


Data Path : U:\HPCHEM1\BNA F\Data\BF011118\
 Data File : BF102006.D
 Acq On : 11 Jan 2018 8:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

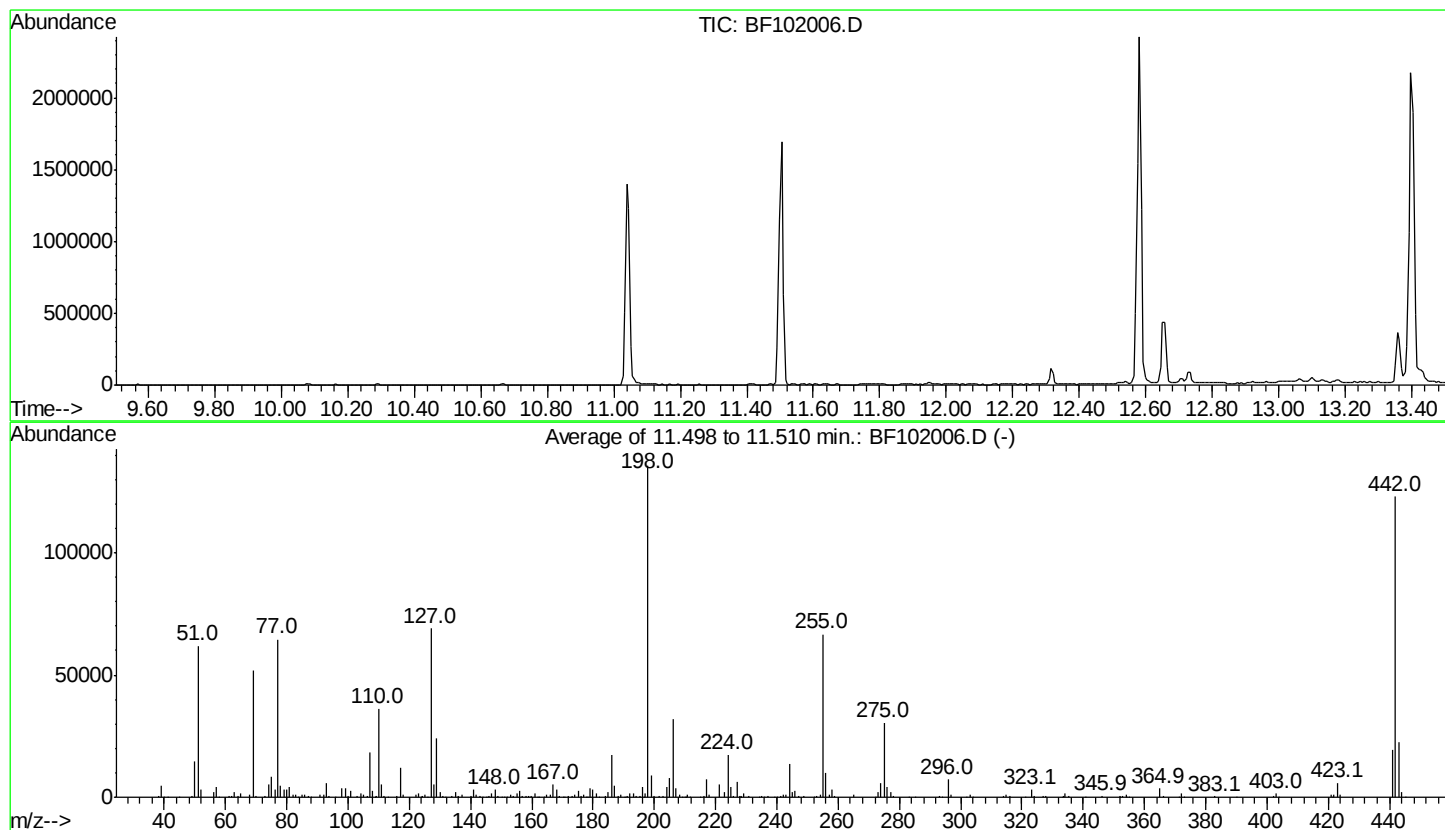

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	61978	PASS
68	69	0.00	2	1.8	953	PASS
69	198	0.00	100	38.1	51701	PASS
70	69	0.00	2	0.6	311	PASS
127	198	10	80	50.9	69069	PASS
197	198	0.00	2	1.1	1488	PASS
198	198	100	100	100.0	135693	PASS
199	198	5	9	6.6	8927	PASS
275	198	10	60	22.5	30568	PASS
365	198	1	100	2.6	3479	PASS
441	443	0.01	100	86.2	19652	PASS
442	198	50	100	90.6	122933	PASS
443	442	15	24	18.5	22800	PASS