


Data Path : U:\HPCHEM1\BNA F\Data\BF011118\
 Data File : BF102017.D
 Acq On : 11 Jan 2018 14:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

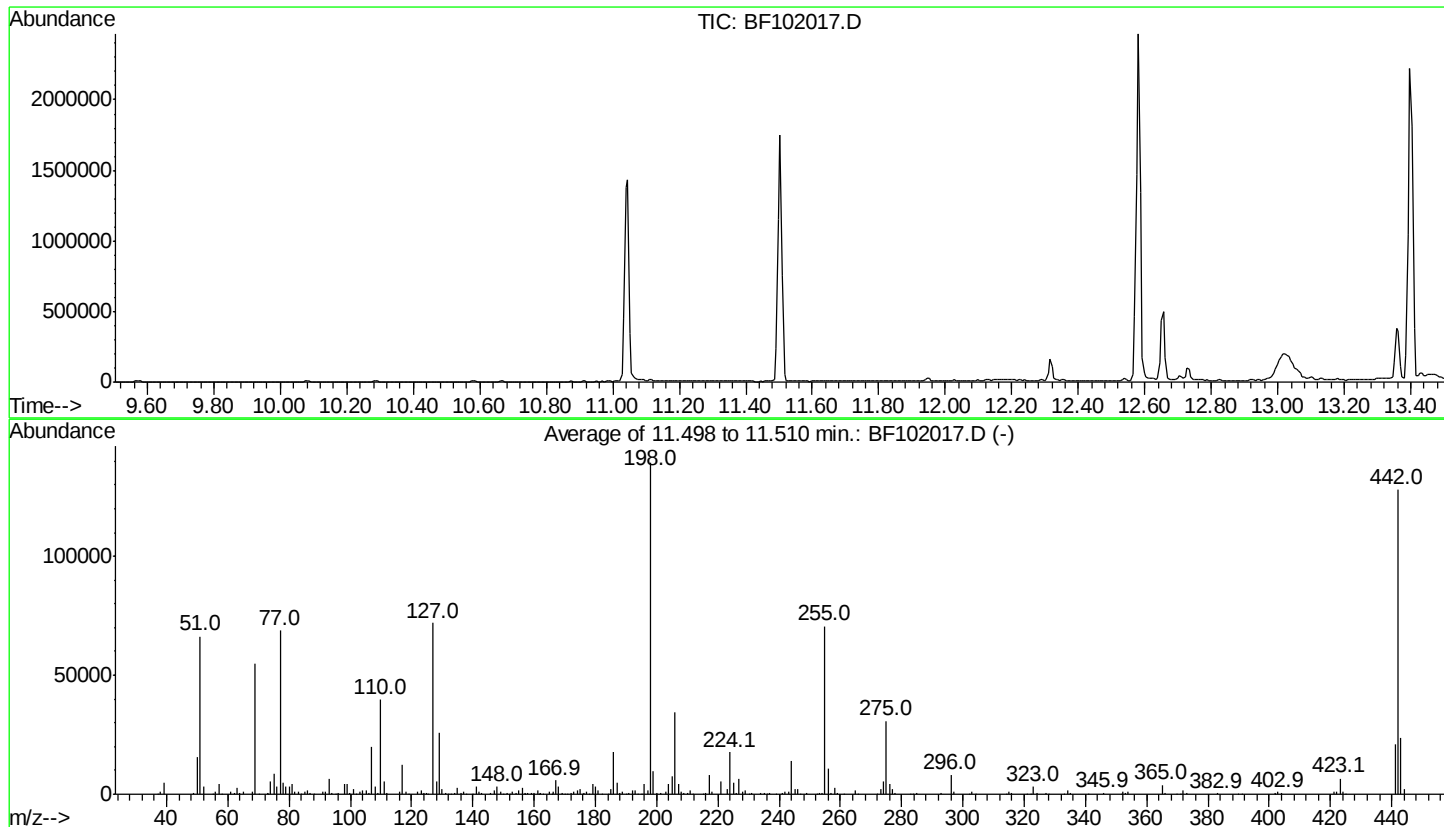

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	66309	PASS
68	69	0.00	2	1.9	1058	PASS
69	198	0.00	100	39.3	54825	PASS
70	69	0.00	2	0.4	244	PASS
127	198	10	80	51.7	72085	PASS
197	198	0.00	2	1.1	1596	PASS
198	198	100	100	100.0	139352	PASS
199	198	5	9	6.9	9581	PASS
275	198	10	60	22.1	30749	PASS
365	198	1	100	2.8	3970	PASS
441	443	0.01	100	87.9	20955	PASS
442	198	50	100	91.8	127877	PASS
443	442	15	24	18.6	23828	PASS