
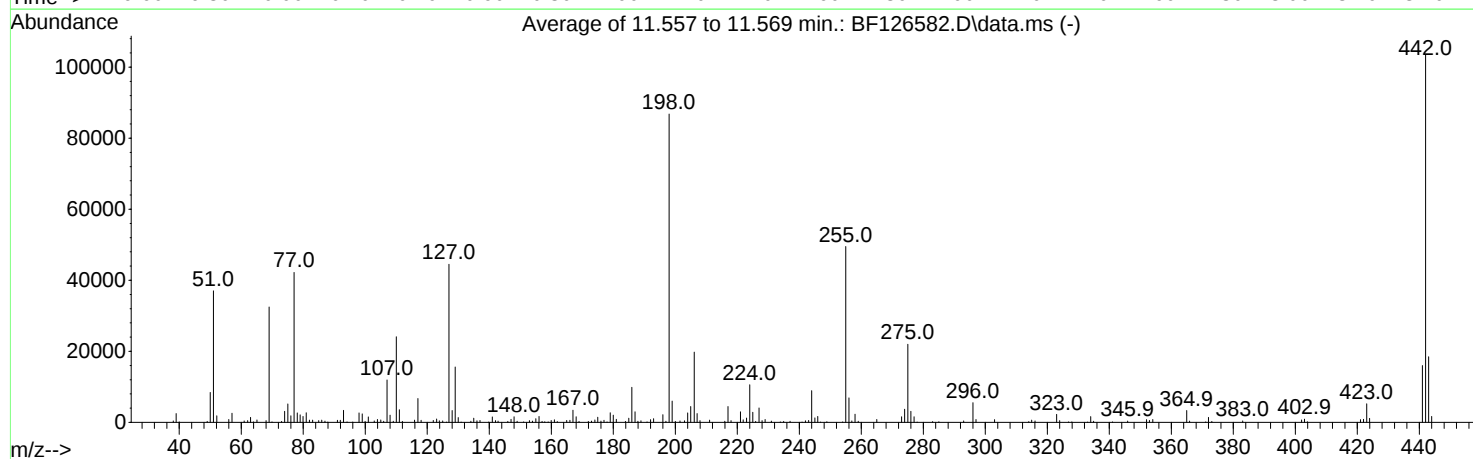


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011122\  
 Data File : BF126582.D  
 Acq On : 11 Jan 2022 9:35  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jan 10 14:50:31 2022

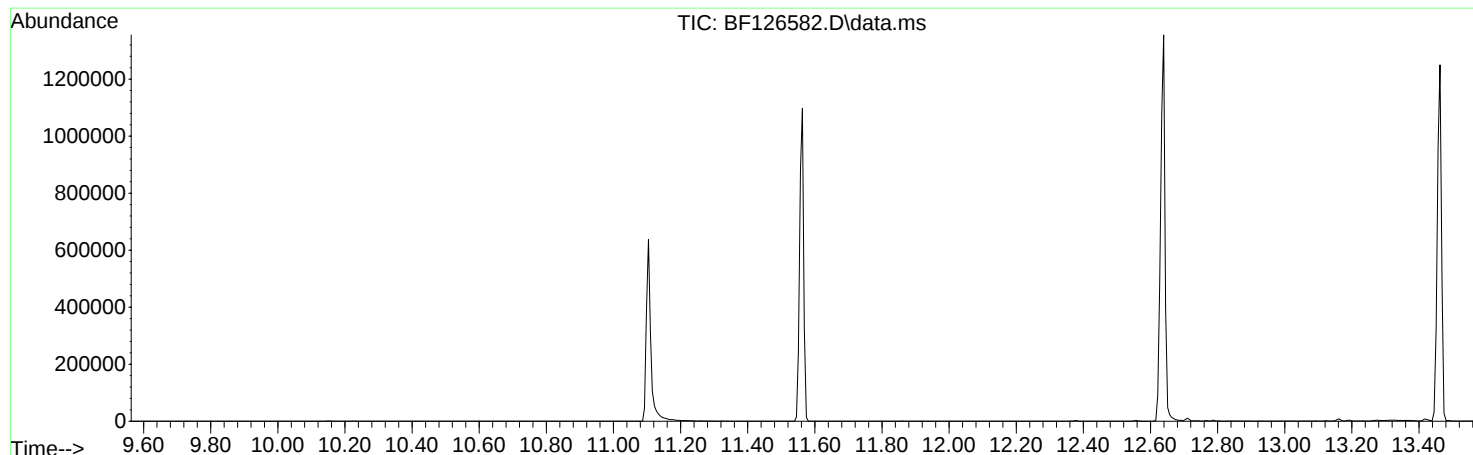

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.6         | 37021      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 491        | PASS                |
| 69             | 198             | 0.00            | 100             | 37.4         | 32456      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 119        | PASS                |
| 127            | 198             | 10              | 80              | 51.3         | 44522      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 333        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 86816      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 5980       | PASS                |
| 275            | 198             | 10              | 60              | 25.3         | 21997      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 3338       | PASS                |
| 441            | 198             | 0.01            | 100             | 18.4         | 15980      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 103560     | PASS                |
| 443            | 442             | 15              | 24              | 17.8         | 18474      | PASS                |

# DDT Breakdown


| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/11/2022     | BNA_F            | <u>BF126582.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 214253           | 13.46              |
| DDD           | 2281             | 13.16              |
| DDE           | 112              | 12.82              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2393          | 216646           | 1.10               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011122\  
Data File : BF126582.D  
Acq On : 11 Jan 2022 9:35  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 11 15:01:45 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 10 14:50:31 2022  
Response via : Initial Calibration

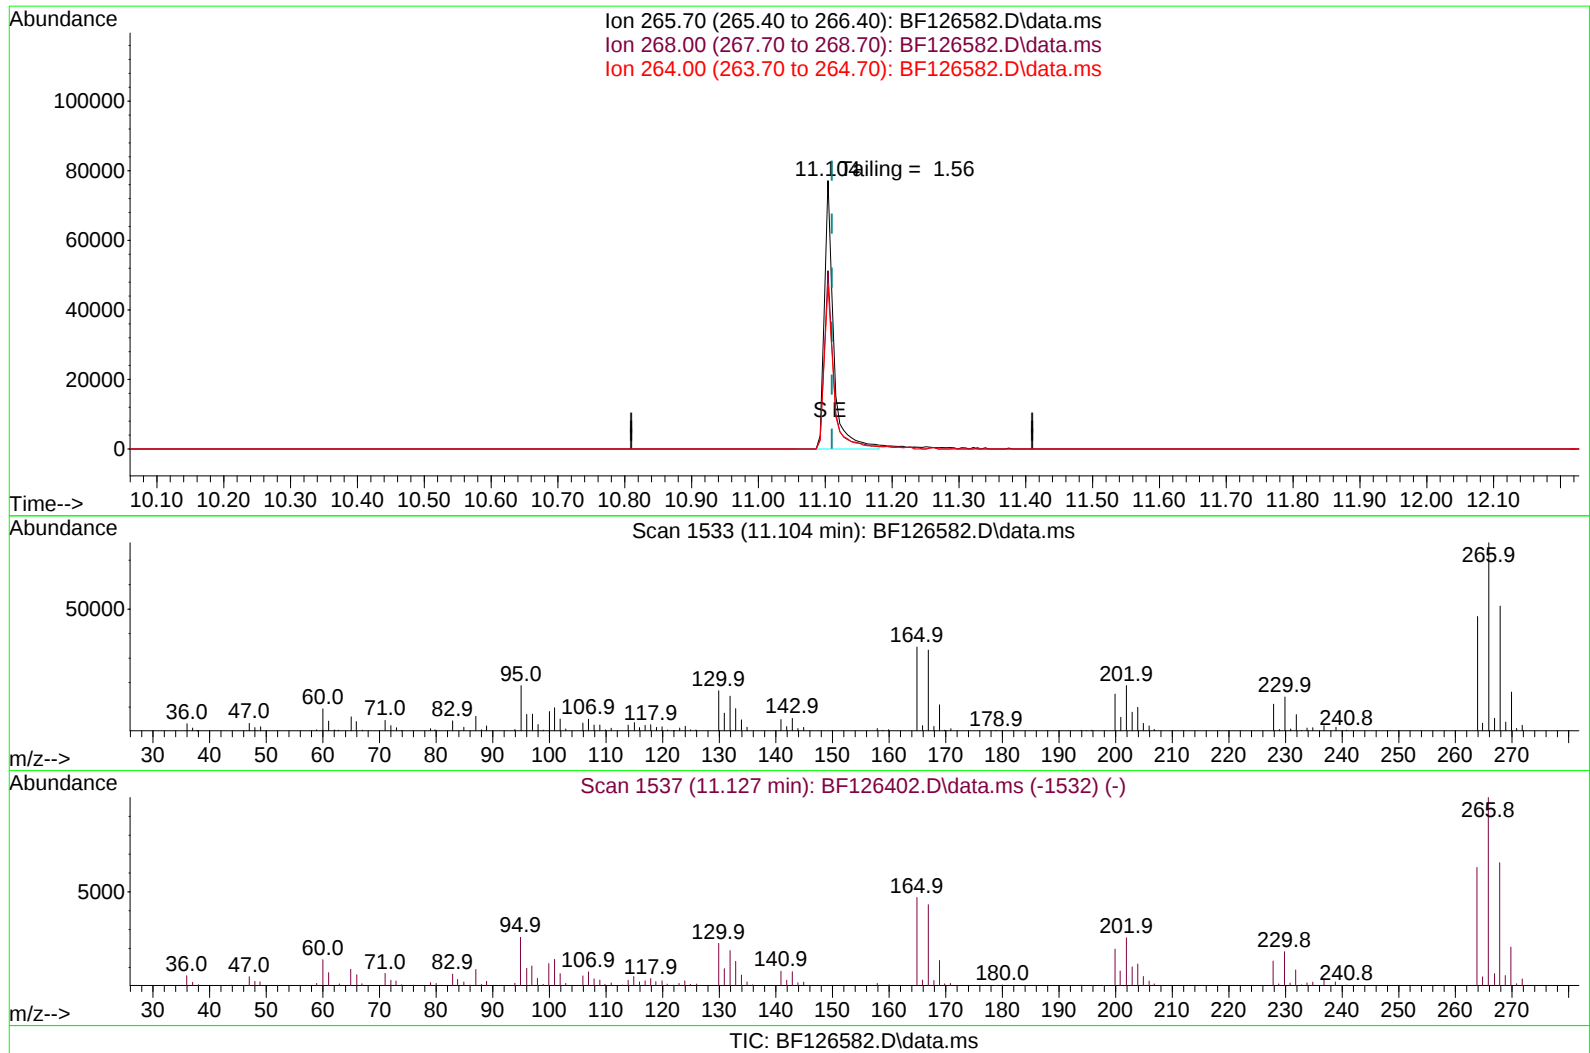

(70) Pentachlorophenol (C)

11.104min (-0.006) 48526.92 ng




response 76462

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.40  | 66.44  |
| 264.00 | 63.00  | 60.95  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011122\  
Data File : BF126582.D  
Acq On : 11 Jan 2022 9:35  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 11 15:01:45 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 10 14:50:31 2022  
Response via : Initial Calibration

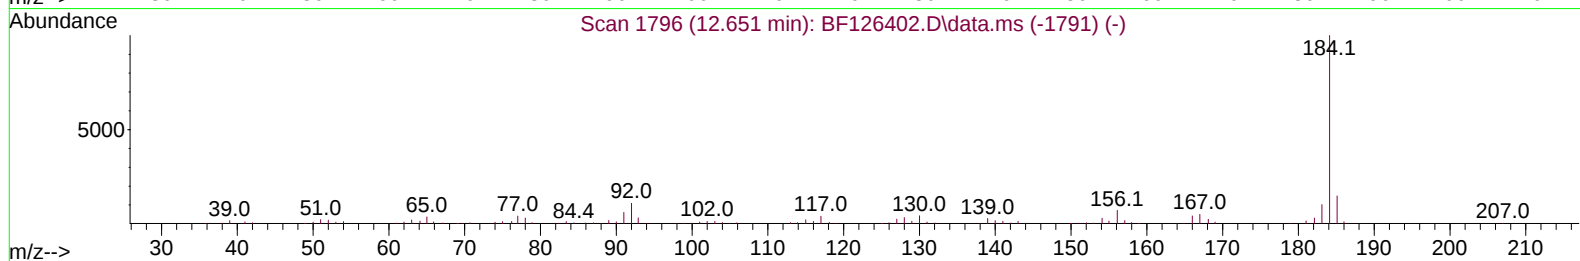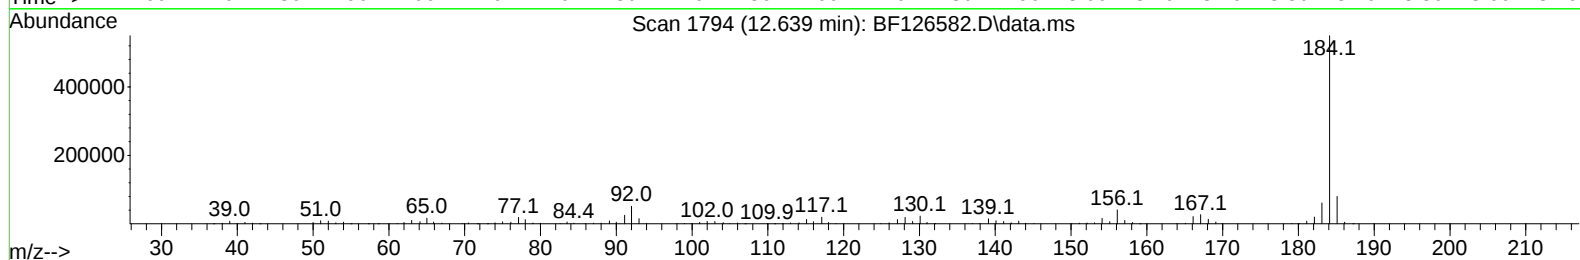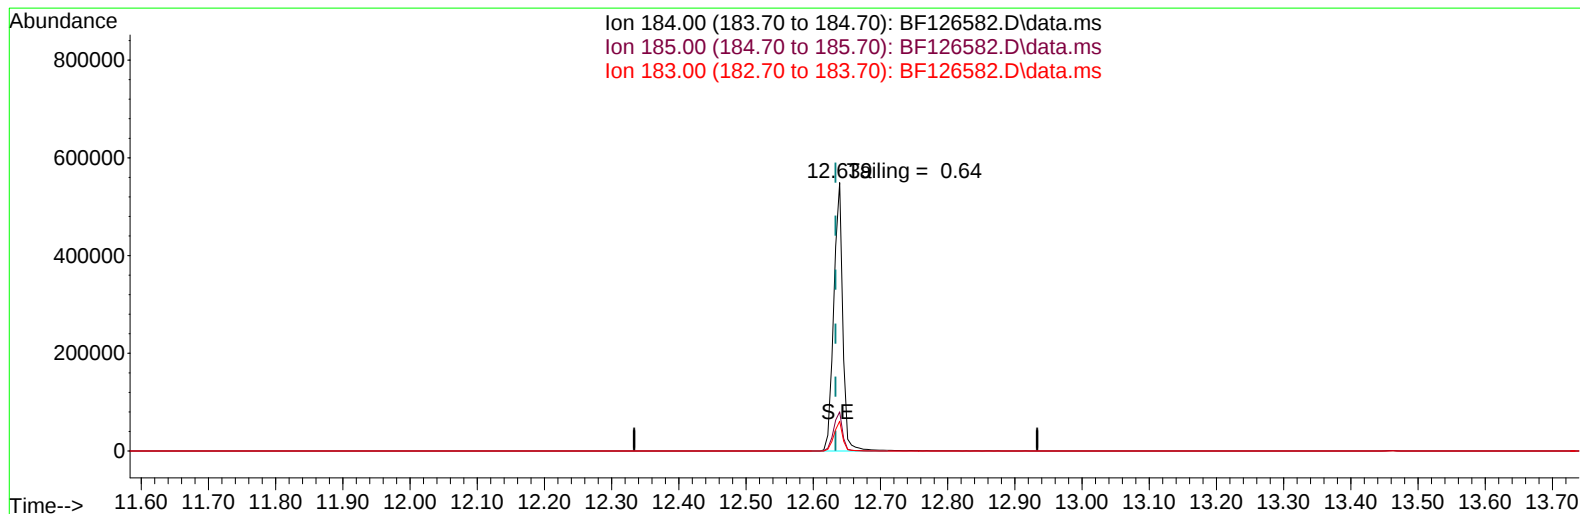

TIC: BF126582.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 0.00 ng

response 510650

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.62  |
| 183.00 | 10.20  | 11.10  |
| 0.00   | 0.00   | 0.00   |