

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011123\
 Data File : BF132021.D
 Acq On : 11 Jan 2023 12:32
 Operator : CG\JU
 Sample : 01079-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SAMPLE-2-INFLUENTRE

Quant Time: Jan 11 14:25:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 00:32:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.775	152	70831	20.000	ng	-0.01
21) Naphthalene-d8	8.069	136	265331	20.000	ng	-0.01
39) Acenaphthene-d10	9.828	164	158373	20.000	ng	-0.01
64) Phenanthrene-d10	11.322	188	299982	20.000	ng	-0.01
76) Chrysene-d12	13.974	240	148531	20.000	ng	#-0.01
86) Perylene-d12	15.445	264	136854	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.393	112	207344	48.236	ng	0.00
7) Phenol-d6	6.422	99	192059	33.698	ng	-0.01
23) Nitrobenzene-d5	7.351	82	624028	97.611	ng	-0.02
42) 2,4,6-Tribromophenol	10.628	330	188952	103.766	ng	-0.01
45) 2-Fluorobiphenyl	9.151	172	1137581	96.967	ng	-0.01
79) Terphenyl-d14	12.922	244	1294843	124.948	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011123\
Data File : BF132021.D
Acq On : 11 Jan 2023 12:32
Operator : CG\JU
Sample : 01079-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SAMPLE-2-INFLUENTRE

Quant Time: Jan 11 14:25:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration




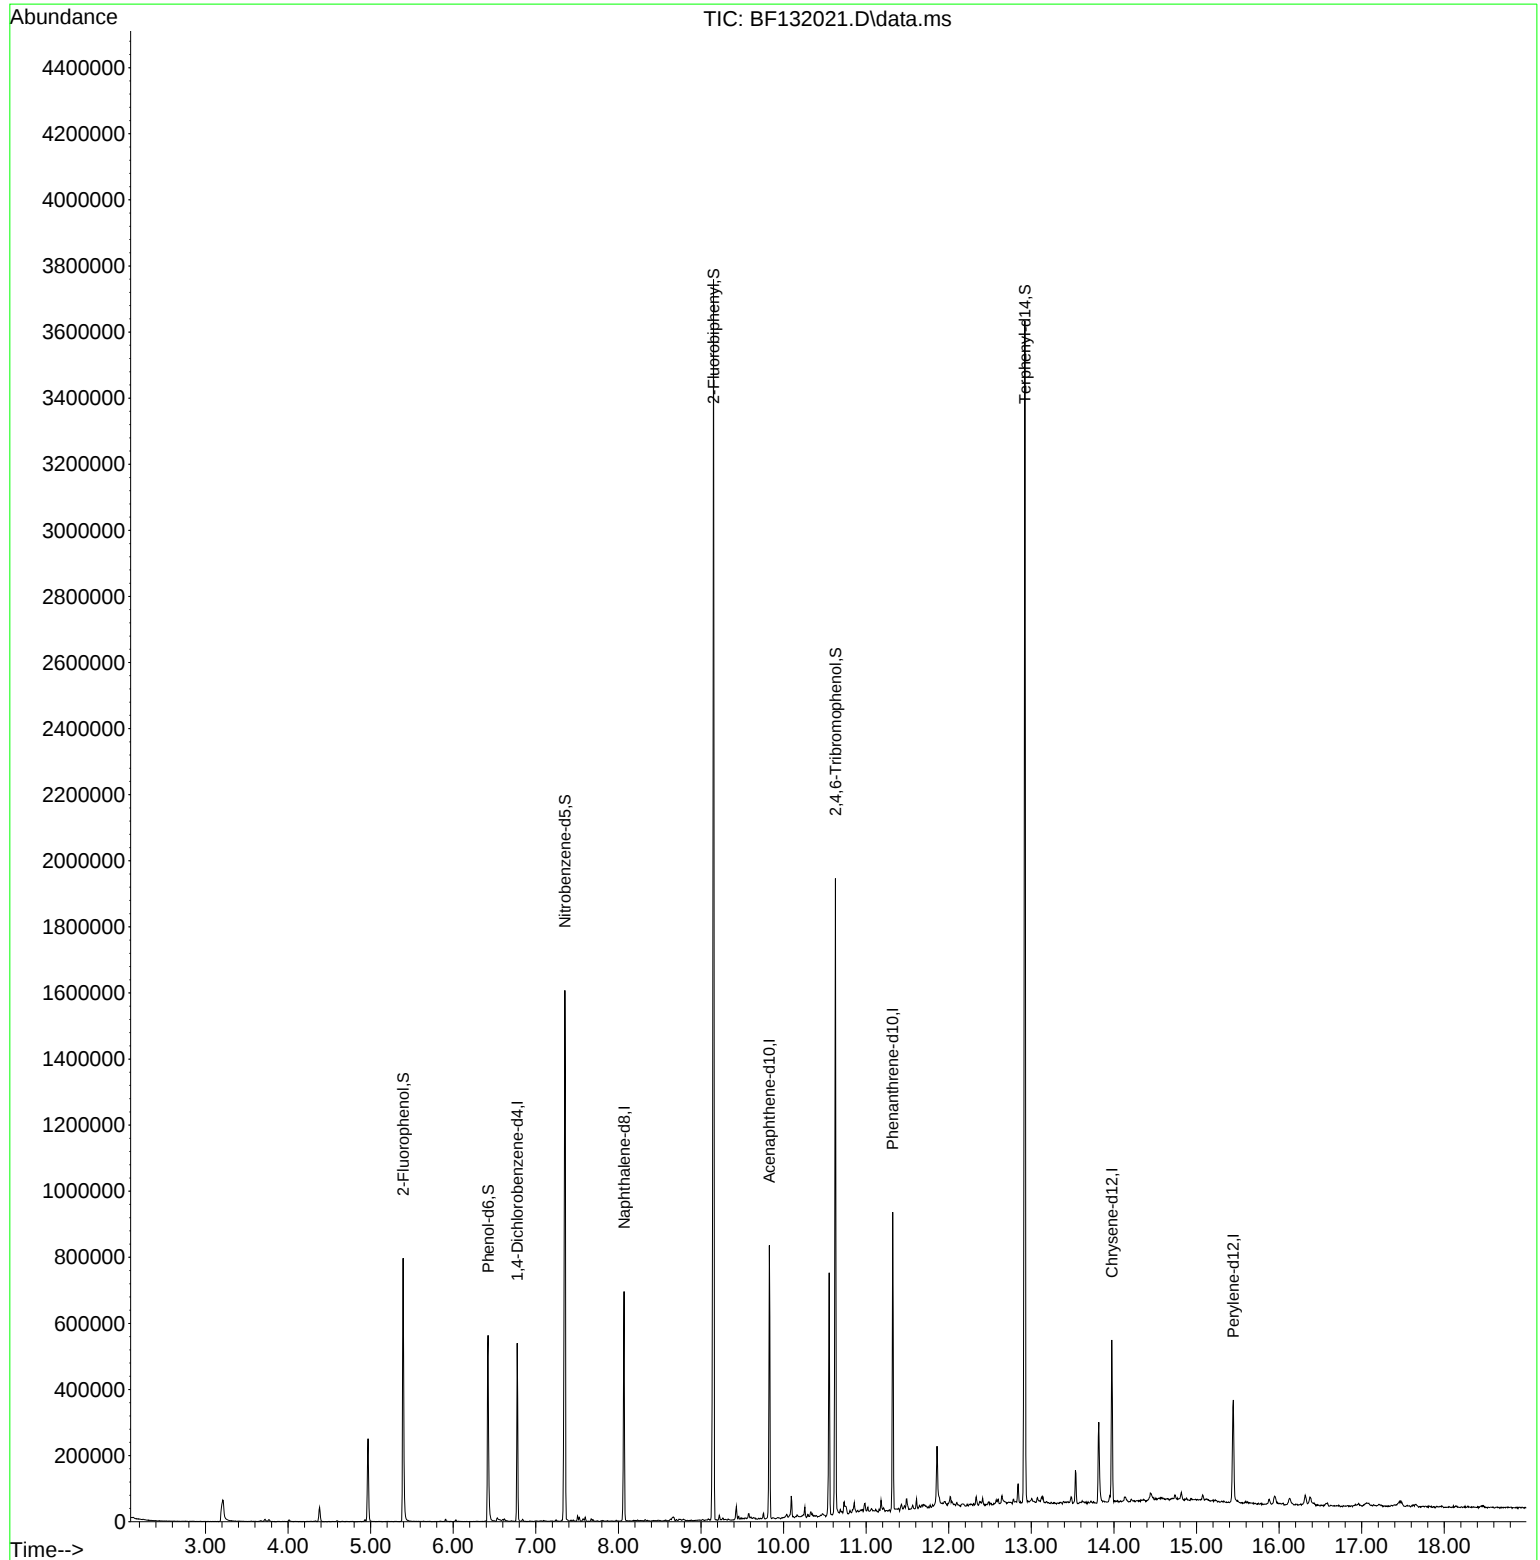


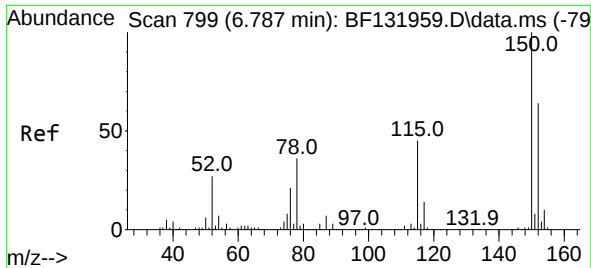

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.775 min Scan# 799
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32




Instrument :
BNA_F
ClientSampleId :
SAMPLE-2-INFLUENTRE


Tgt Ion:152 Resp: 70831
Ion Ratio Lower Upper
152 100
150 142.0 124.6 186.8
115 67.7 55.6 83.4

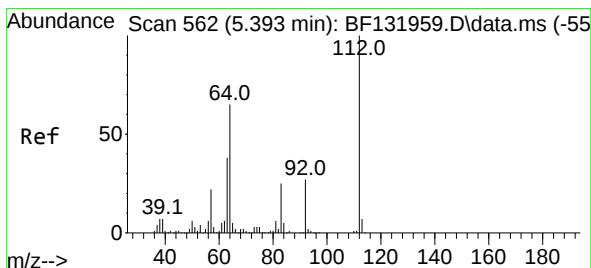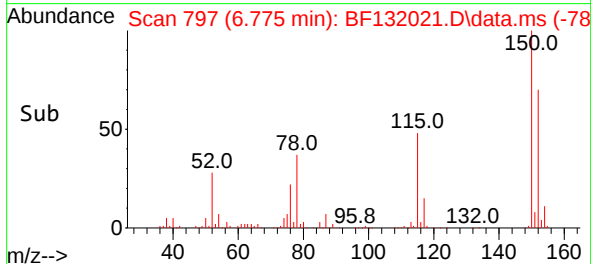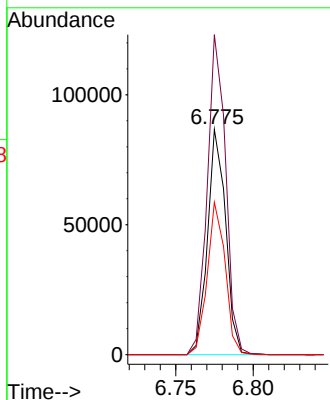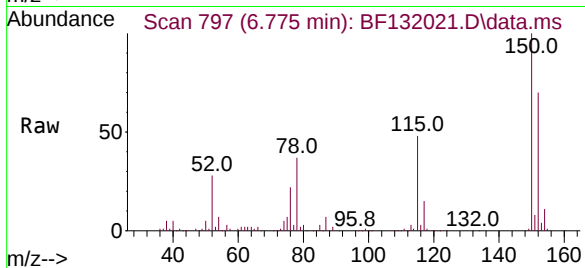

#5
2-Fluorophenol
Concen: 48.236 ng
RT: 5.393 min Scan# 562
Delta R.T. -0.000 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32

Tgt Ion:112 Resp: 207344
Ion Ratio Lower Upper
112 100
64 64.4 51.9 77.9
63 37.0 30.2 45.2


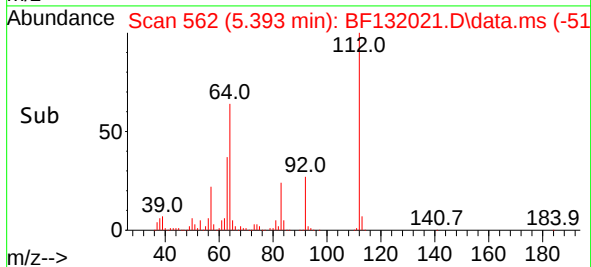
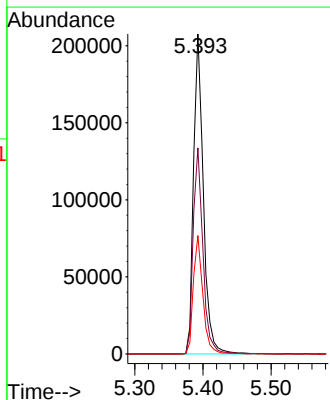
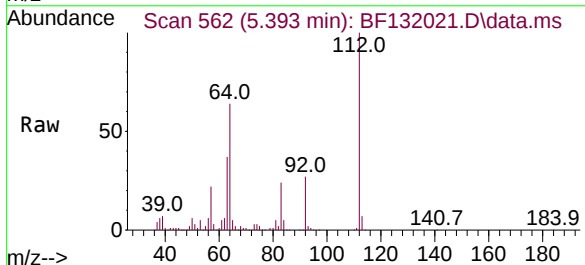


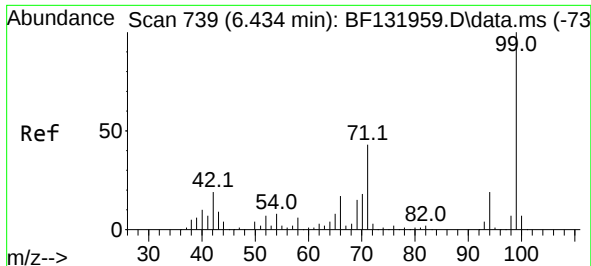

#7
Phenol-d6
Concen: 33.698 ng
RT: 6.422 min Scan# 739
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32




Instrument :
BNA_F
ClientSampleId :
SAMPLE-2-INFLUENTRE


Tgt Ion: 99 Resp: 192059
Ion Ratio Lower Upper
99 100
42 18.1 15.4 23.2
71 42.4 34.6 51.8

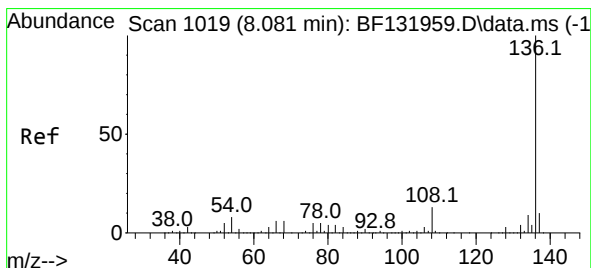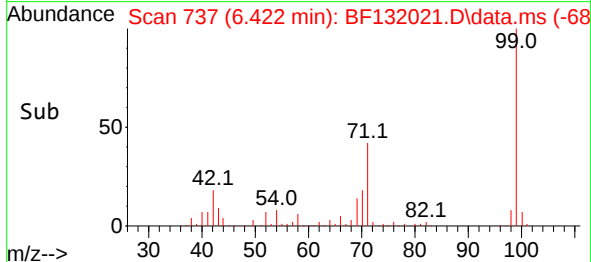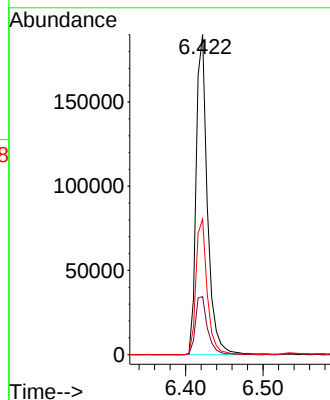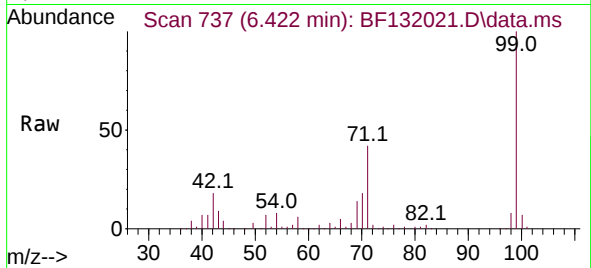

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.069 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32

Tgt Ion: 136 Resp: 265331
Ion Ratio Lower Upper
136 100
137 11.1 8.2 12.2
54 7.6 6.6 9.8
68 5.4 4.5 6.7


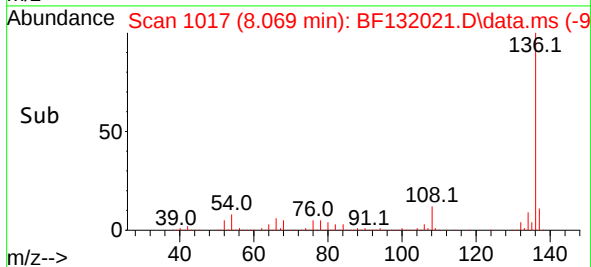
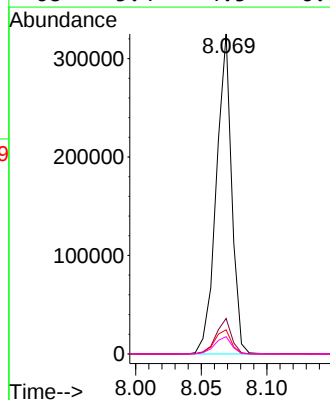
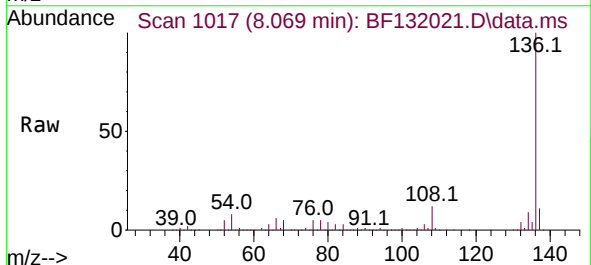


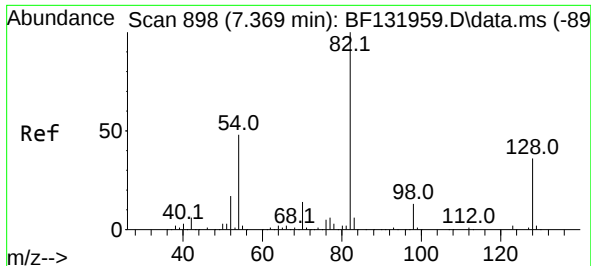

#23
Nitrobenzene-d5
Concen: 97.611 ng
RT: 7.351 min Scan# 89
Delta R.T. -0.018 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32




Instrument :
BNA_F
ClientSampleId :
SAMPLE-2-INFLUENTRE


Tgt Ion: 82 Resp: 624028
Ion Ratio Lower Upper
82 100
128 34.2 28.7 43.1
54 48.9 38.1 57.1

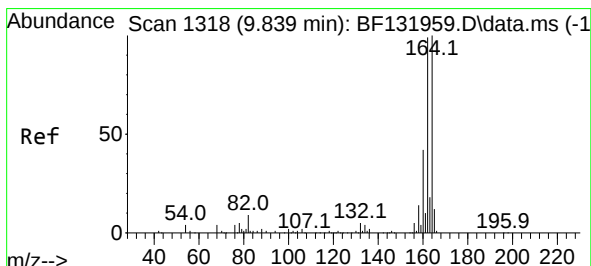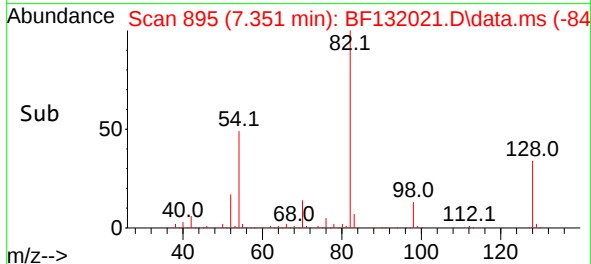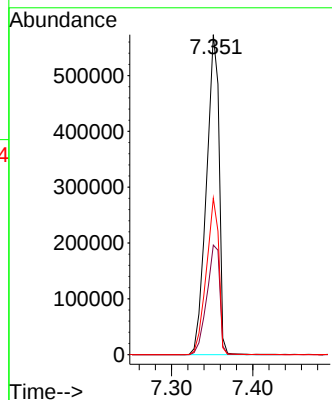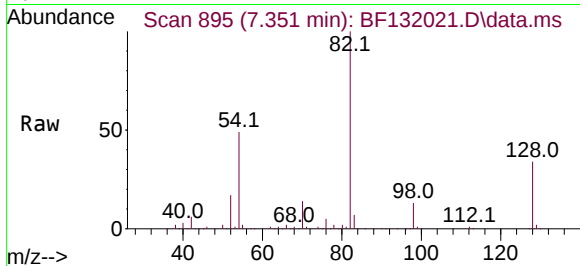

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.828 min Scan# 1316
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32

Tgt Ion:164 Resp: 158373
Ion Ratio Lower Upper
164 100
162 99.9 79.4 119.0
160 45.1 33.9 50.9

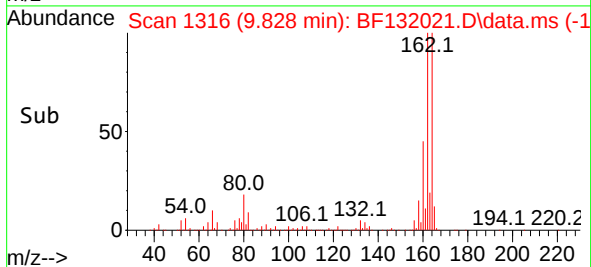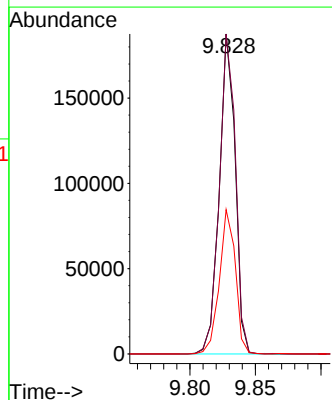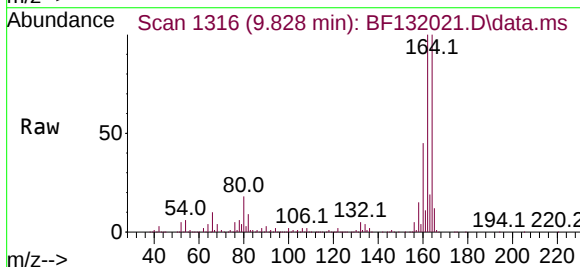

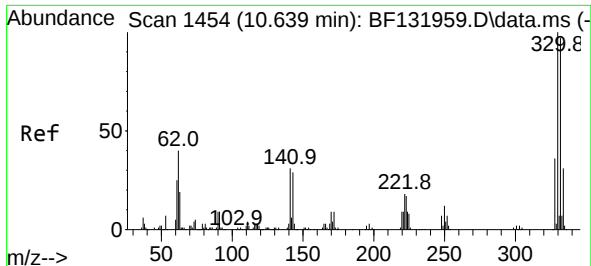

#42

2,4,6-Tribromophenol

Concen: 103.766 ng

RT: 10.628 min Scan# 1454

Delta R.T. -0.012 min

Lab File: BF132021.D


Acq: 11 Jan 2023 12:32

Instrument :

BNA_F

ClientSampleId :

SAMPLE-2-INFLUENTRE

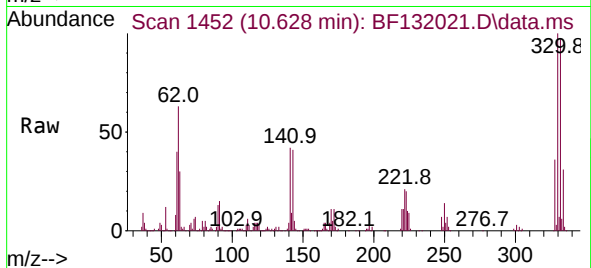




Tgt Ion:330 Resp: 188952

Ion Ratio Lower Upper

330 100

332 97.0 76.9 115.3

141 40.4 31.3 46.9

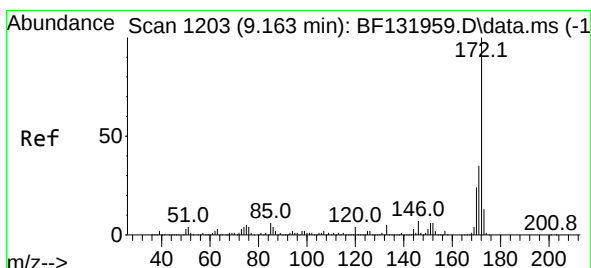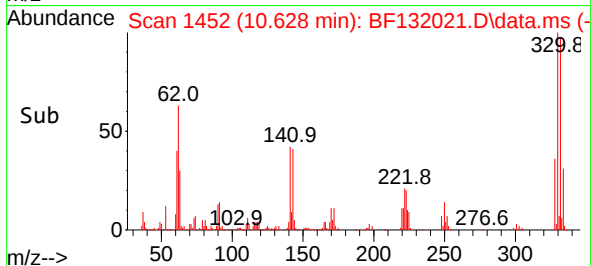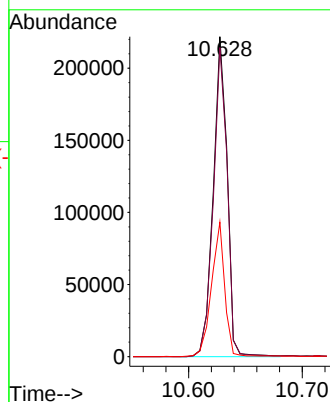

#45

2-Fluorobiphenyl

Concen: 96.967 ng

RT: 9.151 min Scan# 1201

Delta R.T. -0.012 min

Lab File: BF132021.D

Acq: 11 Jan 2023 12:32




Tgt Ion:172 Resp: 1137581


Ion Ratio Lower Upper

172 100

171 34.9 28.0 42.0

170 23.7 18.9 28.3


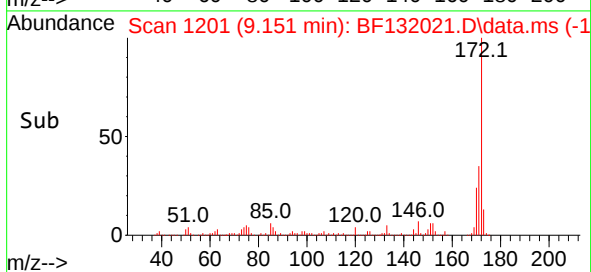
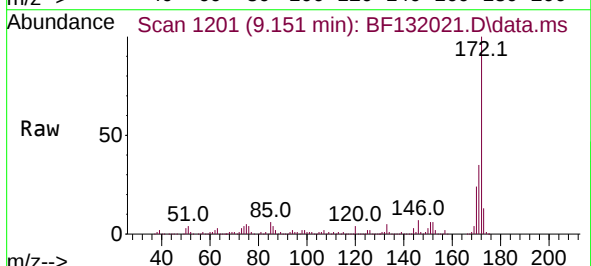
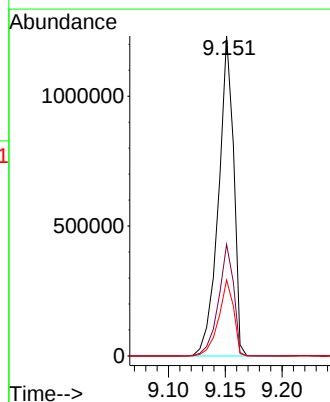


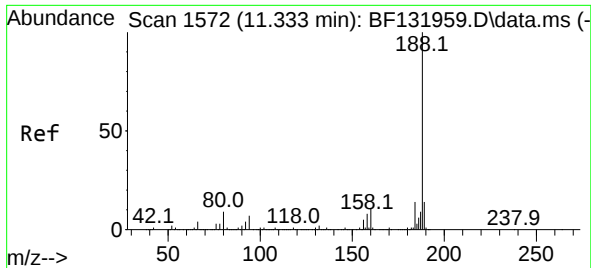

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.322 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32




Instrument :
BNA_F
ClientSampleId :
SAMPLE-2-INFLUENTRE


Tgt Ion:188 Resp: 299982
Ion Ratio Lower Upper
188 100
94 7.8 5.8 8.6
80 9.2 7.4 11.0

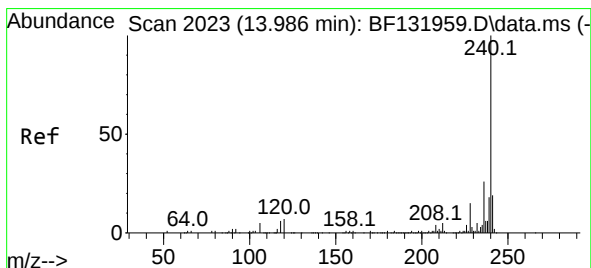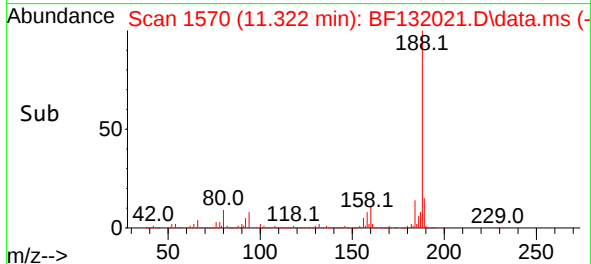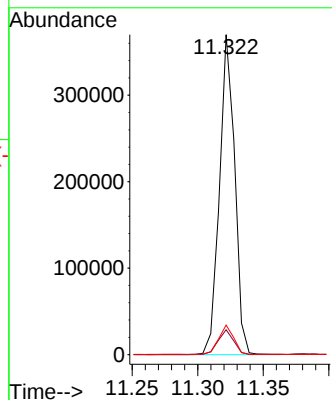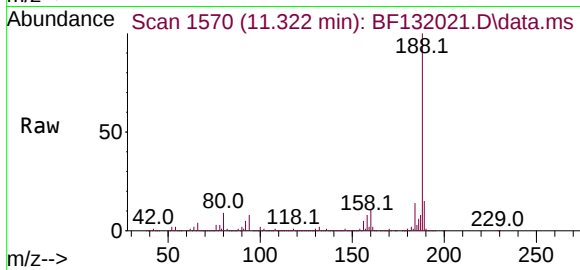

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.974 min Scan# 2021
Delta R.T. -0.012 min
Lab File: BF132021.D
Acq: 11 Jan 2023 12:32

Tgt Ion:240 Resp: 148531
Ion Ratio Lower Upper
240 100
120 8.2 5.4 8.0#
236 26.1 21.1 31.7


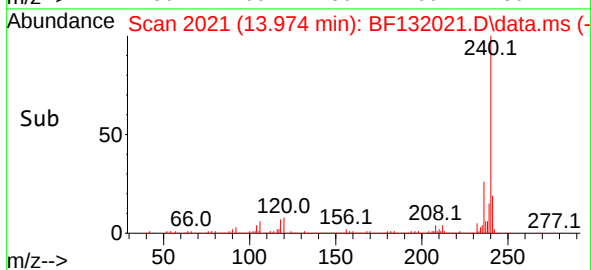
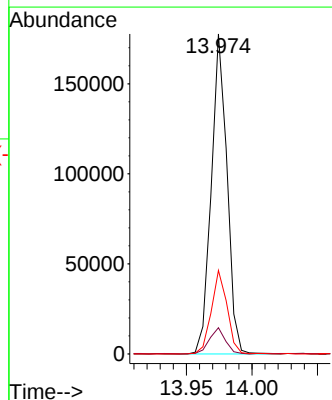
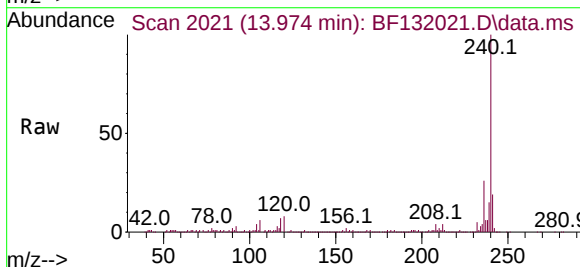


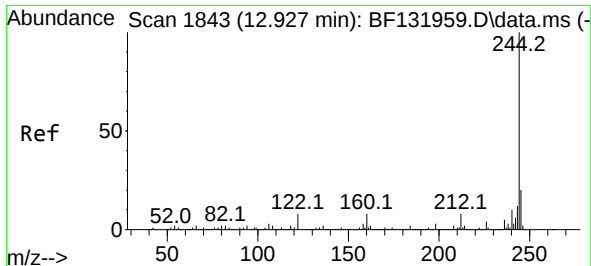

#79
 Terphenyl-d14
 Concen: 124.948 ng
 RT: 12.922 min Scan# 1843
 Delta R.T. -0.006 min
 Lab File: BF132021.D
 Acq: 11 Jan 2023 12:32

Instrument :
 BNA_F
 ClientSampleId :
 SAMPLE-2-INFLUENTRE

Tgt Ion:244 Resp: 1294843
 Ion Ratio Lower Upper
 244 100
 212 8.2 6.3 9.5
 122 9.5 6.8 10.2

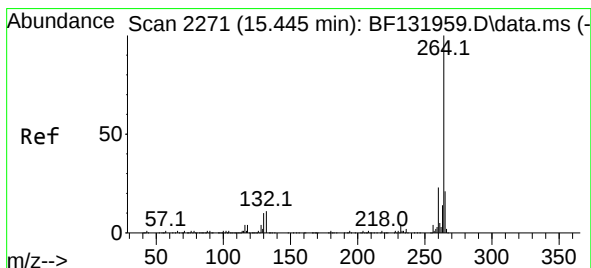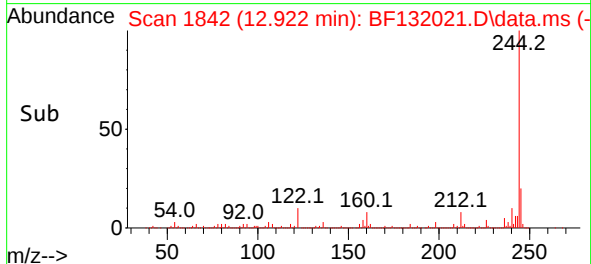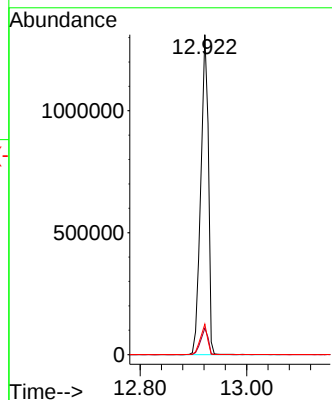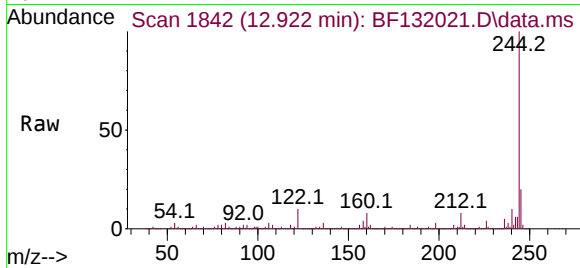

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.445 min Scan# 2271
 Delta R.T. -0.000 min
 Lab File: BF132021.D
 Acq: 11 Jan 2023 12:32

Tgt Ion:264 Resp: 136854
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.3 27.5
 265 21.2 16.9 25.3

