


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011123\  
 Data File : BF132017.D  
 Acq On : 11 Jan 2023 10:14  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jan 10 00:32:25 2023

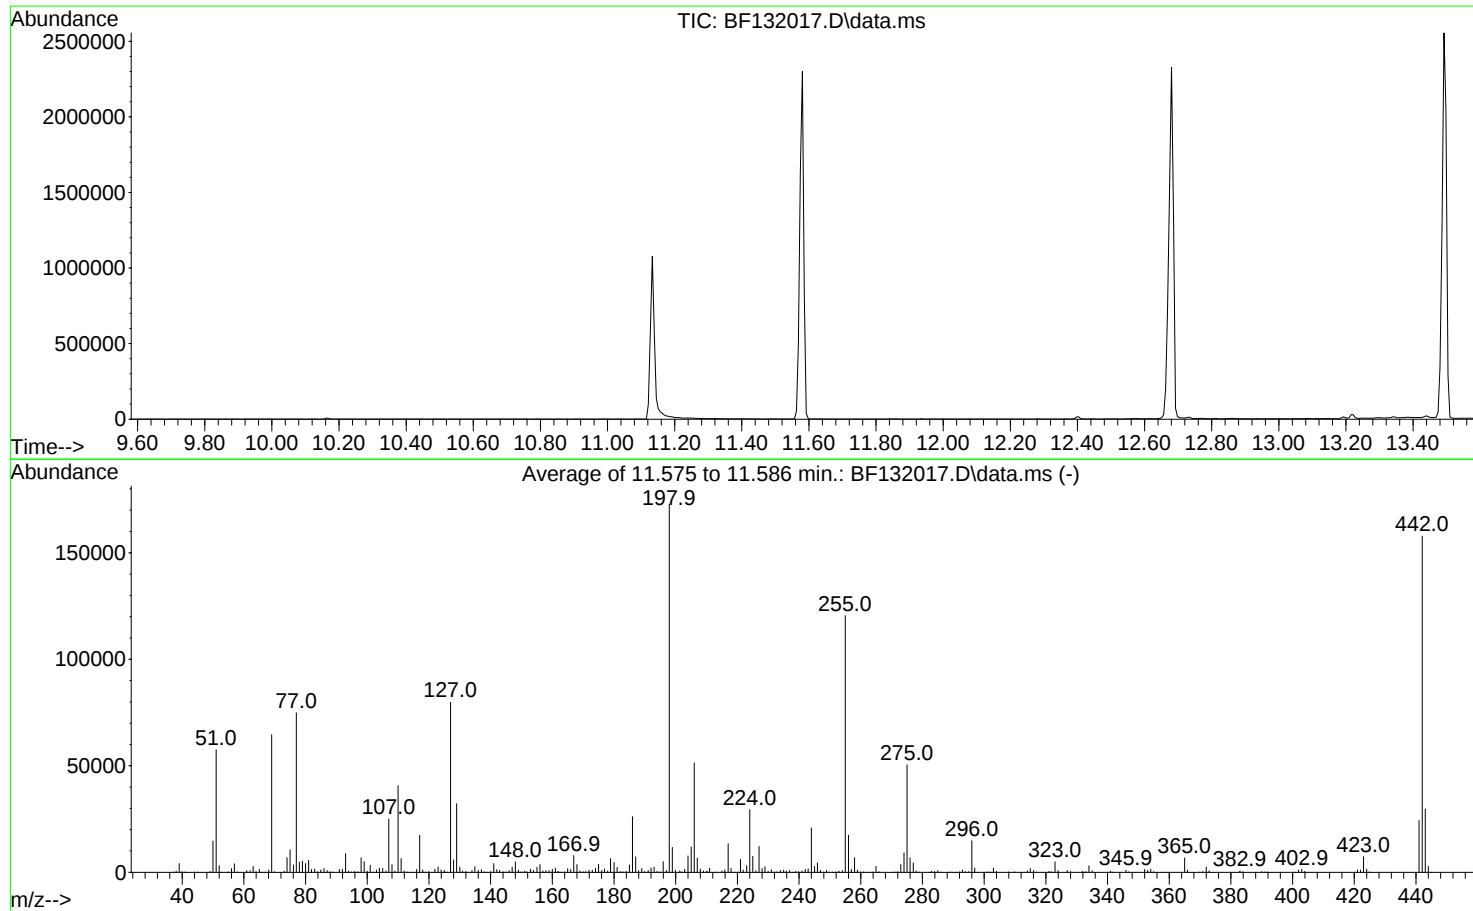




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.3         | 57502      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1135       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.4         | 64579      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 292        | PASS                |
| 127            | 198             | 10              | 80              | 46.2         | 79848      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 779        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 172704     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 11693      | PASS                |
| 275            | 198             | 10              | 60              | 29.2         | 50461      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 6746       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.1         | 24329      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 157816     | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 29749      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011123\  
Data File : BF132017.D  
Acq On : 11 Jan 2023 10:14  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 12 03:29:50 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 10 00:32:25 2023  
Response via : Initial Calibration

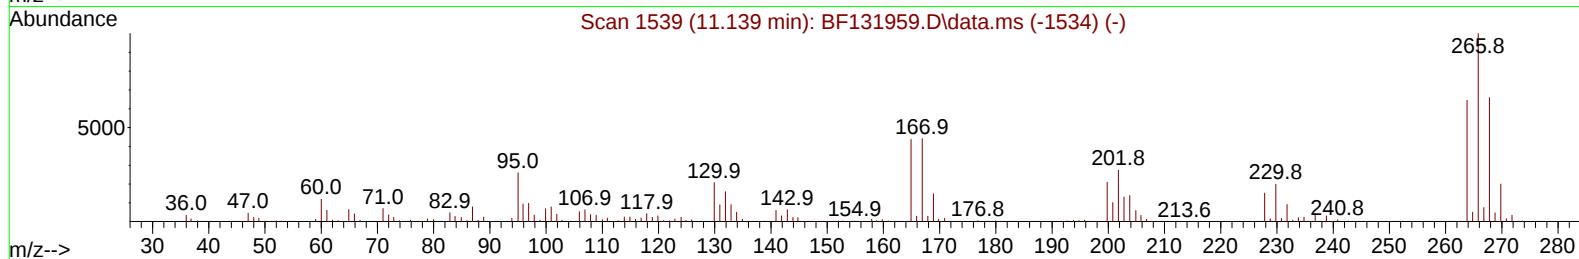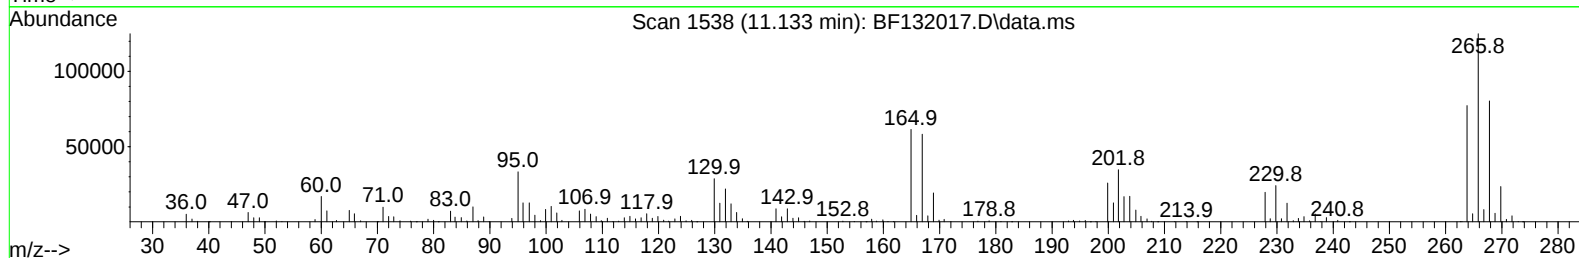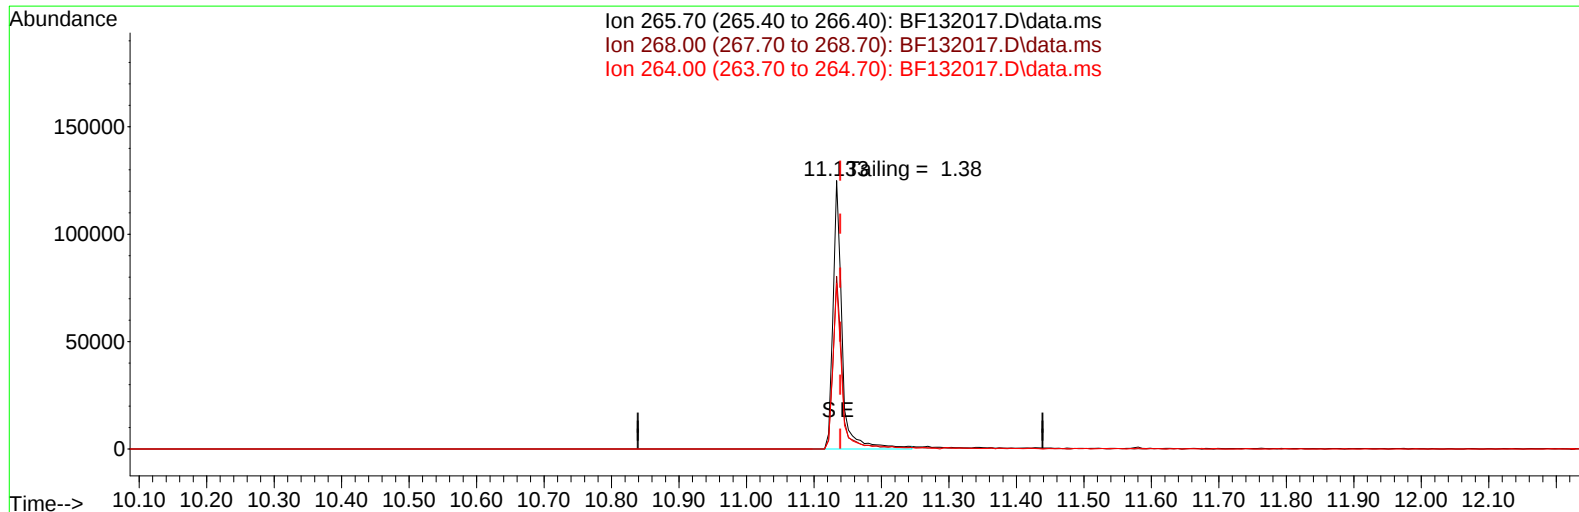

TIC: BF132017.D\data.ms

**(70) Pentachlorophenol (C)**

**11.133min (-0.006) 17874.41 ng**




**response 116191**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.90  | 64.32  |
| 264.00 | 64.50  | 61.80  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011123\  
 Data File : BF132017.D  
 Acq On : 11 Jan 2023 10:14  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 12 03:29:50 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jan 10 00:32:25 2023  
 Response via : Initial Calibration

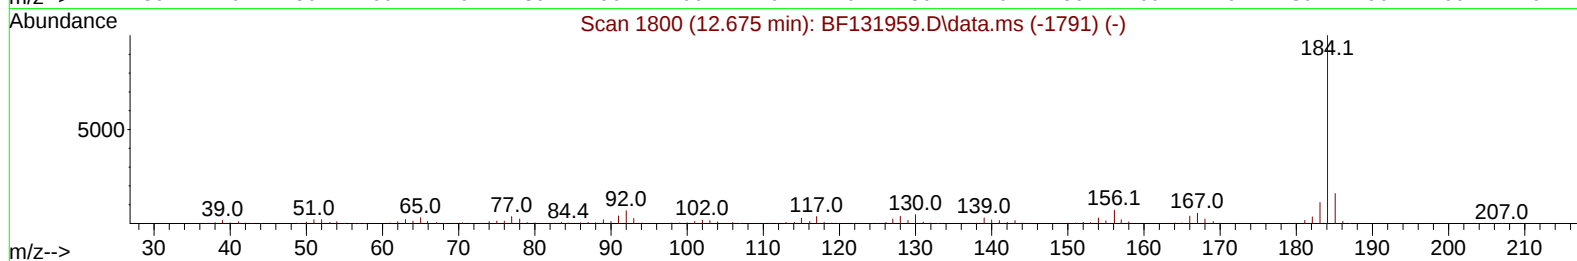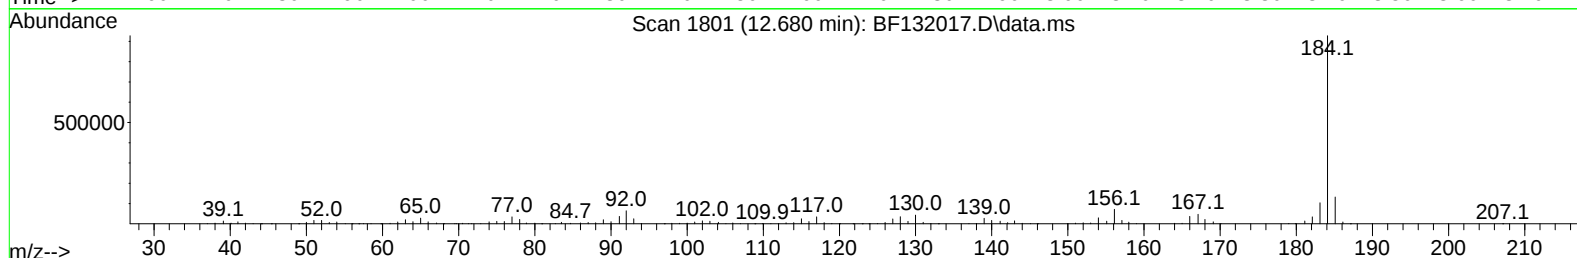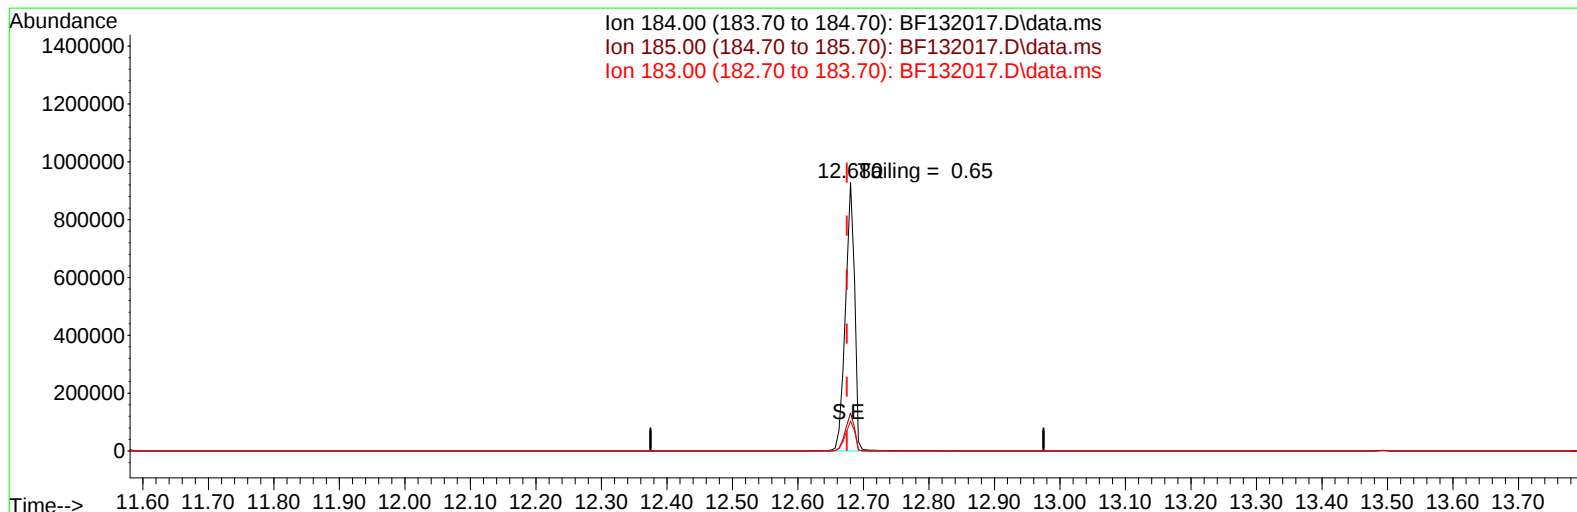

TIC: BF132017.D\data.ms

**(77) Benzidine**

12.680min (+ 0.005) 0.00 ng

response 900922

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 16.00  | 14.22  |
| 183.00 | 11.20  | 11.19  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/11/2023     | BNA_F            | <u>BF132017.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 453435           | 13.492             |
| DDD           | 7105             | 13.222             |
| DDE           | 1026             | 12.857             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 8131          | 461566           | 1.76               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP