
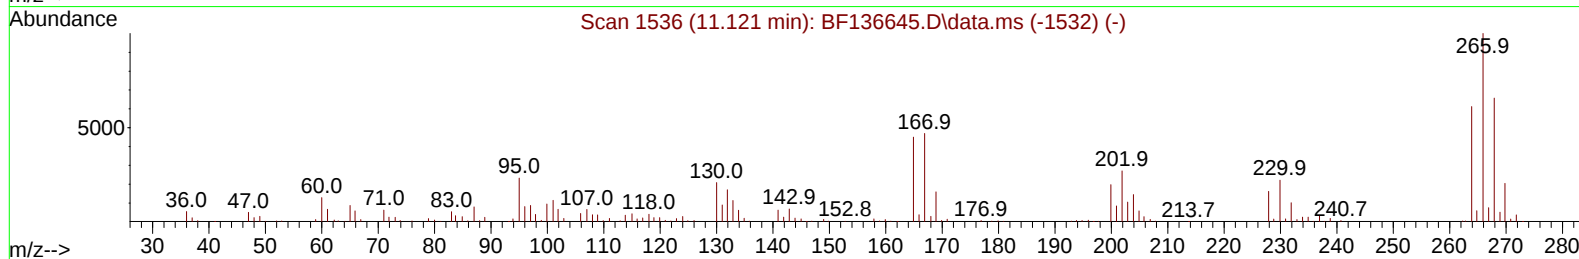
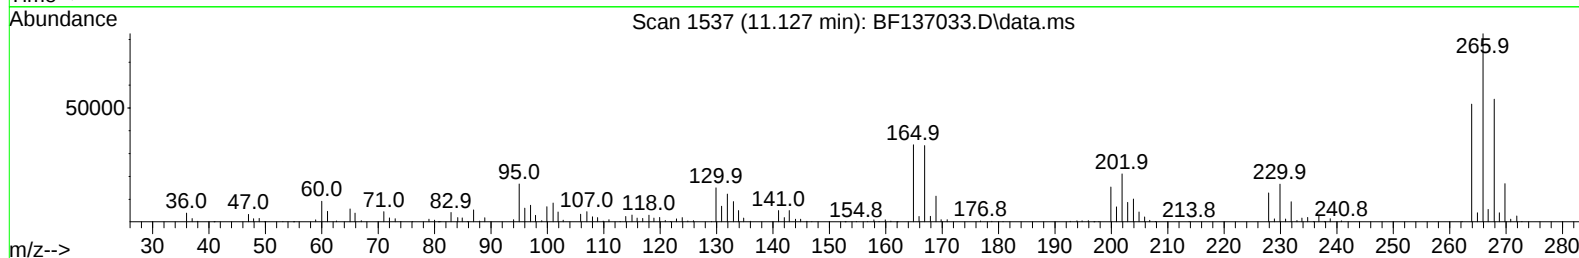


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011124\
Data File : BF137033.D
Acq On : 11 Jan 2024 11:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 12:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

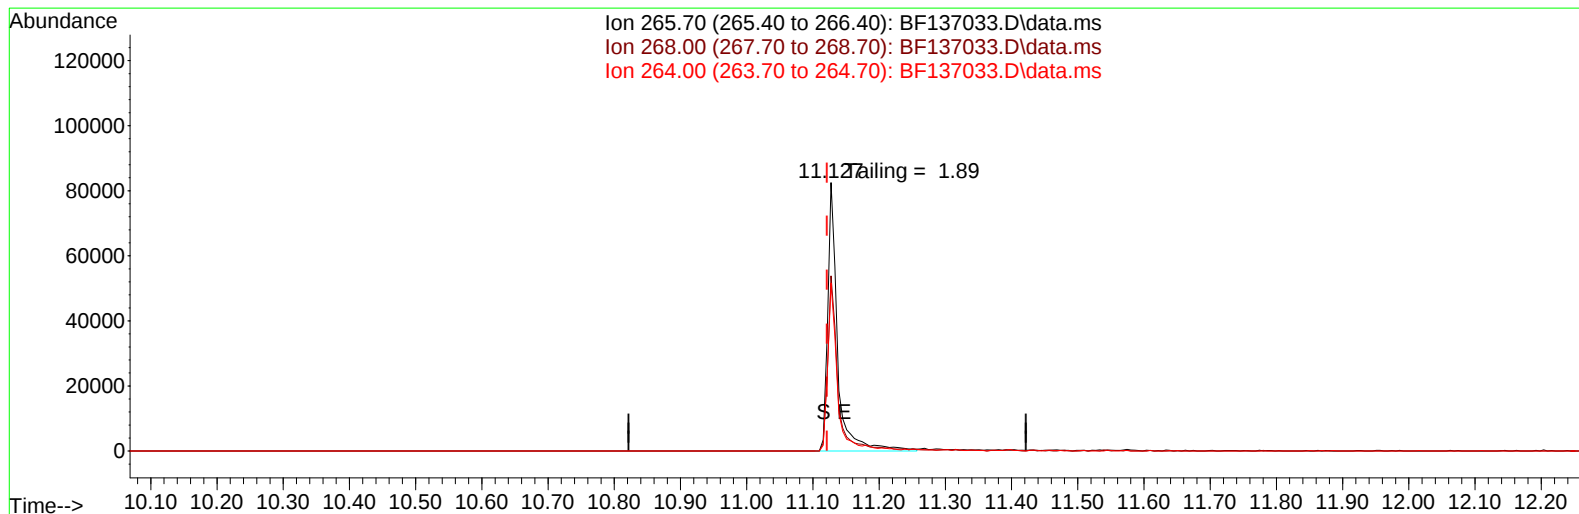

TIC: BF137033.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.006) 31096.62 ng

response 86645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.25
264.00	61.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011124\
Data File : BF137033.D
Acq On : 11 Jan 2024 11:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 12:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

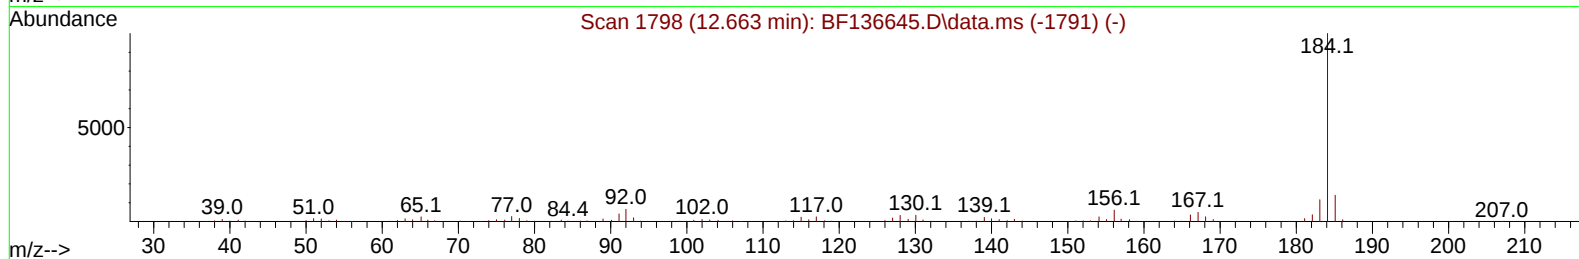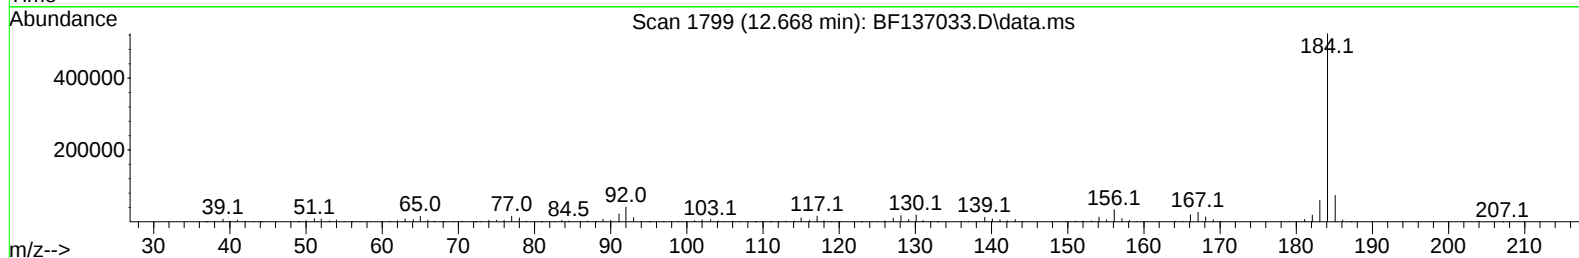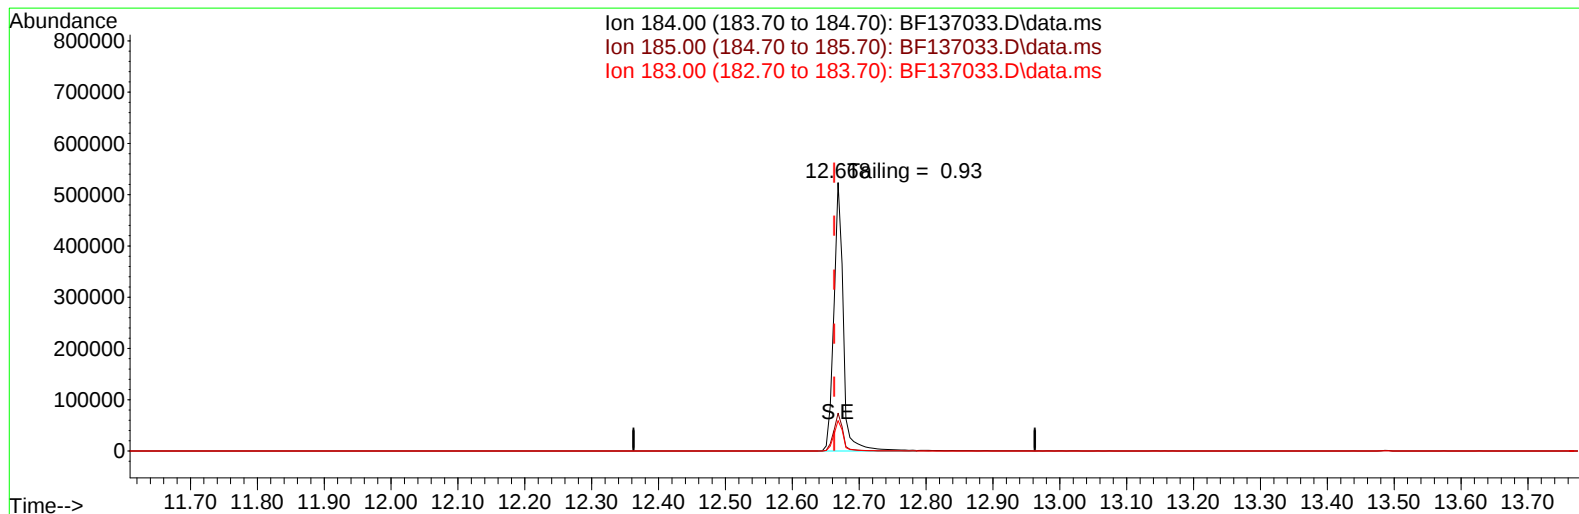

TIC: BF137033.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 157995.44 ng m

response 512447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	11.60	11.37
0.00	0.00	0.00