


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011124\
Data File : BF137033.D
Acq On : 11 Jan 2024 11:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

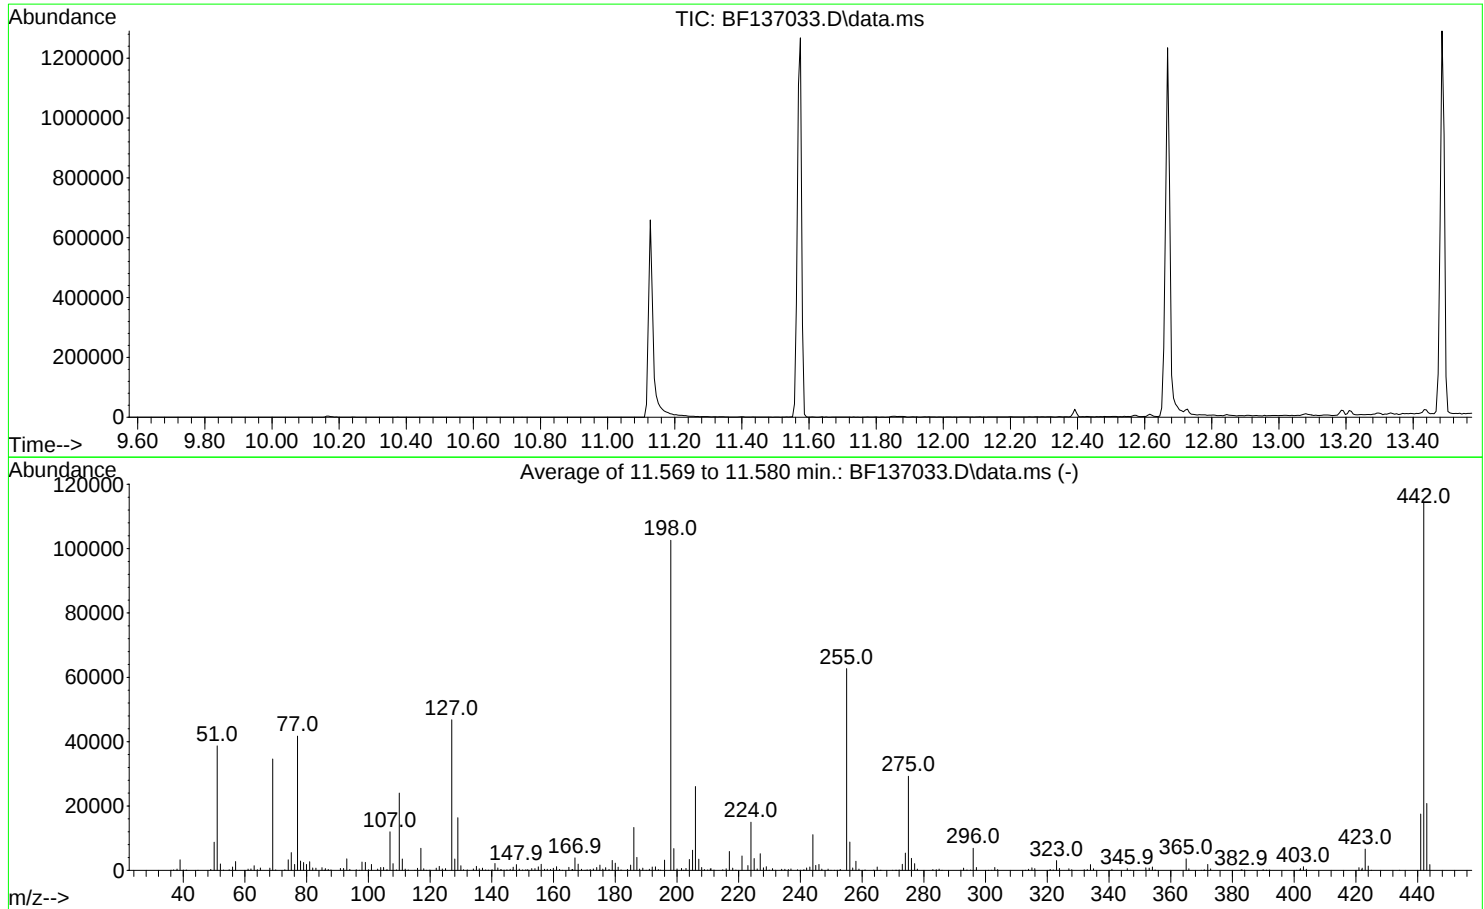




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	38689	PASS
68	69	0.00	2	2.0	683	PASS
69	198	0.00	100	33.7	34595	PASS
70	69	0.00	2	0.5	169	PASS
127	198	10	80	45.6	46786	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102616	PASS
199	198	5	9	6.6	6760	PASS
275	198	10	60	28.5	29258	PASS
365	198	1	100	3.5	3579	PASS
441	198	0.01	100	17.1	17534	PASS
442	442	50	100	100.0	114341	PASS
443	442	15	24	18.2	20797	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011124\
Data File : BF137033.D
Acq On : 11 Jan 2024 11:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 11 12:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

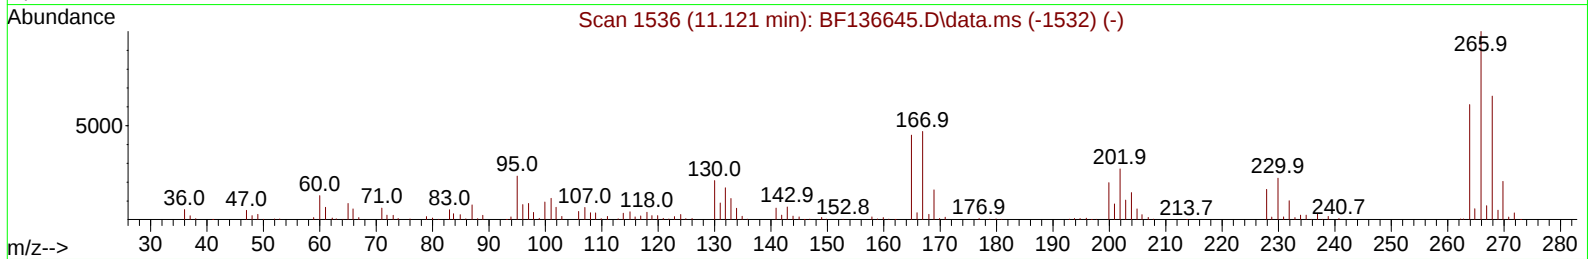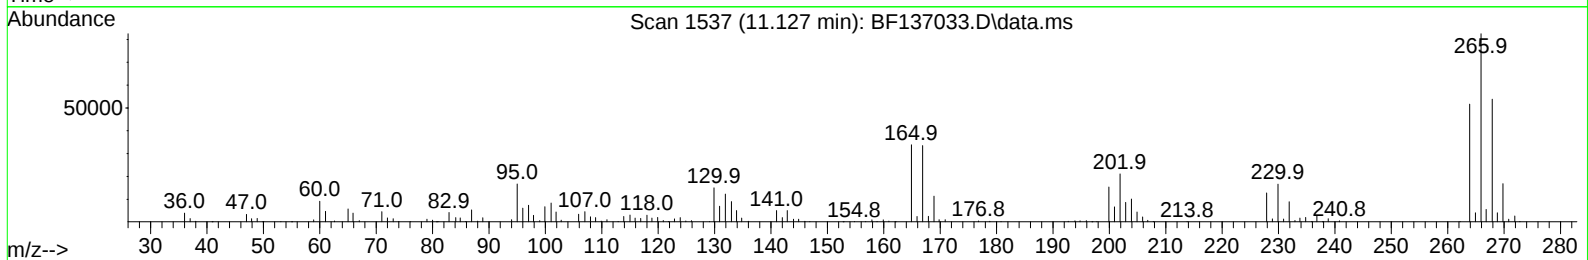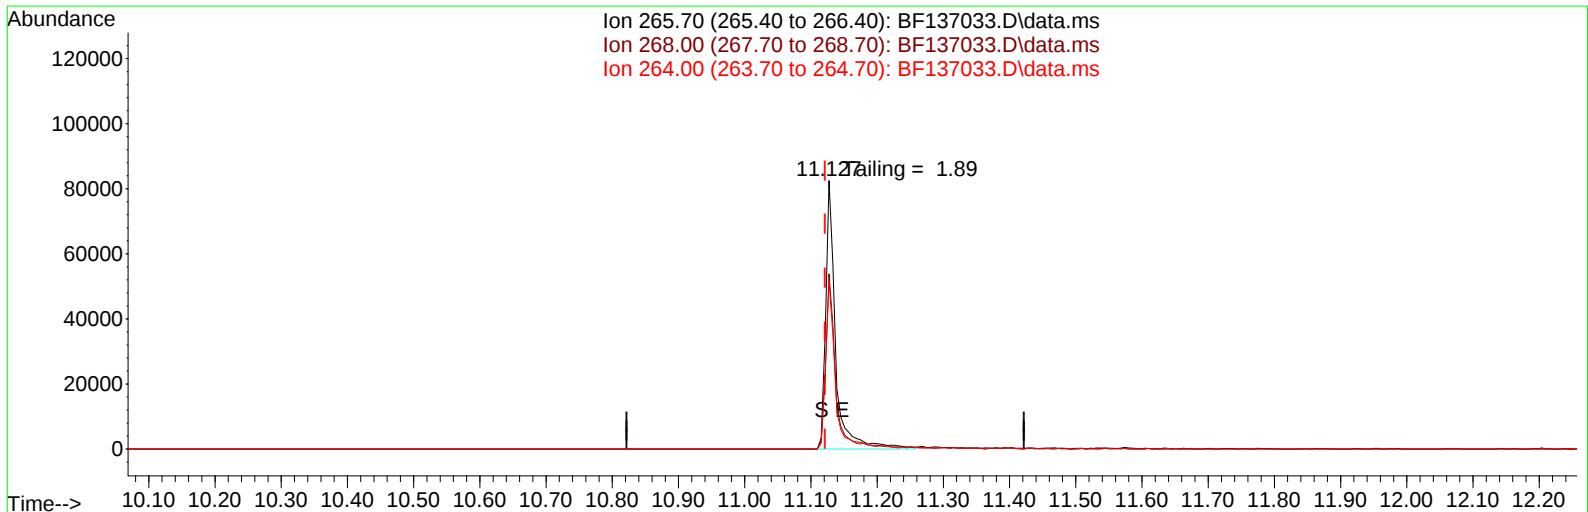

TIC: BF137033.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.006) 31096.62 ng




response 86645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.25
264.00	61.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011124\
Data File : BF137033.D
Acq On : 11 Jan 2024 11:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 11 12:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

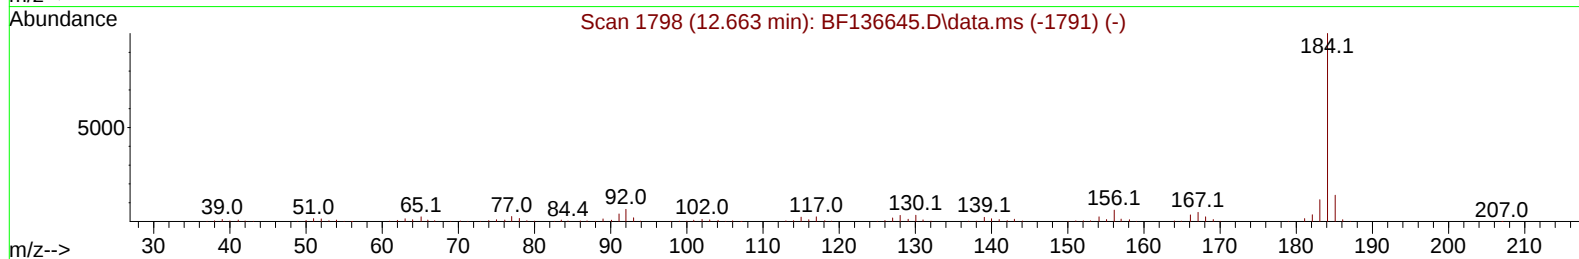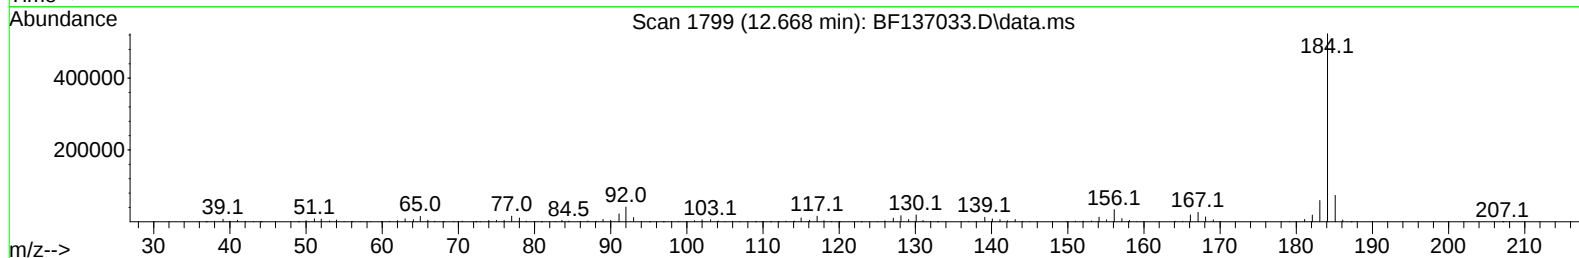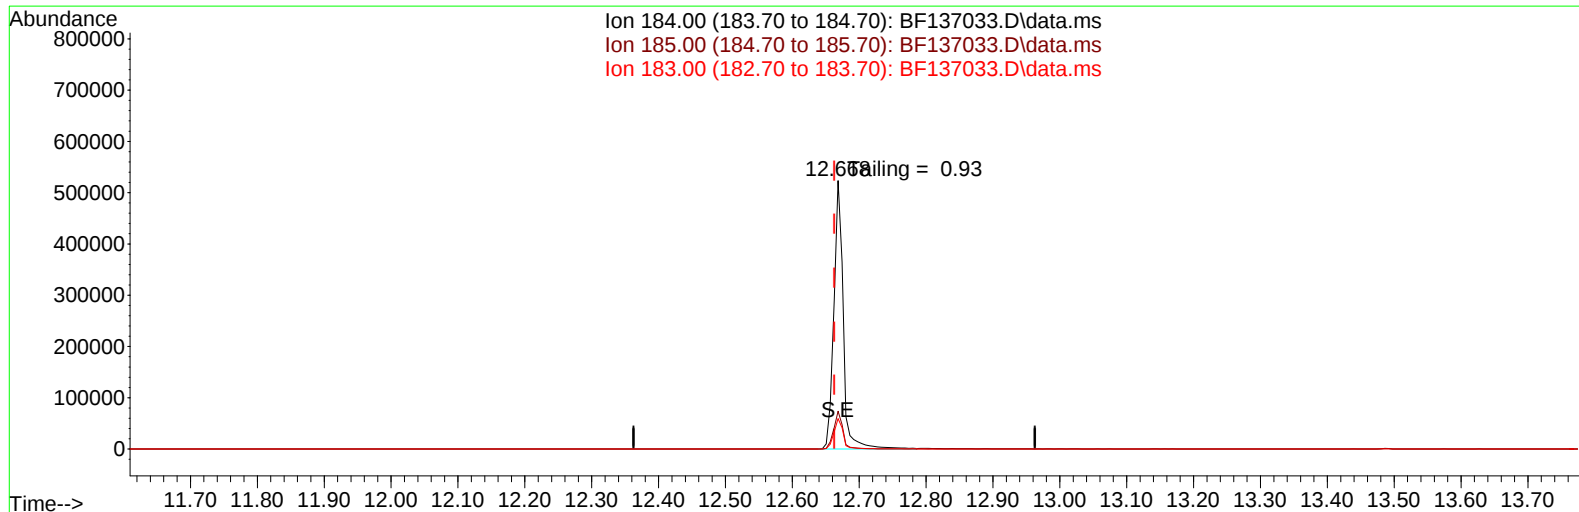

TIC: BF137033.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 157995.44 ng m

response 512447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	11.60	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/11/2024	BNA_F	<u>BF137033.D</u>
Compound Name	Response	Retention Time
DDT	234232	13.486
DDD	6212	13.192
DDE	505	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6717	240949	2.79

Instrument :
BNA_F
ClientSampleId :
DFTPP