

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011215\
 Data File : BF076812.D
 Acq On : 12 Jan 2015 16:38
 Operator : IZ / TP
 Sample : G1056-01
 Misc : S
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FD02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.407	26	28	34	rBV	96599	158724	12.09%	1.774%
2	1.487	34	35	52	rVB	761400	1312819	100.00%	14.672%
3	4.253	274	277	287	rBV	92665	210703	16.05%	2.355%
4	5.167	354	357	369	rBB	396247	695167	52.95%	7.769%
5	7.476	556	559	565	rBV	412780	693295	52.81%	7.748%
6	7.579	565	568	574	rVB	481477	749153	57.06%	8.373%
7	8.082	609	612	616	rBB	135557	202566	15.43%	2.264%
8	8.402	637	640	644	rBV	351011	539046	41.06%	6.024%
9	9.373	722	725	728	rBV	308500	435470	33.17%	4.867%
10	10.985	863	866	870	rBV	190692	295200	22.49%	3.299%
11	13.637	1095	1098	1102	rBV	518545	799389	60.89%	8.934%
12	14.700	1188	1191	1195	rBB	31837	43775	3.33%	0.489%
13	15.123	1225	1228	1232	rBV	217211	326702	24.89%	3.651%
14	16.711	1364	1367	1369	rBB	19341	25279	1.93%	0.283%
15	16.769	1369	1372	1375	rBV	373737	522528	39.80%	5.840%
16	17.854	1464	1467	1470	rBV	316942	342497	26.09%	3.828%
17	18.826	1550	1552	1555	rBV	15556	19634	1.50%	0.219%
18	20.072	1658	1661	1664	rBV	722313	791651	60.30%	8.848%
19	21.340	1766	1772	1775	rBV	307877	381873	29.09%	4.268%
20	22.472	1869	1871	1873	rBV	12507	16150	1.23%	0.180%
21	22.918	1906	1910	1916	rBV3	6419	15922	1.21%	0.178%
22	23.078	1921	1924	1930	rVV	198402	289997	22.09%	3.241%
23	23.318	1940	1945	1947	rBV3	7478	14089	1.07%	0.157%
24	23.706	1975	1979	1981	rBV3	9406	15873	1.21%	0.177%
25	24.106	2011	2014	2017	rBV3	9037	17239	1.31%	0.193%
26	25.009	2089	2093	2096	rBV4	6086	13720	1.05%	0.153%
27	25.581	2140	2143	2150	rVB6	6750	19165	1.46%	0.214%


Sum of corrected areas: 8947626

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011215\
Data File : BF076812.D
Acq On : 12 Jan 2015 16:38
Operator : IZ / TP
Sample : G1056-01
Misc : S
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

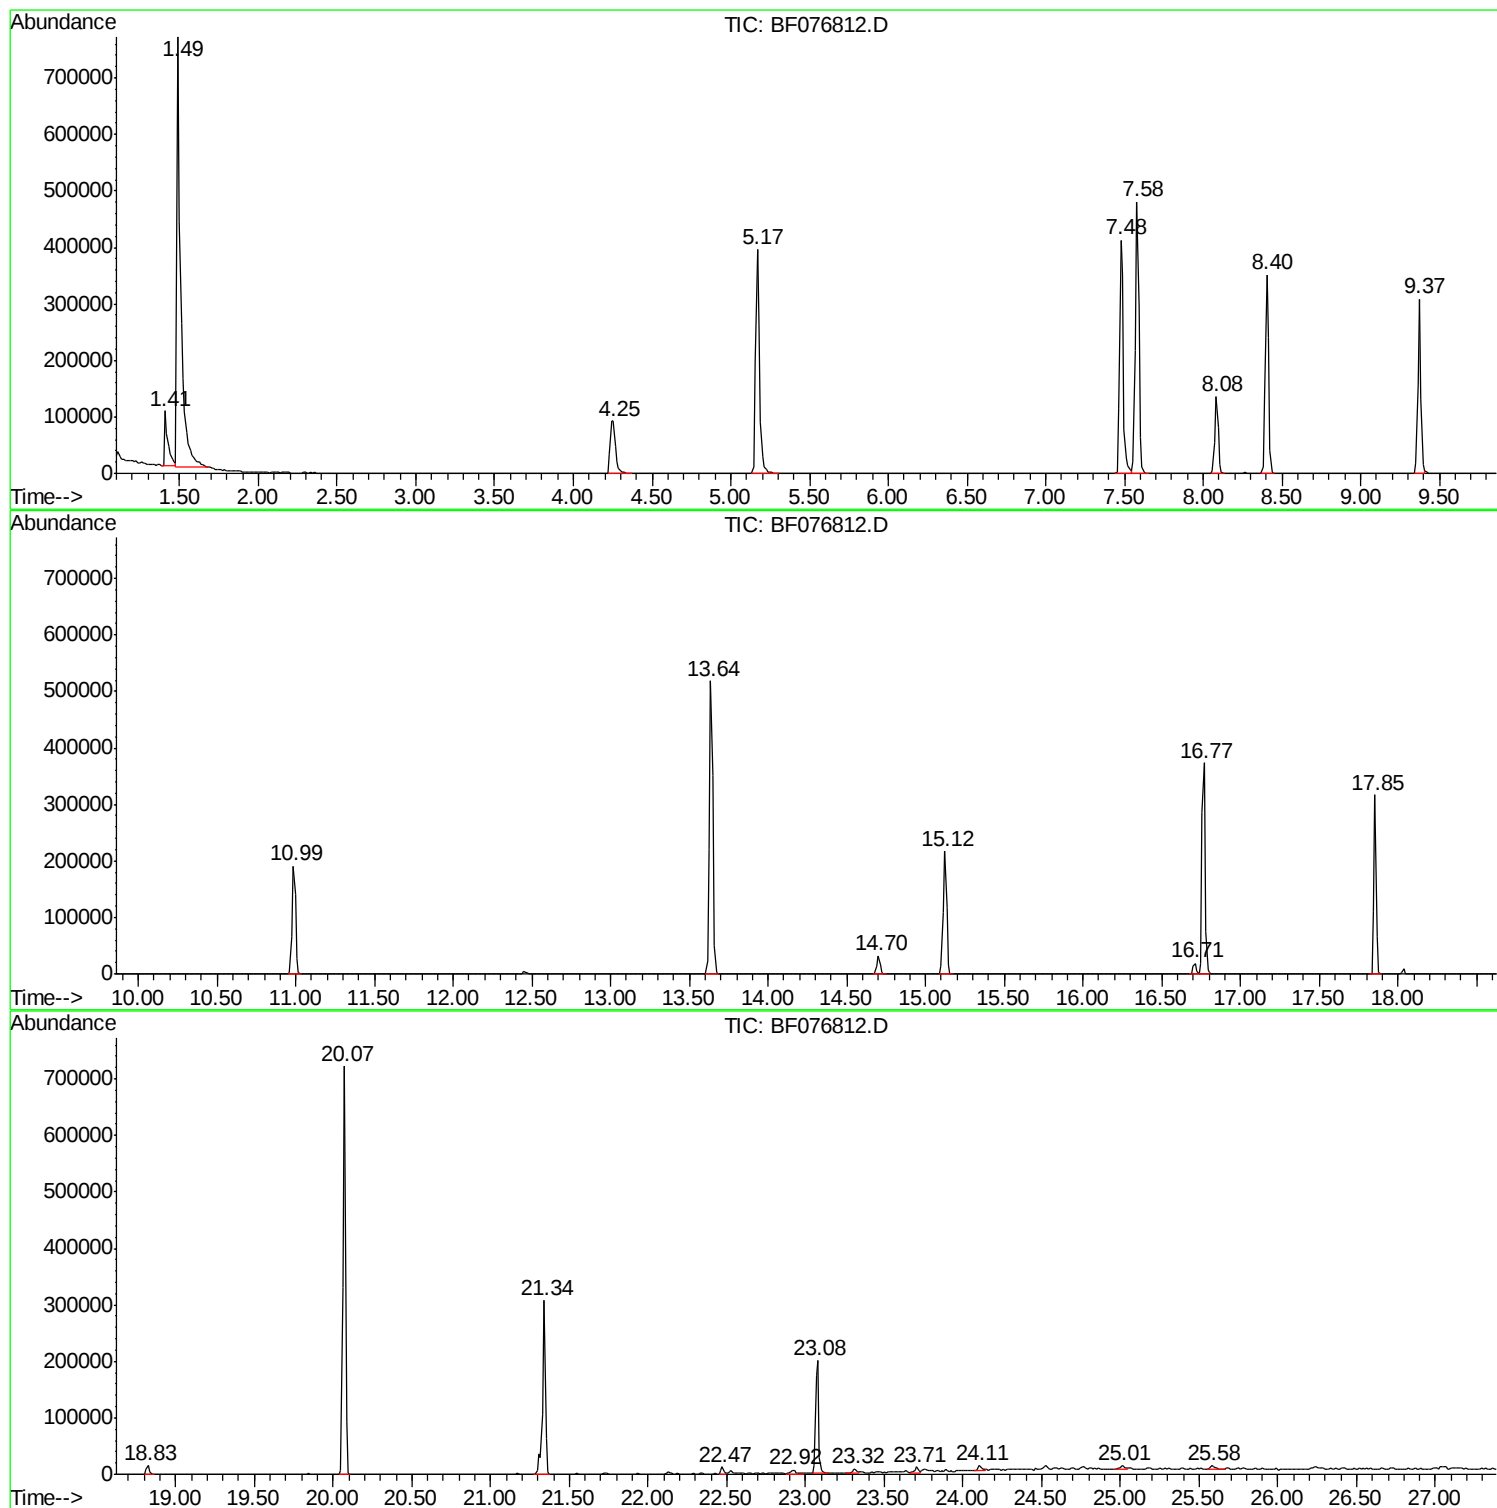

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011215\
Data File : BF076812.D
Acq On : 12 Jan 2015 16:38
Operator : IZ / TP
Sample : G1056-01
Misc : S
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD02










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.25	20.80 ng	210703	1,4-Dichlorobenzene-d4	8.08

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	40
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	17
4			Acetone	58	C3H6O	000067-64-1	9
5			Guanidine	59	CH5N3	000113-00-8	9

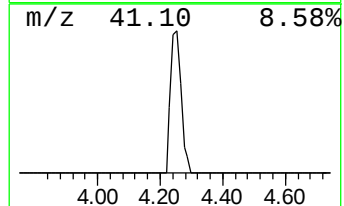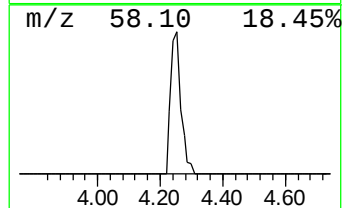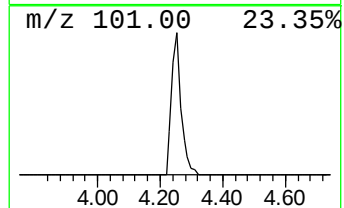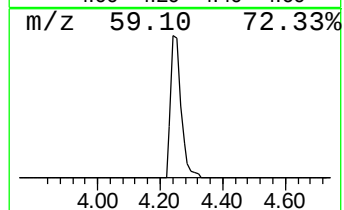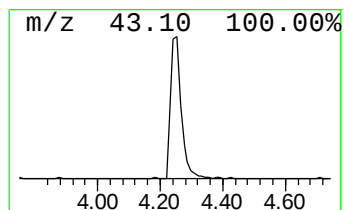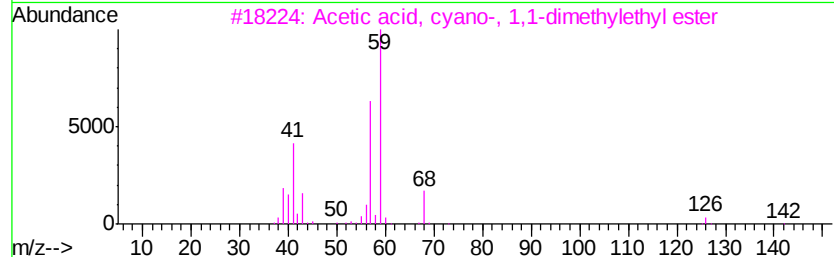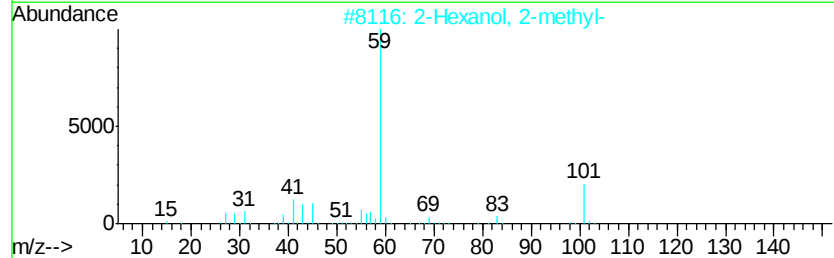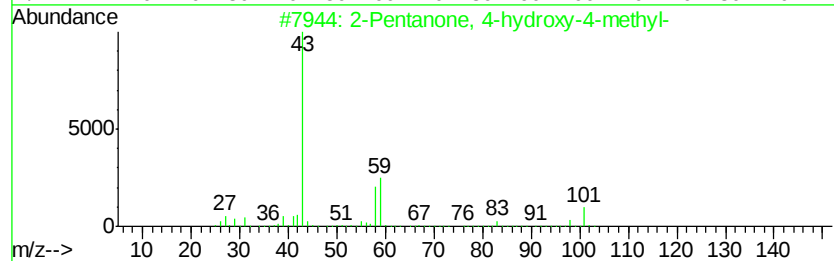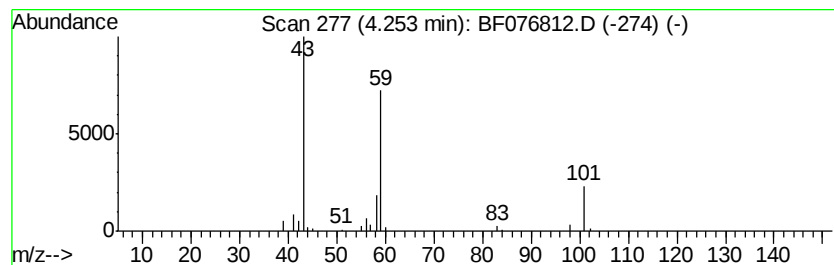

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011215\
Data File : BF076812.D
Acq On : 12 Jan 2015 16:38
Operator : IZ / TP
Sample : G1056-01
Misc : S
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD02










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	73.97 ng	749153	1,4-Dichlorobenzene-d4	8.08

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

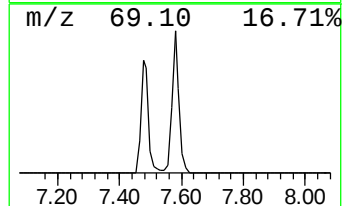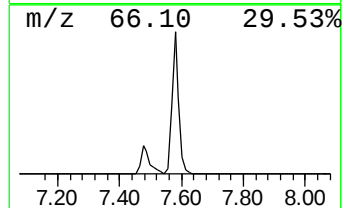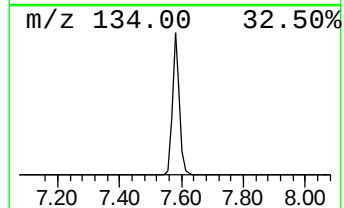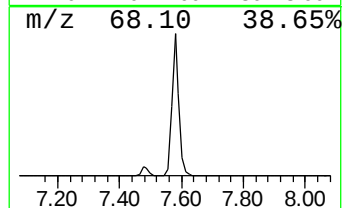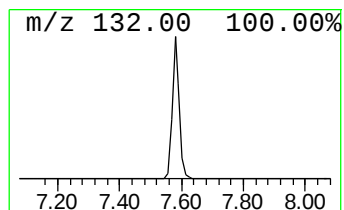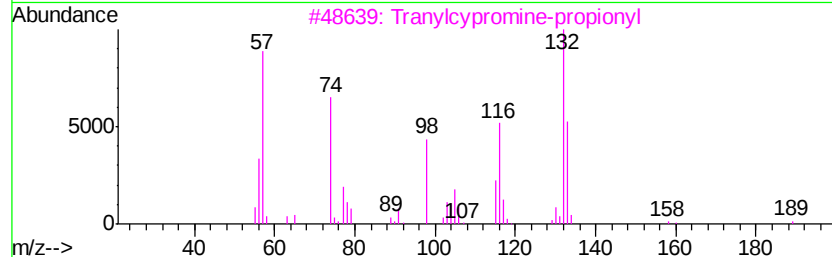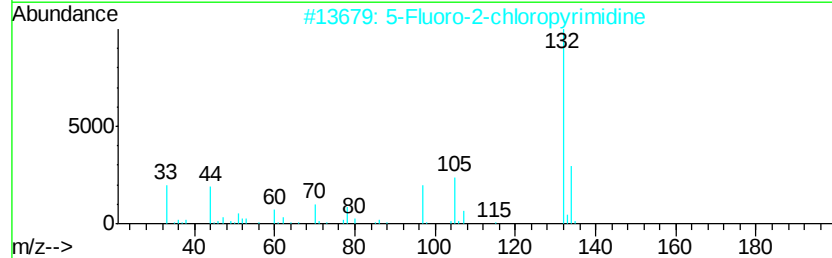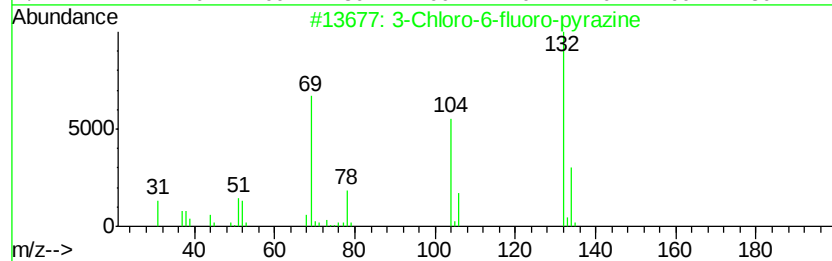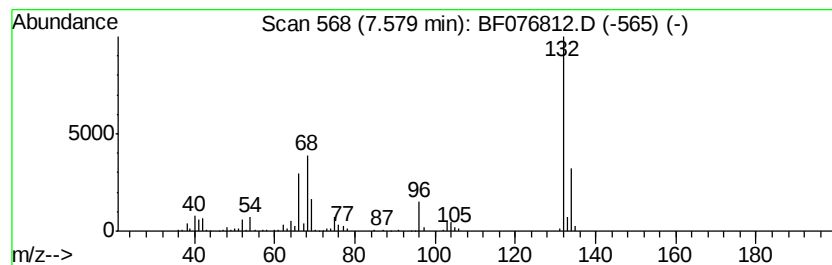

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011215\
Data File : BF076812.D
Acq On : 12 Jan 2015 16:38
Operator : IZ / TP
Sample : G1056-01
Misc : S
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.25	20.8	ng	210703	1	8.08	202566	20.0
unknown7.58	7.58	74.0	ng	749153	1	8.08	202566	20.0