


Data Path : Z:\HPCHEM1\BNA_F\Data\BF011215\
 Data File : BF076807.D
 Acq On : 12 Jan 2015 10:01
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 12 10:43:48 2015

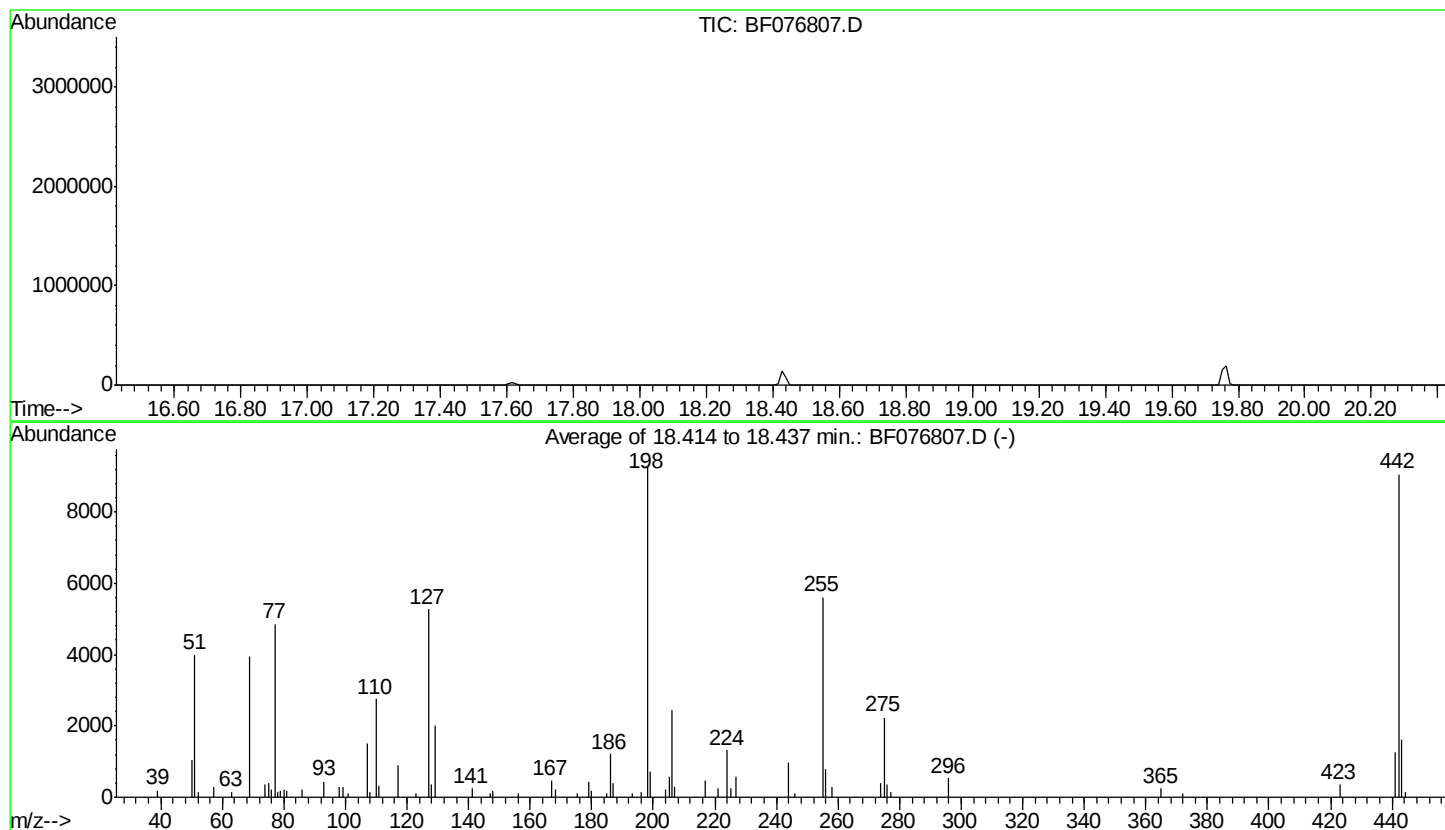

AutoFind: Scans 1516, 1517, 1518; Background Corrected with Scan 1513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	3992	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.3	3933	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.6	5263	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9299	PASS
199	198	5	9	7.6	711	PASS
275	198	10	60	24.0	2235	PASS
365	198	1	100	2.7	247	PASS
441	442	0.01	24	13.8	1248	PASS
442	198	50	100	97.3	9052	PASS
443	442	15	24	18.0	1630	PASS