

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011217\
 Data File : BF092221.D
 Acq On : 12 Jan 2017 21:37
 Operator : UM/SJ
 Sample : I1030-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Quant Time: Jan 12 23:44:16 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.60	152	154694	20.00	ng	-0.05
21) Naphthalene-d8	7.88	136	622007	20.00	ng	-0.06
38) Acenaphthene-d10	9.62	164	307813	20.00	ng	-0.06
63) Phenanthrene-d10	11.11	188	550234	20.00	ng	-0.05
75) Chrysene-d12	13.73	240	318766	20.00	ng	-0.06
86) Perylene-d12	15.09	264	310878	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1072463	115.76	ng	-0.05
7) Phenol-d6	6.26	99	1459052	128.99	ng	-0.05
23) Nitrobenzene-d5	7.17	82	1012420	90.51	ng	-0.05
41) 2,4,6-Tribromophenol	10.42	330	328254	128.86	ng	-0.05
44) 2-Fluorobiphenyl	8.96	172	1650444	114.31	ng	-0.05
78) Terphenyl-d14	12.69	244	1085859	82.62	ng	-0.06
Target Compounds						
10) Phenol	6.28	94	26323	2.04	ng	Qvalue 78
19) n-Nitroso-di-n-propylamine	7.17	70	137253	18.24	ng	# 75
25) Isophorone	7.17	82	1007486	48.82	ng	# 65
37) 2-Methylnaphthalene	8.60	142	1158	Below Cal	#	86
49) Dimethylphthalate	9.36	163	448789	22.80	ng	99
56) 2,4-Dinitrotoluene	9.62	165	39195	7.25	ng	# 20
66) 4-Bromophenyl-phenylether	10.41	248	20216	3.53	ng	# 1
71) Anthracene	11.13	178	11796	Below Cal		97
73) Di-n-butylphthalate	11.68	149	6217	Below Cal	#	99
74) Fluoranthene	12.31	202	23541	Below Cal		99
76) Benizidine	12.69	184	14439	Below Cal		97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011217\
Data File : BF092221.D
Acq On : 12 Jan 2017 21:37
Operator : UM/SJ
Sample : I1030-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-0016

Quant Time: Jan 12 23:44:16 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

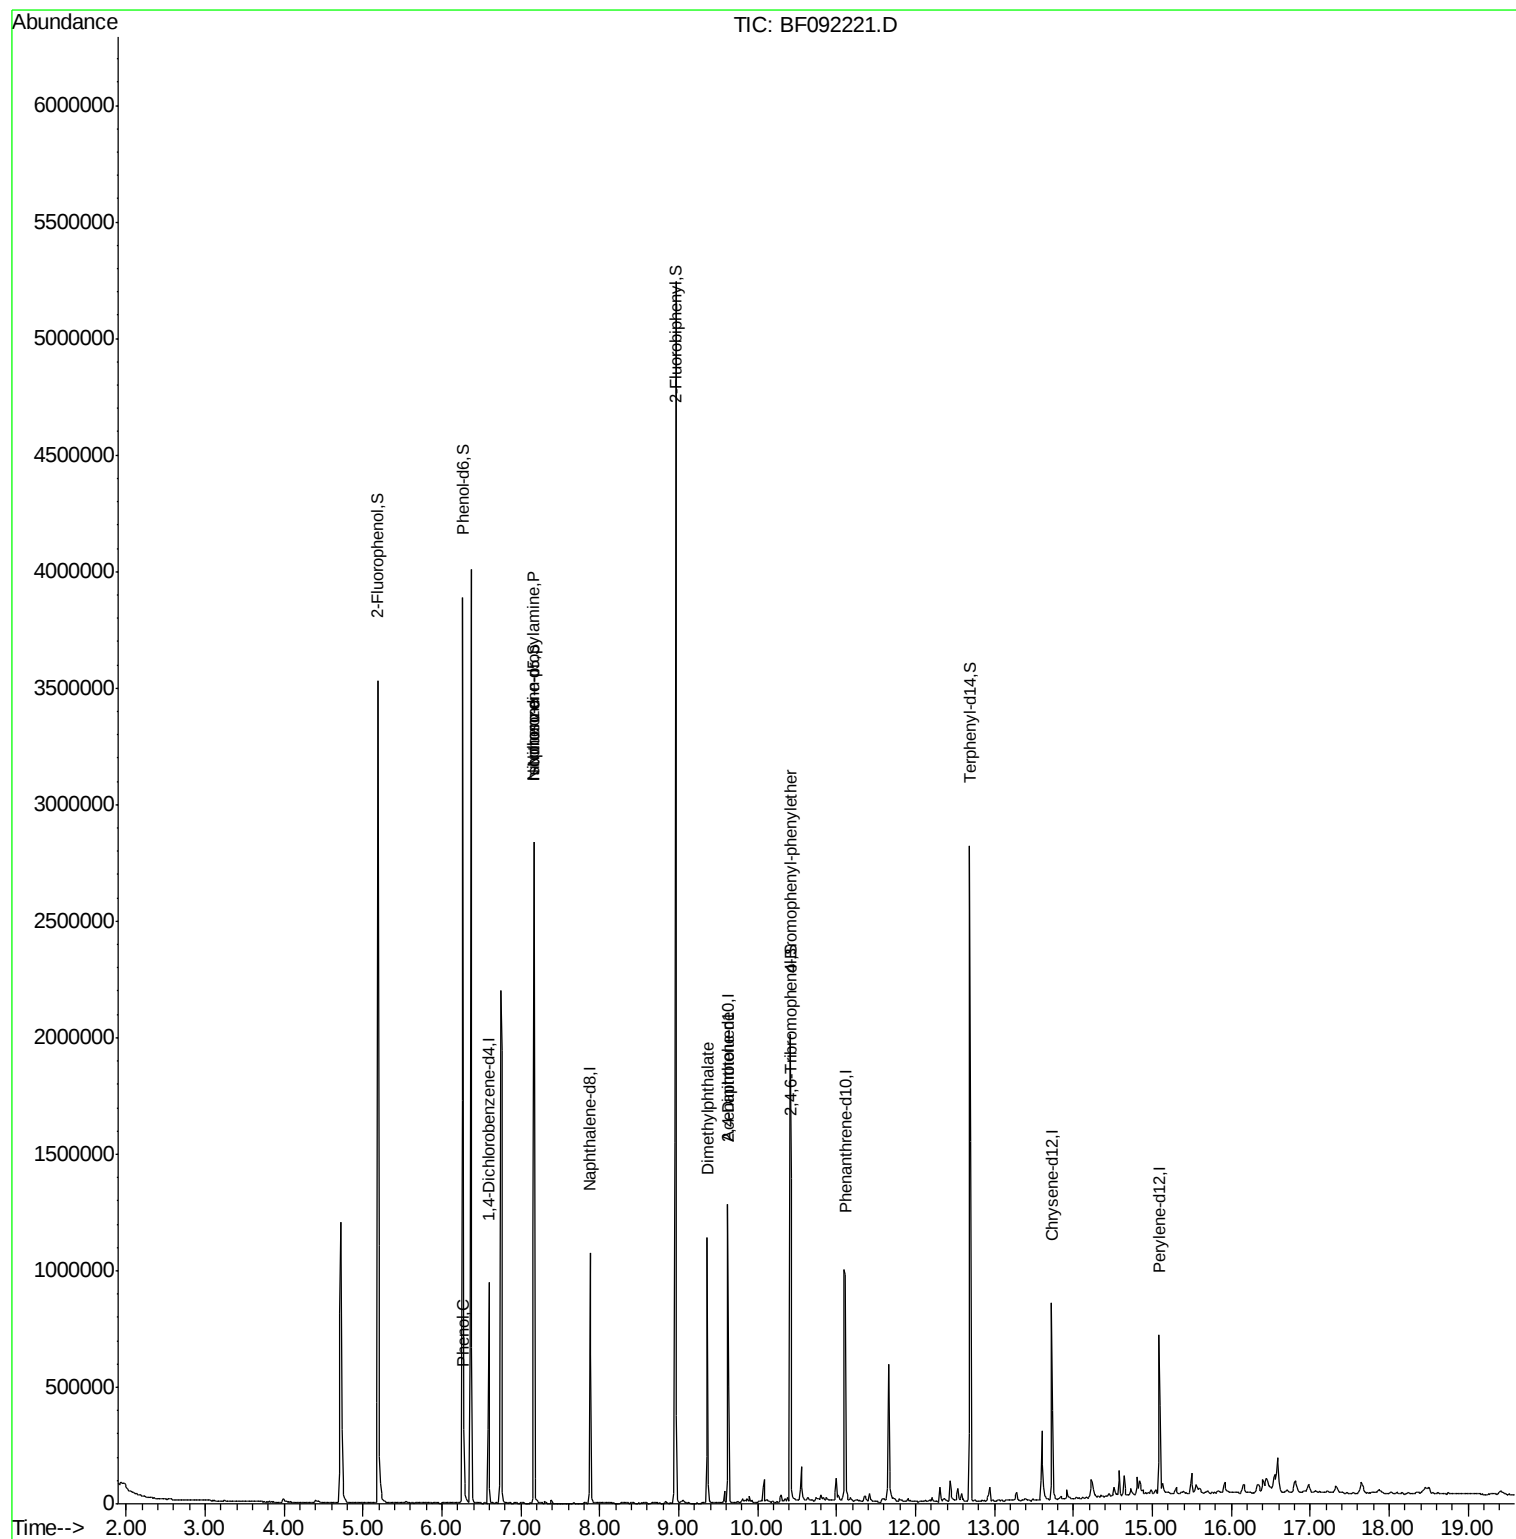

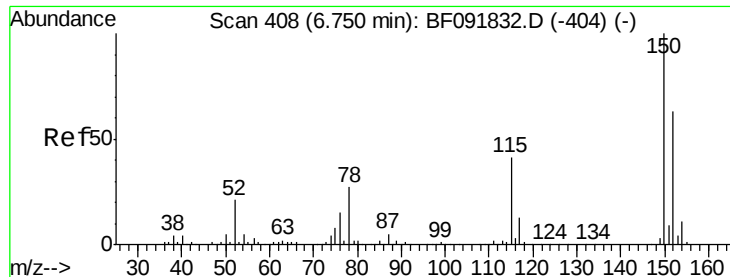

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.60 min Scan# 412

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tgt Ion:152 Resp: 154694

Ion Ratio Lower Upper

152 100

150 156.5 124.9 187.3




115 57.1 46.0 69.0

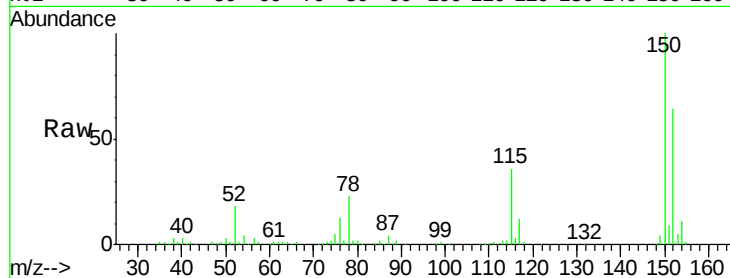

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

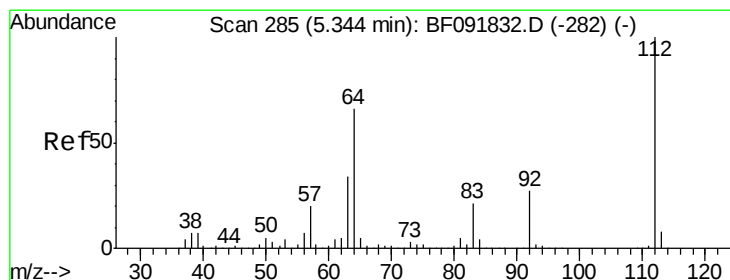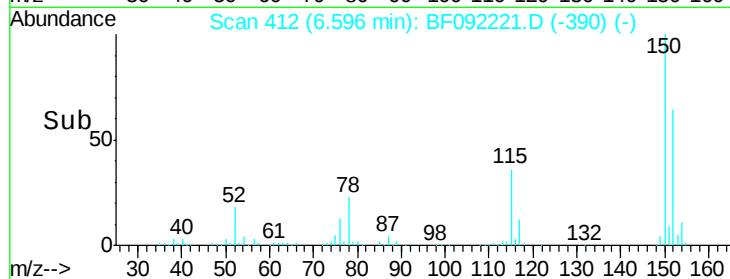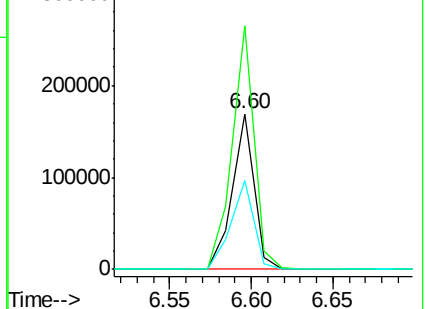

#5

2-Fluorophenol

Concen: 115.76 ng

RT: 5.19 min Scan# 289

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion:112 Resp: 1072463

Ion Ratio Lower Upper

112 100

64 64.8 46.1 69.1



63 33.0 23.8 35.6

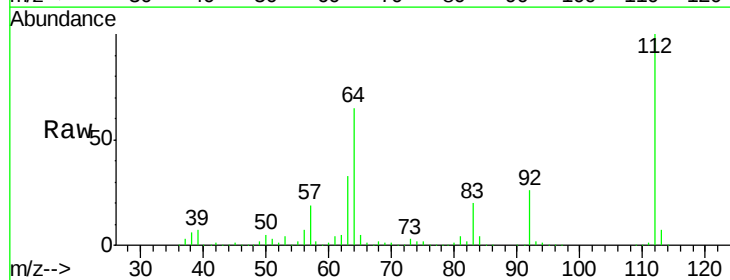

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

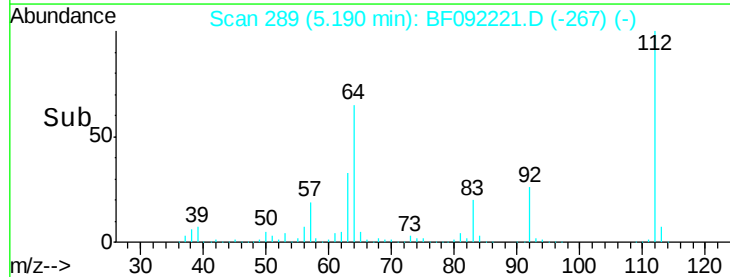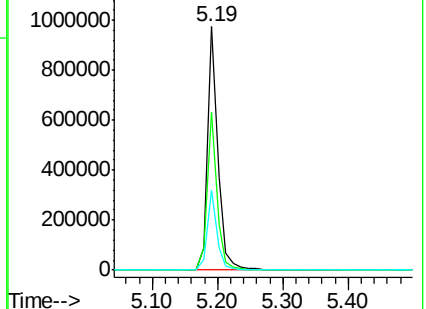



#7

Phenol-d6

Concen: 128.99 ng

RT: 6.26 min Scan# 383

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tgt Ion: 99 Resp: 1459052

Ion Ratio Lower Upper

99 100

42 18.4 15.6 23.4




71 33.7 27.5 41.3

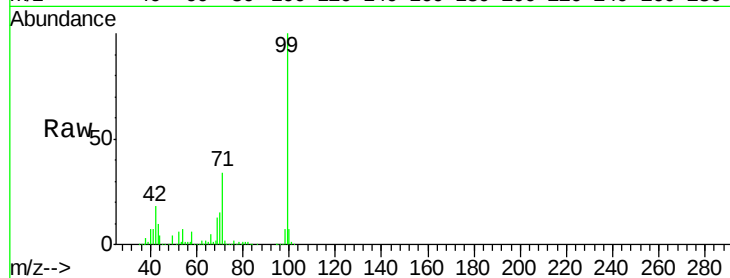

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

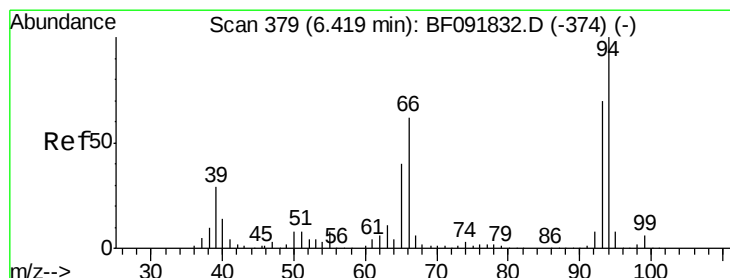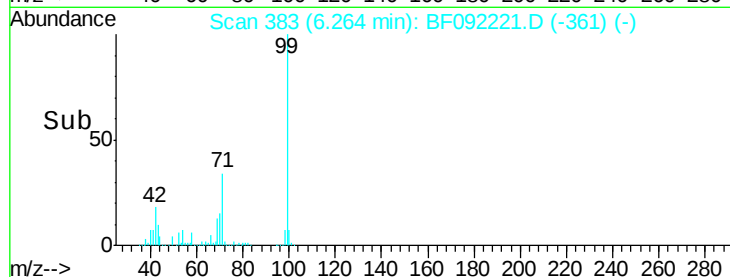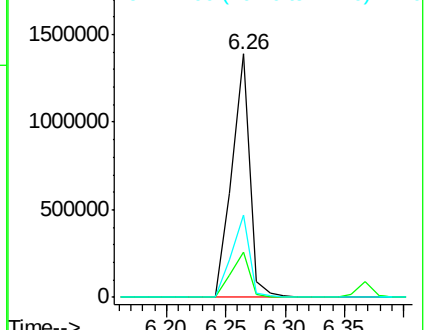

#10

Phenol

Concen: 2.04 ng

RT: 6.28 min Scan# 384

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion: 94 Resp: 26323

Ion Ratio Lower Upper

94 100

65 28.0 21.4 61.4



66 46.3 44.0 84.0


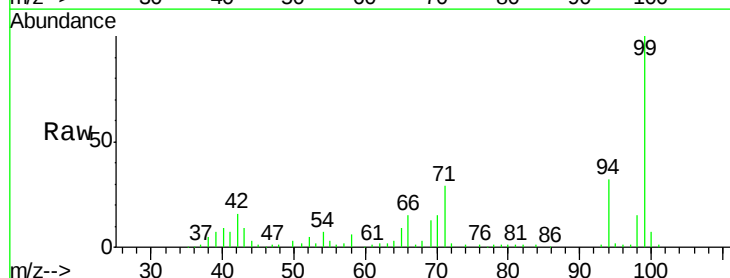


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



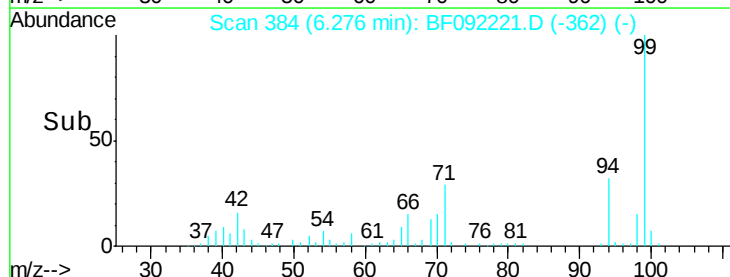
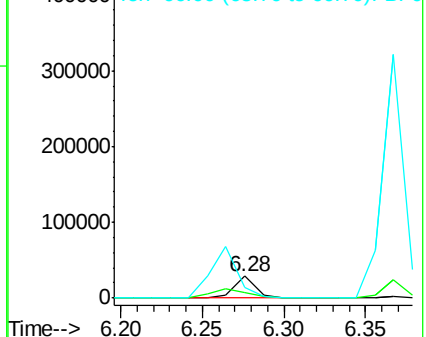


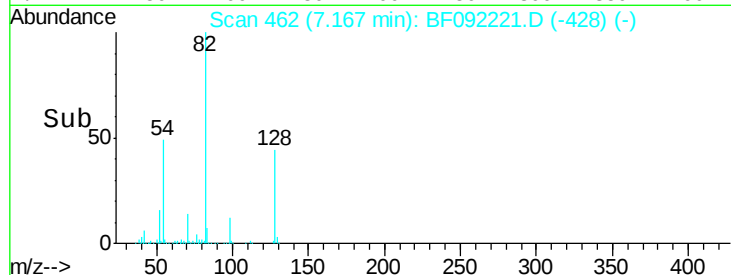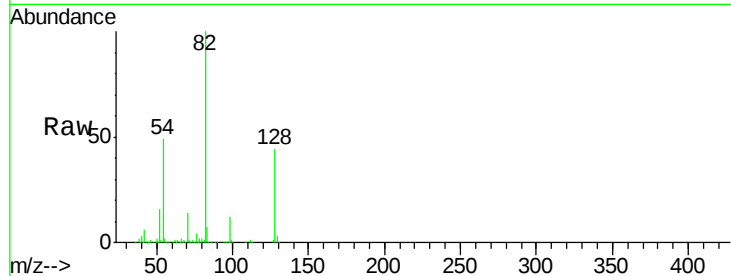

#19
n-Nitroso-di-n-propylamine
Concen: 18.24 ng
RT: 7.17 min Scan# 462
Delta R.T. 0.09 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37


Instrument :
BNA_F
ClientSampleId :
COMP-0016

Tgt Ion:	70	Resp:	137253
Ion	Ratio	Lower	Upper
70	100		
42	44.8	49.4	74.0#
101	0.0	7.4	11.2#
130	2.0	14.2	21.4#

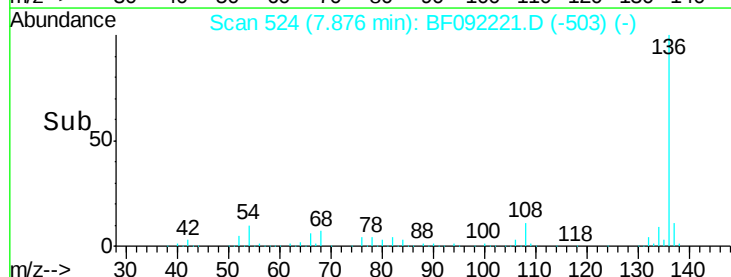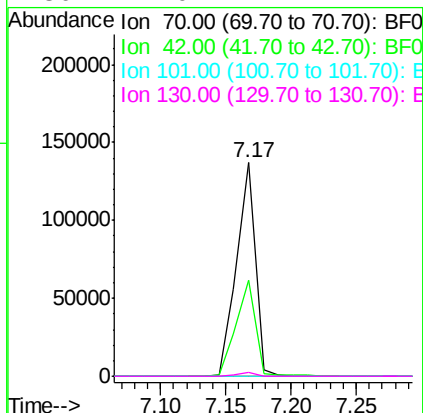

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.88 min Scan# 524
Delta R.T. -0.06 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37

Tgt Ion:	136	Resp:	622007
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	10.0	4.5	6.7#
68	7.2	3.6	5.4#

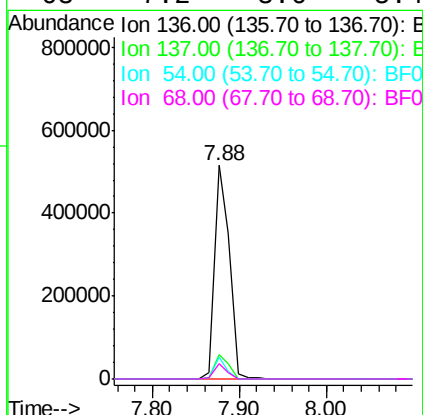







#23
 Nitrobenzene-d5
 Concen: 90.51 ng
 RT: 7.17 min Scan# 462
 Delta R.T. -0.05 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Tgt Ion: 82 Resp: 1012420
 Ion Ratio Lower Upper
 82 100
 128 43.6 34.6 52.0
 54 49.2 39.5 59.3

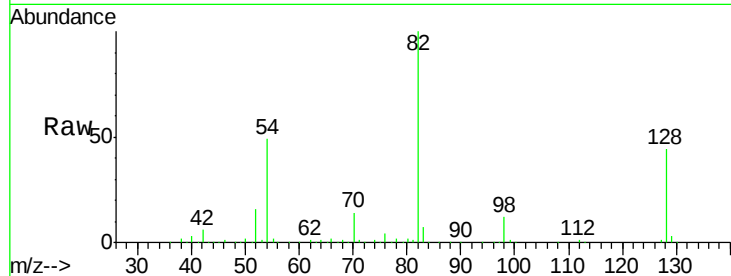


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

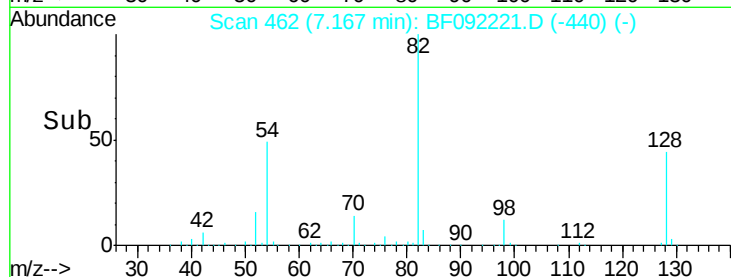
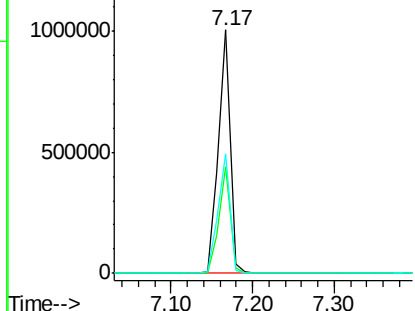



#25
 Isophorone
 Concen: 48.82 ng
 RT: 7.17 min Scan# 462
 Delta R.T. -0.31 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Tgt Ion: 82 Resp: 1007486
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.6 8.4#
 138 0.0 14.6 22.0#



Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0



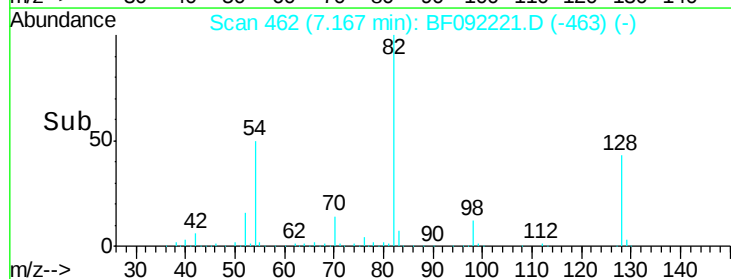
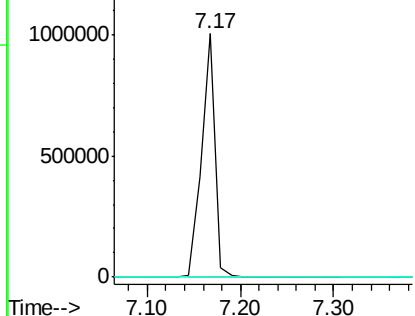


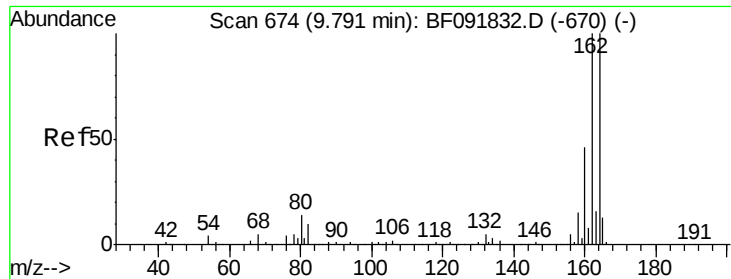

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.62 min Scan# 677
Delta R.T. -0.06 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37




Instrument :
BNA_F
ClientSampleId :
COMP-0016


Tgt Ion:164 Resp: 307813
Ion Ratio Lower Upper
164 100
162 102.1 80.2 120.2
160 45.0 36.9 55.3

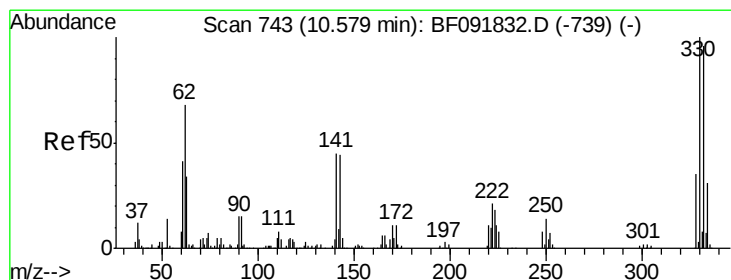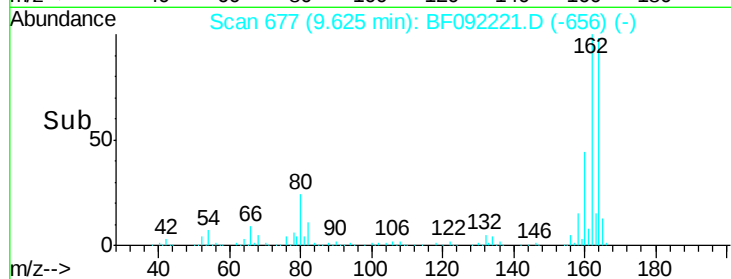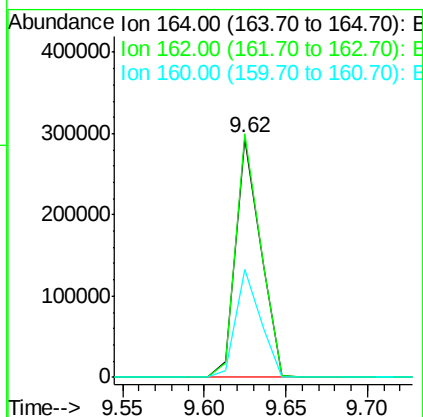

#41
2,4,6-Tribromophenol
Concen: 128.86 ng
RT: 10.42 min Scan# 747
Delta R.T. -0.05 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37

Tgt Ion:330 Resp: 328254
Ion Ratio Lower Upper
330 100
332 95.4 77.4 116.2
141 33.3 34.1 51.1#

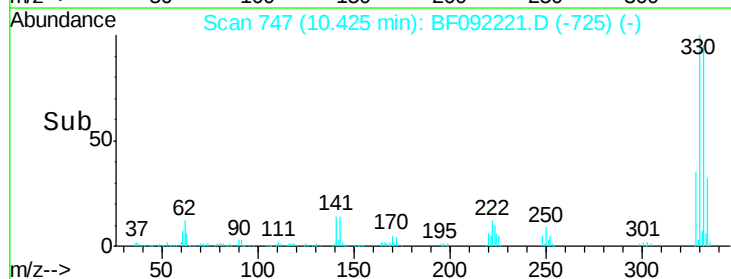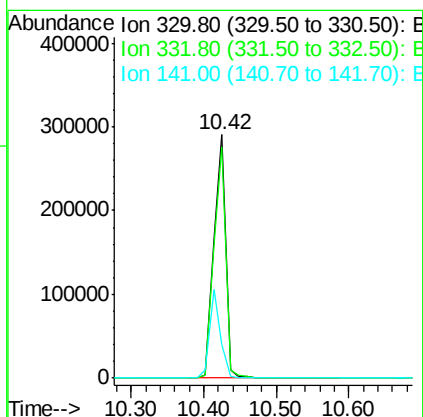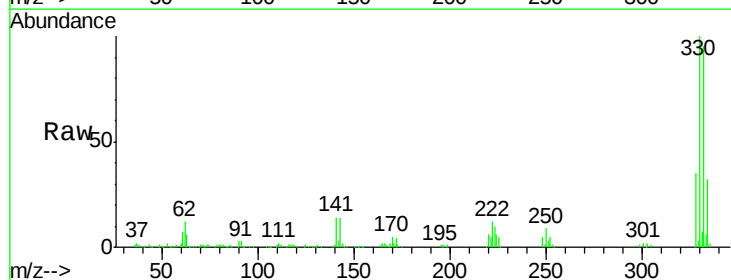


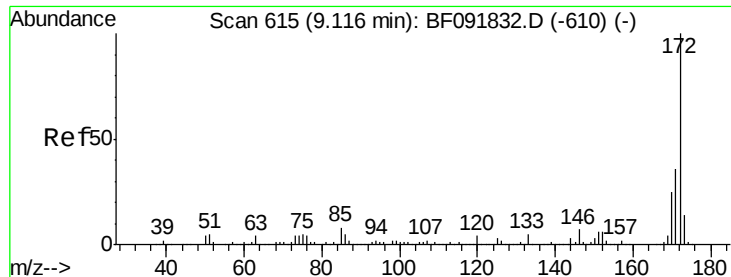




#44
 2-Fluorobiphenyl
 Concen: 114.31 ng
 RT: 8.96 min Scan# 619
 Delta R.T. -0.05 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Tgt Ion:172 Resp: 1650444
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.4 44.0
 170 24.6 20.2 30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

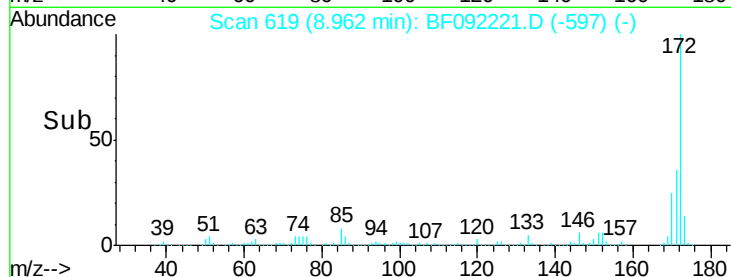
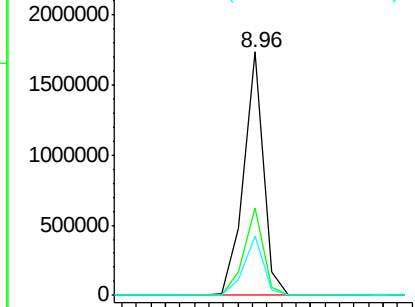



#49
 Dimethylphthalate
 Concen: 22.80 ng
 RT: 9.36 min Scan# 654
 Delta R.T. -0.06 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Tgt Ion:163 Resp: 448789
 Ion Ratio Lower Upper
 163 100
 194 3.1 3.0 4.4
 164 10.3 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



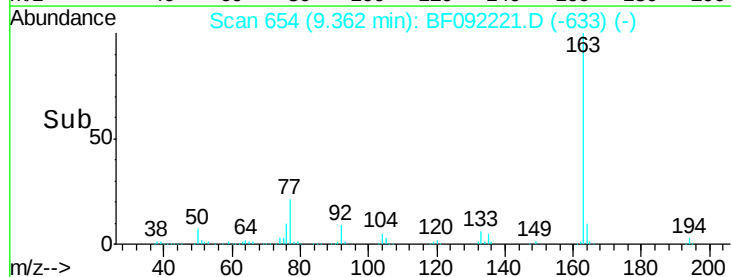
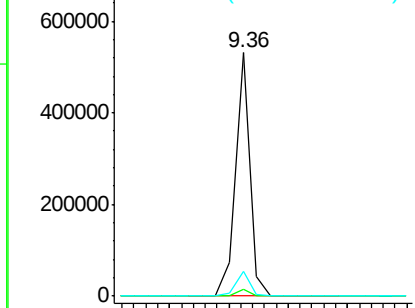


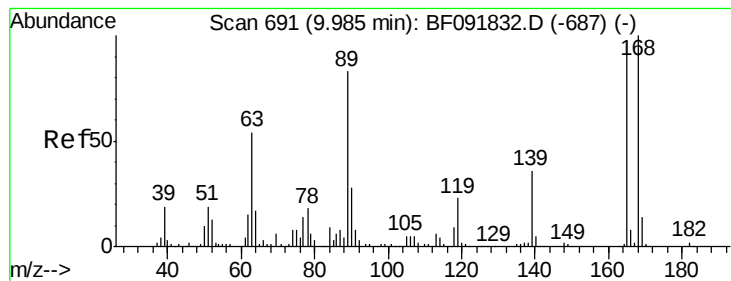

#56
 2,4-Dinitrotoluene
 Concen: 7.25 ng
 RT: 9.62 min Scan# 677
 Delta R.T. -0.26 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37




Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.9	40.2	60.4#
89	1.3	62.5	93.7#
182	0.0	1.8	2.8#

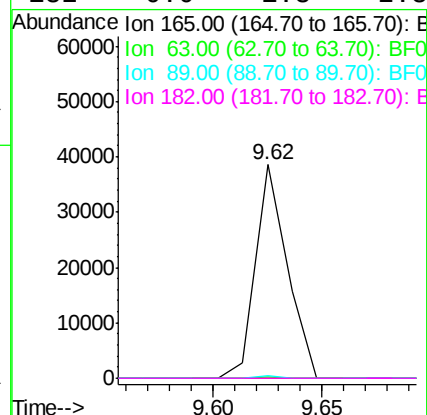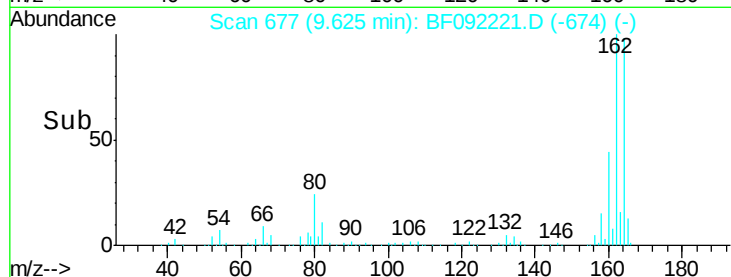

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.11 min Scan# 807
 Delta R.T. -0.05 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Tgt Ion	Ratio	Lower	Upper
188	100		
94	6.7	10.0	15.0#
80	6.8	11.2	16.8#

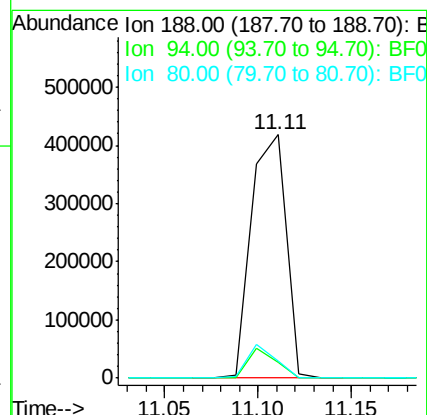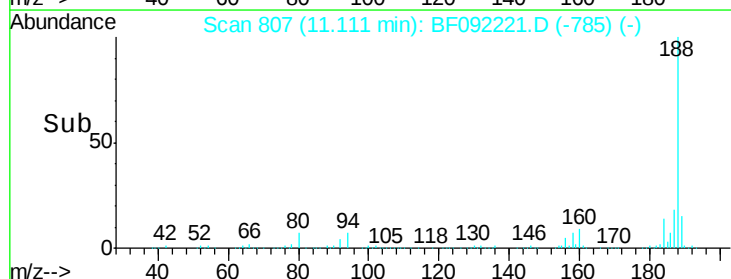

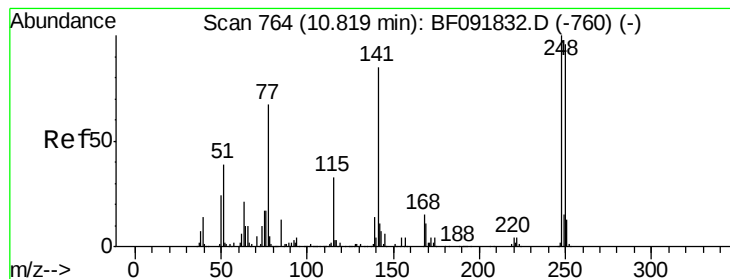

#66

4-Bromophenyl-phenylether

Concen: 3.53 ng

RT: 10.41 min Scan# 746

Delta R.T. -0.30 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tgt Ion:248 Resp: 20216

Ion Ratio Lower Upper

248 100

250 194.0 76.9 115.3#




141 731.2 68.2 102.4#

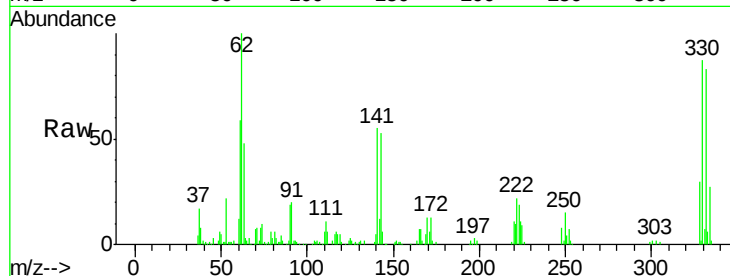

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

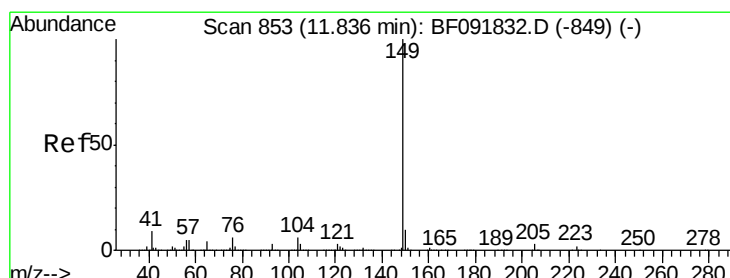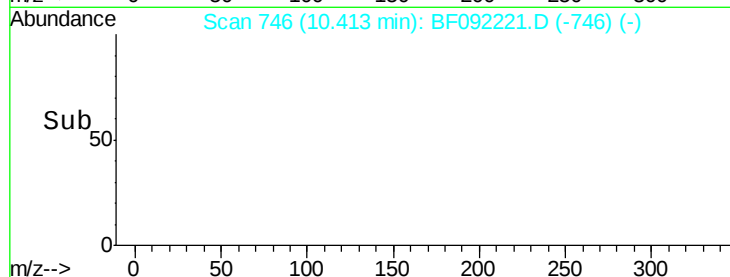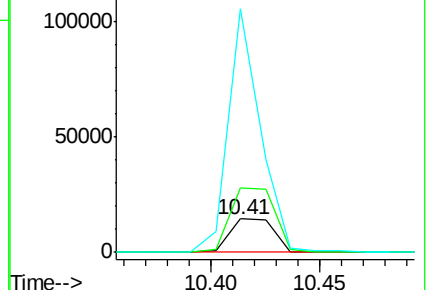

#73

Di-n-butylphthalate

Concen: Below Cal

RT: 11.68 min Scan# 857

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion:149 Resp: 6217

Ion Ratio Lower Upper

149 100

150 10.2 8.1 12.1



104 4.6 4.6 7.0#

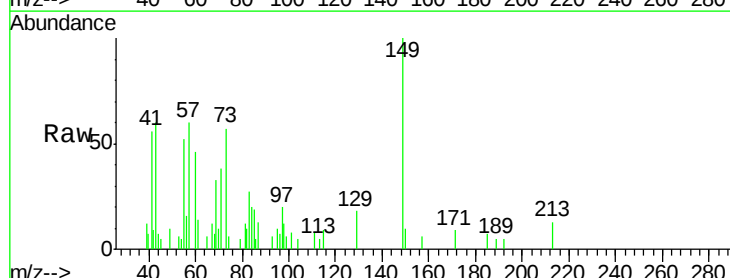


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

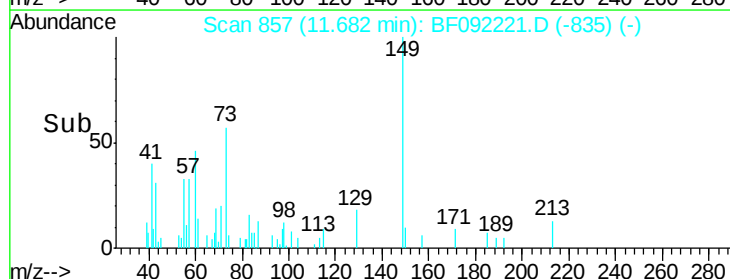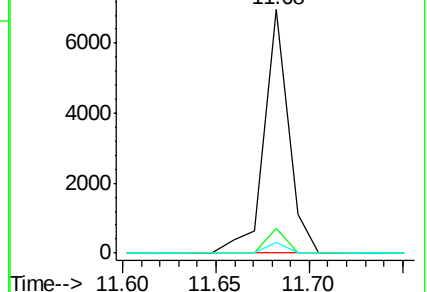

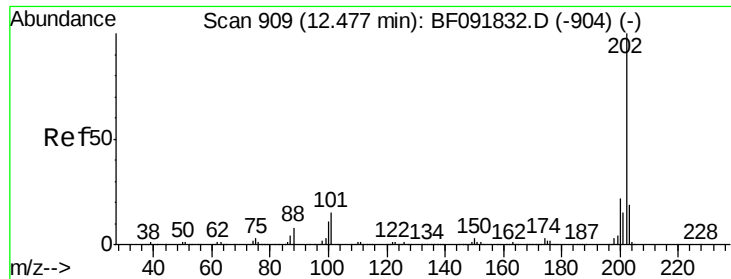

#74

Fluoranthene

Concen: Below Cal

RT: 12.31 min Scan# 912

Delta R.T. -0.06 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016





Tgt Ion:202 Resp: 23541

Ion Ratio Lower Upper

202 100

101 13.9 0.0 34.6

203 18.2 0.0 38.7

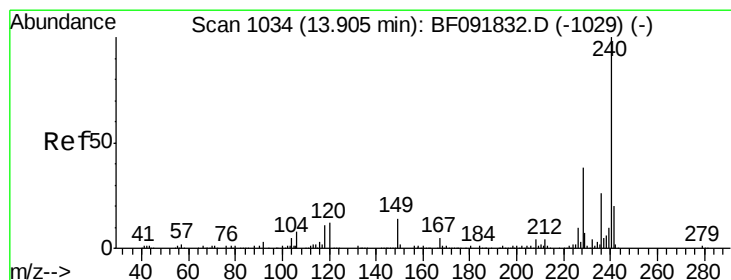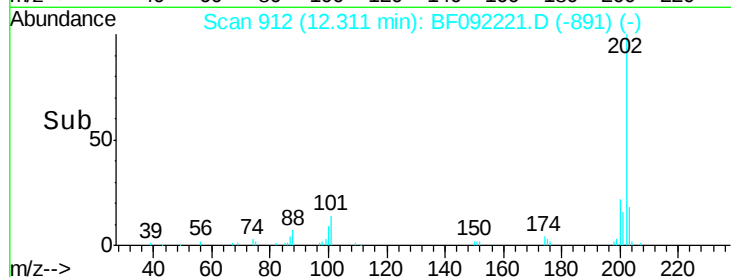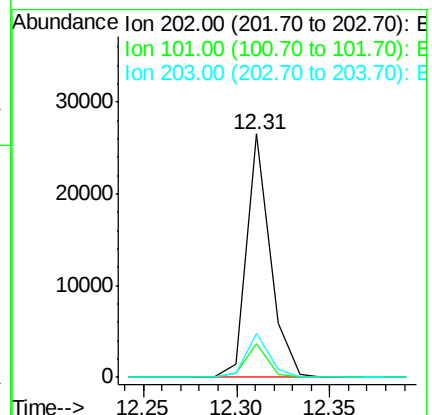

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.73 min Scan# 1036

Delta R.T. -0.06 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37




Tgt Ion:240 Resp: 318766


Ion Ratio Lower Upper

240 100

120 15.6 12.9 19.3

236 24.6 20.9 31.3


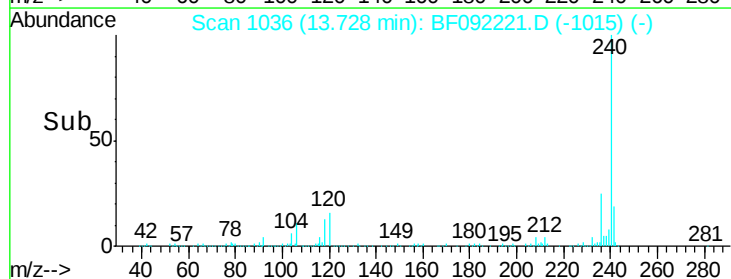
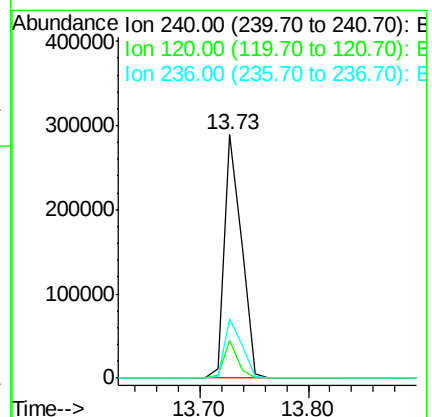
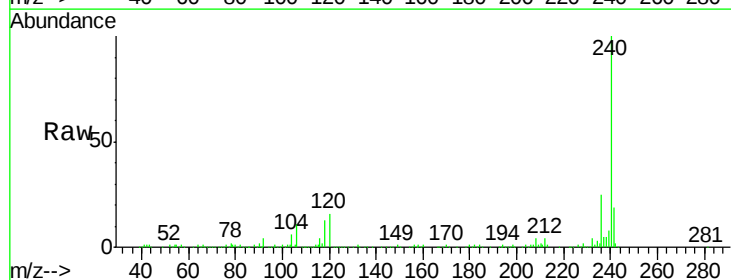


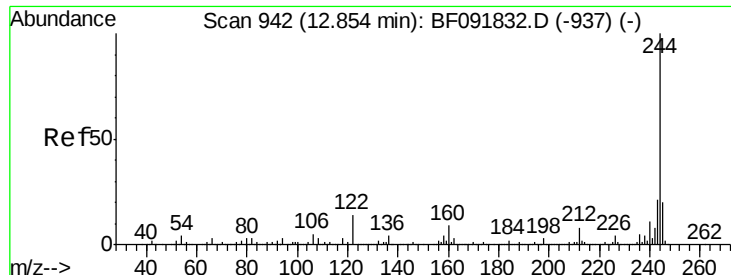

#78
 Terphenyl-d14
 Concen: 82.62 ng
 RT: 12.69 min Scan# 945
 Delta R.T. -0.06 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Tgt Ion:244 Resp: 1085859
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.2 9.2
 122 15.0 11.4 17.2

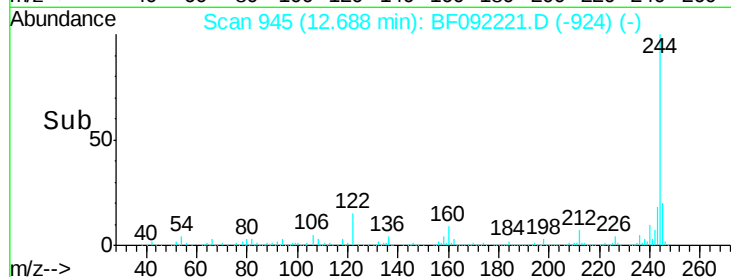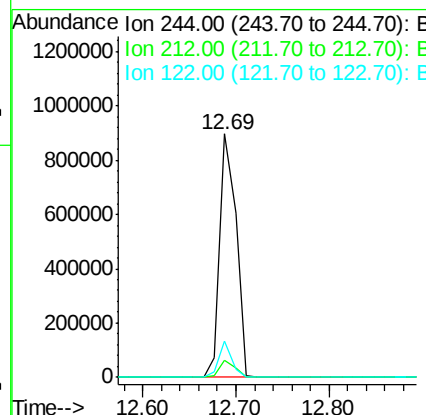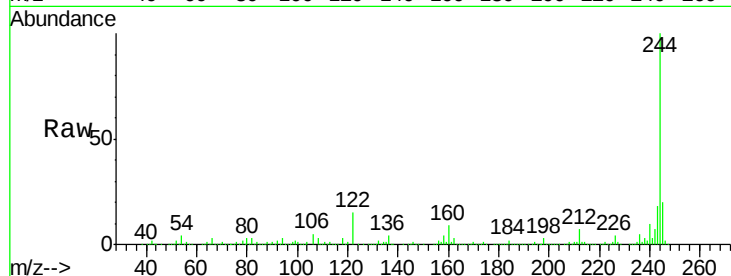

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.09 min Scan# 1155
 Delta R.T. -0.06 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Tgt Ion:264 Resp: 310878
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.2 28.8
 265 22.5 17.4 26.0

