

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
 Data File : BF092220.D
 Acq On : 12 Jan 2017 21:08
 Operator : UM/SJ
 Sample : I1030-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0015

Quant Time: Jan 13 00:15:00 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.60	152	218745	20.00	ng	-0.05
21) Naphthalene-d8	7.88	136	861434	20.00	ng	-0.06
38) Acenaphthene-d10	9.62	164	455068	20.00	ng	-0.06
63) Phenanthrene-d10	11.11	188	690090	20.00	ng	-0.05
75) Chrysene-d12	13.73	240	510450	20.00	ng	-0.06
86) Perylene-d12	15.09	264	467781	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1362376	103.99	ng	-0.05
7) Phenol-d6	6.26	99	1822509	113.95	ng	-0.05
23) Nitrobenzene-d5	7.17	82	1177768	76.03	ng	-0.05
41) 2,4,6-Tribromophenol	10.42	330	412716	109.59	ng	-0.05
44) 2-Fluorobiphenyl	8.96	172	1609839	70.24	ng	-0.05
78) Terphenyl-d14	12.69	244	1454295	69.10	ng	-0.06
Target Compounds						Qvalue
49) Dimethylphthalate	9.36	163	500985	17.21	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
Data File : BF092220.D
Acq On : 12 Jan 2017 21:08
Operator : UM/SJ
Sample : I1030-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-0015

Quant Time: Jan 13 00:15:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

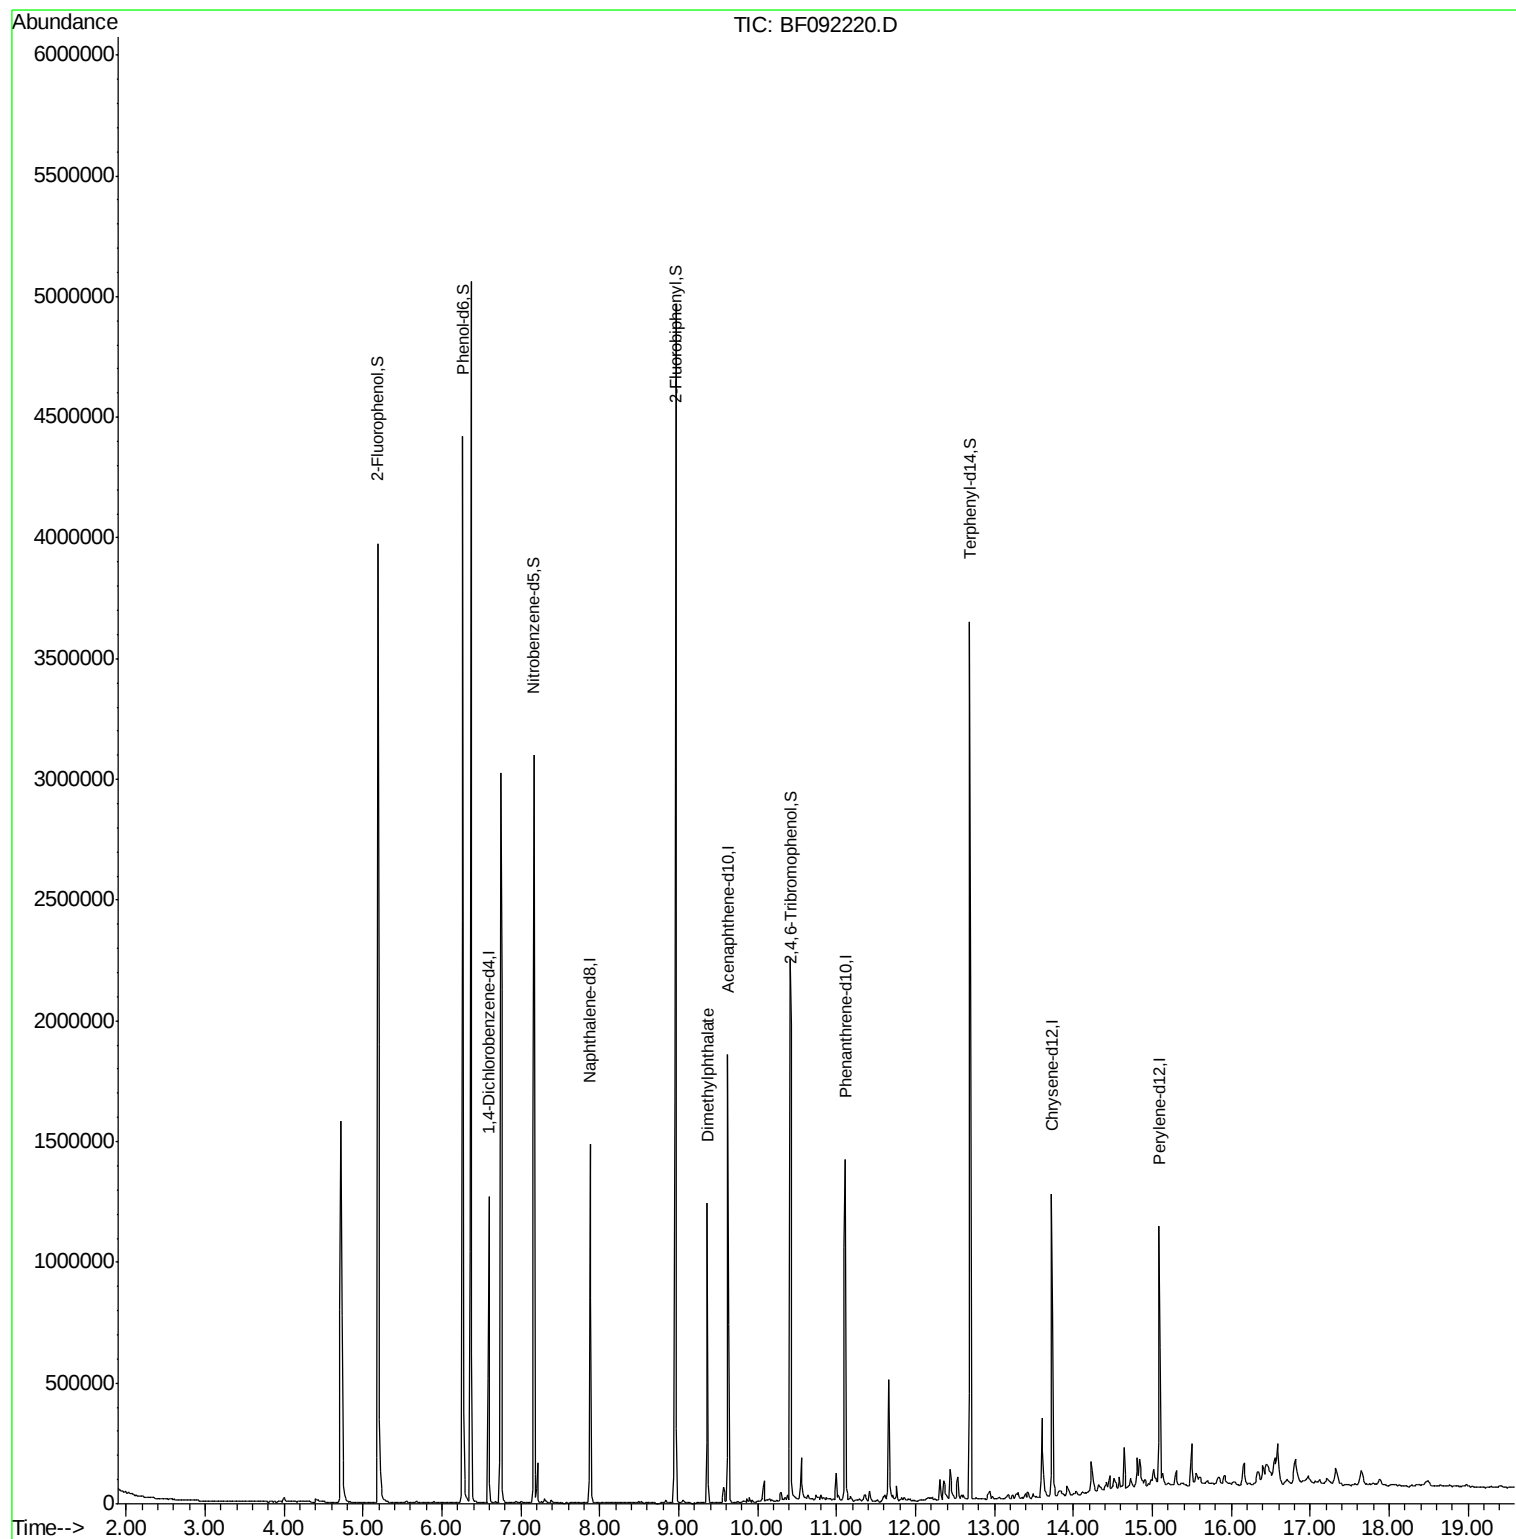

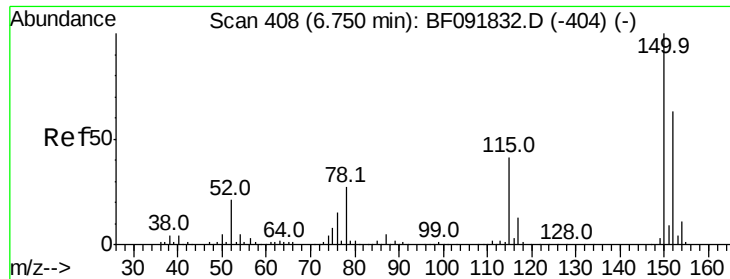

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.60 min Scan# 412

Delta R.T. -0.05 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Instrument :

BNA_F

ClientSampleId :

COMP-0015


Tot Ion:152 Resp: 218745

Ion Ratio Lower Upper

152 100

150 156.0 124.9 187.3




115 57.1 46.0 69.0

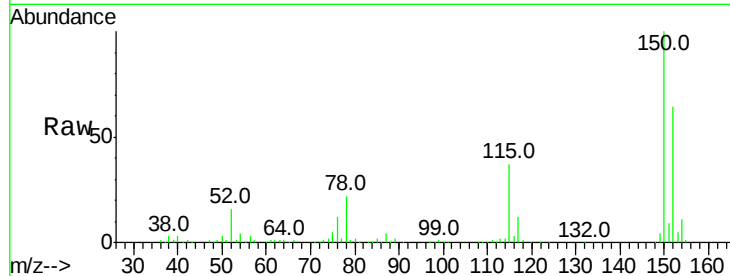

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

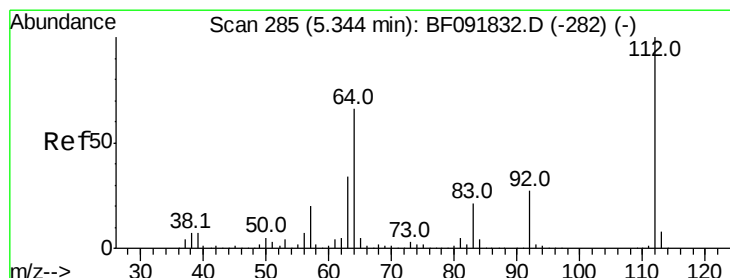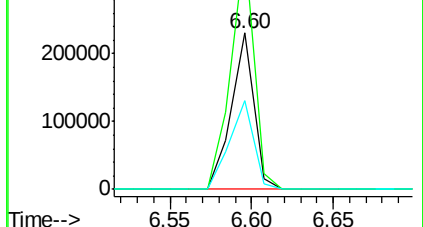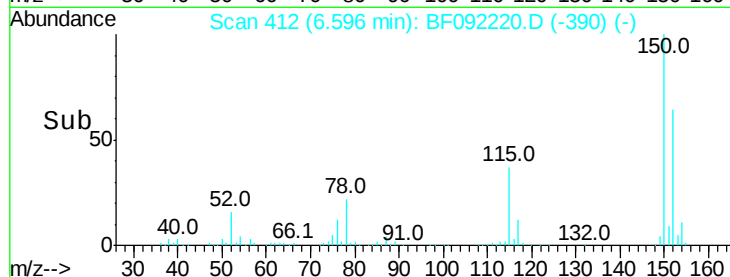

#5

2-Fluorophenol

Concen: 103.99 ng

RT: 5.19 min Scan# 289

Delta R.T. -0.05 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08


Tgt Ion:112 Resp: 1362376

Ion Ratio Lower Upper

112 100

64 65.7 46.1 69.1



63 32.8 23.8 35.6

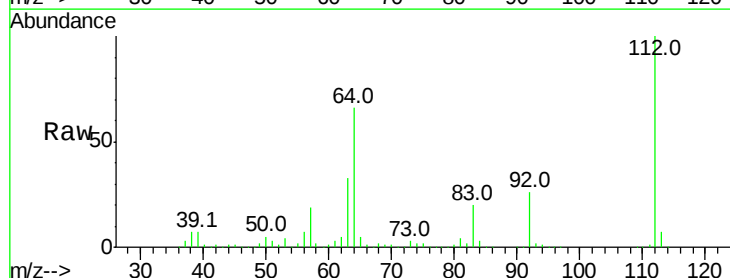

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

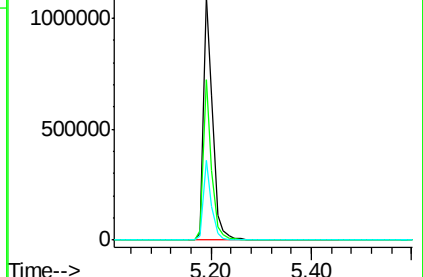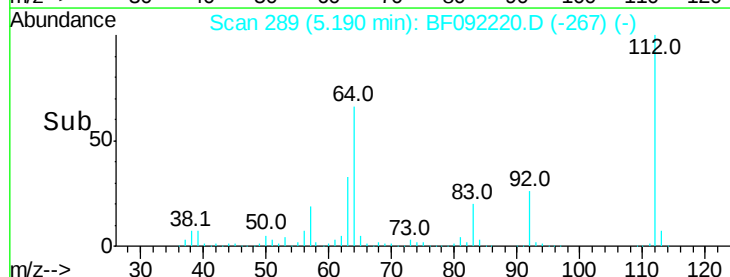



#7

Phenol-d6

Concen: 113.95 ng

RT: 6.26 min Scan# 383

Delta R.T. -0.05 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Instrument :

BNA_F

ClientSampleId :

COMP-0015





Tot Ion: 99 Resp: 1822509

Ion Ratio Lower Upper

99 100

42 17.3 15.6 23.4

71 32.1 27.5 41.3

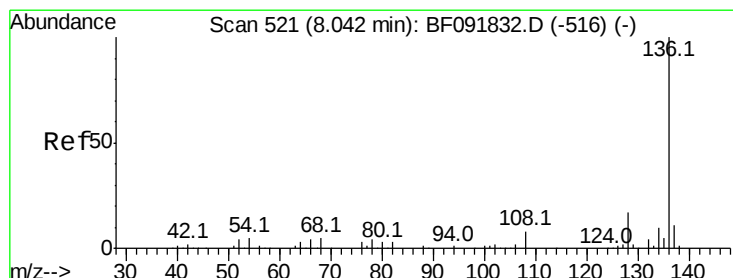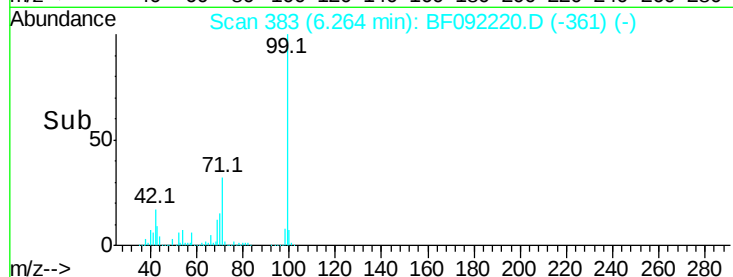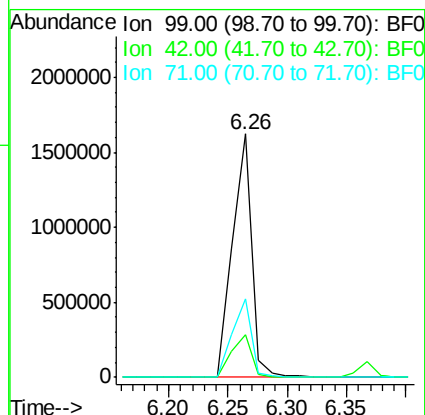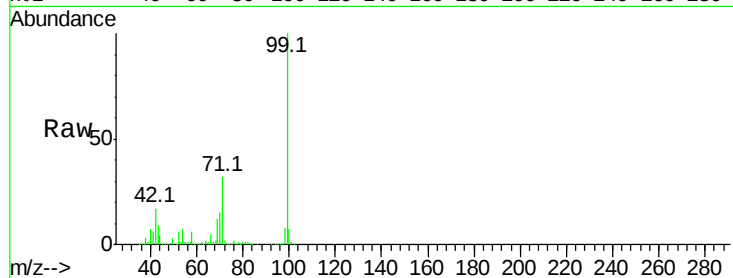

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.88 min Scan# 524

Delta R.T. -0.06 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Tgt Ion: 136 Resp: 861434




Ion Ratio Lower Upper


136 100

137 11.5 8.4 12.6

54 9.7 4.5 6.7#

68 7.5 3.6 5.4#

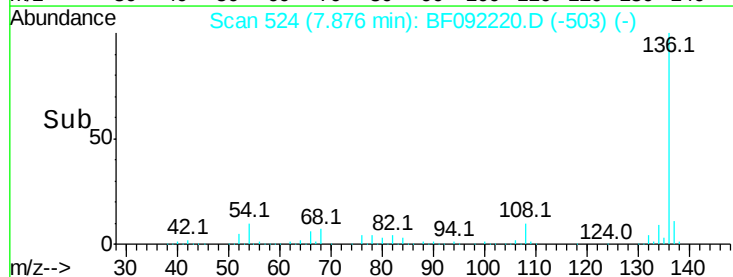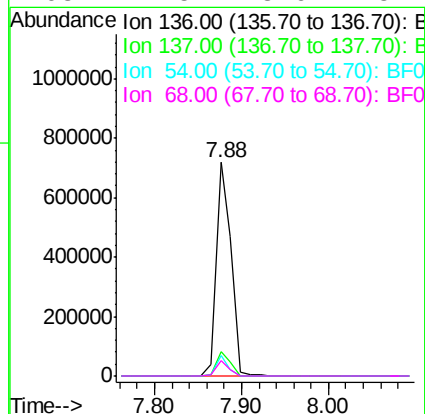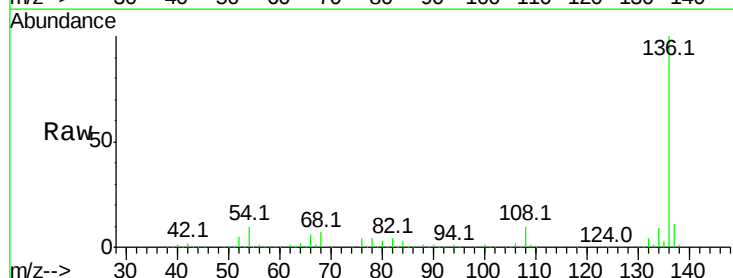

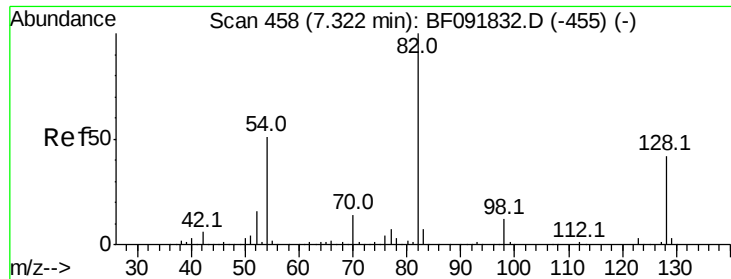

#23

Nitrobenzene-d5

Concen: 76.03 ng

RT: 7.17 min Scan# 462

Delta R.T. -0.05 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Instrument :

BNA_F

ClientSampleId :

COMP-0015


Tot Ion: 82 Resp: 1177768

Ion Ratio Lower Upper

82 100

128 44.9 34.6 52.0




54 48.1 39.5 59.3

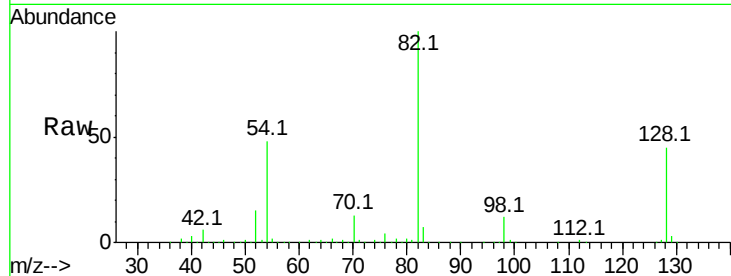

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

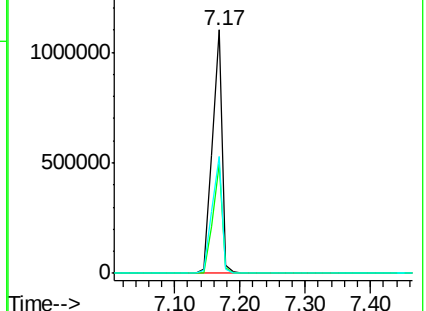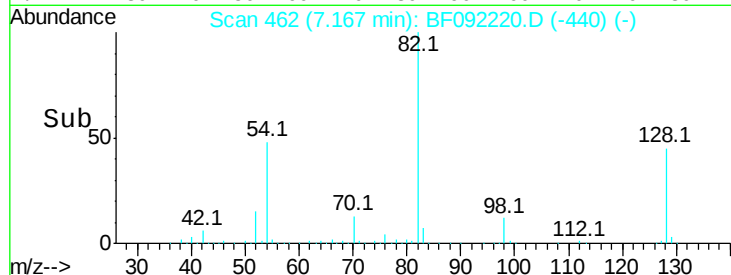

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.62 min Scan# 677

Delta R.T. -0.06 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08


Tgt Ion:164 Resp: 455068

Ion Ratio Lower Upper

164 100

162 100.6 80.2 120.2



160 45.2 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

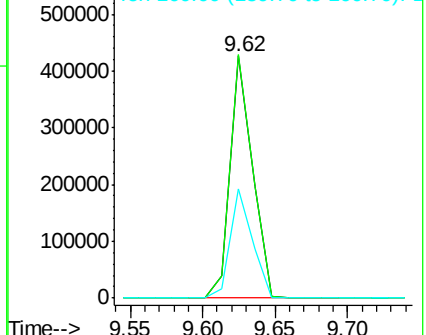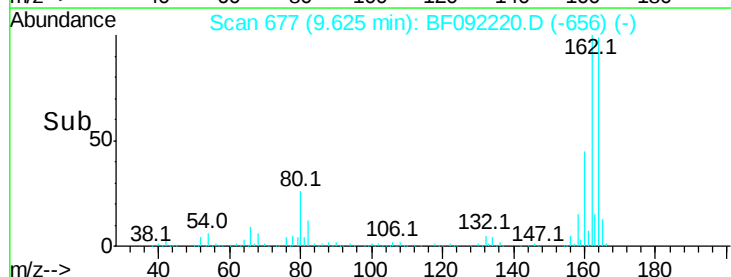







#41
 2,4,6-Tribromophenol
 Concen: 109.59 ng
 RT: 10.42 min Scan# 747
 Delta R.T. -0.05 min
 Lab File: BF092220.D
 Acq: 12 Jan 2017 21:08

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0015

Tot Ion:330 Resp: 412716
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.4 116.2
 141 32.7 34.1 51.1#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

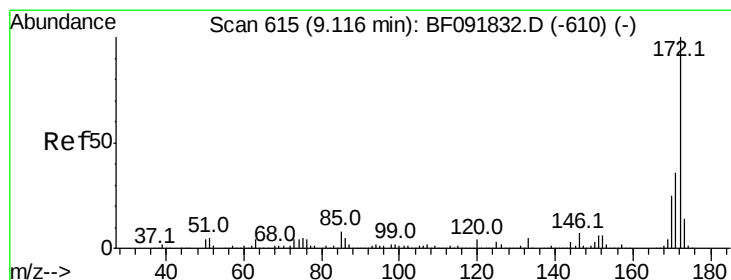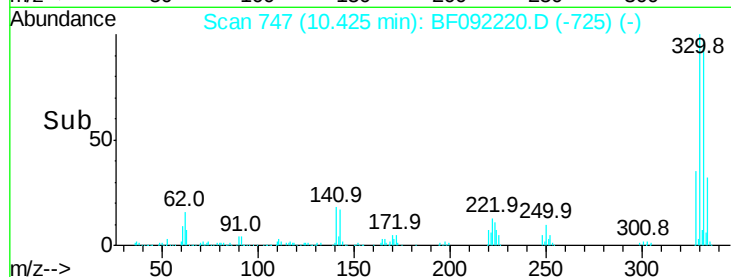
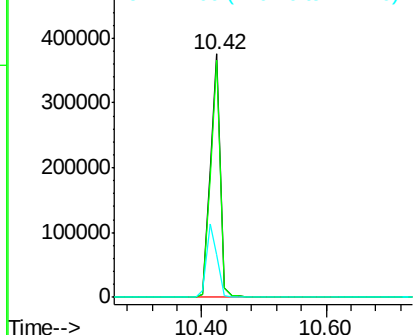



#44
 2-Fluorobiphenyl
 Concen: 70.24 ng
 RT: 8.96 min Scan# 619
 Delta R.T. -0.05 min
 Lab File: BF092220.D
 Acq: 12 Jan 2017 21:08

Tgt Ion:172 Resp: 1609839
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.4 44.0
 170 24.1 20.2 30.4

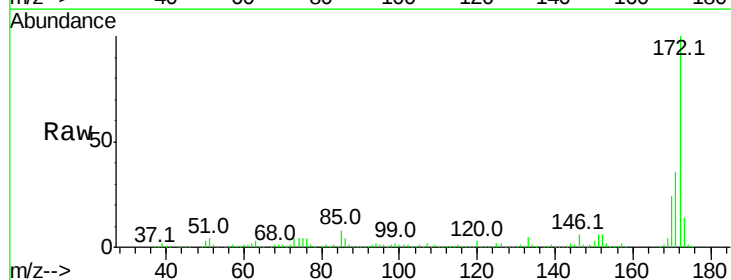

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

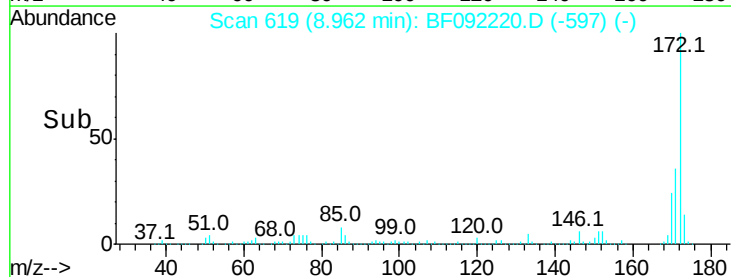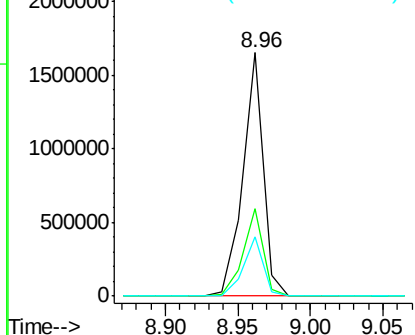

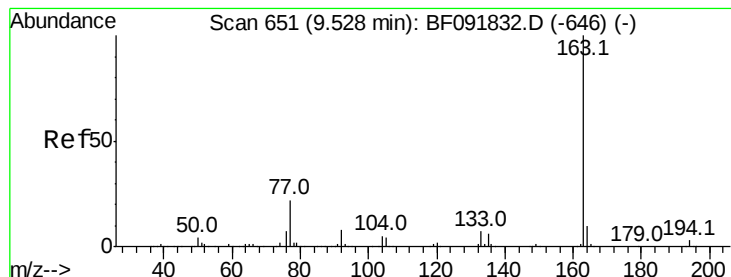

#49

Dimethylphthalate

Concen: 17.21 ng

RT: 9.36 min Scan# 654

Delta R.T. -0.06 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Instrument :

BNA_F

ClientSampleId :

COMP-0015


Tot Ion:163 Resp: 500985

Ion Ratio Lower Upper

163 100

194 3.1 3.0 4.4




164 10.2 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

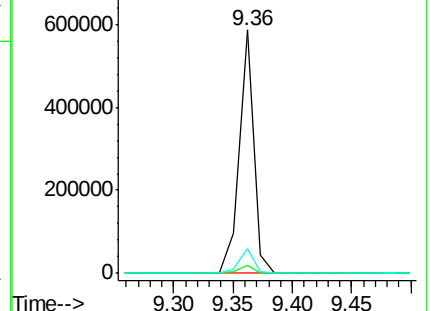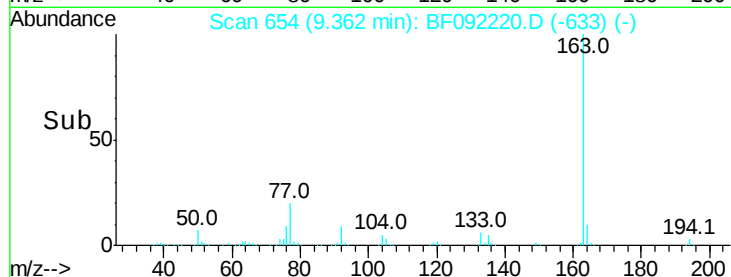

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.11 min Scan# 807

Delta R.T. -0.05 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08


Tgt Ion:188 Resp: 690090

Ion Ratio Lower Upper

188 100

94 7.3 10.0 15.0#



80 7.8 11.2 16.8#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

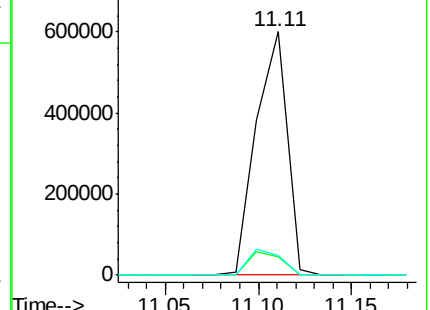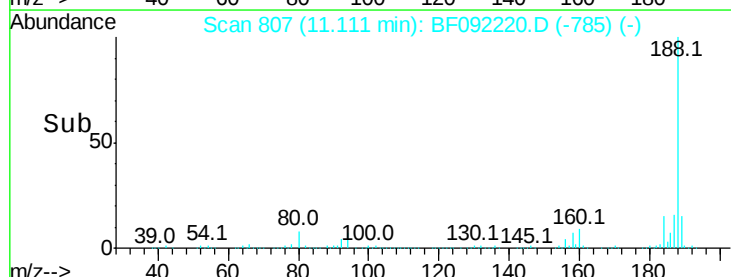

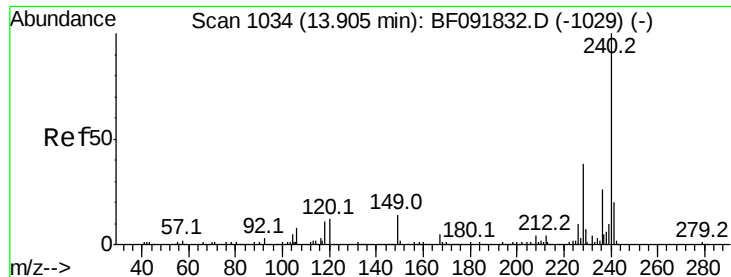

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.73 min Scan# 1036

Delta R.T. -0.06 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08

Instrument :

BNA_F

ClientSampled :

COMP-0015


Tot Ion:240 Resp: 510450

Ion Ratio Lower Upper

240 100

120 17.2 12.9 19.3




236 24.5 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

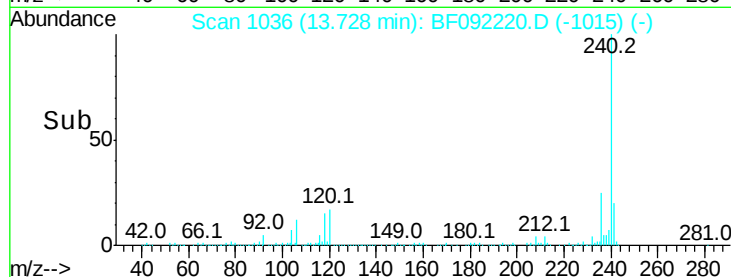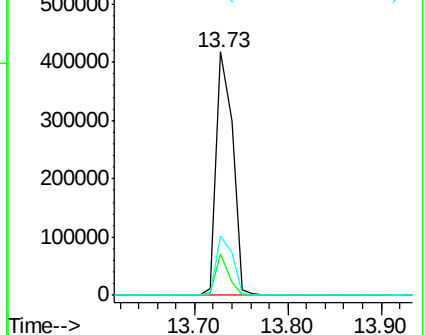

#78

Terphenyl-d14

Concen: 69.10 ng

RT: 12.69 min Scan# 945

Delta R.T. -0.06 min

Lab File: BF092220.D

Acq: 12 Jan 2017 21:08


Tgt Ion:244 Resp: 1454295

Ion Ratio Lower Upper

244 100

212 7.1 6.2 9.2



122 15.7 11.4 17.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

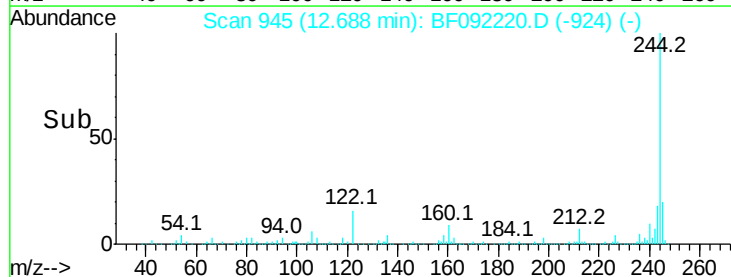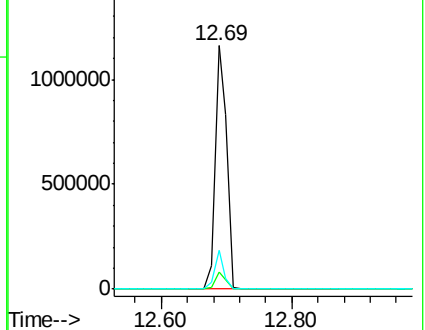


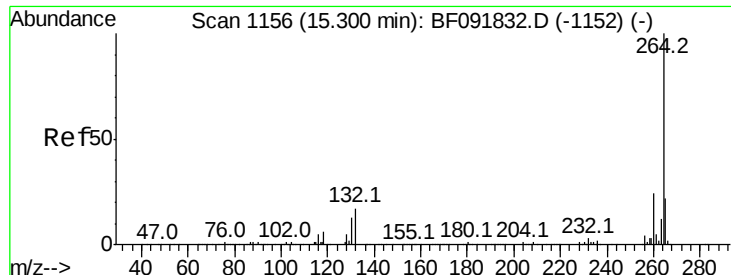

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.09 min Scan# 1155
 Delta R.T. -0.06 min
 Lab File: BF092220.D
 Acq: 12 Jan 2017 21:08

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0015

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.8	17.4	26.0



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

