

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
 Data File : BF092221.D
 Acq On : 12 Jan 2017 21:37
 Operator : UM/SJ
 Sample : I1030-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Quant Time: Jan 13 00:17:54 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.60	152	154694	20.00	ng	-0.05
21) Naphthalene-d8	7.88	136	622007	20.00	ng	-0.06
38) Acenaphthene-d10	9.62	164	307813	20.00	ng	-0.06
63) Phenanthrene-d10	11.11	188	550234	20.00	ng	-0.05
75) Chrysene-d12	13.73	240	318766	20.00	ng	-0.06
86) Perylene-d12	15.09	264	310878	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1072463	115.76	ng	-0.05
7) Phenol-d6	6.26	99	1459052	128.99	ng	-0.05
23) Nitrobenzene-d5	7.17	82	1012420	90.51	ng	-0.05
41) 2,4,6-Tribromophenol	10.42	330	328254	128.86	ng	-0.05
44) 2-Fluorobiphenyl	8.96	172	1650444	114.31	ng	-0.05
78) Terphenyl-d14	12.69	244	1085859	82.62	ng	-0.06
Target Compounds						
10) Phenol	6.28	94	26323	2.04	ng	78
49) Dimethylphthalate	9.36	163	448789	22.80	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
Data File : BF092221.D
Acq On : 12 Jan 2017 21:37
Operator : UM/SJ
Sample : I1030-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-0016

Quant Time: Jan 13 00:17:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

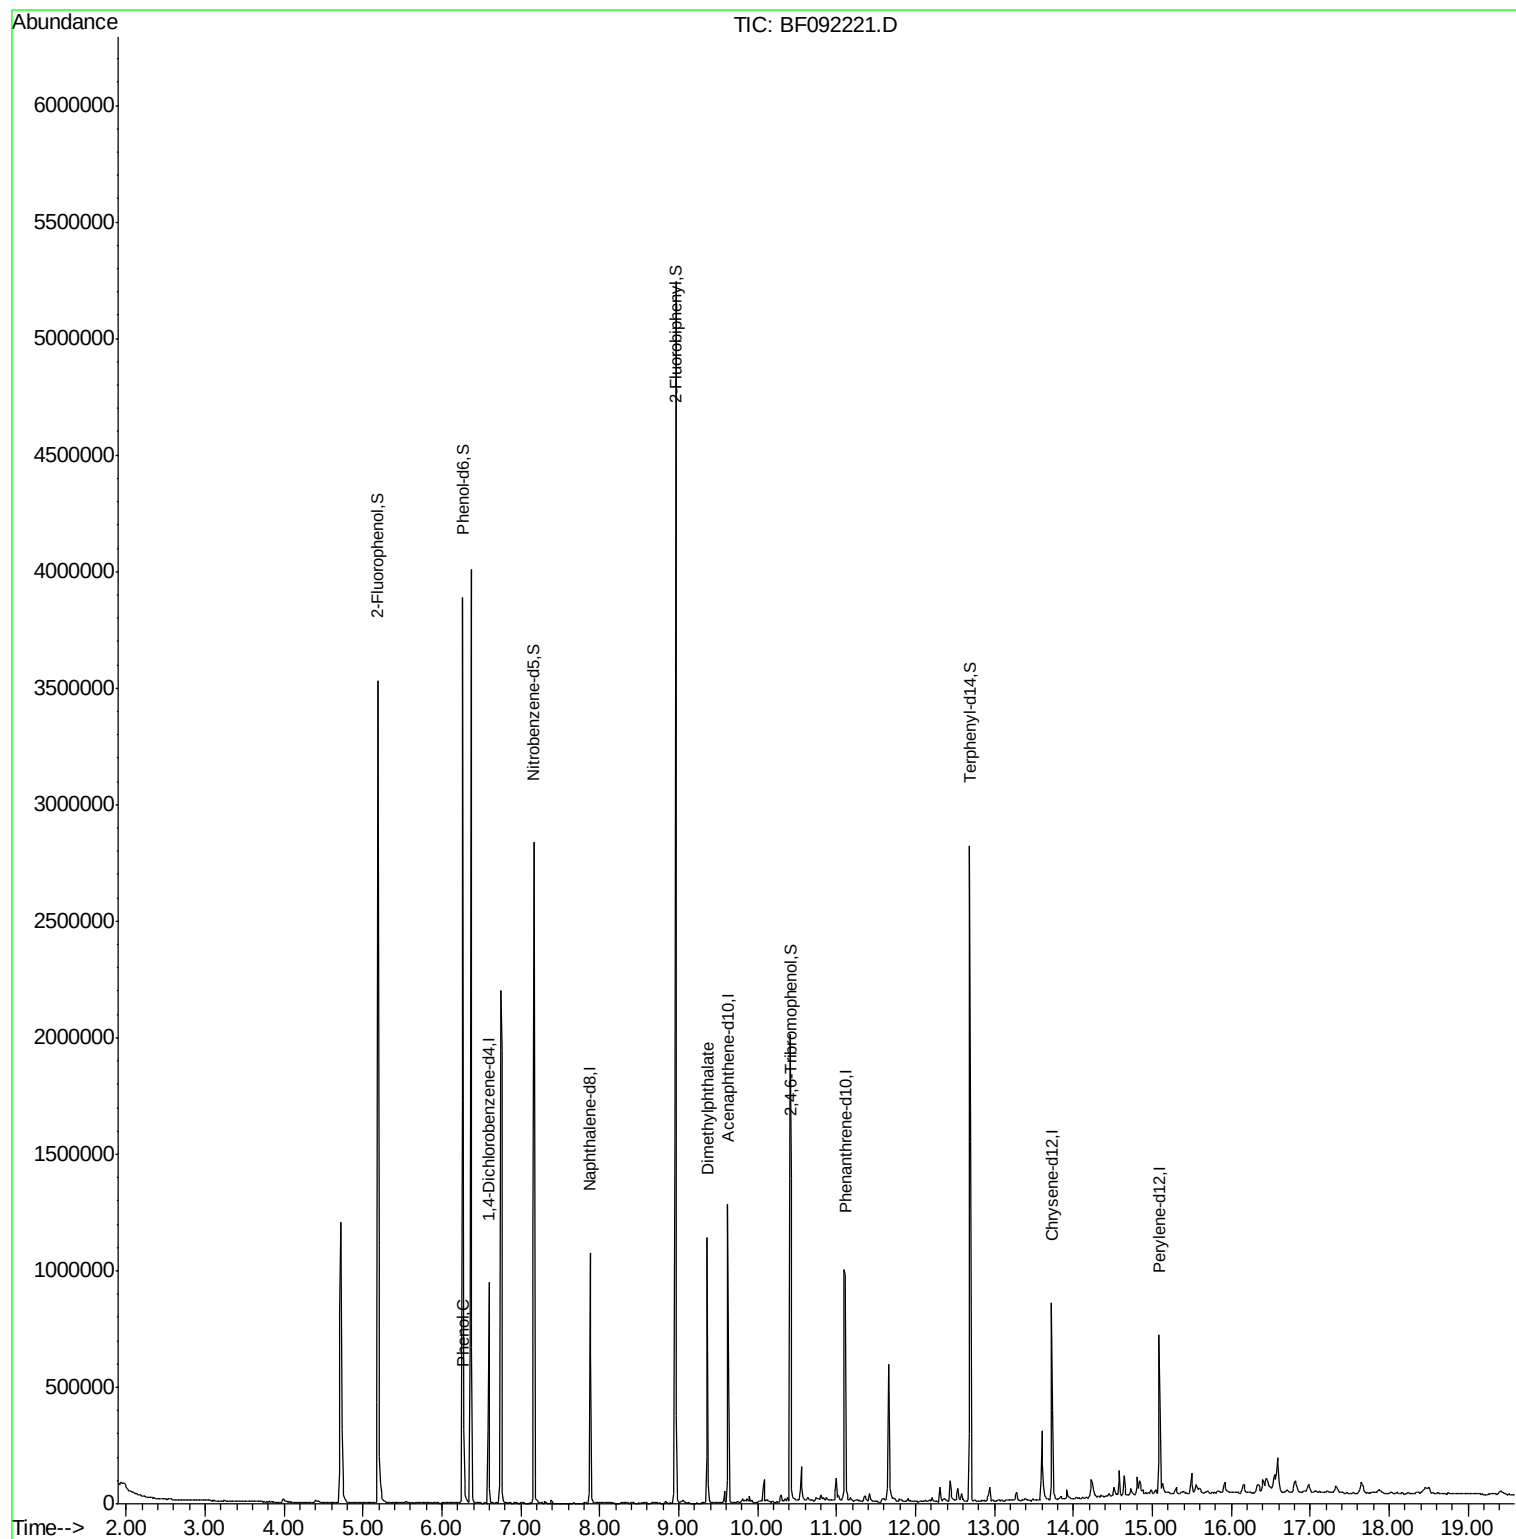

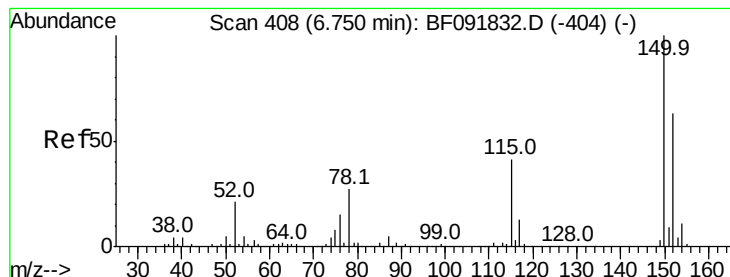

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.60 min Scan# 412

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tot Ion:152 Resp: 154694

Ion Ratio Lower Upper

152 100

150 156.5 124.9 187.3




115 57.1 46.0 69.0

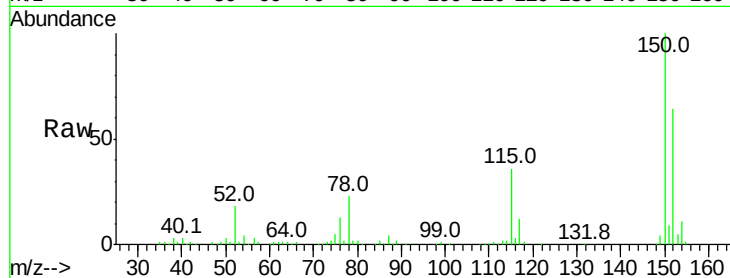

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

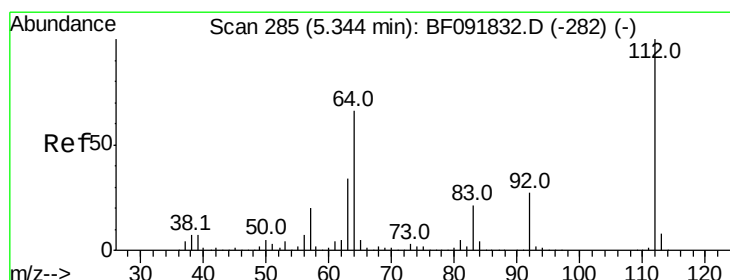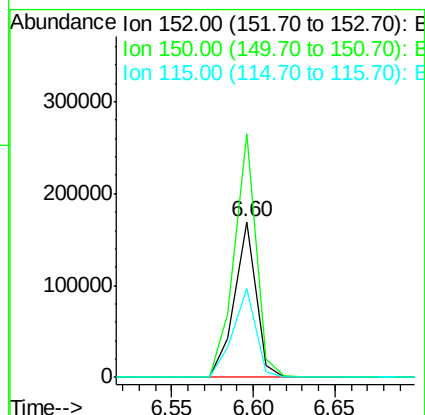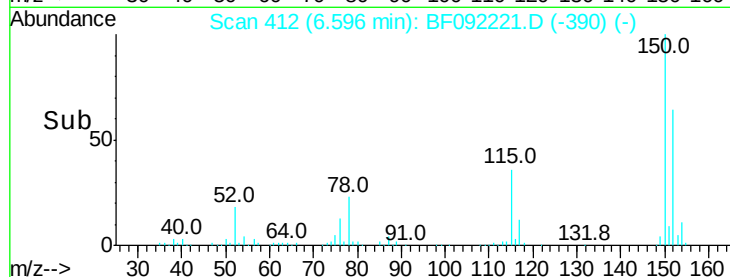

#5

2-Fluorophenol

Concen: 115.76 ng

RT: 5.19 min Scan# 289

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion:112 Resp: 1072463

Ion Ratio Lower Upper

112 100

64 64.8 46.1 69.1



63 33.0 23.8 35.6

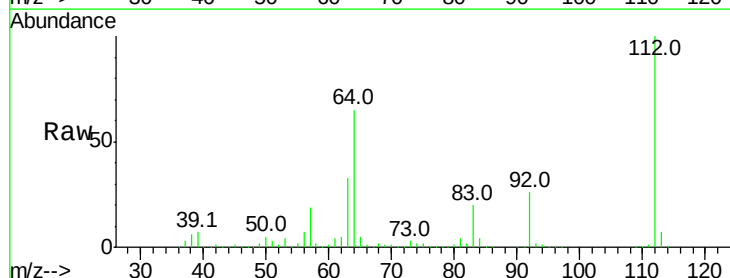


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

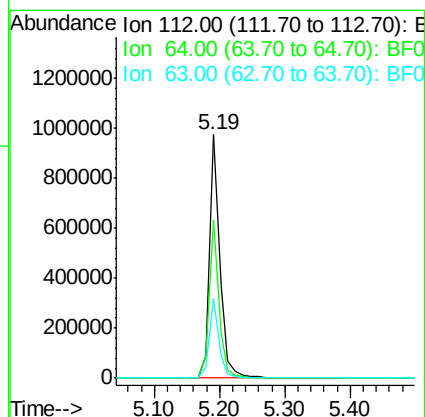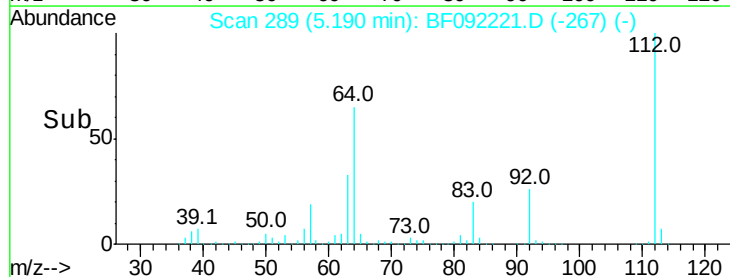

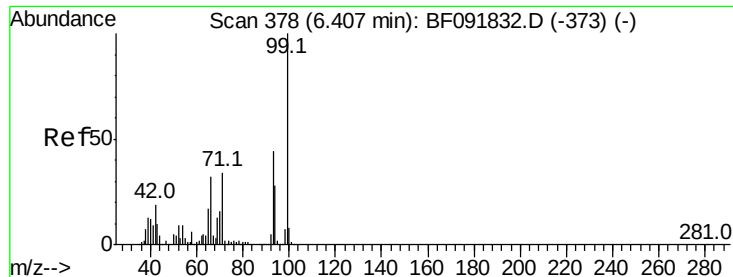

#7

Phenol-d6

Concen: 128.99 ng

RT: 6.26 min Scan# 383

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tot Ion: 99 Resp: 1459052

Ion Ratio Lower Upper

99 100

42 18.4 15.6 23.4




71 33.7 27.5 41.3

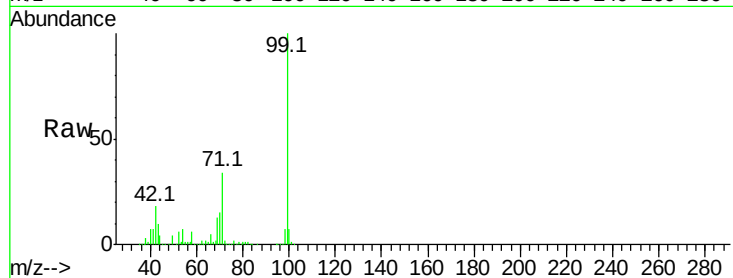

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

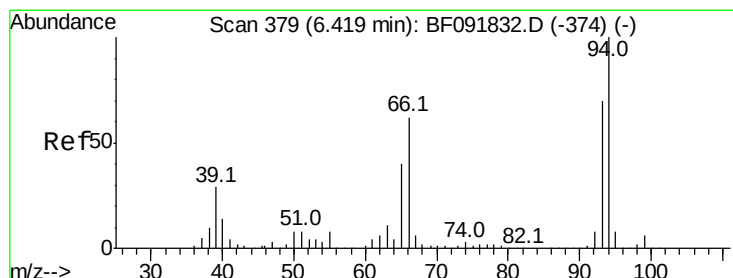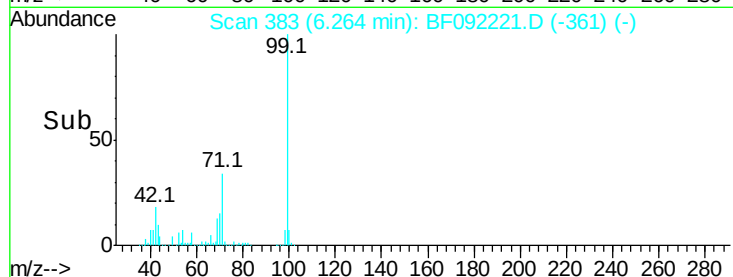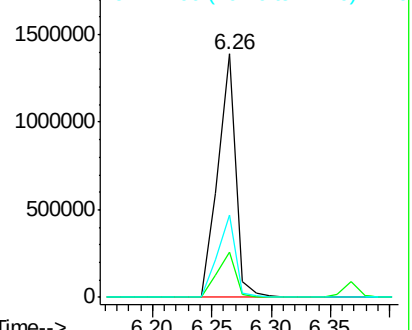

#10

Phenol

Concen: 2.04 ng

RT: 6.28 min Scan# 384

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion: 94 Resp: 26323

Ion Ratio Lower Upper

94 100

65 28.0 21.4 61.4



66 46.3 44.0 84.0

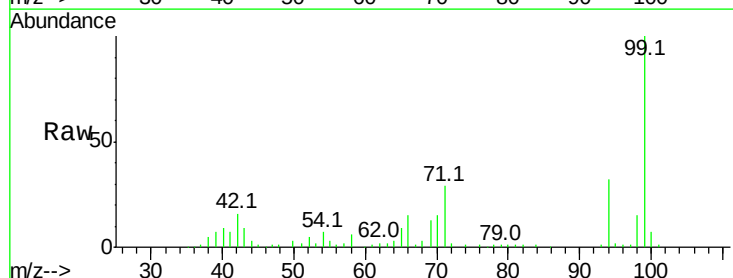


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

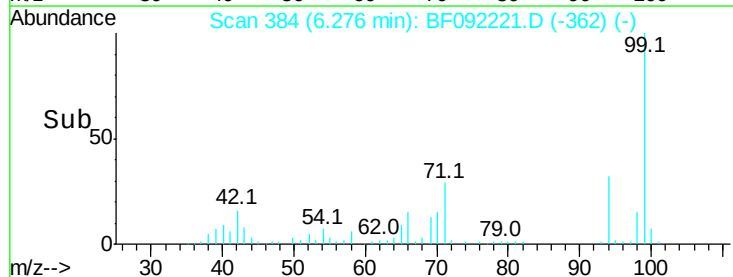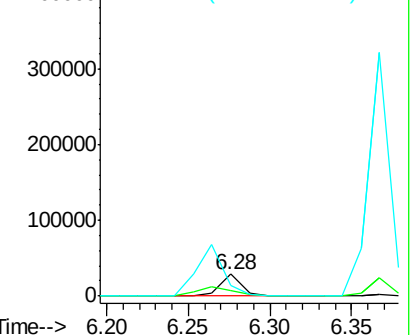


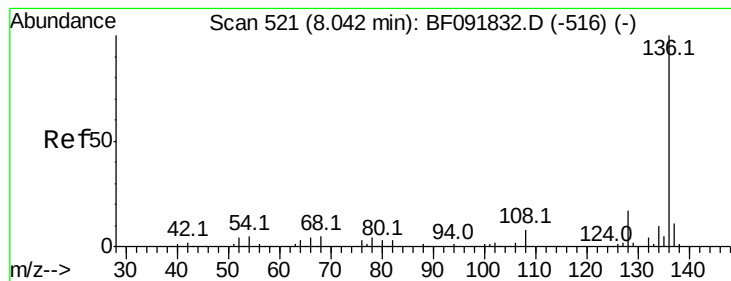




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.88 min Scan# 524
Delta R.T. -0.06 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37

Instrument :
BNA_F
ClientSampleId :
COMP-0016

Tot Ion:136	Resp:	622007	
Ion Ratio	Lower	Upper	
136 100			
137 11.2	8.4	12.6	
54 10.0	4.5	6.7#	
68 7.2	3.6	5.4#	

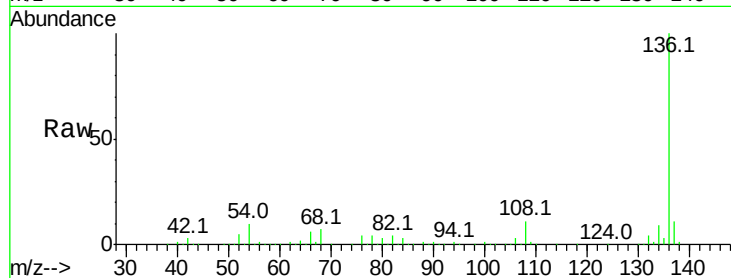


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

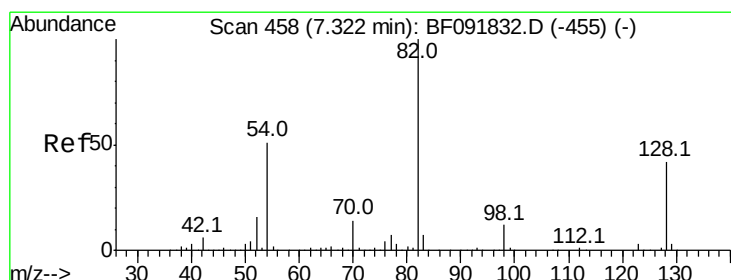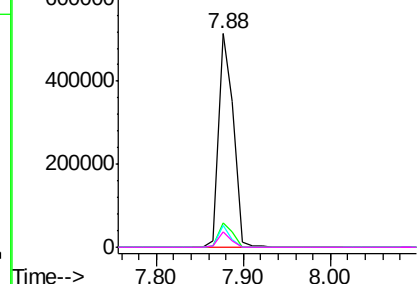
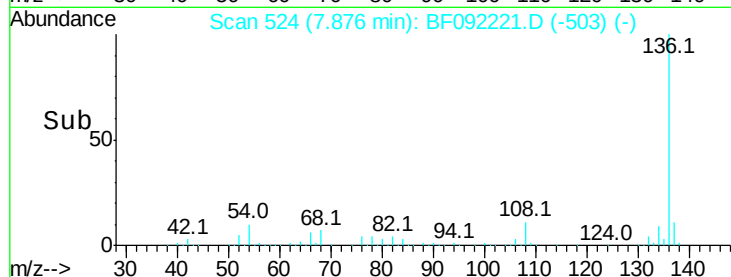



#23
Nitrobenzene-d5
Concen: 90.51 ng
RT: 7.17 min Scan# 462
Delta R.T. -0.05 min
Lab File: BF092221.D
Acq: 12 Jan 2017 21:37

Tgt Ion: 82	Resp: 1012420
Ion Ratio	Lower Upper
82 100	
128 43.6	34.6 52.0
54 49.2	39.5 59.3

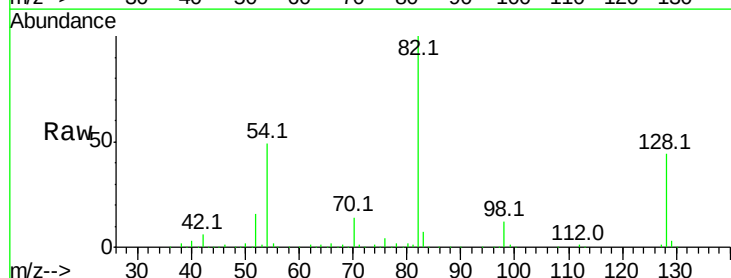

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

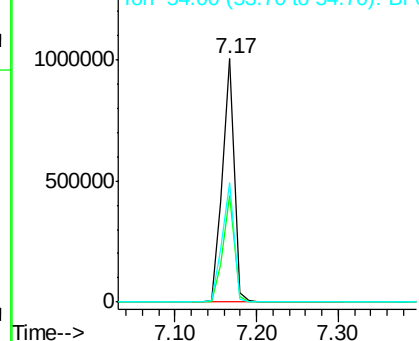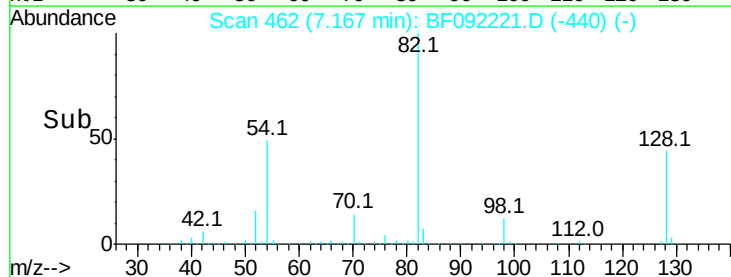

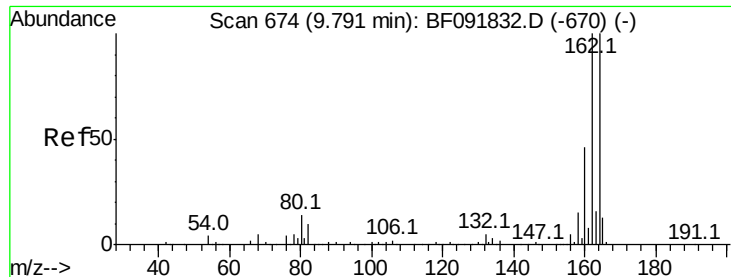

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.62 min Scan# 677

Delta R.T. -0.06 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tot Ion:164 Resp: 307813

Ion Ratio Lower Upper

164 100

162 102.1 80.2 120.2




160 45.0 36.9 55.3

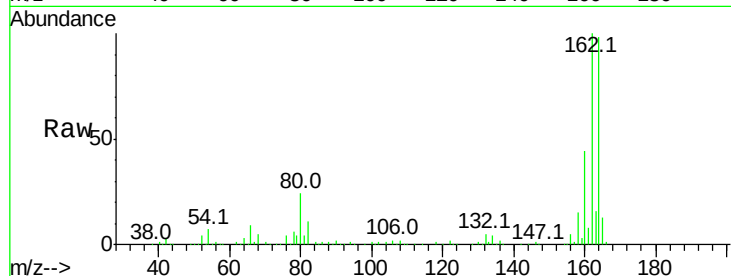

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

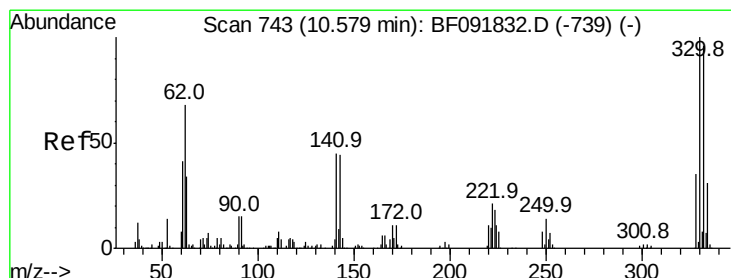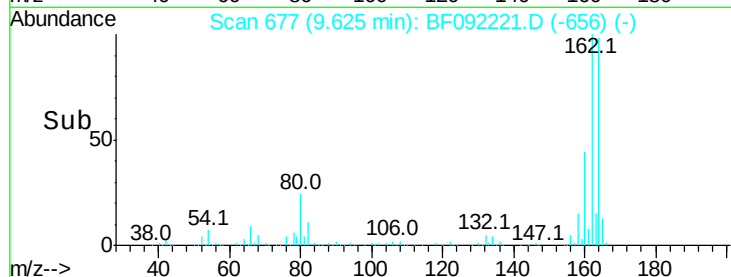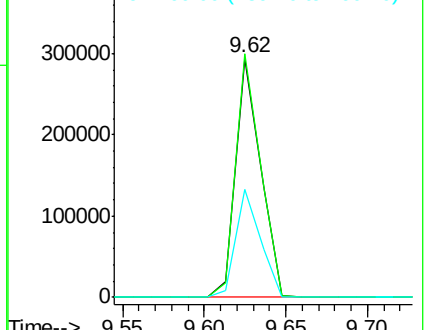

#41

2,4,6-Tribromophenol

Concen: 128.86 ng

RT: 10.42 min Scan# 747

Delta R.T. -0.05 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion:330 Resp: 328254

Ion Ratio Lower Upper

330 100

332 95.4 77.4 116.2



141 33.3 34.1 51.1#

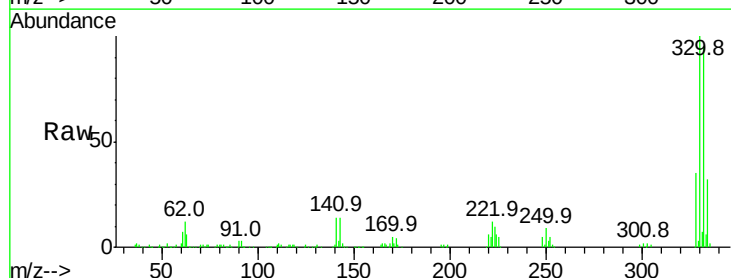


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

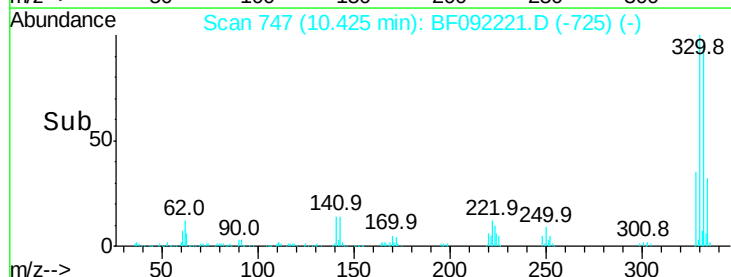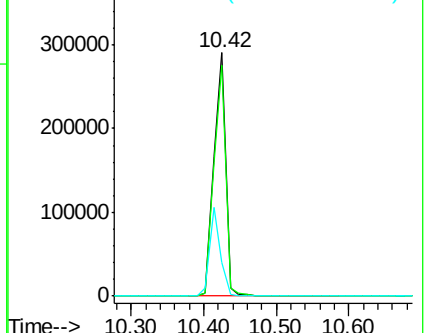

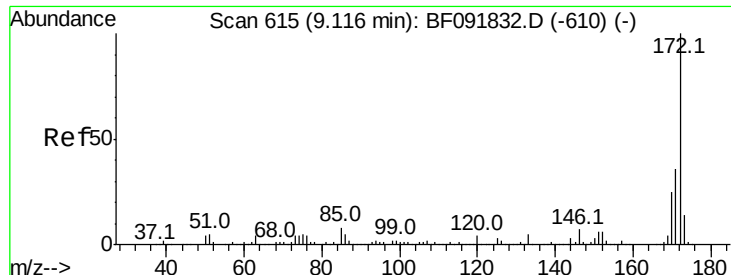


#44
 2-Fluorobiphenyl
 Concen: 114.31 ng
 RT: 8.96 min Scan# 619
 Delta R.T. -0.05 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37




Instrument :
 BNA_F
 ClientSampleId :
 COMP-0016

Tot Ion:172 Resp: 1650444

Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.4	44.0
170	24.6	20.2	30.4

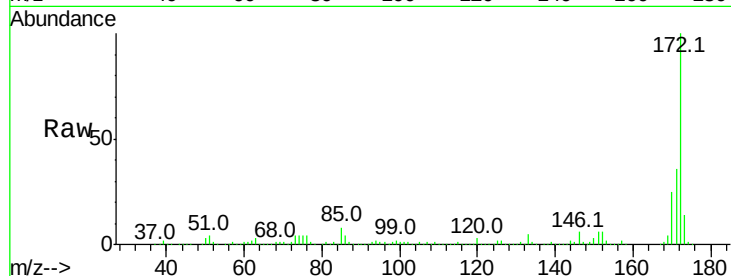


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

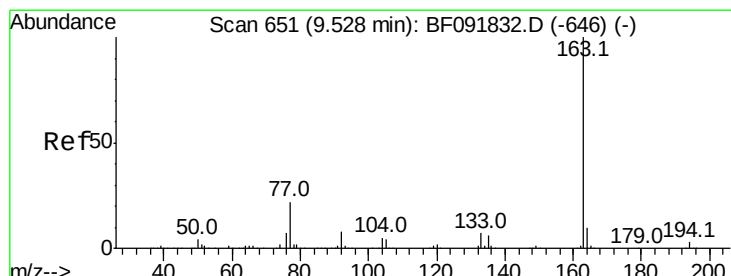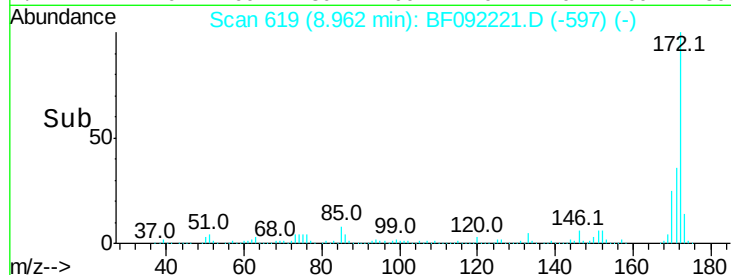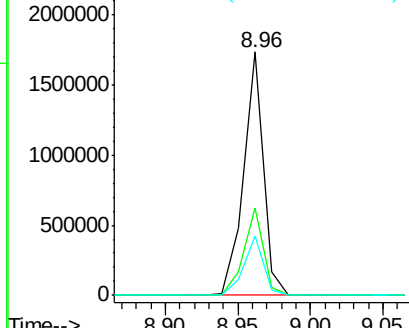



#49
 Dimethylphthalate
 Concen: 22.80 ng
 RT: 9.36 min Scan# 654
 Delta R.T. -0.06 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37


Tgt Ion:163 Resp: 448789

Ion	Ratio	Lower	Upper
163	100		
194	3.1	3.0	4.4
164	10.3	8.0	12.0

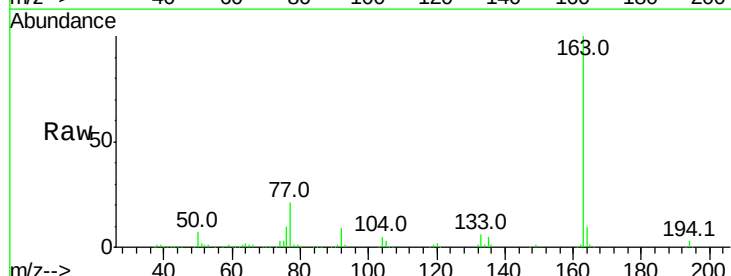

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



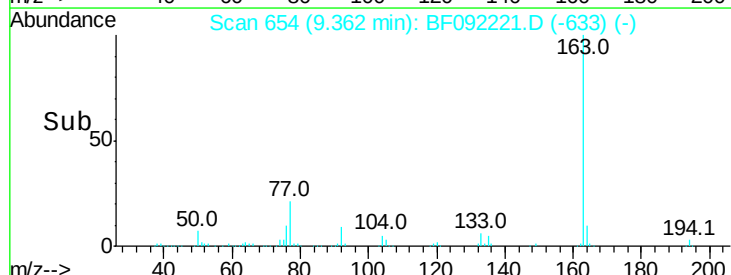
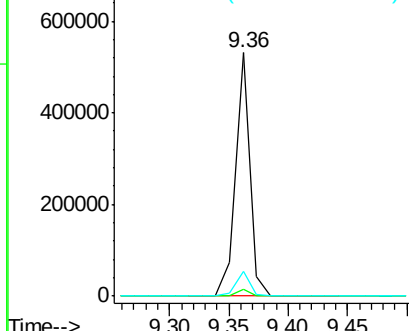


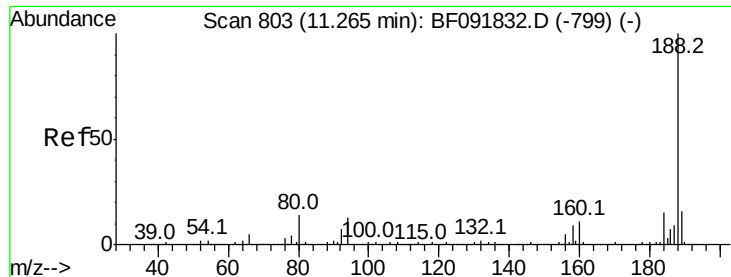

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.11 min Scan# 807
 Delta R.T. -0.05 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37




Instrument :
 BNA_F
 ClientSampled :
 COMP-0016


Tot Ion:188 Resp: 550234
 Ion Ratio Lower Upper
 188 100
 94 6.7 10.0 15.0#
 80 6.8 11.2 16.8#

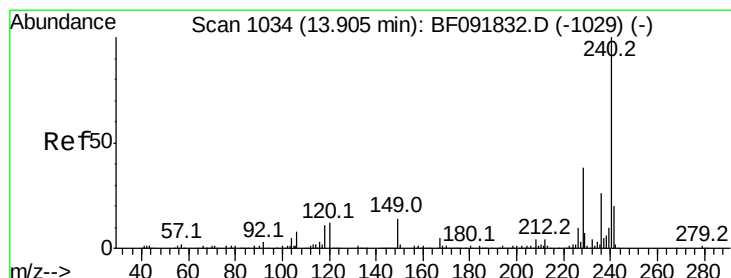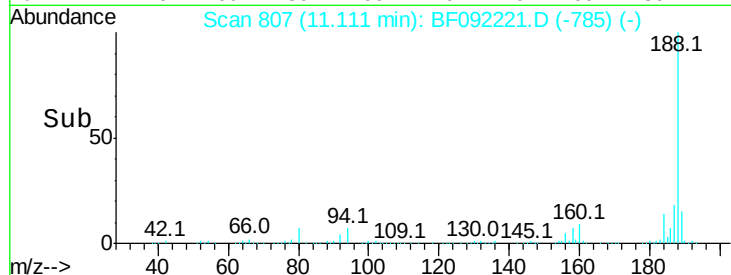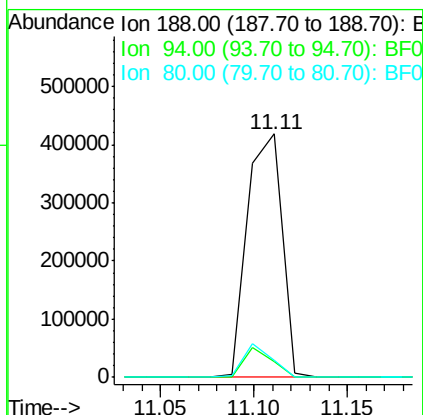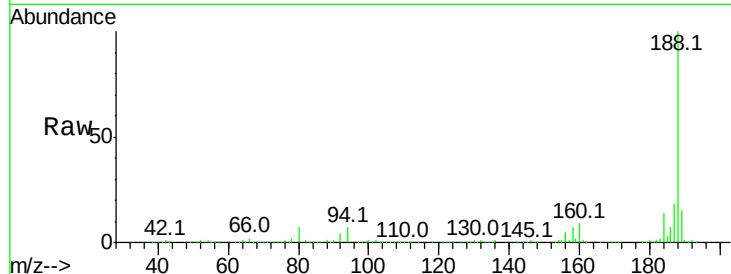

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.73 min Scan# 1036
 Delta R.T. -0.06 min
 Lab File: BF092221.D
 Acq: 12 Jan 2017 21:37

Tgt Ion:240 Resp: 318766
 Ion Ratio Lower Upper
 240 100
 120 15.6 12.9 19.3
 236 24.6 20.9 31.3

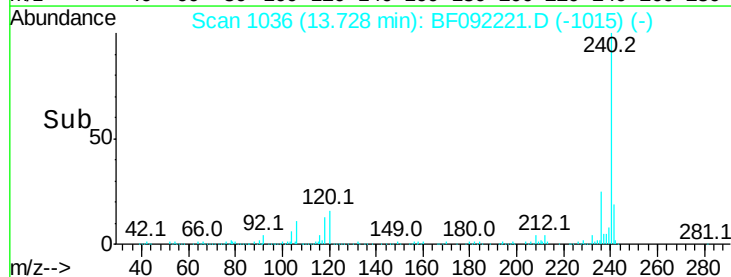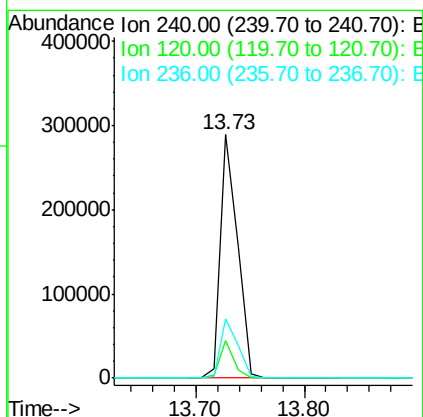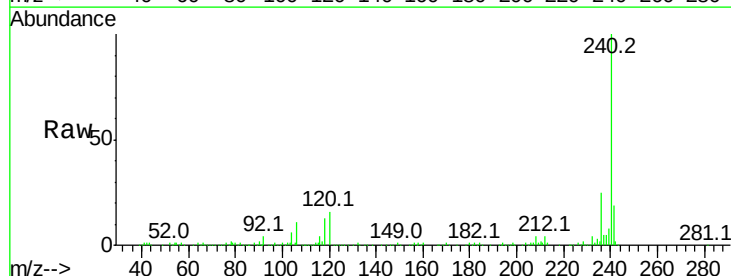

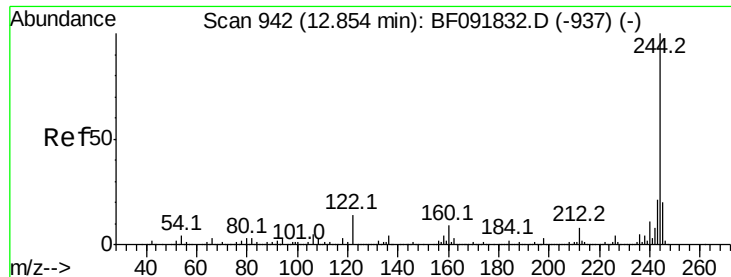

#78

Terphenyl-d14

Concen: 82.62 ng

RT: 12.69 min Scan# 945

Delta R.T. -0.06 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37

Instrument :

BNA_F

ClientSampleId :

COMP-0016


Tot Ion:244 Resp: 1085859

Ion Ratio Lower Upper

244 100

212 7.3 6.2 9.2




122 15.0 11.4 17.2

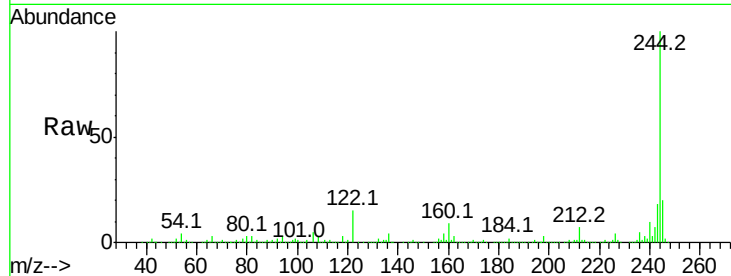

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

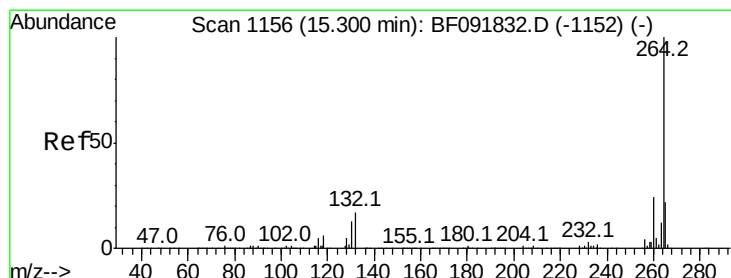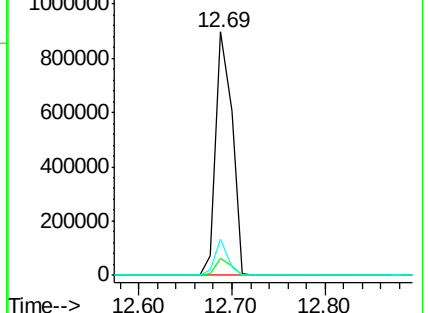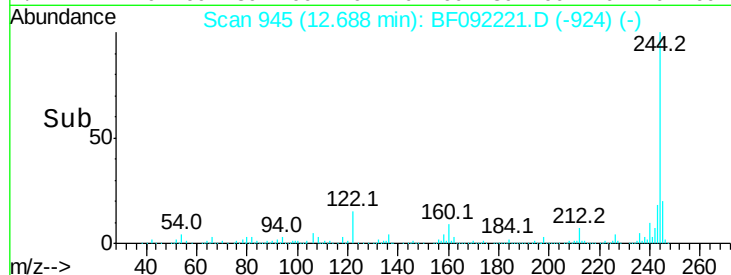

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.09 min Scan# 1155

Delta R.T. -0.06 min

Lab File: BF092221.D

Acq: 12 Jan 2017 21:37


Tgt Ion:264 Resp: 310878

Ion Ratio Lower Upper

264 100

260 24.2 19.2 28.8

265 22.5 17.4 26.0

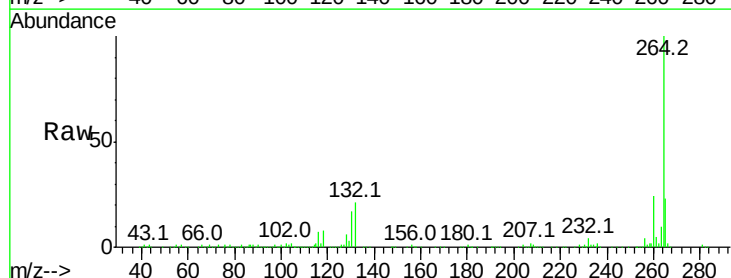

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

