

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
 Data File : BF092225.D
 Acq On : 12 Jan 2017 23:31
 Operator : UM/SJ
 Sample : I1030-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-0020

Quant Time: Jan 13 00:34:05 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.60	152	172684	20.00	ng	-0.05
21) Naphthalene-d8	7.88	136	638723	20.00	ng	-0.06
38) Acenaphthene-d10	9.62	164	309555	20.00	ng	-0.06
63) Phenanthrene-d10	11.11	188	538458	20.00	ng	-0.05
75) Chrysene-d12	13.73	240	319306	20.00	ng	-0.06
86) Perylene-d12	15.09	264	312731	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	860857	83.24	ng	-0.05
7) Phenol-d6	6.26	99	1223502	96.90	ng	-0.05
23) Nitrobenzene-d5	7.17	82	872631	75.97	ng	-0.05
41) 2,4,6-Tribromophenol	10.42	330	254314	99.27	ng	-0.05
44) 2-Fluorobiphenyl	8.96	172	1065344	67.92	ng	-0.05
78) Terphenyl-d14	12.69	244	887748	67.43	ng	-0.06
Target Compounds						
10) Phenol	6.28	94	61327	4.26	ng	Qvalue # 67
49) Dimethylphthalate	9.36	163	127175	6.42	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
Data File : BF092225.D
Acq On : 12 Jan 2017 23:31
Operator : UM/SJ
Sample : I1030-19
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-0020

Quant Time: Jan 13 00:34:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

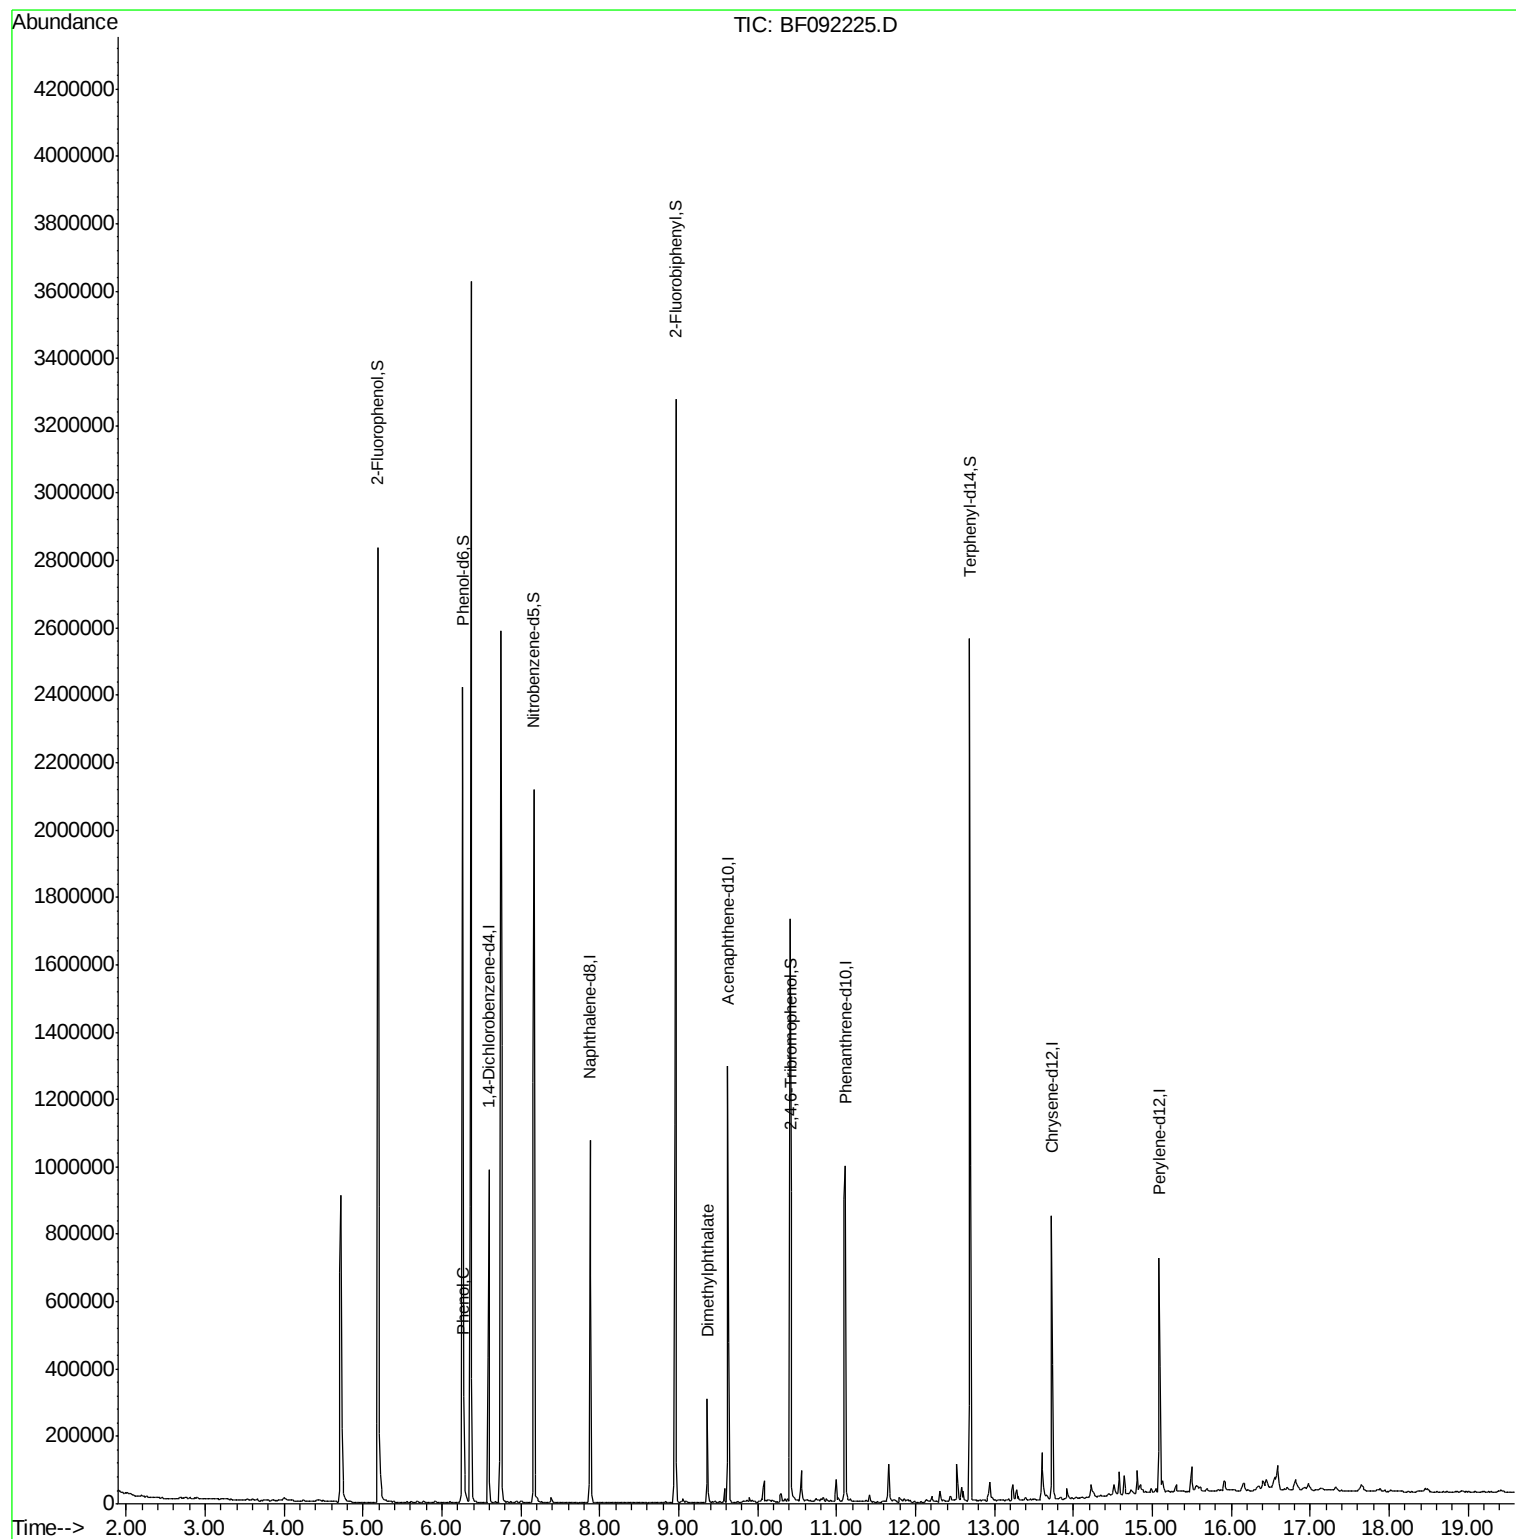

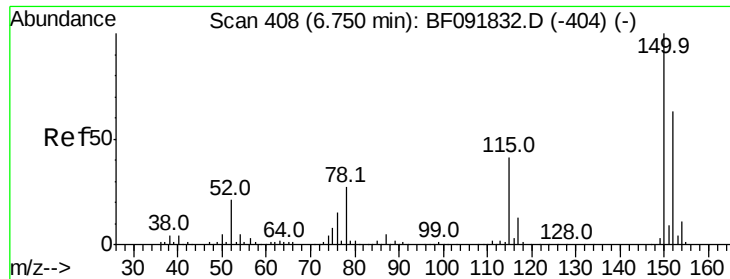


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.60 min Scan# 412
Delta R.T. -0.05 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Instrument :
BNA_F
ClientSampleId :
COMP-0020

Tot Ion:152 Resp: 172684
Ion Ratio Lower Upper
152 100
150 153.4 124.9 187.3
115 56.8 46.0 69.0

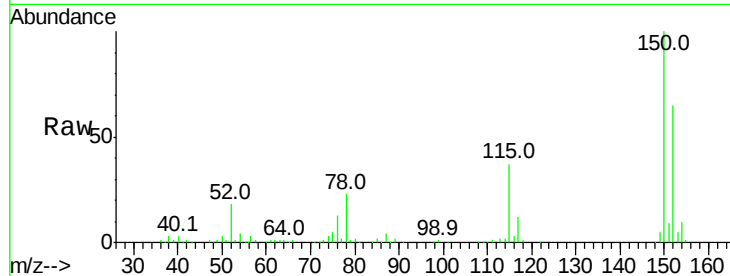


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

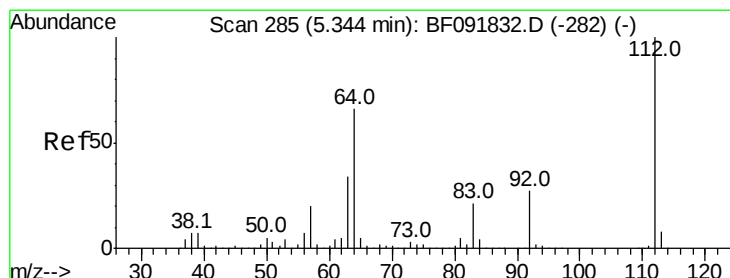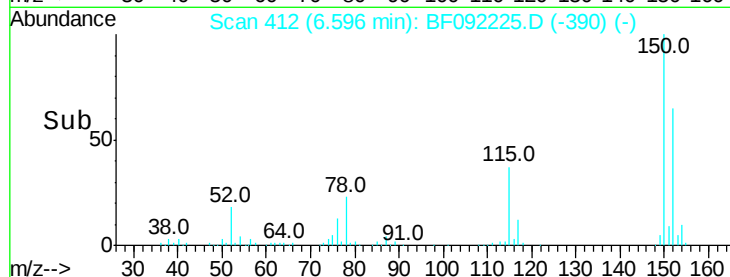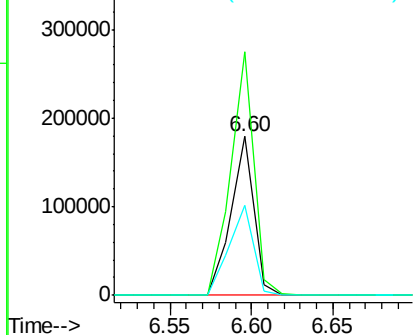



#5

2-Fluorophenol
Concen: 83.24 ng
RT: 5.19 min Scan# 289
Delta R.T. -0.05 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Tgt Ion:112 Resp: 860857
Ion Ratio Lower Upper
112 100
64 63.3 46.1 69.1
63 32.4 23.8 35.6

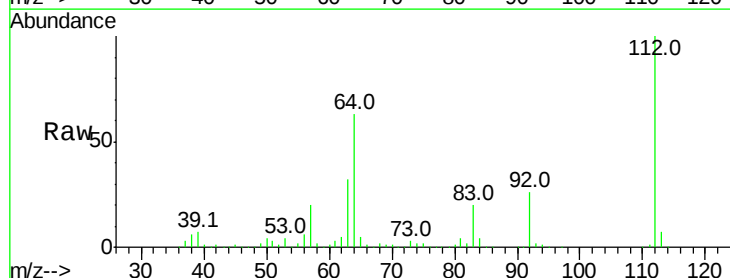

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

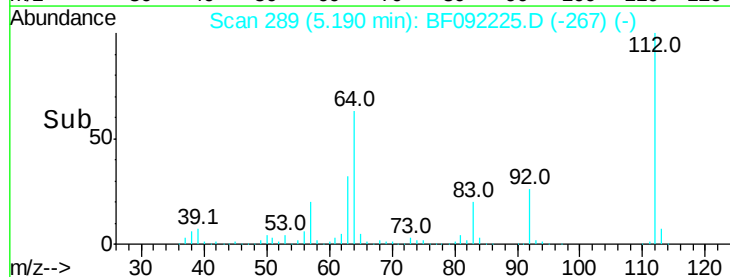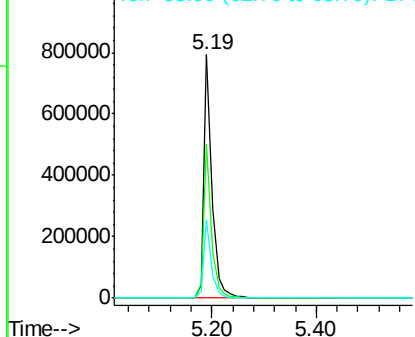



#7

Phenol-d6

Concen: 96.90 ng

RT: 6.26 min Scan# 383

Delta R.T. -0.05 min

Lab File: BF092225.D

Acq: 12 Jan 2017 23:31

Instrument :





BNA_F

ClientSampleId :

COMP-0020

Tot Ion: 99 Resp: 1223502

Ion	Ratio	Lower	Upper
99	100		
42	14.0	15.6	23.4#
71	28.9	27.5	41.3

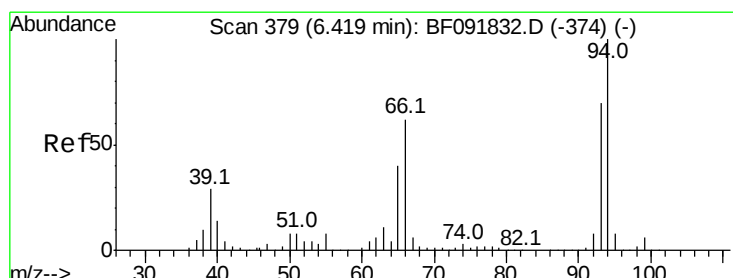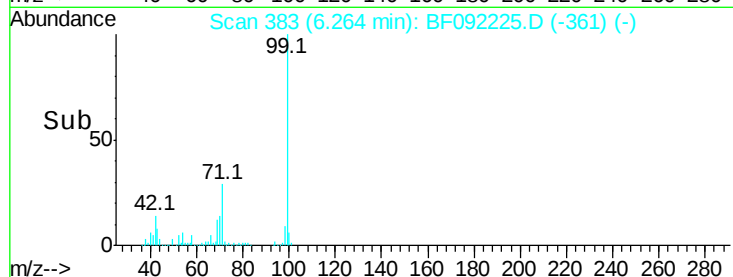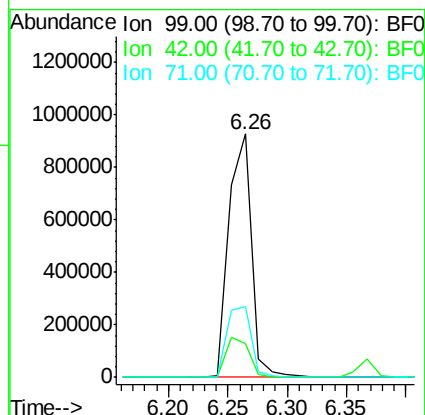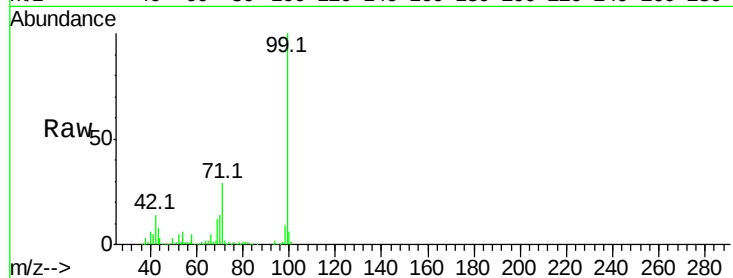

#10

Phenol

Concen: 4.26 ng

RT: 6.28 min Scan# 384




Delta R.T. -0.05 min


Lab File: BF092225.D

Acq: 12 Jan 2017 23:31

Tgt Ion: 94 Resp: 61327

Ion	Ratio	Lower	Upper
94	100		
65	24.2	21.4	61.4
66	35.7	44.0	84.0#

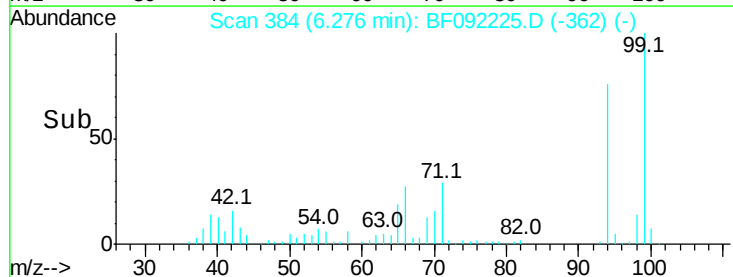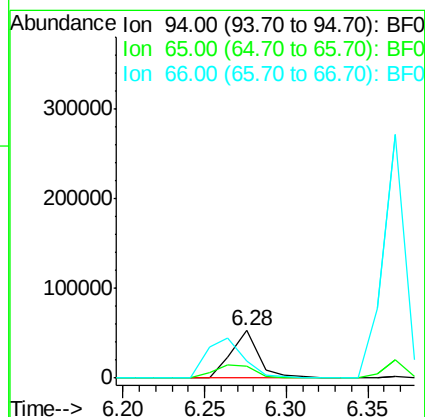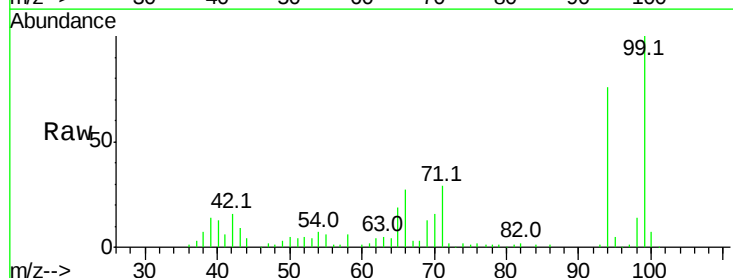


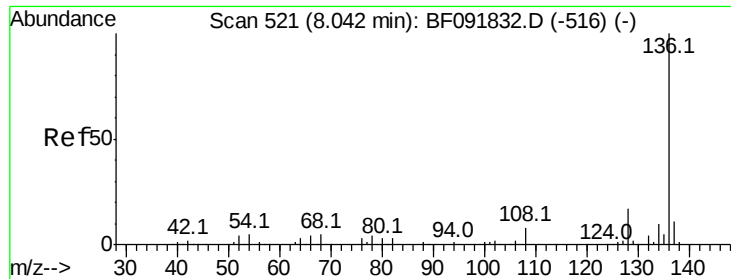




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.88 min Scan# 524
Delta R.T. -0.06 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Instrument :
BNA_F
ClientSampleId :
COMP-0020

Tot Ion:	136	Resp:	638723
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	9.6	4.5	6.7#
68	7.5	3.6	5.4#

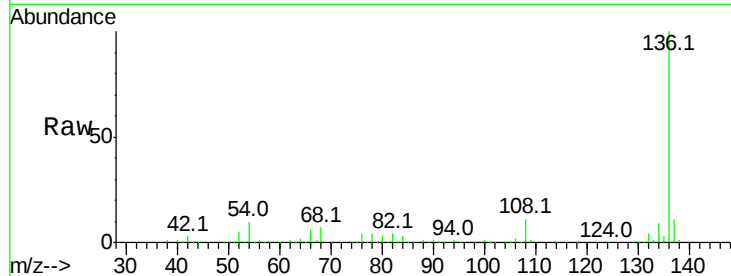


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

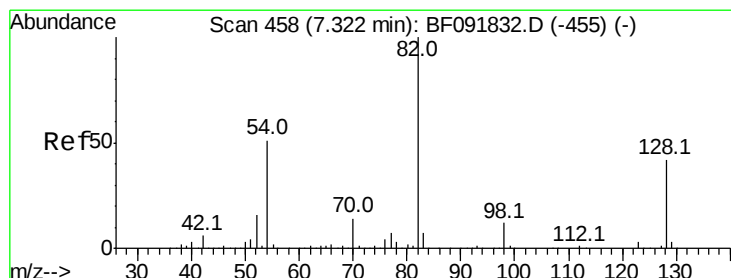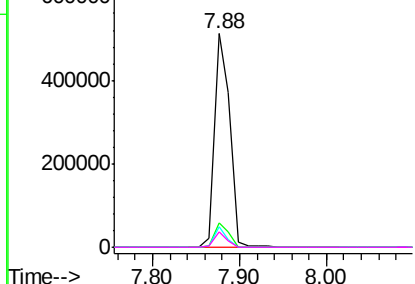
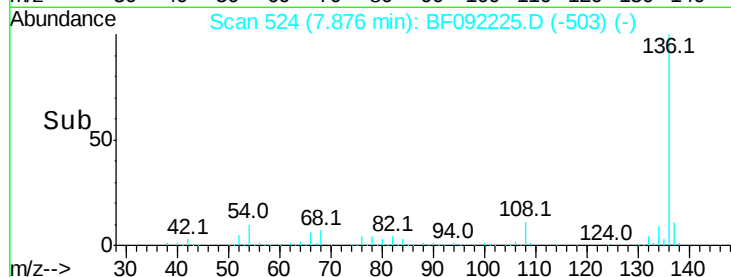



#23
Nitrobenzene-d5
Concen: 75.97 ng
RT: 7.17 min Scan# 462
Delta R.T. -0.05 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Tgt Ion:	82	Resp:	872631
Ion	Ratio	Lower	Upper
82	100		
128	48.5	34.6	52.0
54	44.1	39.5	59.3

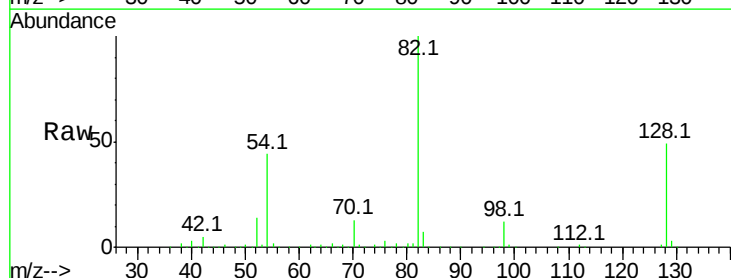

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

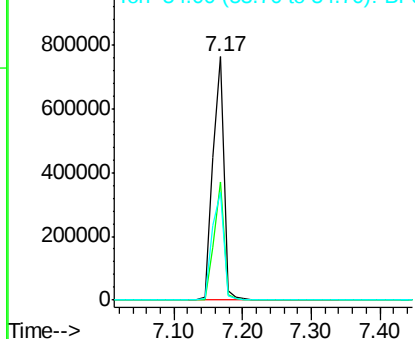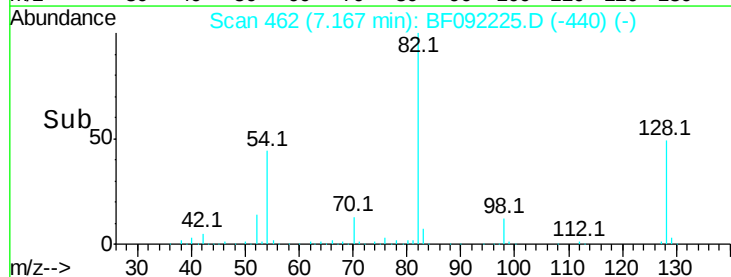

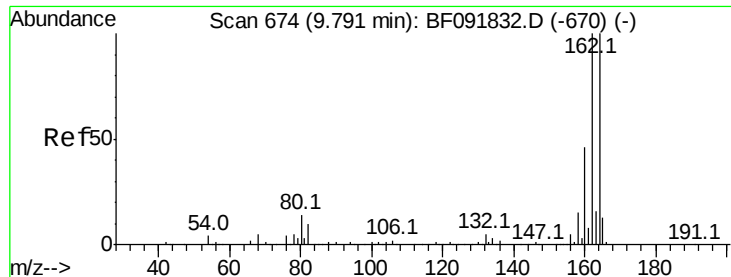

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.62 min Scan# 677

Delta R.T. -0.06 min

Lab File: BF092225.D

Acq: 12 Jan 2017 23:31

Instrument :

BNA_F

ClientSampleId :

COMP-0020


Tot Ion:164 Resp: 309555

Ion Ratio Lower Upper

164 100

162 102.2 80.2 120.2




160 45.3 36.9 55.3

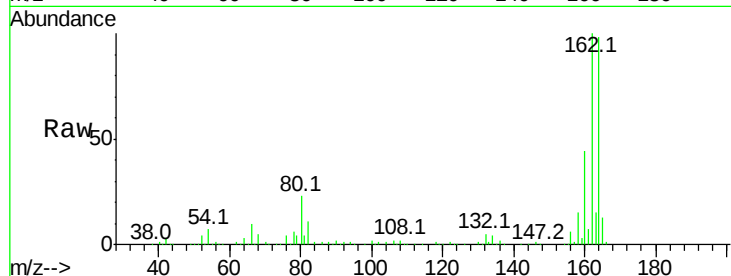

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

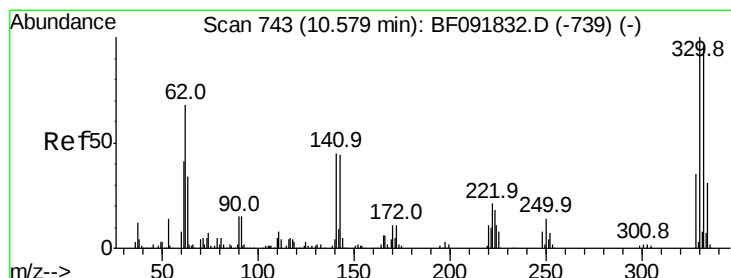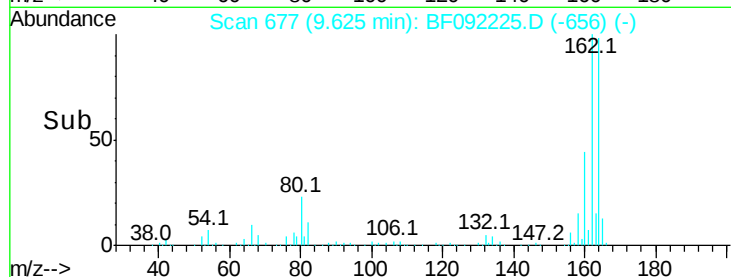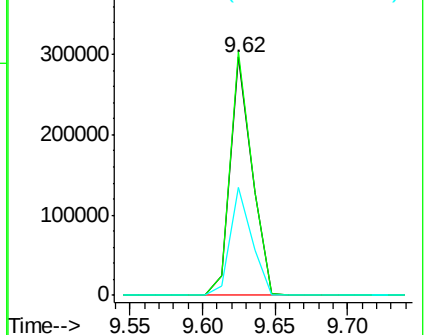

#41

2,4,6-Tribromophenol

Concen: 99.27 ng

RT: 10.42 min Scan# 747

Delta R.T. -0.05 min

Lab File: BF092225.D

Acq: 12 Jan 2017 23:31


Tgt Ion:330 Resp: 254314

Ion Ratio Lower Upper

330 100

332 95.2 77.4 116.2



141 33.7 34.1 51.1#

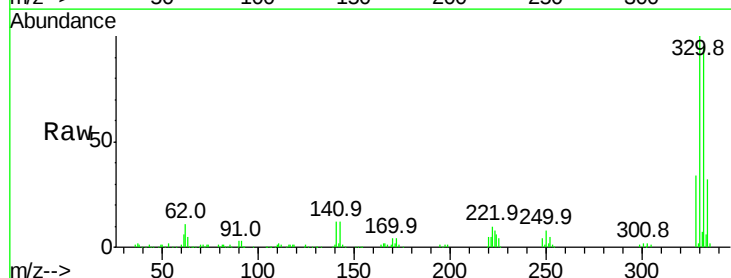

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

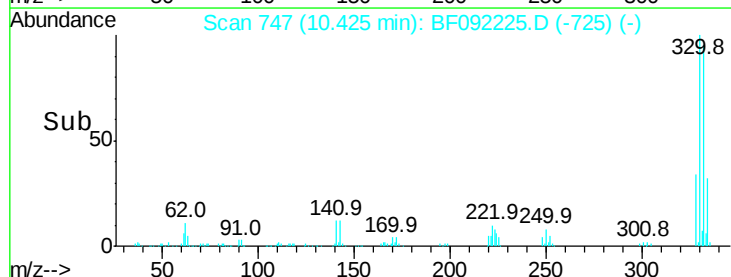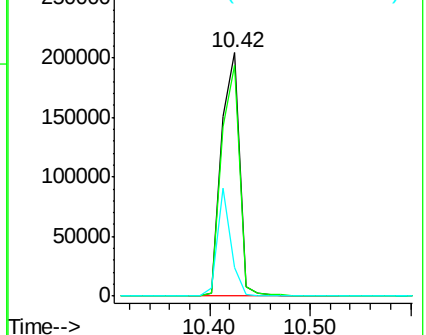







#44
2-Fluorobiphenyl
Concen: 67.92 ng
RT: 8.96 min Scan# 619
Delta R.T. -0.05 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Instrument :
BNA_F
ClientSampleId :
COMP-0020

Tot Ion:172 Resp: 1065344
Ion Ratio Lower Upper
172 100
171 35.7 29.4 44.0
170 23.9 20.2 30.4

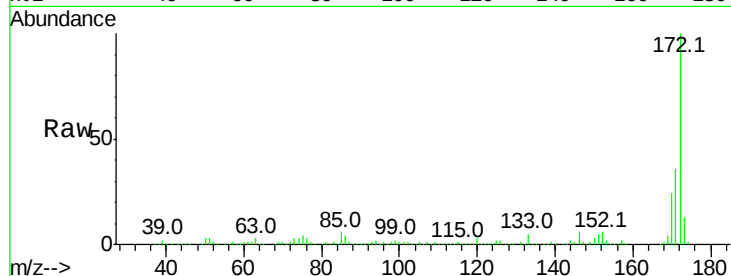


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

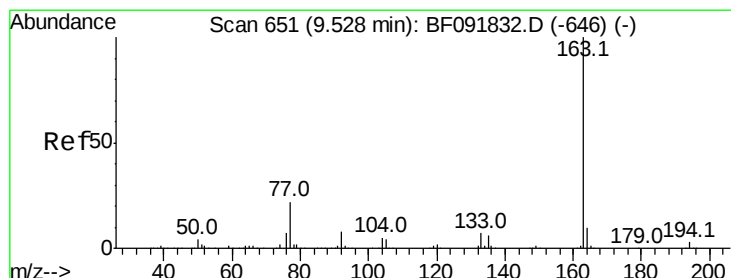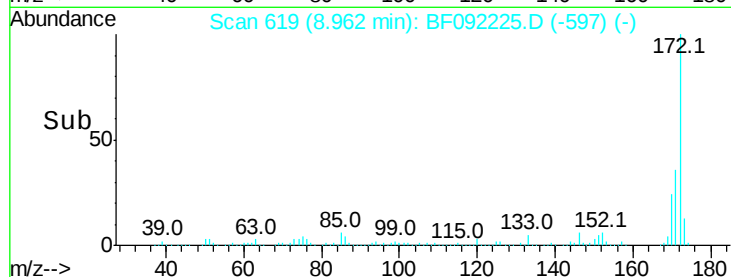
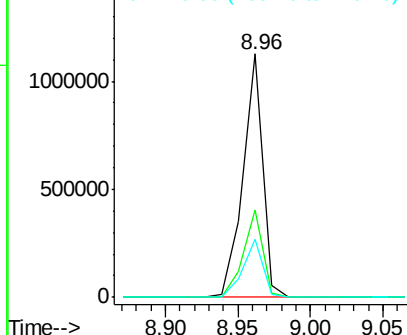



#49
Dimethylphthalate
Concen: 6.42 ng
RT: 9.36 min Scan# 654
Delta R.T. -0.06 min
Lab File: BF092225.D
Acq: 12 Jan 2017 23:31

Tgt Ion:163 Resp: 127175
Ion Ratio Lower Upper
163 100
194 3.0 3.0 4.4
164 9.9 8.0 12.0

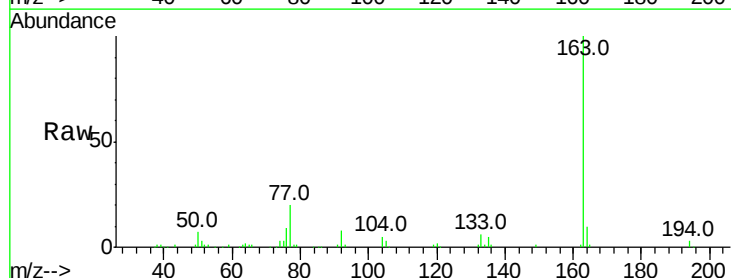

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



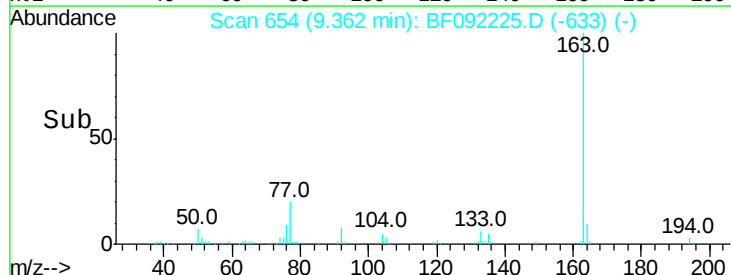
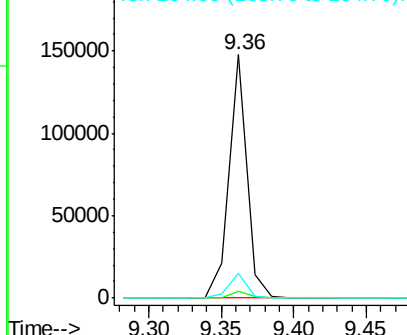


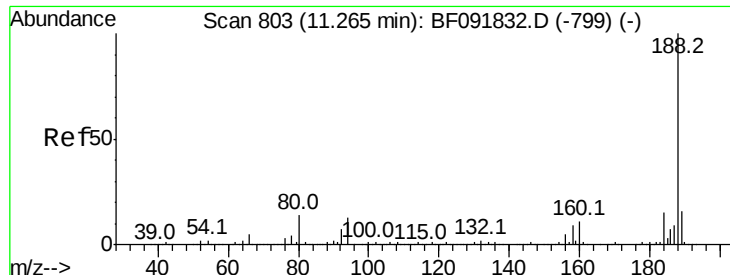

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.11 min Scan# 807
 Delta R.T. -0.05 min
 Lab File: BF092225.D
 Acq: 12 Jan 2017 23:31




Instrument :
 BNA_F
 ClientSampleId :
 COMP-0020


Tot Ion	Ratio	Lower	Upper
188	100		
94	6.4	10.0	15.0#
80	6.6	11.2	16.8#

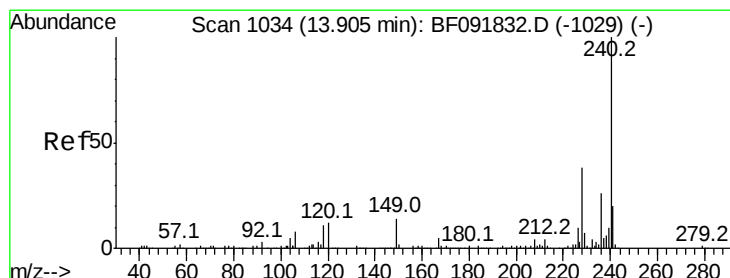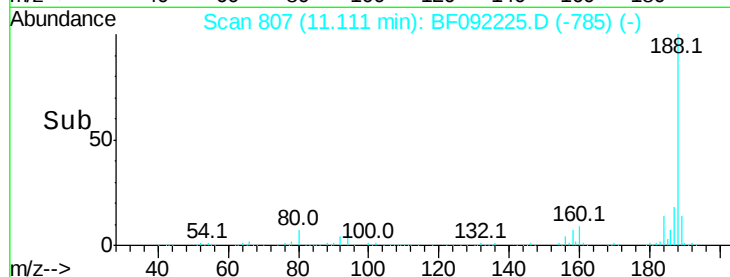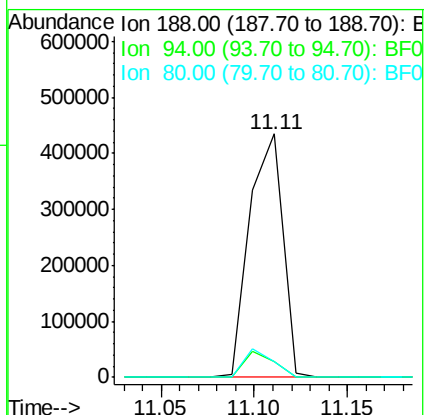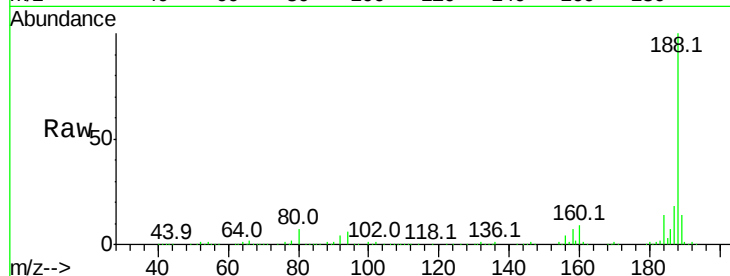

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.73 min Scan# 1036
 Delta R.T. -0.06 min
 Lab File: BF092225.D
 Acq: 12 Jan 2017 23:31

Tgt Ion	Ratio	Lower	Upper
240	100		
120	15.5	12.9	19.3
236	25.5	20.9	31.3

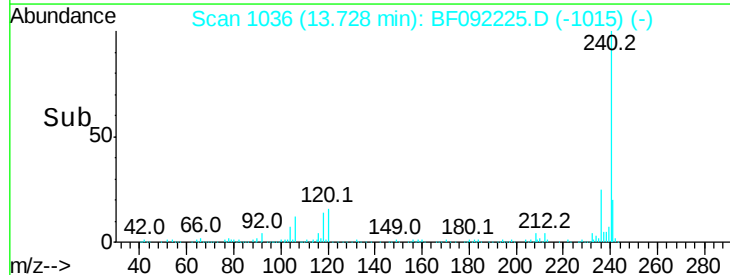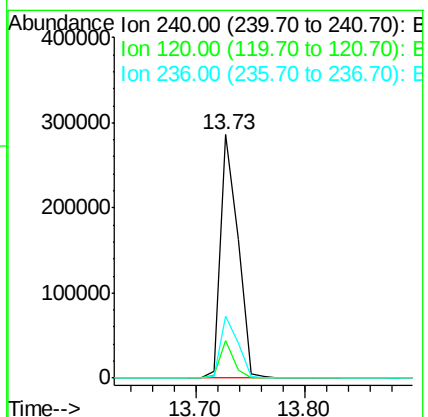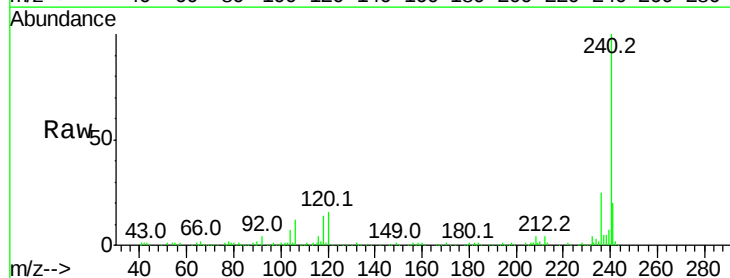

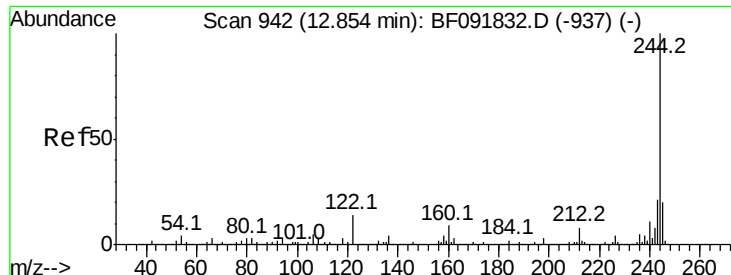

#78

Terphenyl-d14

Concen: 67.43 ng

RT: 12.69 min Scan# 945

Delta R.T. -0.06 min

Lab File: BF092225.D

Acq: 12 Jan 2017 23:31

Instrument :

BNA_F

ClientSampleId :

COMP-0020


Tot Ion:244 Resp: 887748

Ion Ratio Lower Upper

244 100

212 7.5 6.2 9.2




122 14.9 11.4 17.2

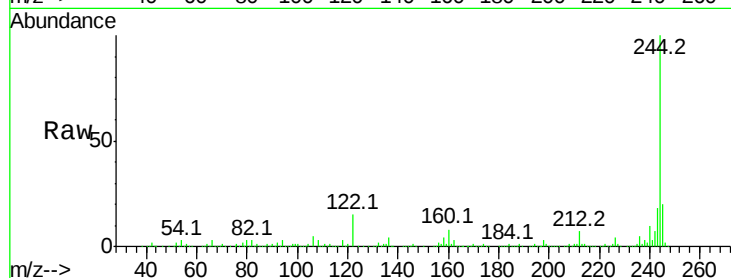

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

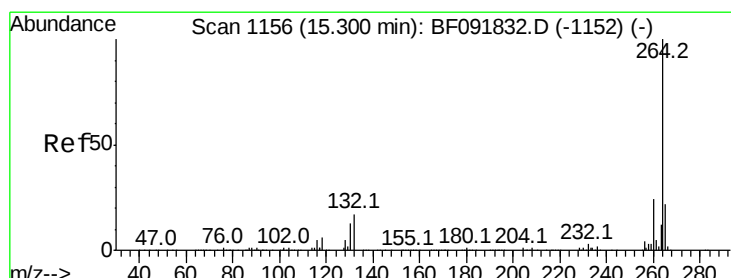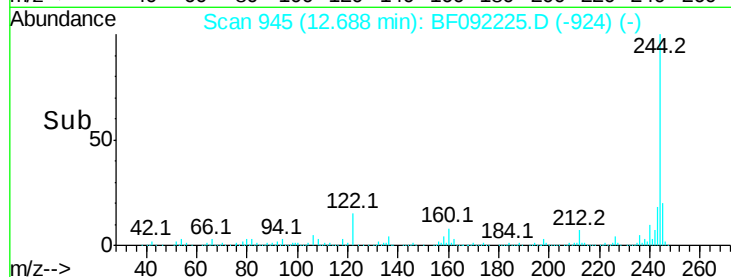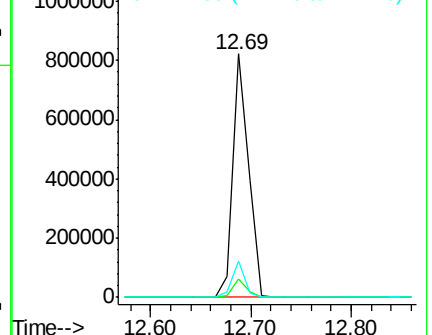

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.09 min Scan# 1155

Delta R.T. -0.06 min

Lab File: BF092225.D

Acq: 12 Jan 2017 23:31


Tgt Ion:264 Resp: 312731

Ion Ratio Lower Upper

264 100

260 23.2 19.2 28.8

265 22.2 17.4 26.0

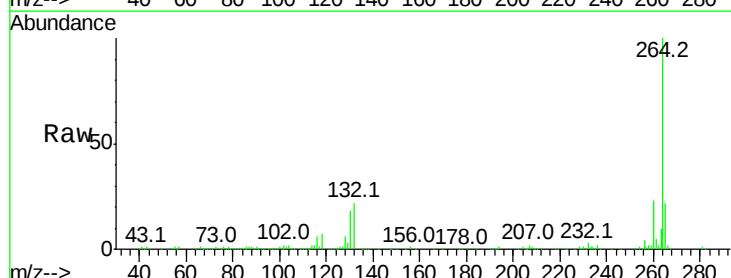

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

