


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
 Data File : BF092204.D
 Acq On : 12 Jan 2017 12:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

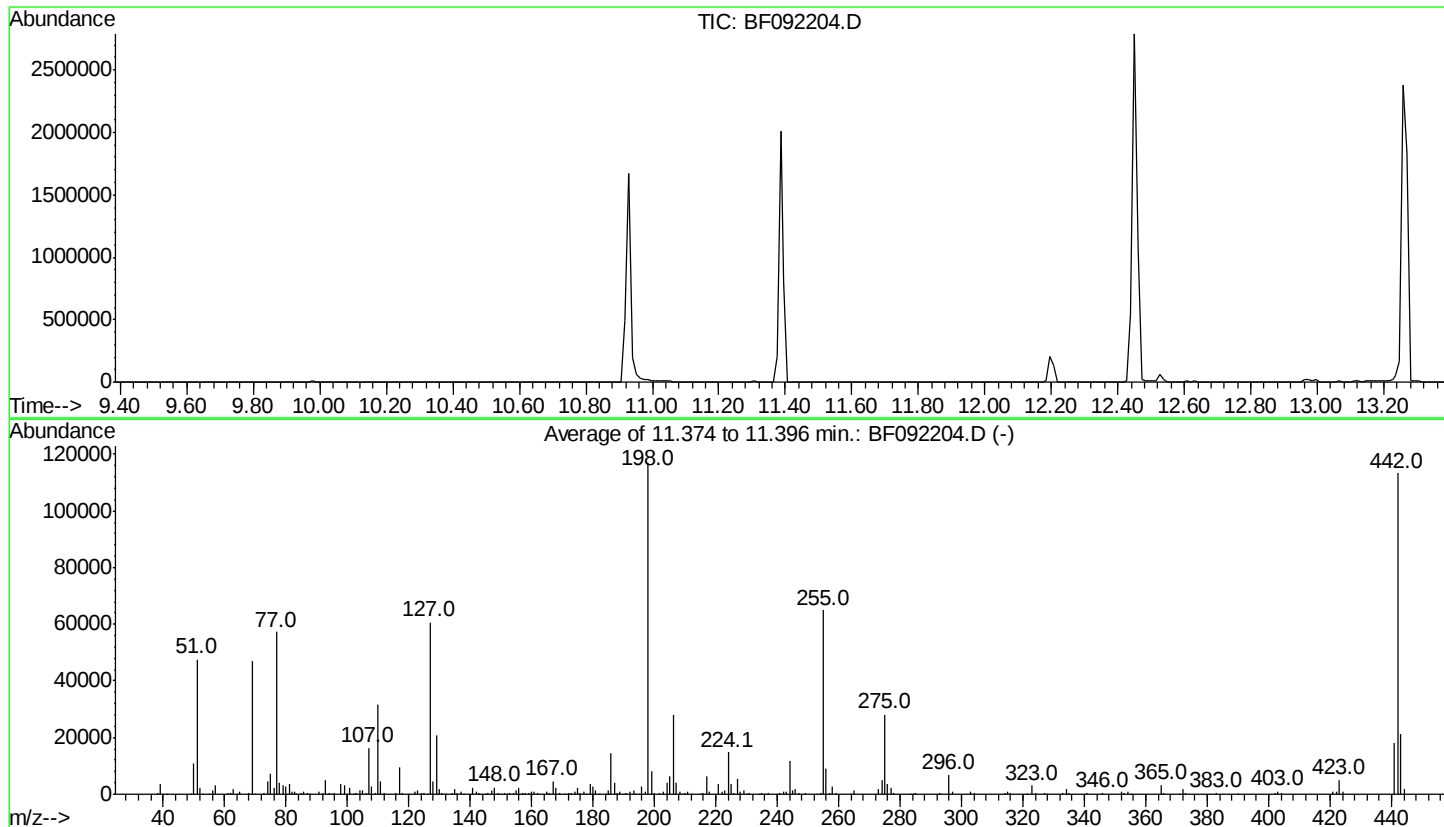

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	47469	PASS
68	69	0.00	2	1.1	506	PASS
69	198	0.00	100	40.1	46987	PASS
70	69	0.00	2	0.4	194	PASS
127	198	10	80	51.9	60749	PASS
197	198	0.00	2	0.7	801	PASS
198	198	100	100	100.0	117034	PASS
199	198	5	9	6.9	8130	PASS
275	198	10	60	24.1	28237	PASS
365	198	1	100	2.9	3365	PASS
441	442	0.01	24	15.9	17964	PASS
442	198	50	100	96.8	113309	PASS
443	442	15	24	18.9	21468	PASS