


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011217\
 Data File : BF092227.D
 Acq On : 13 Jan 2017 1:26
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

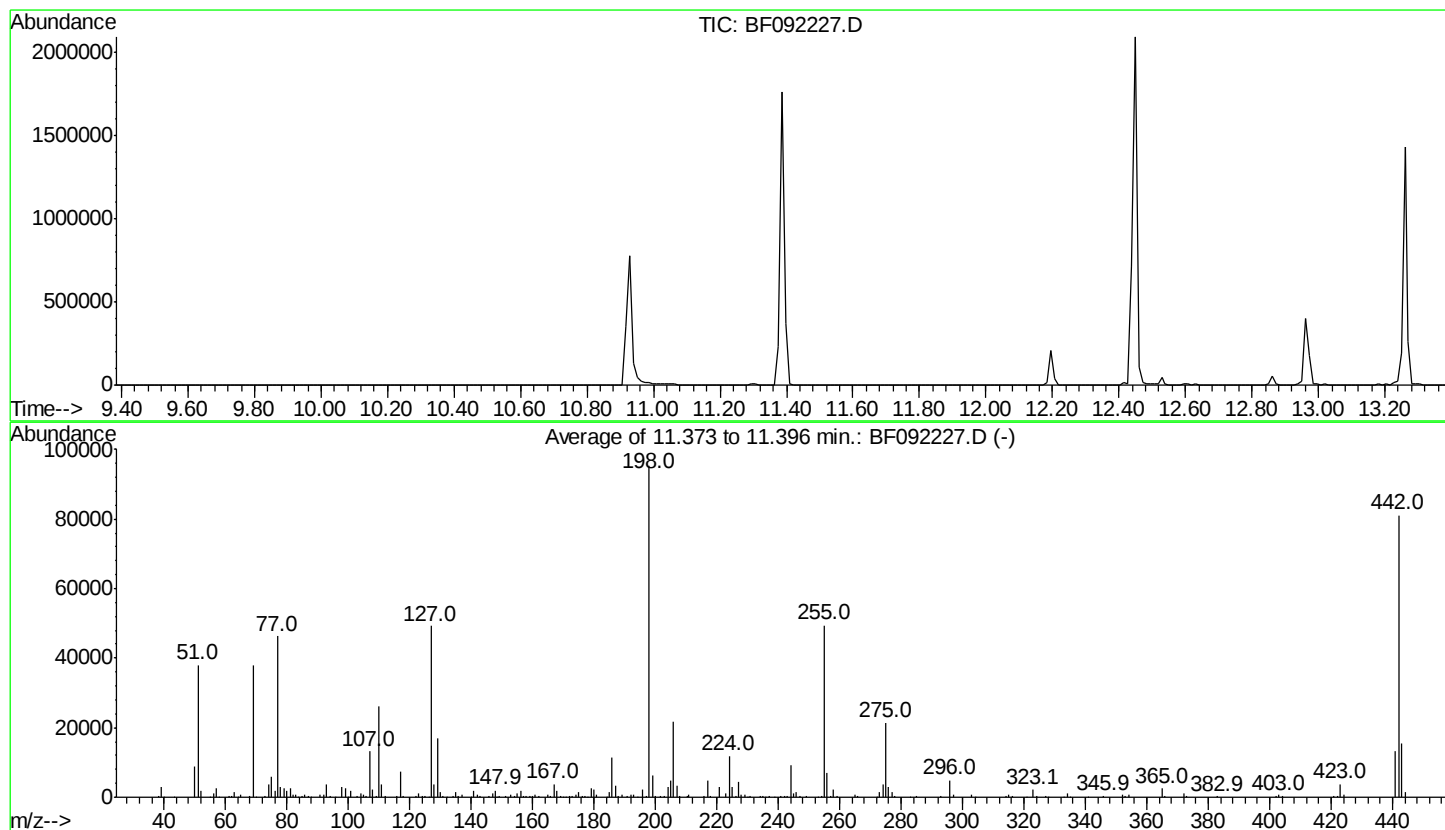

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	38050	PASS
68	69	0.00	2	1.4	546	PASS
69	198	0.00	100	39.8	37933	PASS
70	69	0.00	2	0.5	190	PASS
127	198	10	80	51.7	49312	PASS
197	198	0.00	2	0.4	423	PASS
198	198	100	100	100.0	95346	PASS
199	198	5	9	6.7	6383	PASS
275	198	10	60	22.4	21369	PASS
365	198	1	100	2.6	2499	PASS
441	442	0.01	24	16.3	13266	PASS
442	198	50	100	85.1	81171	PASS
443	442	15	24	19.1	15500	PASS