
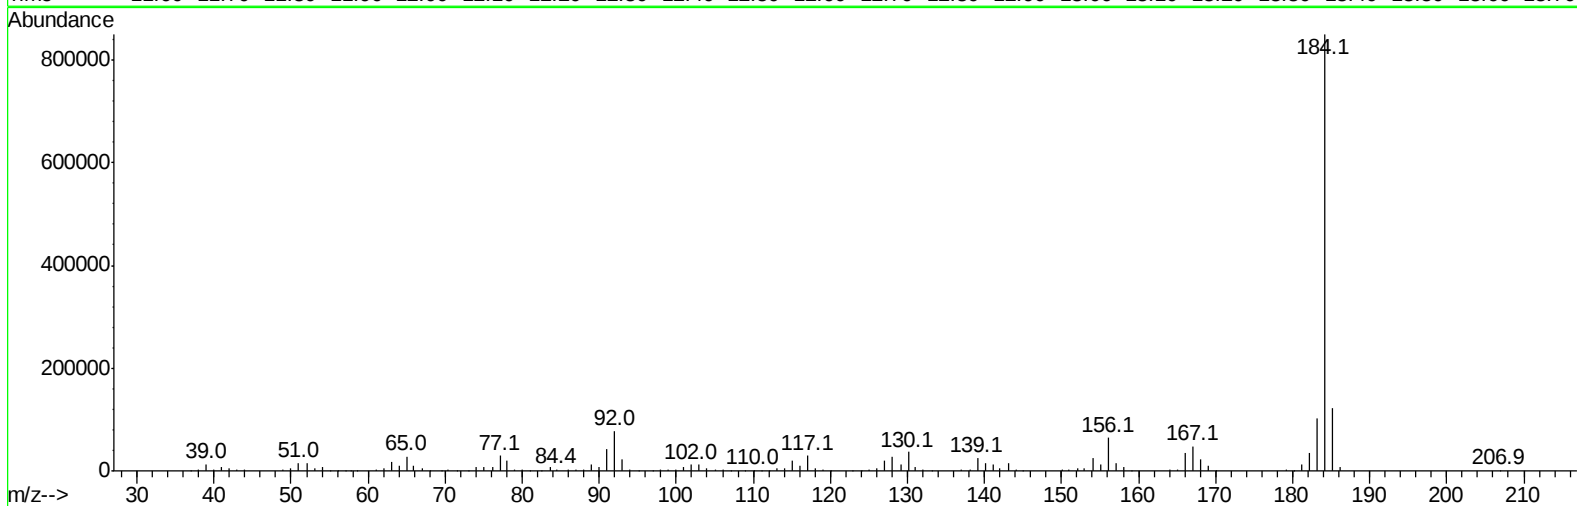


Data Path : U:\HPCHEM1\BNA F\DATA\BF011218\
Data File : BF102041.D
Acq On : 12 Jan 2018 14:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 02:13:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

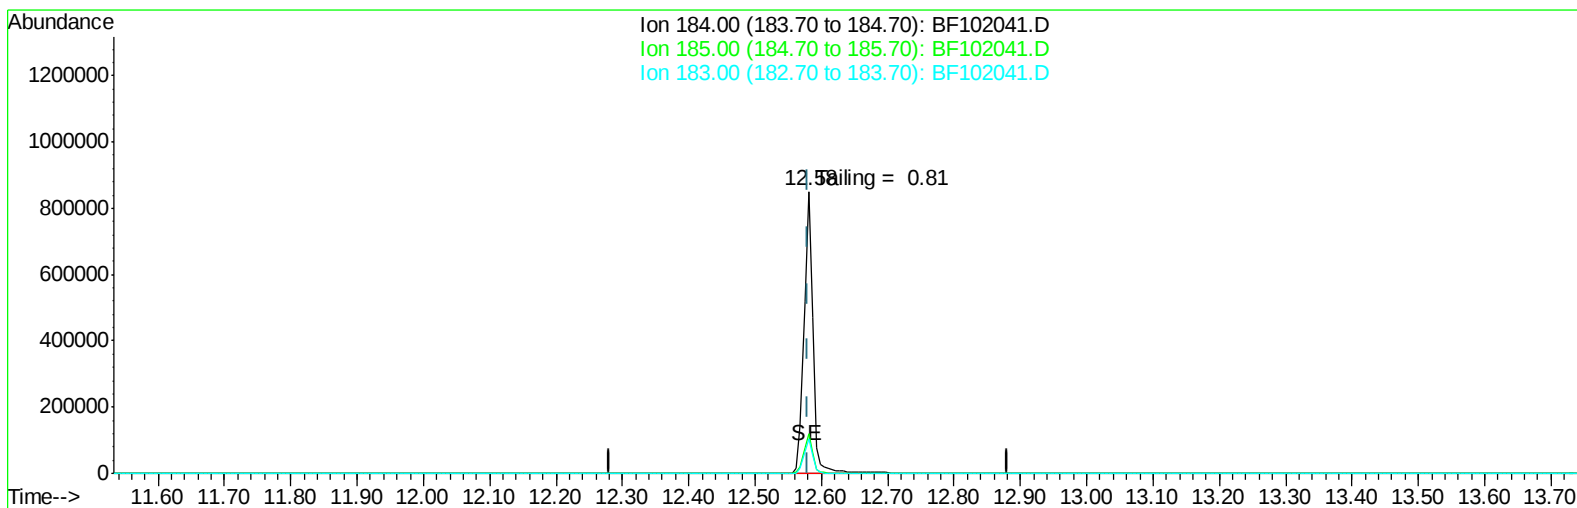

TIC: BF102041.D

(76) Benzidine



12.580min (-0.000) 0.00ng

response 784219

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.27
183.00	11.60	12.08
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011218\
Data File : BF102041.D
Acq On : 12 Jan 2018 14:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 02:13:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

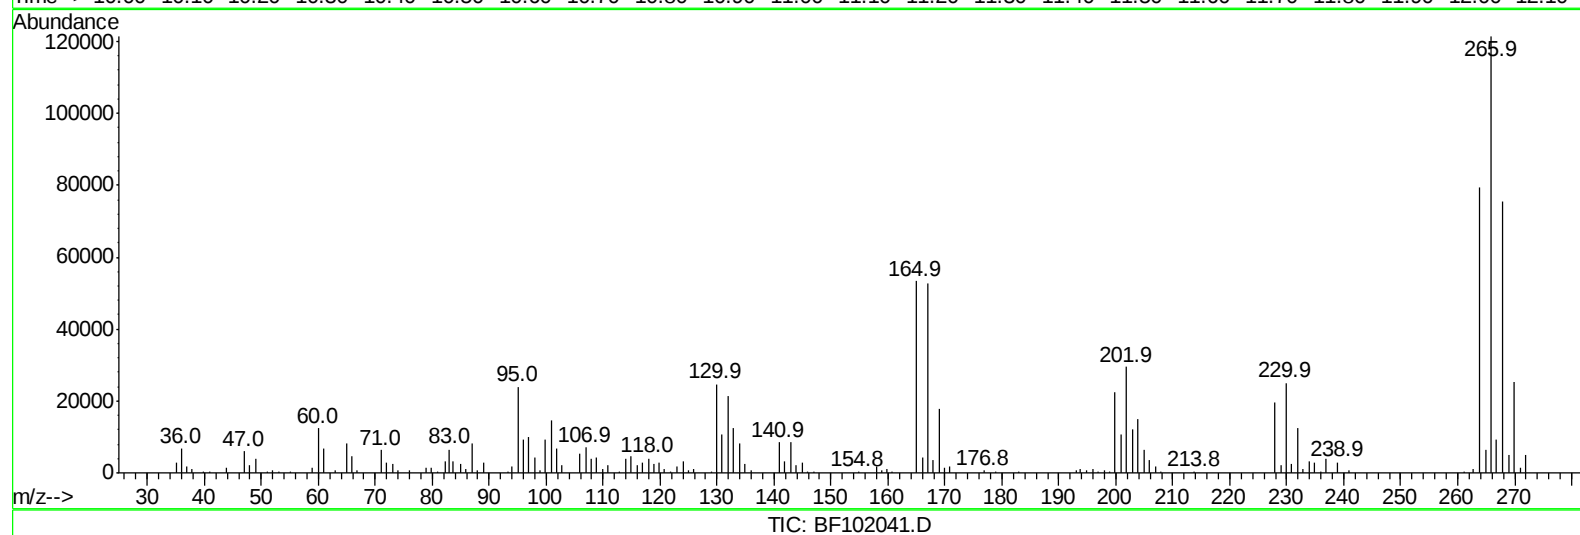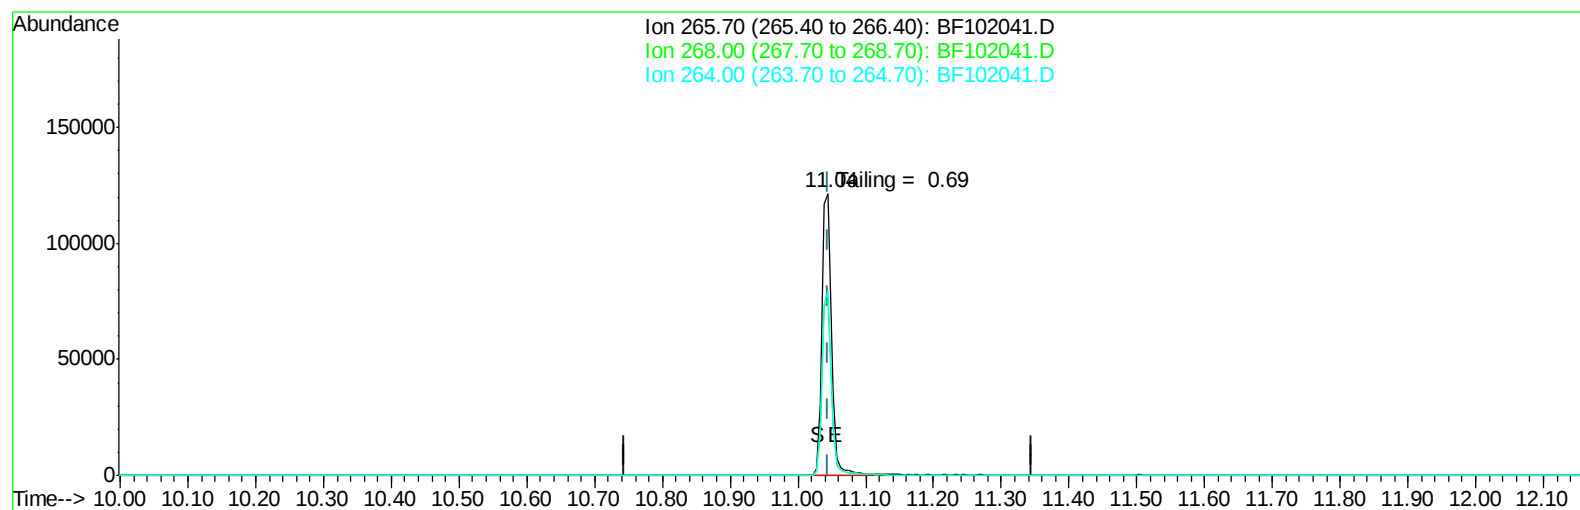

(69) Pentachlorophenol (C)

11.045min (-0.000) 34530.21ng

response 117006

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.24
264.00	61.90	65.45
0.00	0.00	0.00