


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_F\Data\BF011218\
 Data File : BF102041.D
 Acq On : 12 Jan 2018 14:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

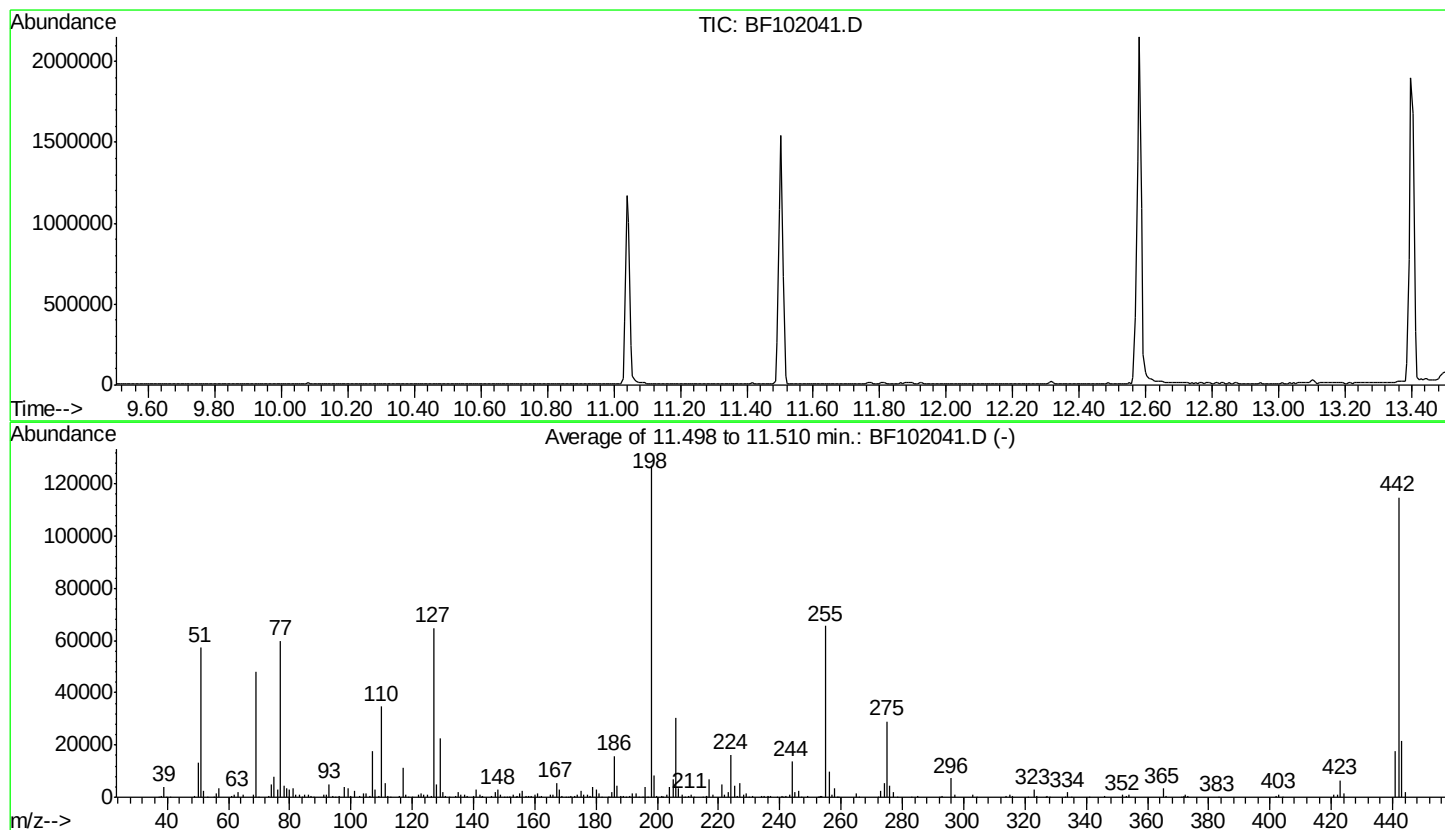

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	57307	PASS
68	69	0.00	2	1.6	766	PASS
69	198	0.00	100	38.0	48290	PASS
70	69	0.00	2	0.5	230	PASS
127	198	10	80	51.1	64866	PASS
197	198	0.00	2	0.2	217	PASS
198	198	100	100	100.0	127013	PASS
199	198	5	9	6.6	8397	PASS
275	198	10	60	22.9	29117	PASS
365	198	1	100	2.7	3424	PASS
441	443	0.01	100	82.3	17811	PASS
442	198	50	100	90.4	114770	PASS
443	442	15	24	18.8	21631	PASS