
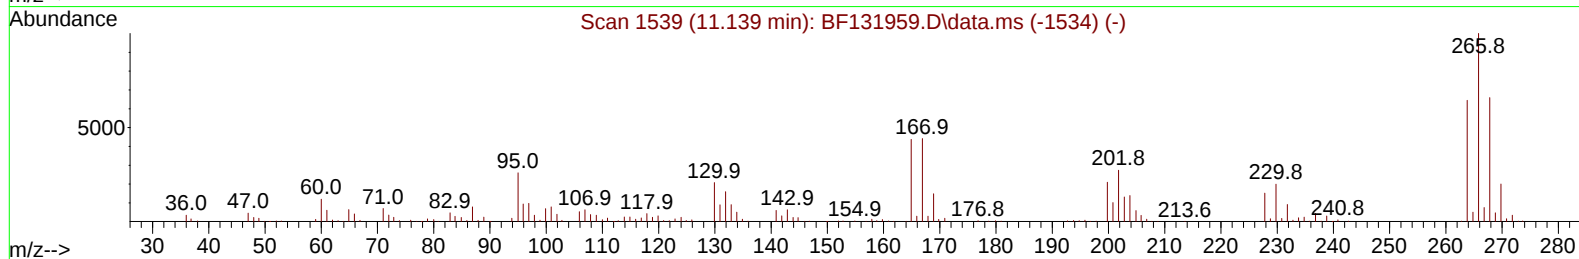
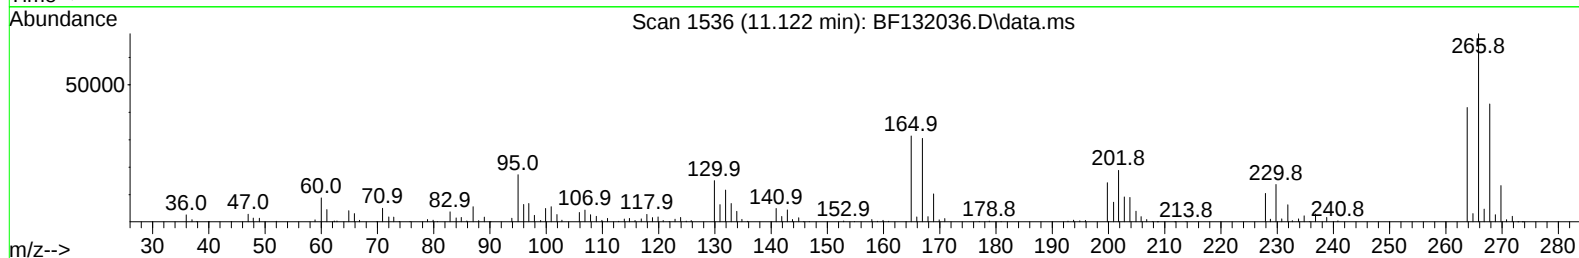


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011223\
Data File : BF132036.D
Acq On : 12 Jan 2023 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 03:39:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 23:59:08 2023
Response via : Initial Calibration

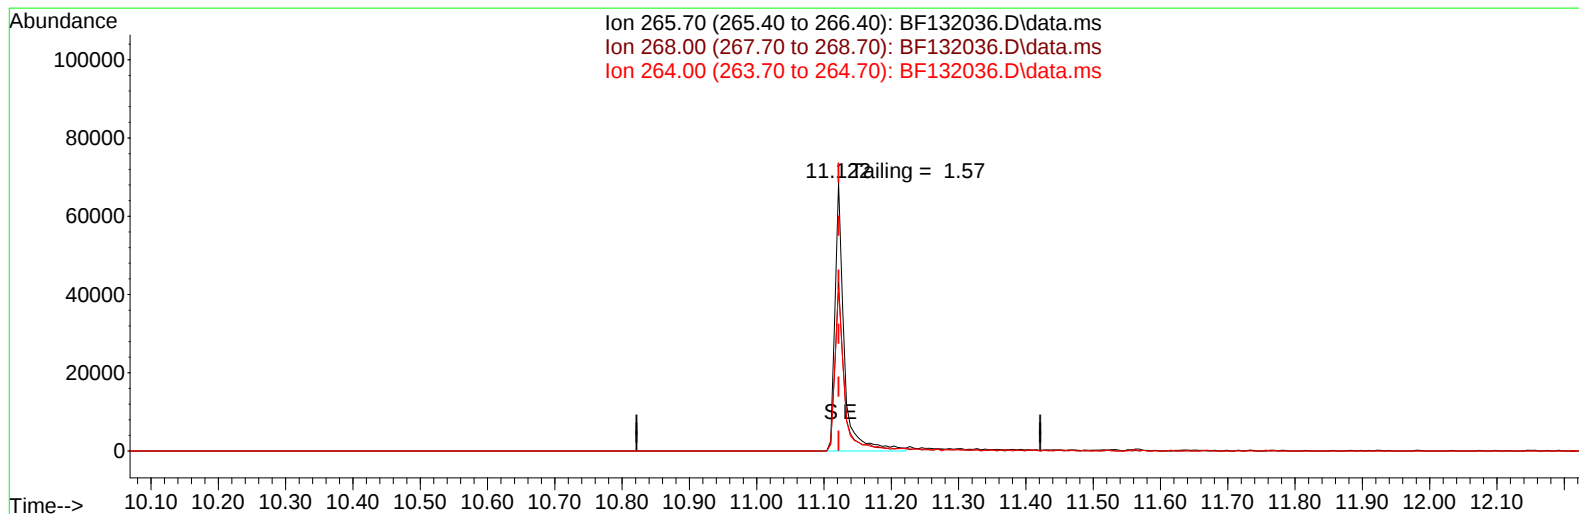

TIC: BF132036.D\data.ms

(70) Pentachlorophenol (C)




11.122min (+ 0.000) 19045.98 ng

response 65098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.74
264.00	64.50	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011223\
 Data File : BF132036.D
 Acq On : 12 Jan 2023 10:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 03:39:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 23:59:08 2023
 Response via : Initial Calibration

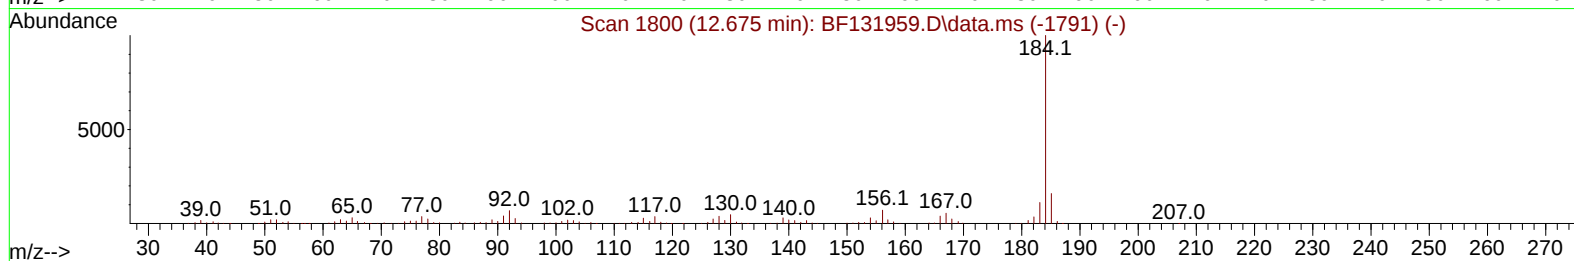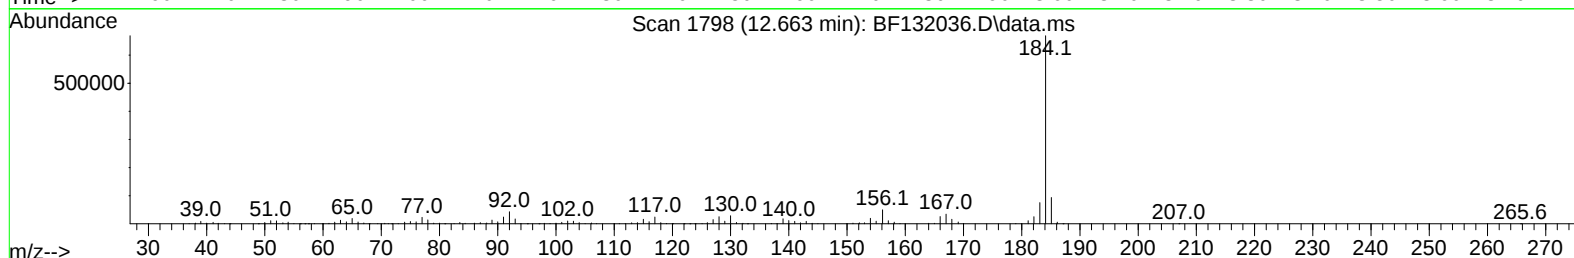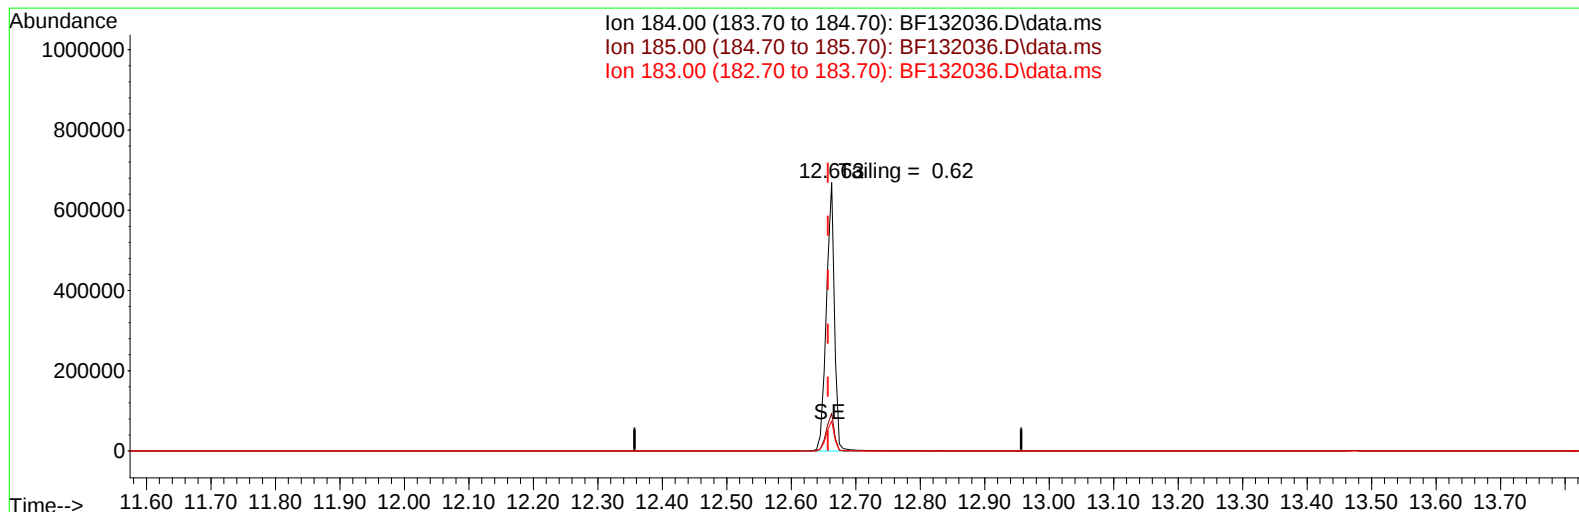

TIC: BF132036.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 0.00 ng

response 583787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.02
183.00	11.20	11.23
0.00	0.00	0.00