
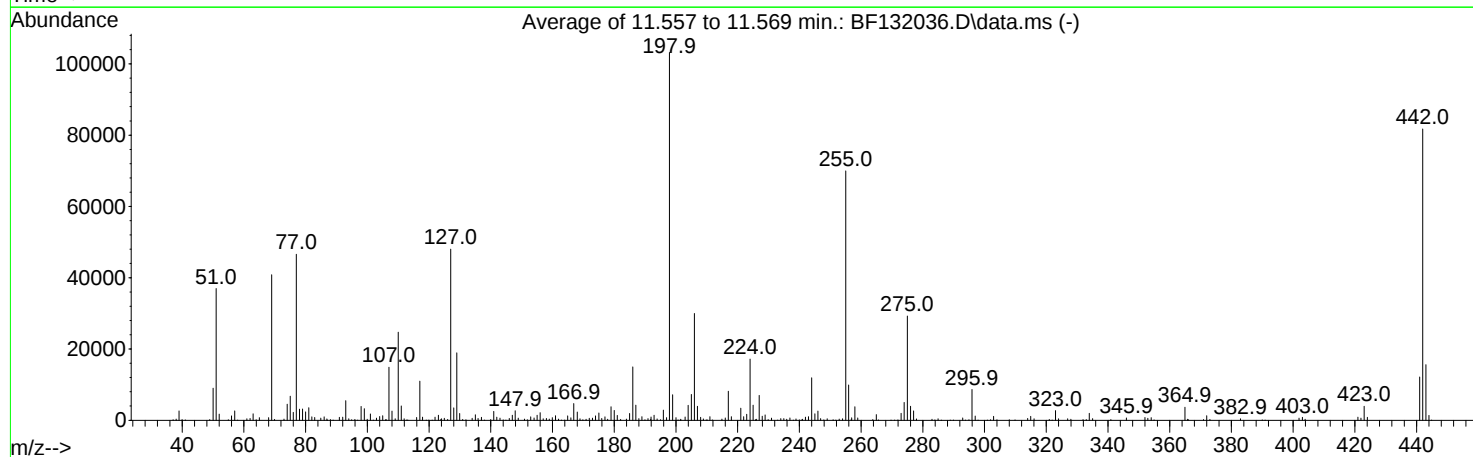


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011223\
Data File : BF132036.D
Acq On : 12 Jan 2023 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 12 23:59:08 2023

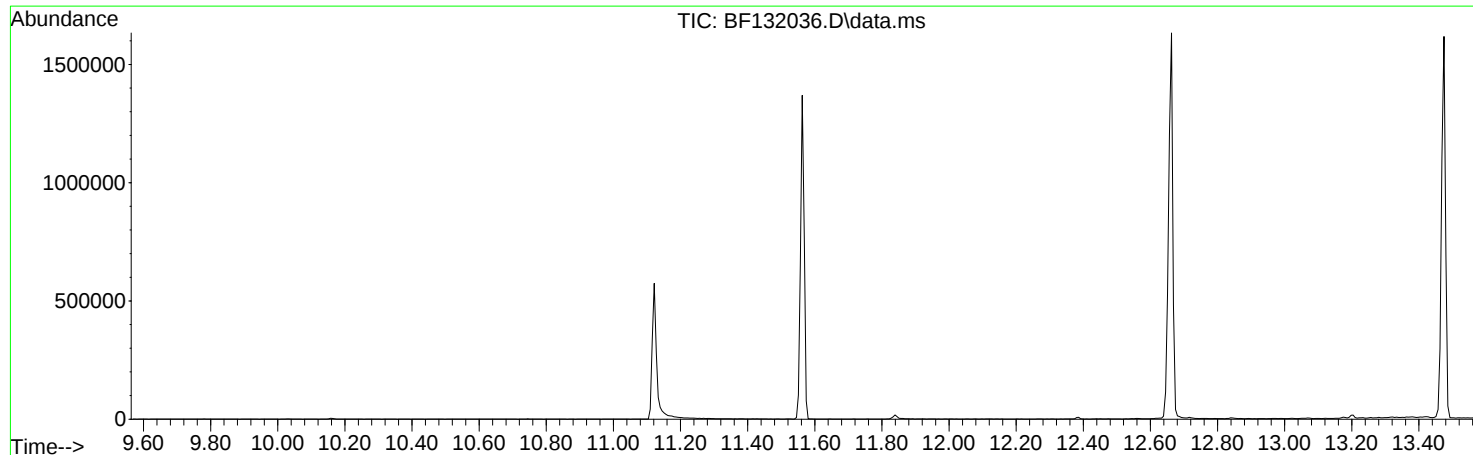




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	36952	PASS
68	69	0.00	2	1.8	738	PASS
69	198	0.00	100	39.6	40843	PASS
70	69	0.00	2	0.6	241	PASS
127	198	10	80	46.5	48035	PASS
197	198	0.00	2	0.7	727	PASS
198	198	100	100	100.0	103219	PASS
199	198	5	9	7.0	7180	PASS
275	198	10	60	28.4	29267	PASS
365	198	1	100	3.6	3670	PASS
441	198	0.01	100	11.8	12134	PASS
442	442	50	100	100.0	81736	PASS
443	442	15	24	19.1	15609	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011223\
Data File : BF132036.D
Acq On : 12 Jan 2023 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 13 03:39:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 23:59:08 2023
Response via : Initial Calibration

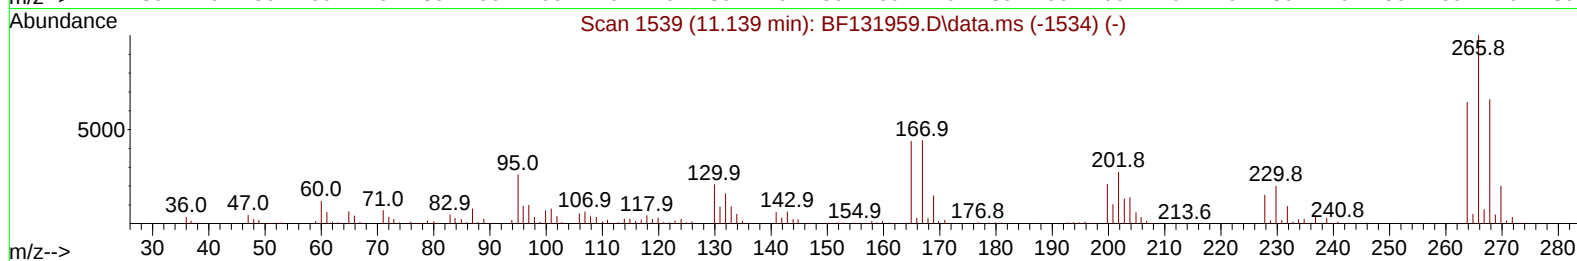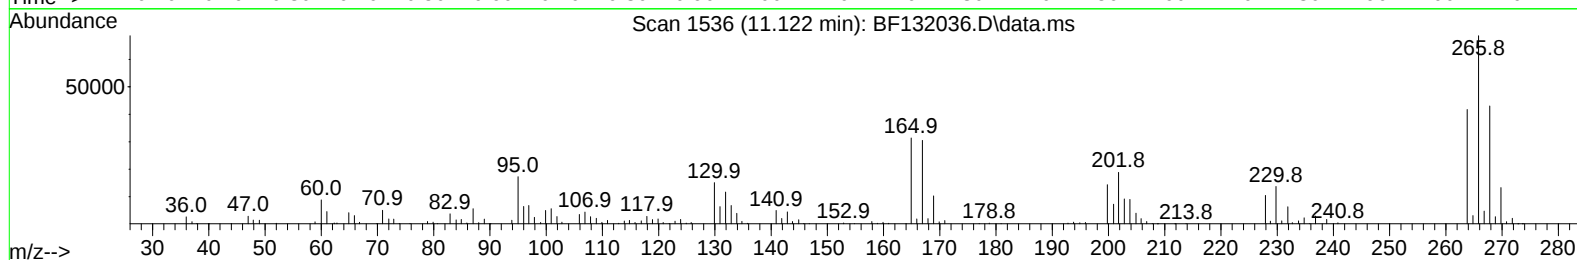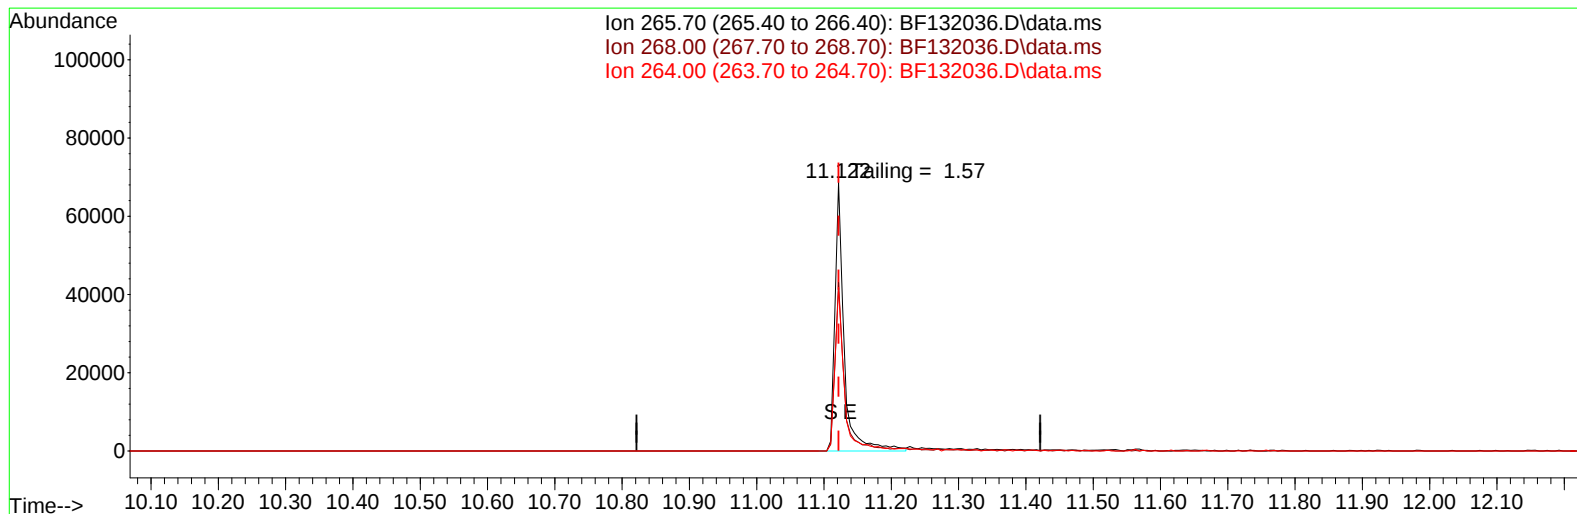

TIC: BF132036.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 19045.98 ng




response 65098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.74
264.00	64.50	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011223\
 Data File : BF132036.D
 Acq On : 12 Jan 2023 10:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 03:39:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 23:59:08 2023
 Response via : Initial Calibration

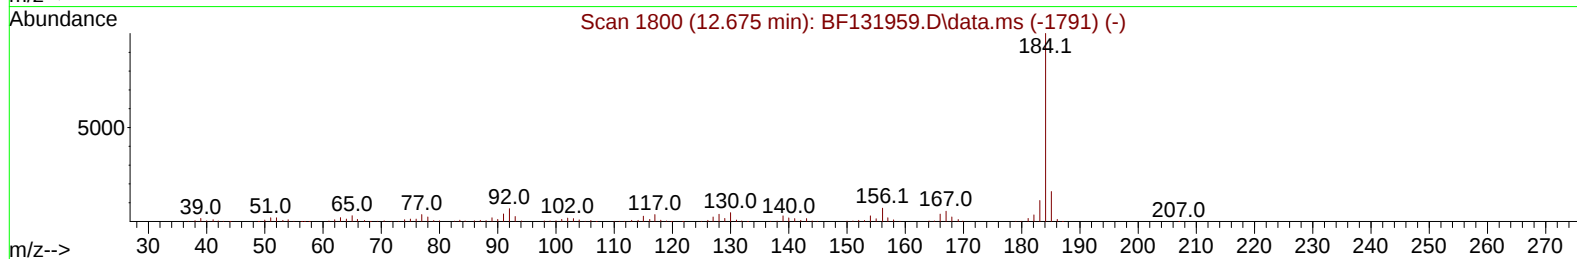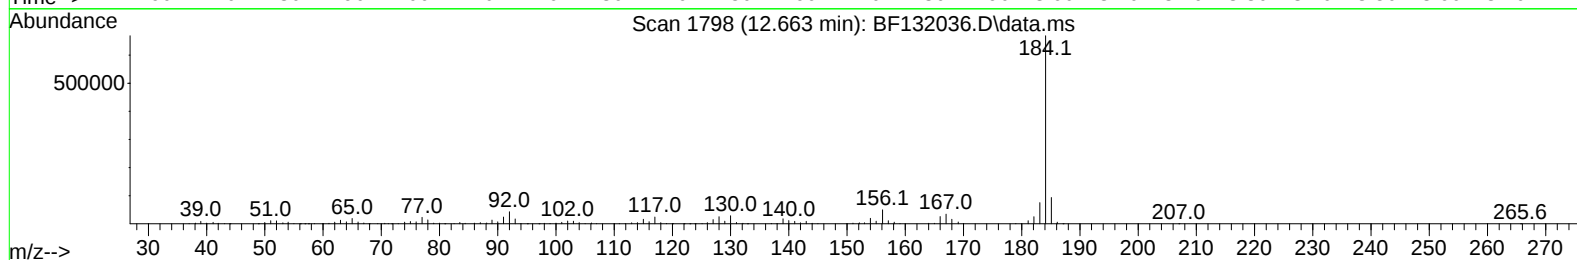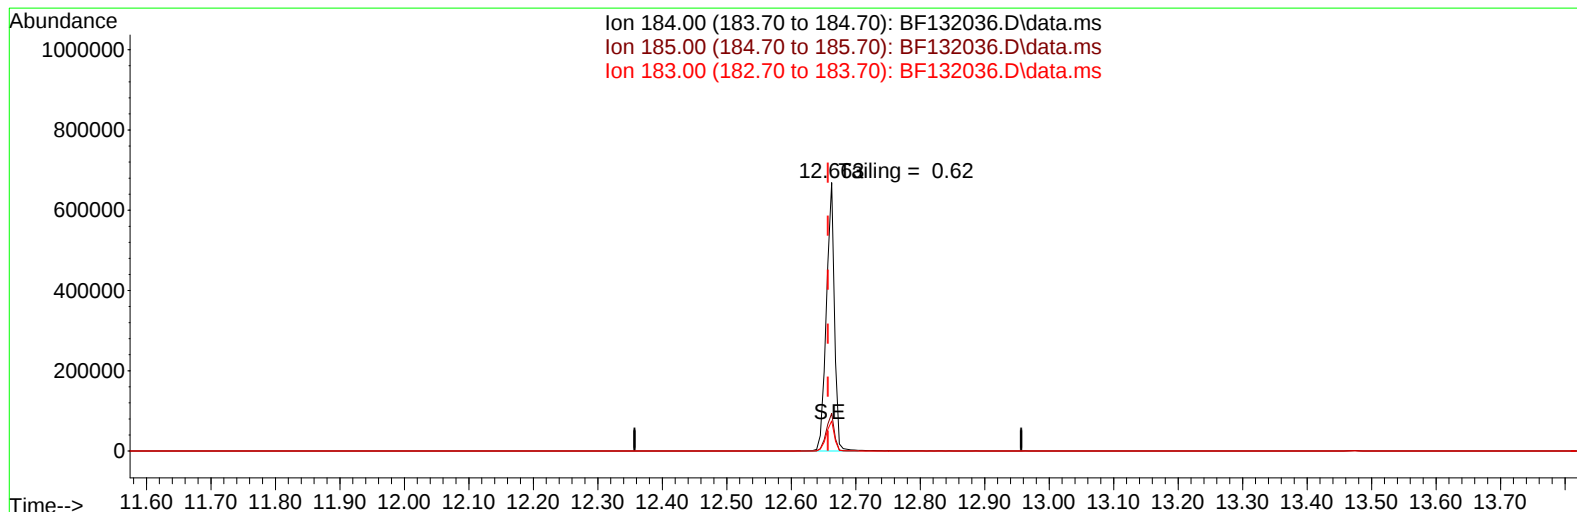

TIC: BF132036.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 0.00 ng

response 583787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.02
183.00	11.20	11.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2023	BNA_F	<u>BF132036.D</u>
Compound Name	Response	Retention Time
DDT	258453	13.474
DDD	4131	13.204
DDE	917	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5048	263501	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP