

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011224\
 Data File : BF137051.D
 Acq On : 12 Jan 2024 16:28
 Operator : CG\JU
 Sample : P1117-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S1-COMPOSITE

Quant Time: Jan 12 16:45:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	59770	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	227058	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	112132	20.000	ng	-0.01
64) Phenanthrene-d10	11.310	188	193400	20.000	ng	0.00
76) Chrysene-d12	13.969	240	115562	20.000	ng	0.00
86) Perylene-d12	15.463	264	134395	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	306640	80.048	ng	0.00
7) Phenol-d6	6.434	99	382489	77.058	ng	0.00
23) Nitrobenzene-d5	7.345	82	239197	53.907	ng	-0.01
42) 2,4,6-Tribromophenol	10.616	330	102228	77.410	ng	0.00
45) 2-Fluorobiphenyl	9.139	172	461088	55.306	ng	-0.01
79) Terphenyl-d14	12.904	244	356199	43.074	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.345	70	31369	10.425	ng	# 74
25) Isophorone	7.345	82	239193	29.625	ng	# 65
50) Dimethylphthalate	9.816	163	21465	2.621	ng	# 1
51) 2,6-Dinitrotoluene	9.816	165	14993	8.066	ng	# 31
57) 2,4-Dinitrotoluene	9.816	165	14993	6.213	ng	# 22
67) 4-Bromophenyl-phenylether	10.610	248	6169	2.872	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011224\
Data File : BF137051.D
Acq On : 12 Jan 2024 16:28
Operator : CG\JU
Sample : P1117-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

Quant Time: Jan 12 16:45:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration



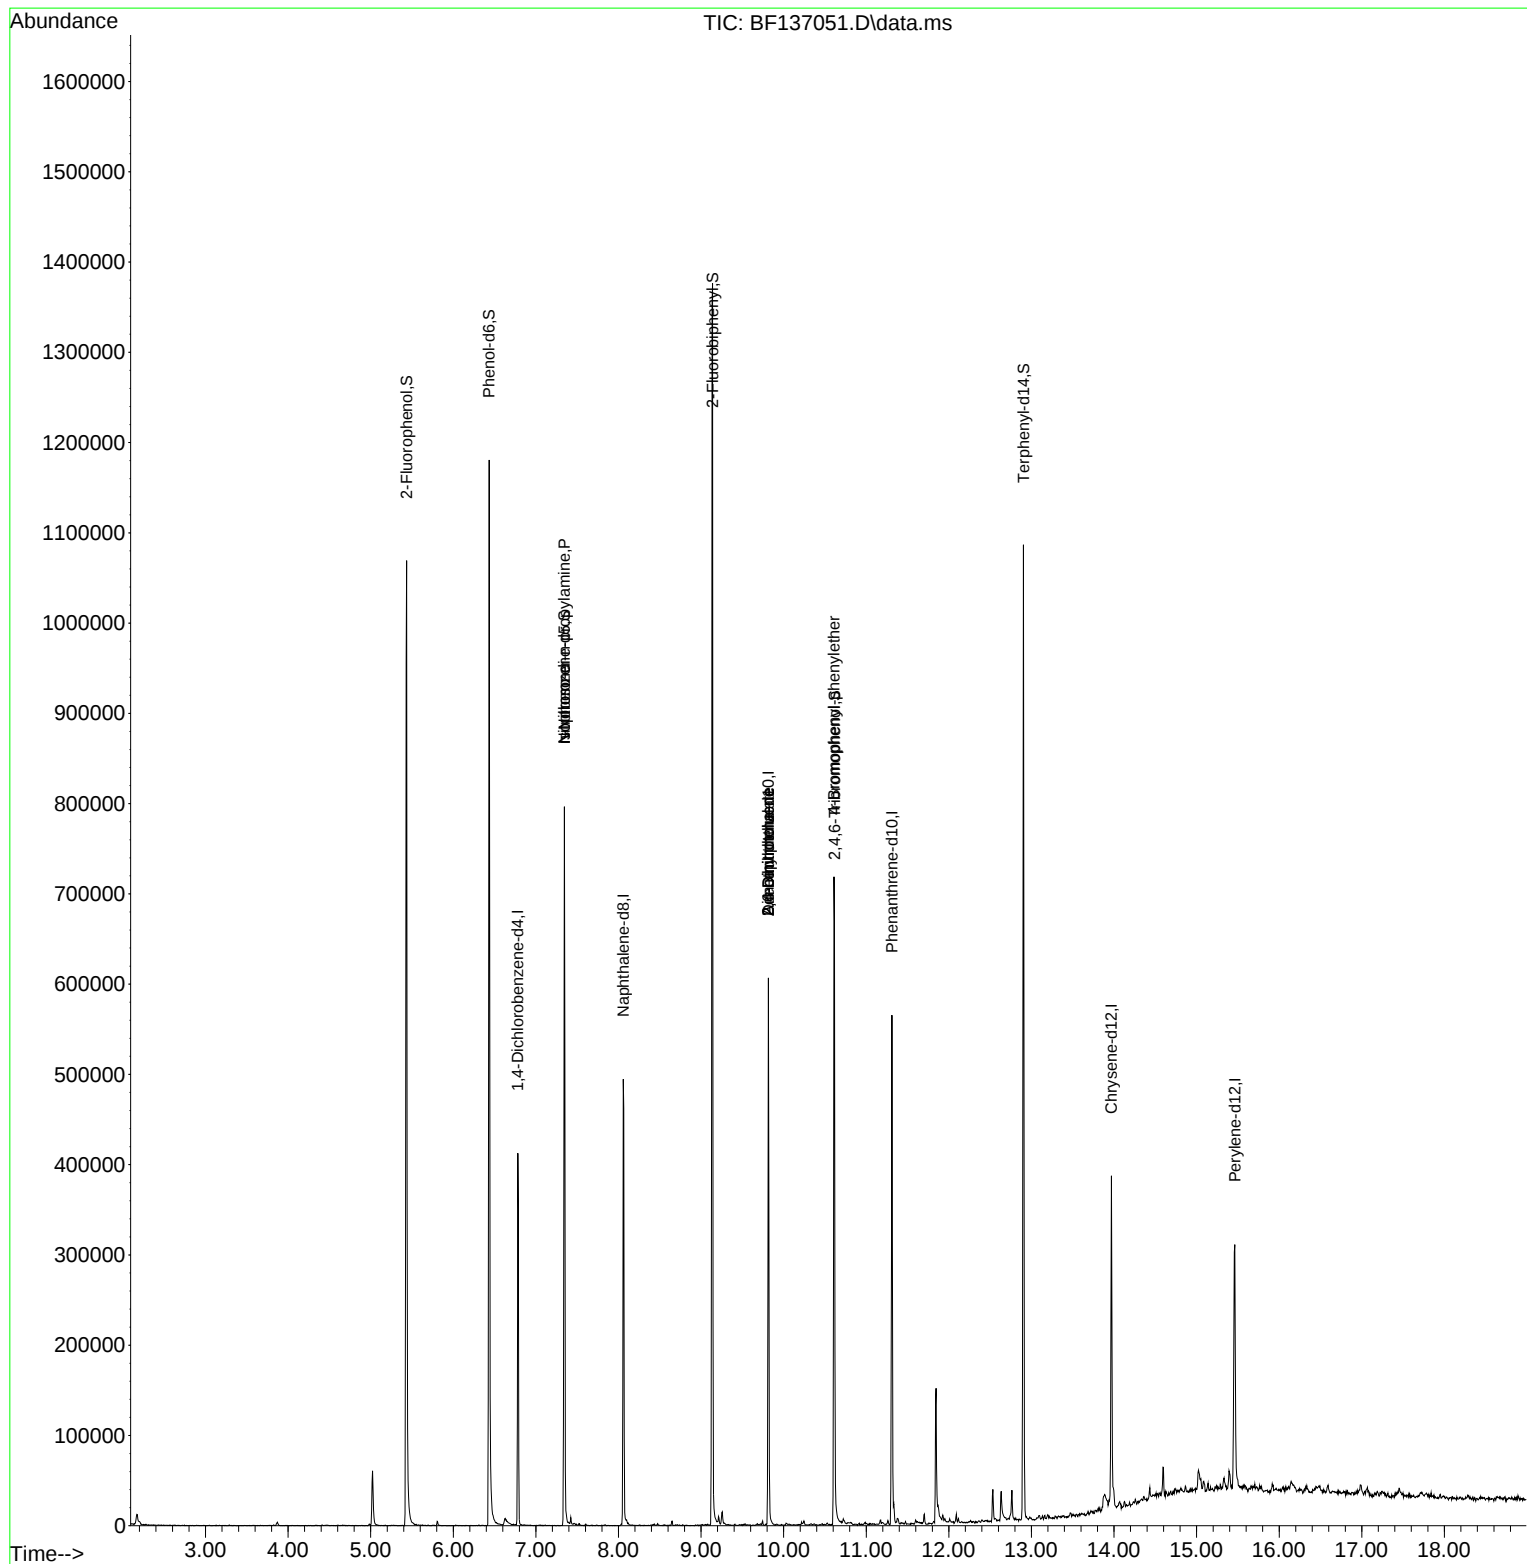




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE


Tgt Ion:152 Resp: 59770
Ion Ratio Lower Upper
152 100
150 159.7 127.0 190.6
115 62.8 49.0 73.4

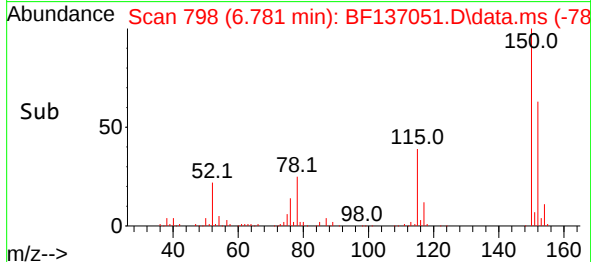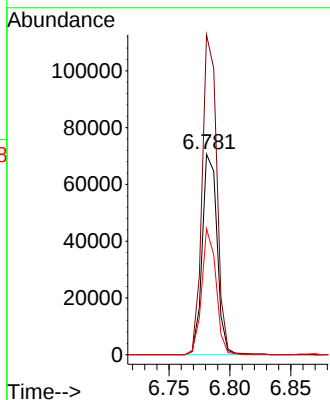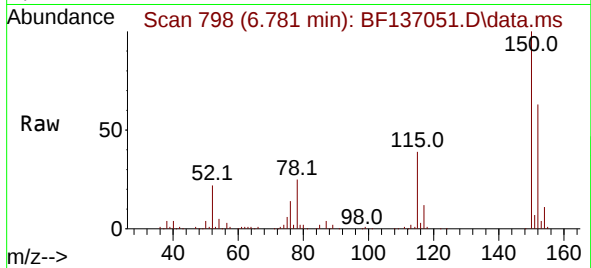

#5
2-Fluorophenol
Concen: 80.048 ng
RT: 5.434 min Scan# 569
Delta R.T. 0.006 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28


Tgt Ion:112 Resp: 306640
Ion Ratio Lower Upper
112 100
64 58.2 51.1 76.7
63 28.8 26.1 39.1

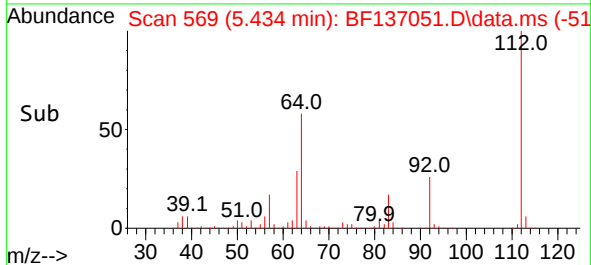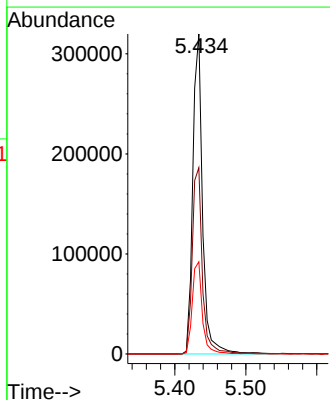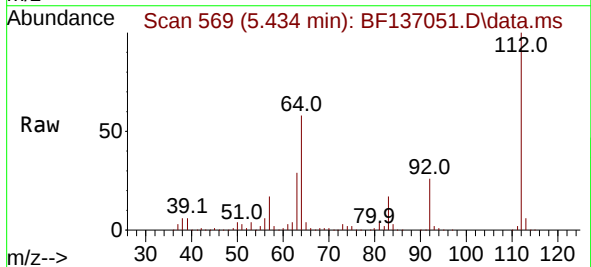


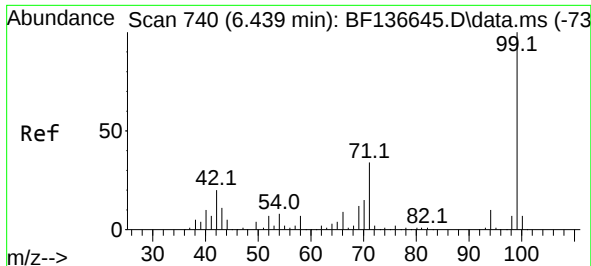


#7
Phenol-d6
Concen: 77.058 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28


Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

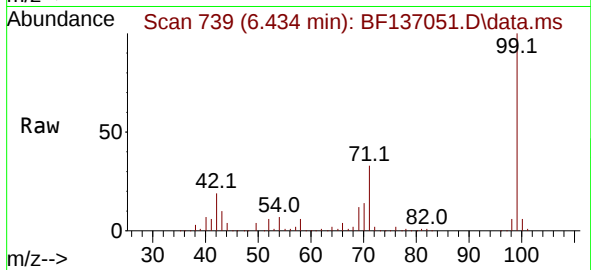



Tgt Ion: 99 Resp: 382489
Ion Ratio Lower Upper
99 100
42 19.0 16.1 24.1
71 33.0 27.4 41.2

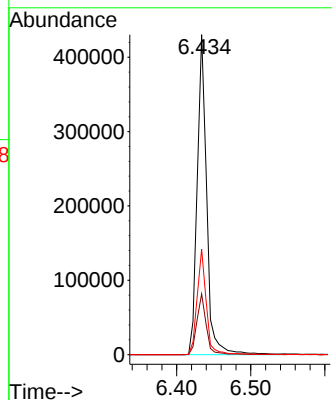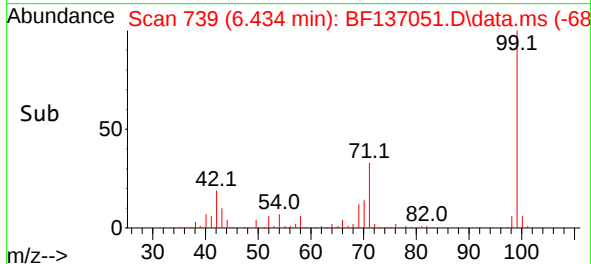


#19
n-Nitroso-di-n-propylamine
Concen: 10.425 ng
RT: 7.345 min Scan# 894
Delta R.T. 0.135 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28

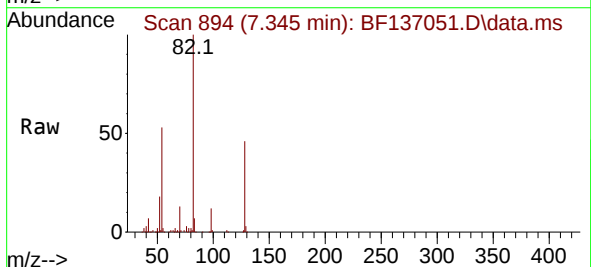

Tgt Ion: 70 Resp: 31369
Ion Ratio Lower Upper
70 100
42 49.7 54.2 81.4#
101 0.0 7.6 11.4#
130 3.0 17.1 25.7#


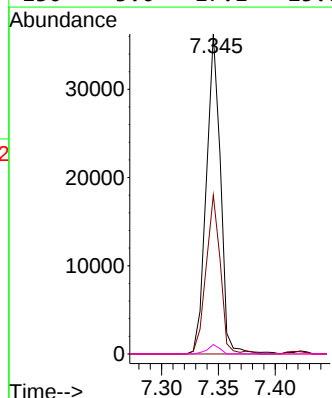
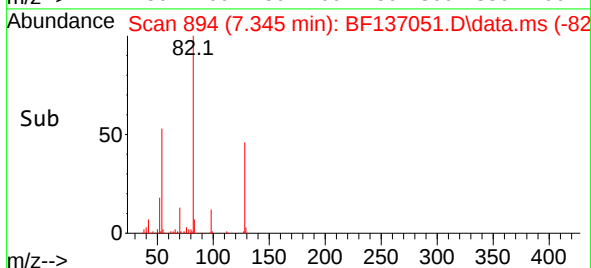


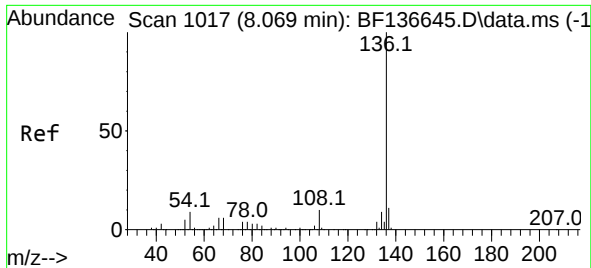

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

Tgt Ion:136 Resp: 227058
Ion Ratio Lower Upper
136 100
137 10.8 9.0 13.4
54 8.6 7.2 10.8
68 6.0 4.9 7.3

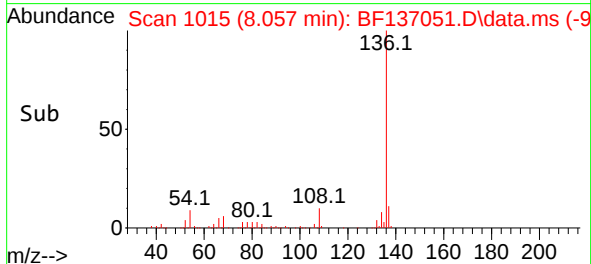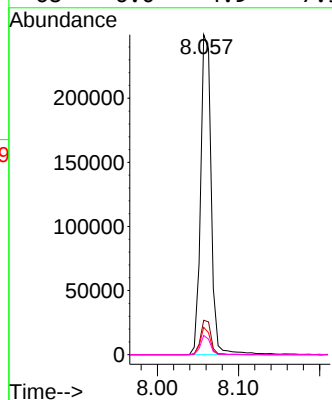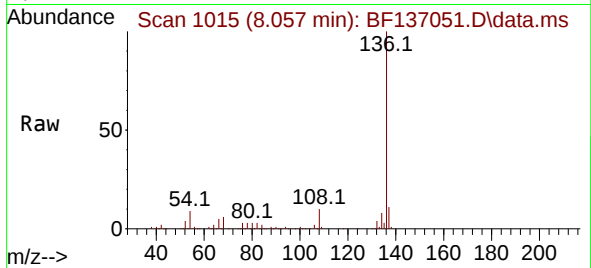

#23
Nitrobenzene-d5
Concen: 53.907 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.012 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28

Tgt Ion: 82 Resp: 239197
Ion Ratio Lower Upper
82 100
128 45.9 35.3 52.9
54 53.0 44.5 66.7


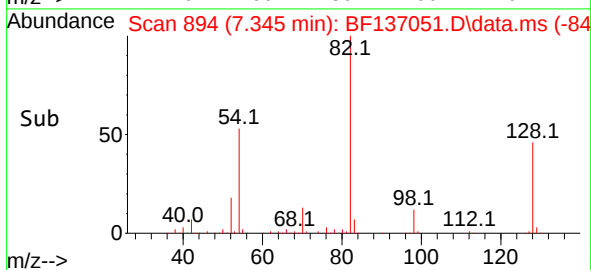
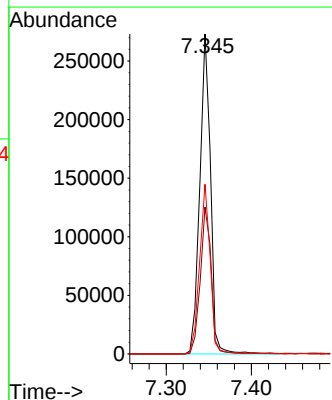
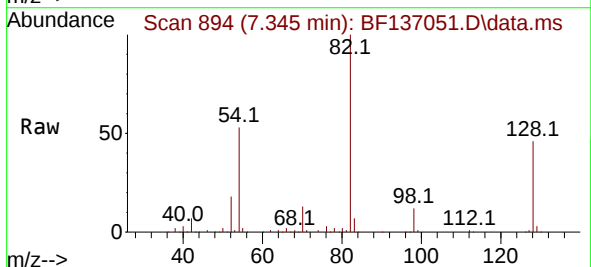




#25
Isophorone
Concen: 29.625 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.270 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

Tgt Ion: 82 Resp: 239193
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 14.5 21.7#

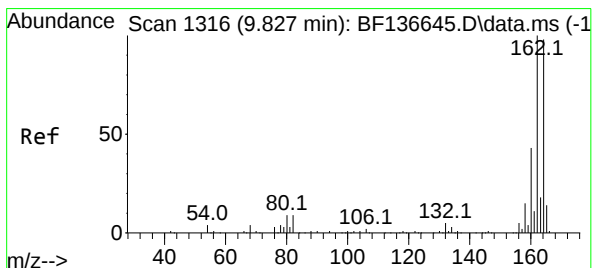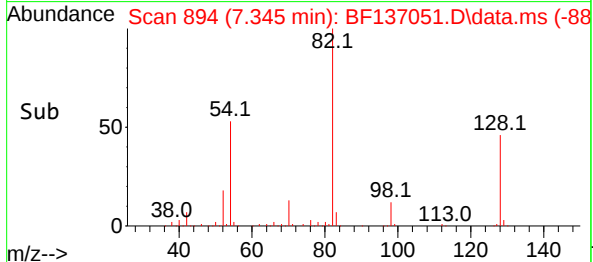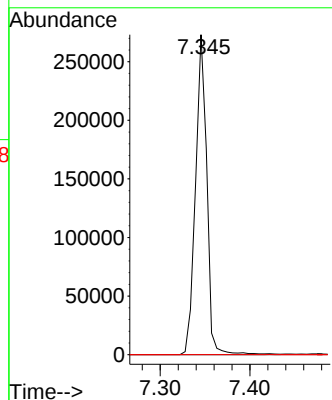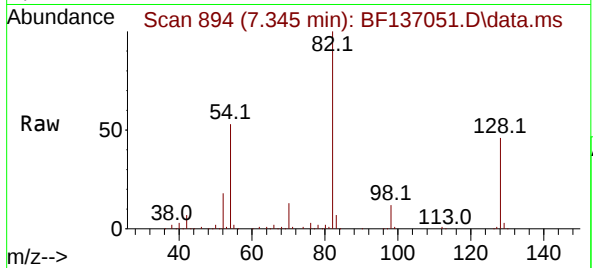

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.816 min Scan# 1314
Delta R.T. -0.012 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28

Tgt Ion:164 Resp: 112132
Ion Ratio Lower Upper
164 100
162 100.3 81.6 122.4
160 44.2 34.9 52.3

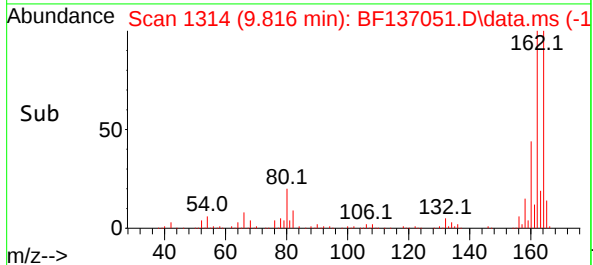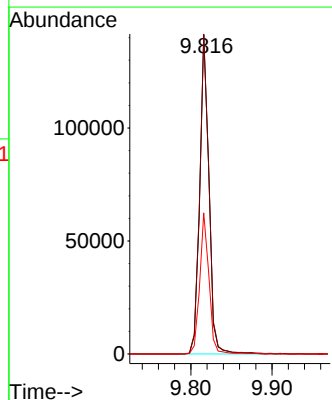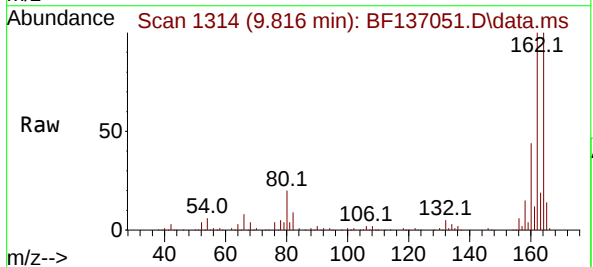



#42

2,4,6-Tribromophenol

Concen: 77.410 ng

RT: 10.616 min Scan# 1451

Delta R.T. -0.006 min

Lab File: BF137051.D


Acq: 12 Jan 2024 16:28

Instrument :

BNA_F

ClientSampleId :

S1-COMPOSITE

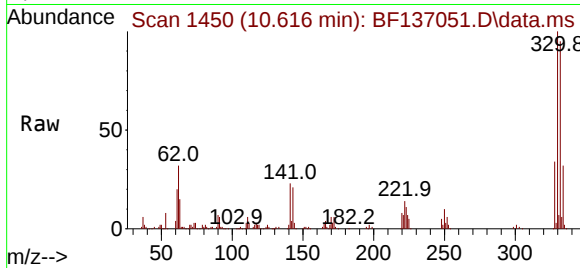



Tgt Ion:330 Resp: 102228

Ion Ratio Lower Upper

330 100

332 96.3 77.4 116.0

141 28.7 23.4 35.2

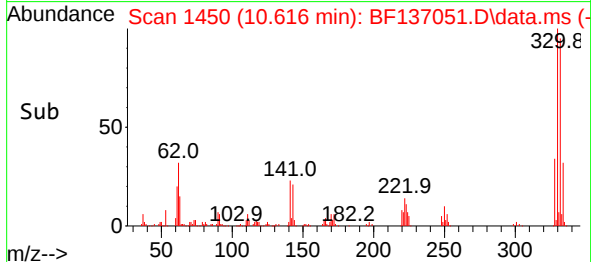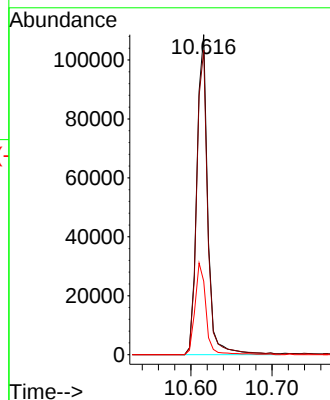

#45

2-Fluorobiphenyl

Concen: 55.306 ng

RT: 9.139 min Scan# 1199

Delta R.T. -0.012 min

Lab File: BF137051.D

Acq: 12 Jan 2024 16:28




Tgt Ion:172 Resp: 461088


Ion Ratio Lower Upper

172 100

171 35.7 29.0 43.6

170 23.4 19.0 28.4

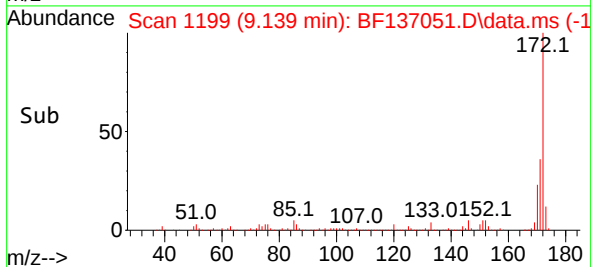
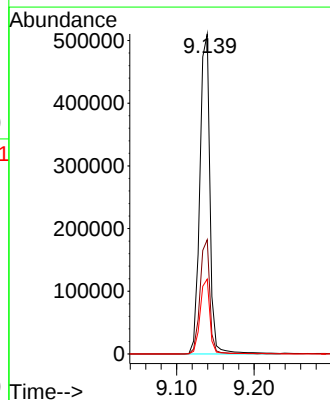
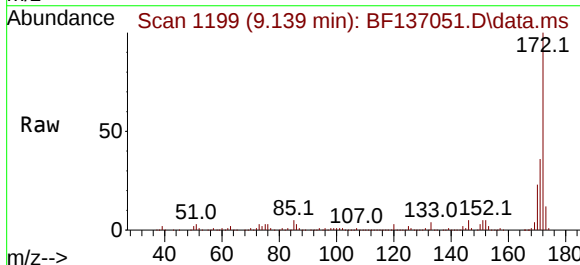


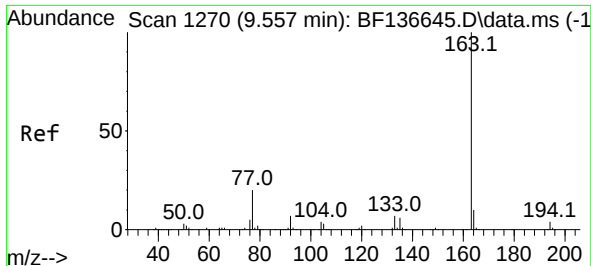

#50
Dimethylphthalate
Concen: 2.621 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.259 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

Tgt Ion:163 Resp: 21465
Ion Ratio Lower Upper
163 100
194 0.0 3.3 4.9#
164 527.4 7.8 11.6#

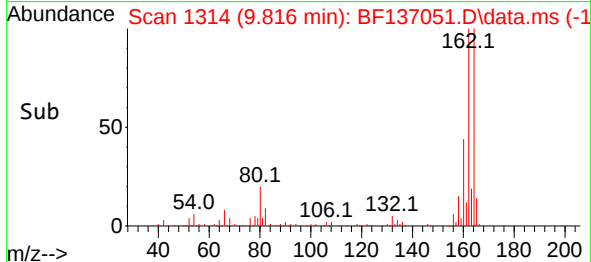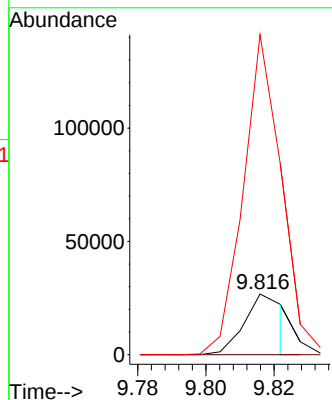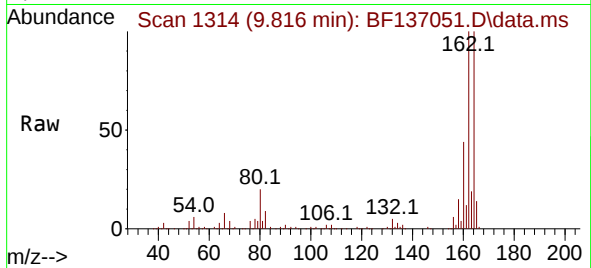

#51
2,6-Dinitrotoluene
Concen: 8.066 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.194 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28

Tgt Ion:165 Resp: 14993
Ion Ratio Lower Upper
165 100
63 1.4 39.8 59.6#
89 2.2 38.8 58.2#


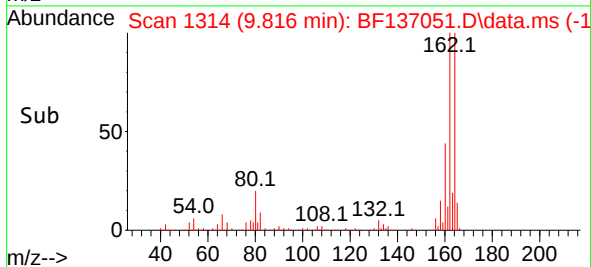
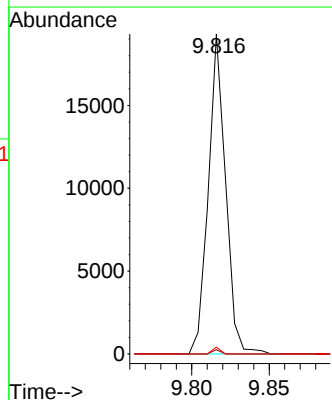
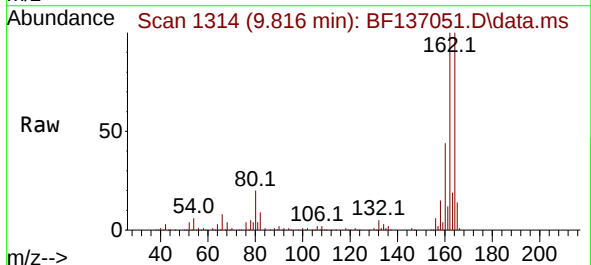




#57
2,4-Dinitrotoluene
Concen: 6.213 ng
RT: 9.816 min Scan# 11
Delta R.T. -0.206 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE


Tgt Ion:165 Resp: 14993
Ion Ratio Lower Upper
165 100
63 1.4 41.0 61.6#
89 2.2 59.9 89.9#
182 0.0 2.0 3.0#

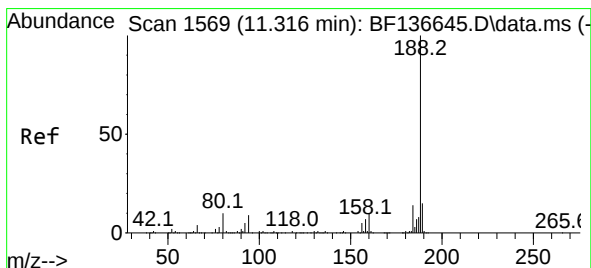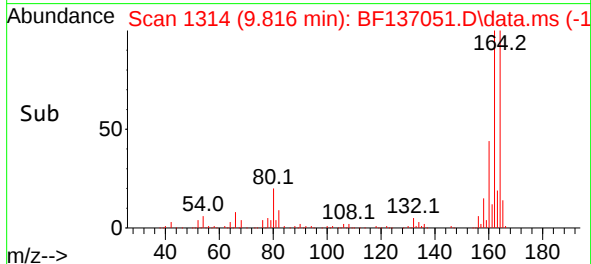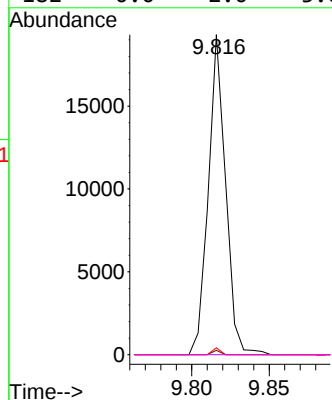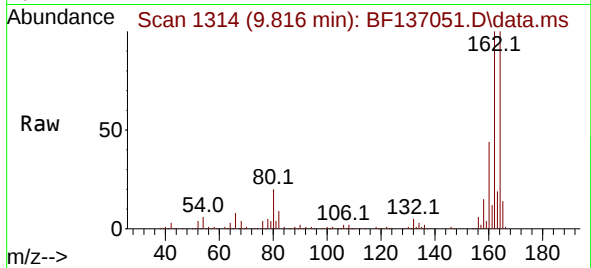

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28

Tgt Ion:188 Resp: 193400
Ion Ratio Lower Upper
188 100
94 9.3 7.5 11.3
80 9.3 8.1 12.1


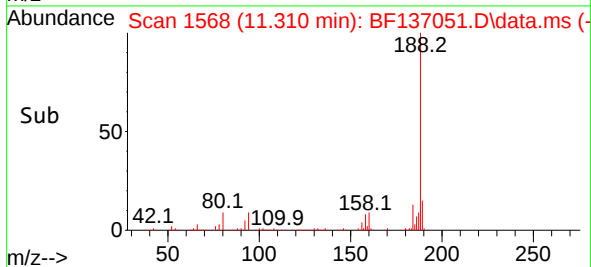
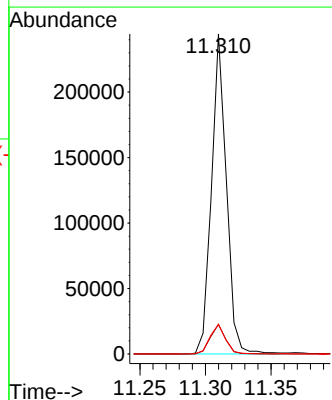
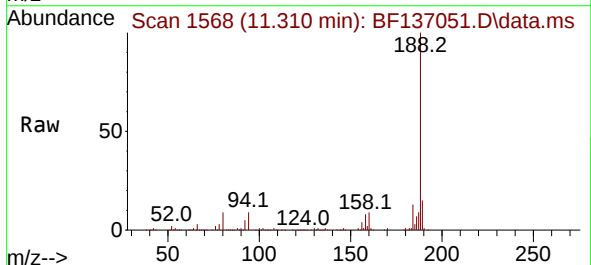


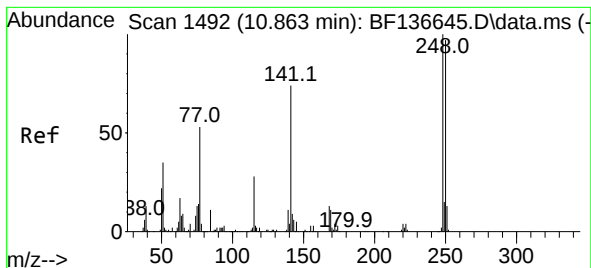

#67
4-Bromophenyl-phenylether
Concen: 2.872 ng
RT: 10.610 min Scan# 1492
Delta R.T. -0.253 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28




Instrument :
BNA_F
ClientSampleId :
S1-COMPOSITE

Tgt Ion:248 Resp: 6169
Ion Ratio Lower Upper
248 100
250 167.0 77.8 116.6#
141 474.6 59.2 88.8#

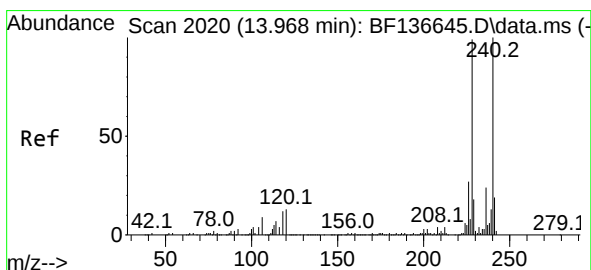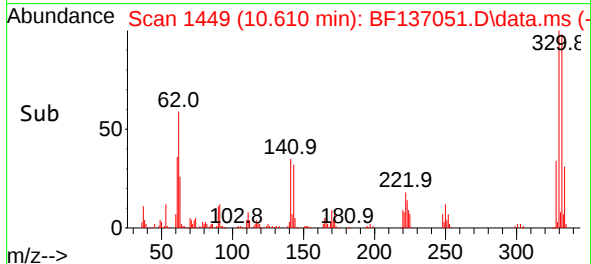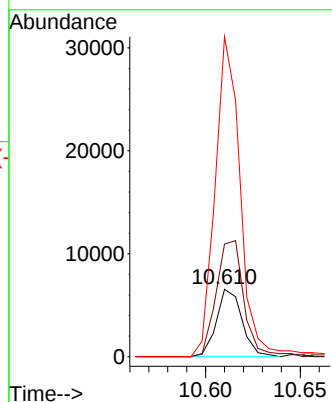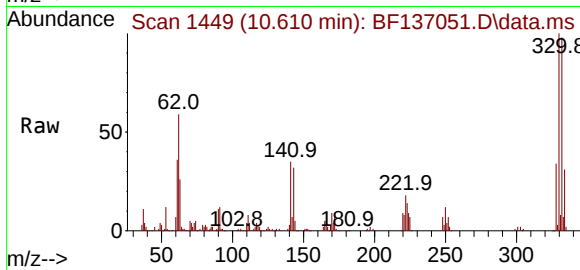

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.969 min Scan# 2020
Delta R.T. 0.000 min
Lab File: BF137051.D
Acq: 12 Jan 2024 16:28


Tgt Ion:240 Resp: 115562
Ion Ratio Lower Upper
240 100
120 11.2 10.3 15.5
236 24.2 19.4 29.2

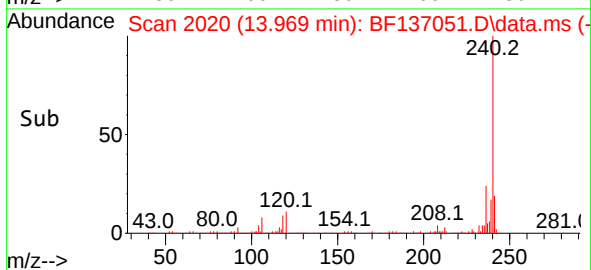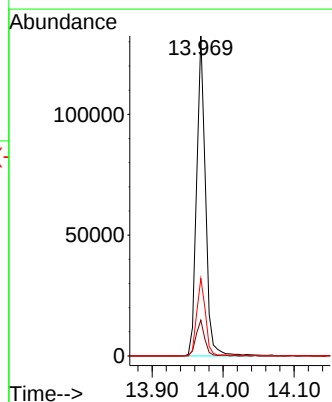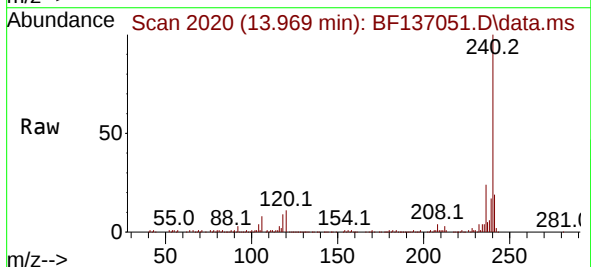






#79
 Terphenyl-d14
 Concen: 43.074 ng
 RT: 12.904 min Scan# 1839
 Delta R.T. -0.012 min
 Lab File: BF137051.D
 Acq: 12 Jan 2024 16:28

Instrument :
 BNA_F
 ClientSampleId :
 S1-COMPOSITE

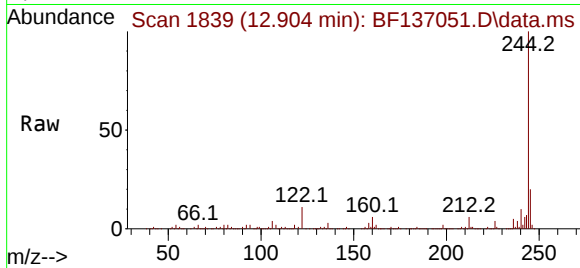

Tgt Ion:244 Resp: 356199
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.0 7.4
 122 11.2 9.0 13.4

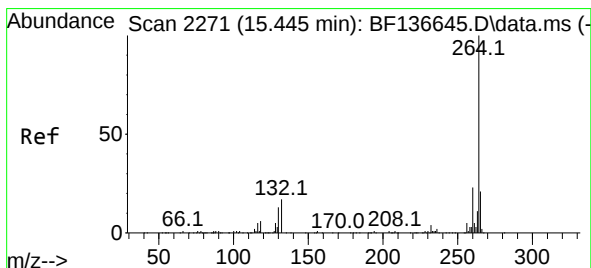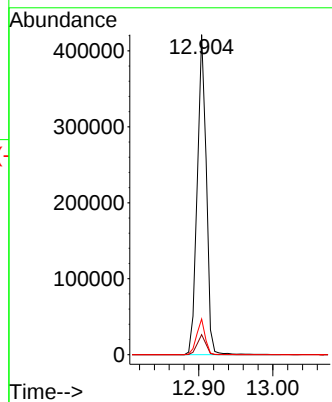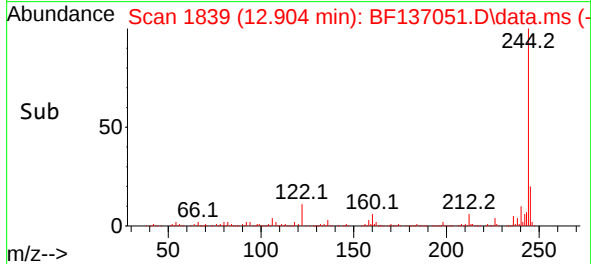

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.463 min Scan# 2274
 Delta R.T. 0.018 min
 Lab File: BF137051.D
 Acq: 12 Jan 2024 16:28

Tgt Ion:264 Resp: 134395
 Ion Ratio Lower Upper
 264 100
 260 25.4 18.3 27.5
 265 20.7 17.0 25.6

