
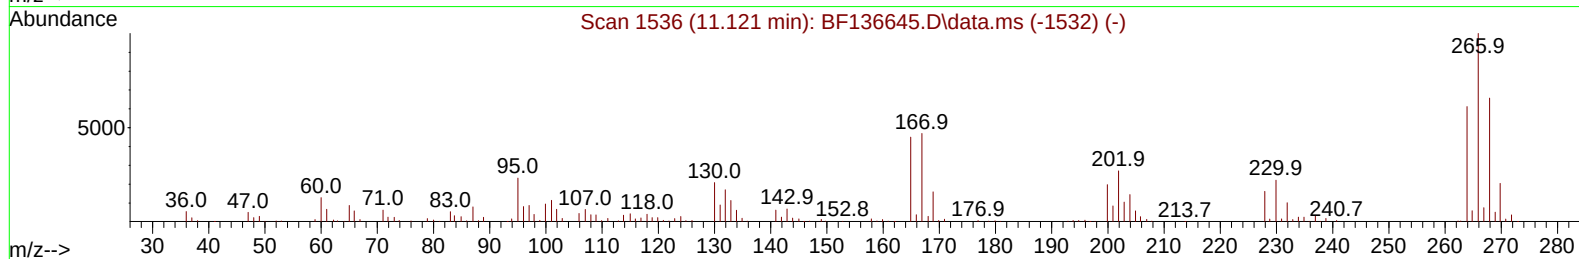
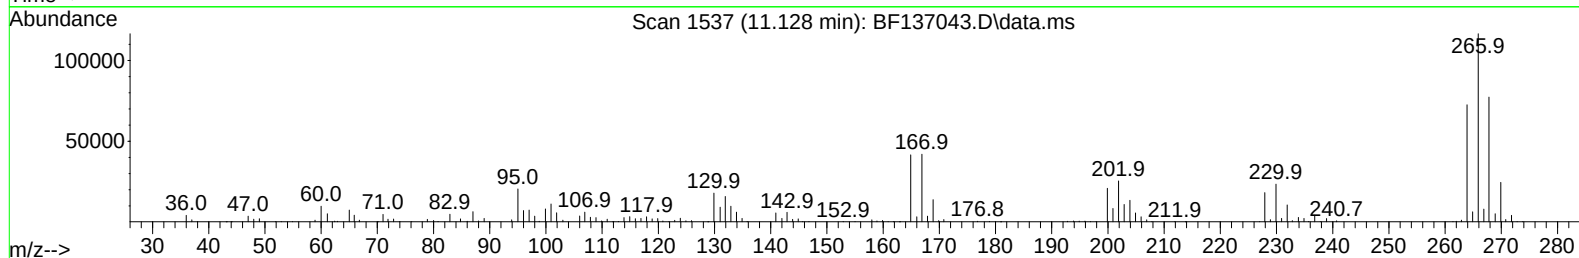


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011224\
Data File : BF137043.D
Acq On : 12 Jan 2024 12:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 14:57:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

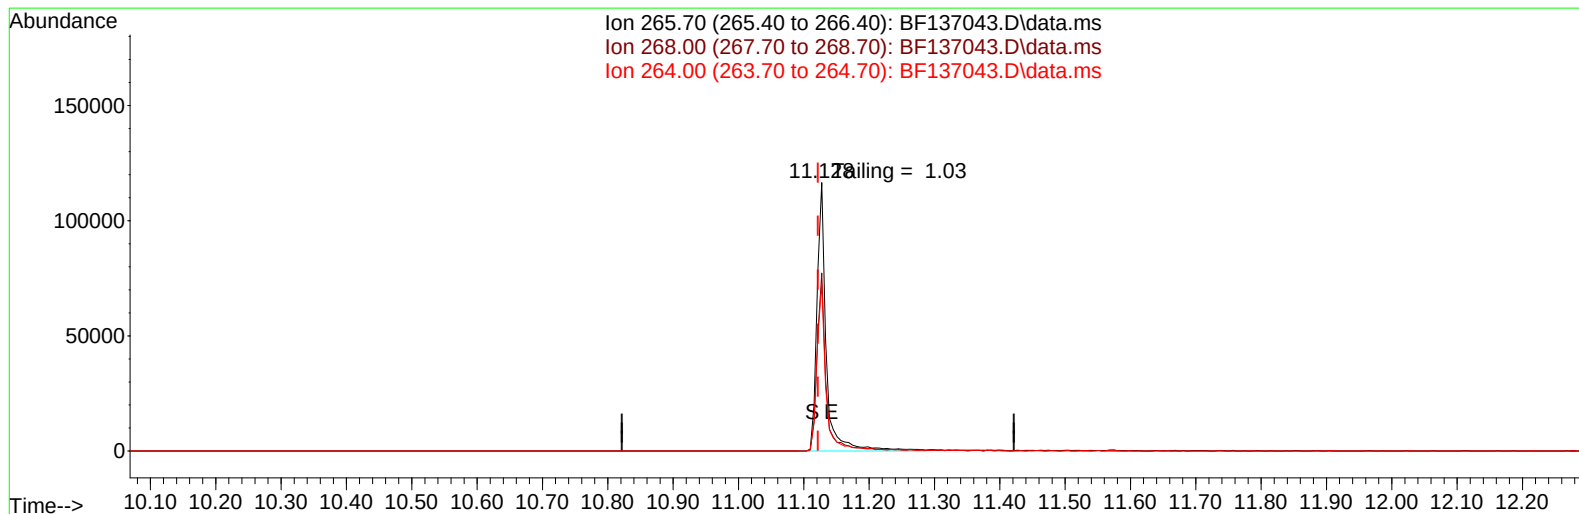

TIC: BF137043.D\data.ms

(70) Pentachlorophenol (C)




11.128min (+ 0.006) 80510.76 ng

response 116112

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.32
264.00	61.20	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011224\
Data File : BF137043.D
Acq On : 12 Jan 2024 12:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 14:57:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

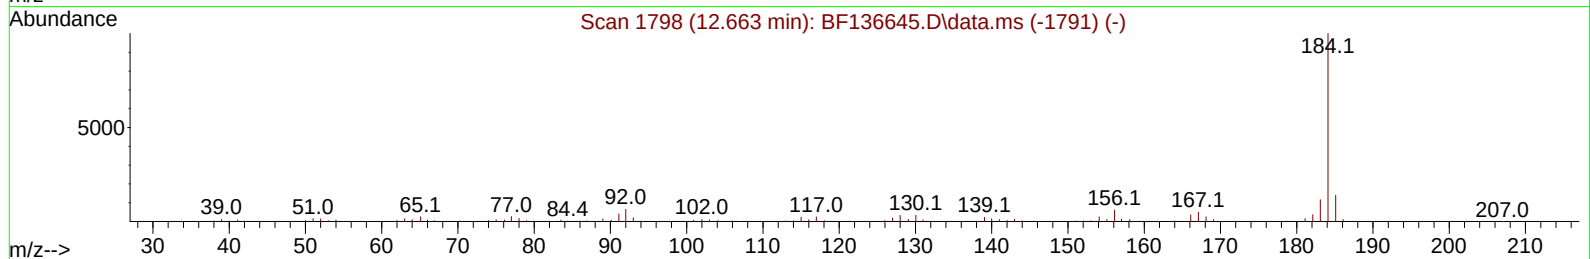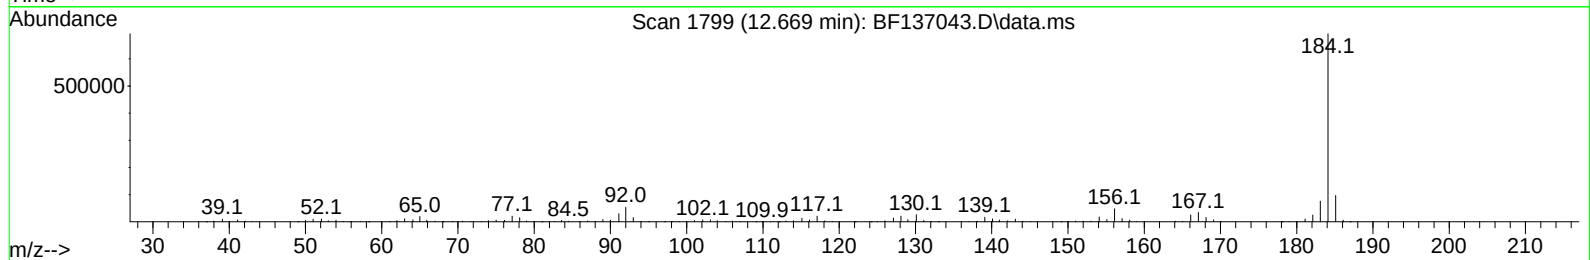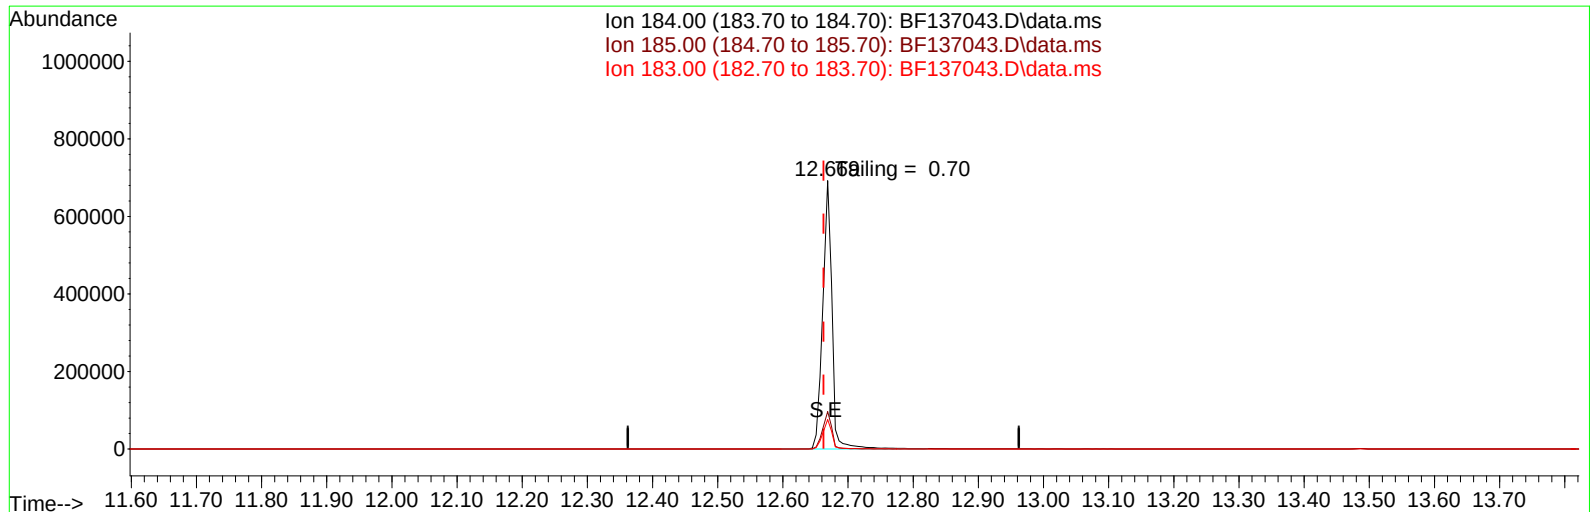

TIC: BF137043.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 310810.36 ng

response 687335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.96
183.00	11.60	11.02
0.00	0.00	0.00