


Data Path : Z:\HPCHEM1\BNA F\Data\BF011316\
 Data File : BF084444.D
 Acq On : 13 Jan 2016 15:01
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

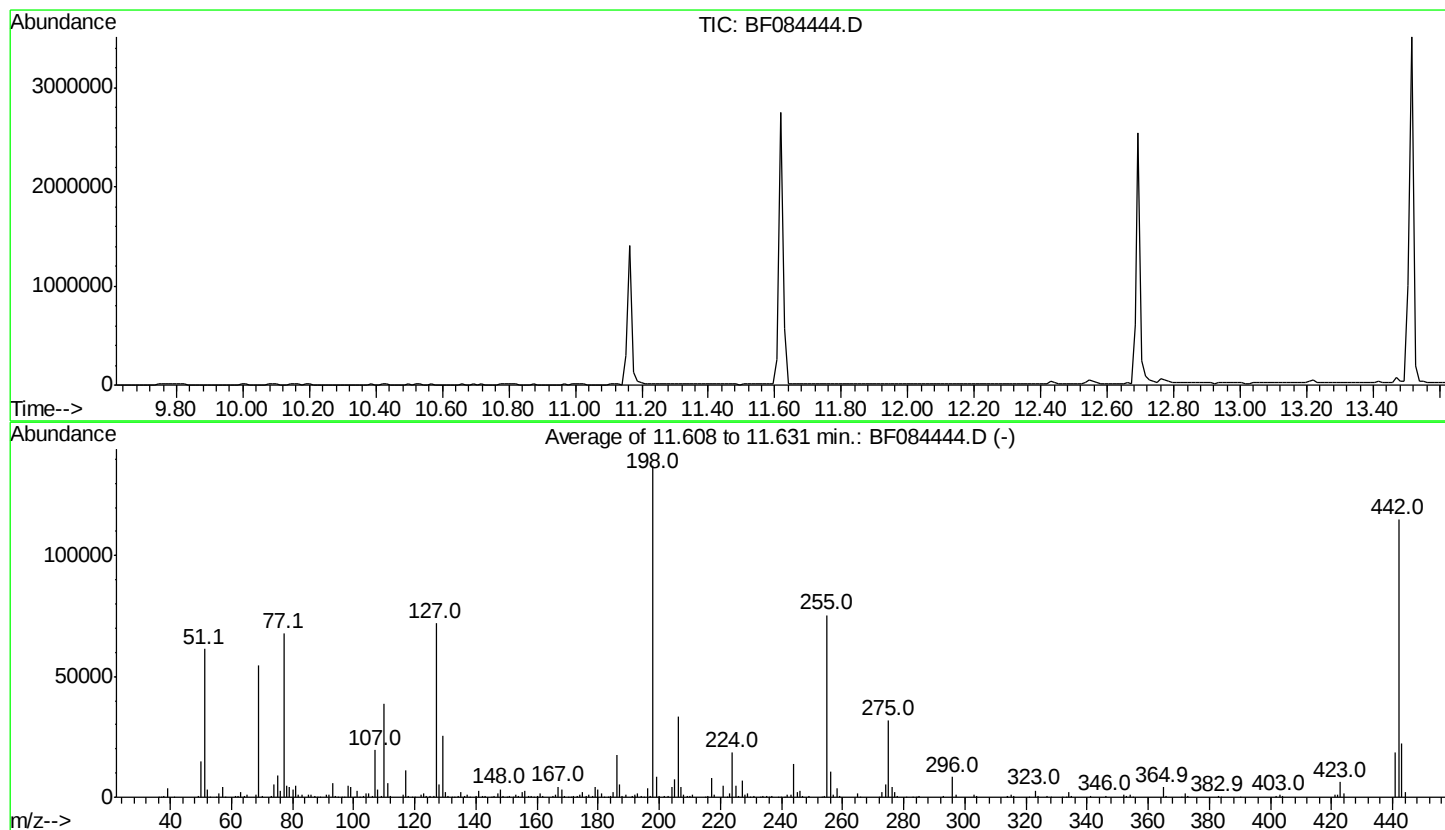

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	61378	PASS
68	69	0.00	2	1.7	955	PASS
69	198	0.00	100	39.8	54690	PASS
70	69	0.00	2	0.7	363	PASS
127	198	10	80	52.4	71957	PASS
197	198	0.00	2	0.5	649	PASS
198	198	100	100	100.0	137285	PASS
199	198	5	9	6.4	8762	PASS
275	198	10	60	23.0	31644	PASS
365	198	1	100	2.9	4029	PASS
441	442	0.01	24	16.2	18618	PASS
442	198	50	100	83.7	114884	PASS
443	442	15	24	19.5	22429	PASS