

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092280.D
 Acq On : 14 Jan 2017 12:55
 Operator : UM/SJ
 Sample : I1162-14
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

Quant Time: Jan 16 03:18:40 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 16 01:02:36 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	231361	20.00	ng	-0.01
21) Naphthalene-d8	7.86	136	805313	20.00	ng	-0.02
38) Acenaphthene-d10	9.60	164	360564	20.00	ng	-0.02
63) Phenanthrene-d10	11.09	188	509786	20.00	ng	-0.01
75) Chrysene-d12	13.71	240	424113	20.00	ng	-0.02
86) Perylene-d12	15.07	264	424472	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.17	112	1507026	108.76	ng	0.00
7) Phenol-d6	6.24	99	1975935	116.80	ng	-0.01
23) Nitrobenzene-d5	7.15	82	1198101	82.73	ng	-0.01
41) 2,4,6-Tribromophenol	10.40	330	316404	106.04	ng	-0.01
44) 2-Fluorobiphenyl	8.94	172	1589562	91.28	ng	-0.01
78) Terphenyl-d14	12.67	244	1027133	58.74	ng	-0.02
Target Compounds						
10) Phenol	6.26	94	132226	6.86	ng	# 66
19) n-Nitroso-di-n-propylamine	7.15	70	159285	14.15	ng	# 76
25) Isophorone	7.15	82	1193584	44.67	ng	# 65
37) 2-Methylnaphthalene	8.58	142	879	Below Cal	#	72
49) Dimethylphthalate	9.34	163	276778	12.00	ng	99
56) 2,4-Dinitrotoluene	9.60	165	46983	7.42	ng	# 20
66) 4-Bromophenyl-phenylether	10.40	248	19825	3.74	ng	# 1
71) Anthracene	11.16	178	6346	Below Cal		95
73) Di-n-butylphthalate	11.66	149	3026	Below Cal	#	84
74) Fluoranthene	12.29	202	41708	Below Cal		97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
Data File : BF092280.D
Acq On : 14 Jan 2017 12:55
Operator : UM/SJ
Sample : I1162-14
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-08-COMP

Quant Time: Jan 16 03:18:40 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 16 01:02:36 2017
Response via : Initial Calibration

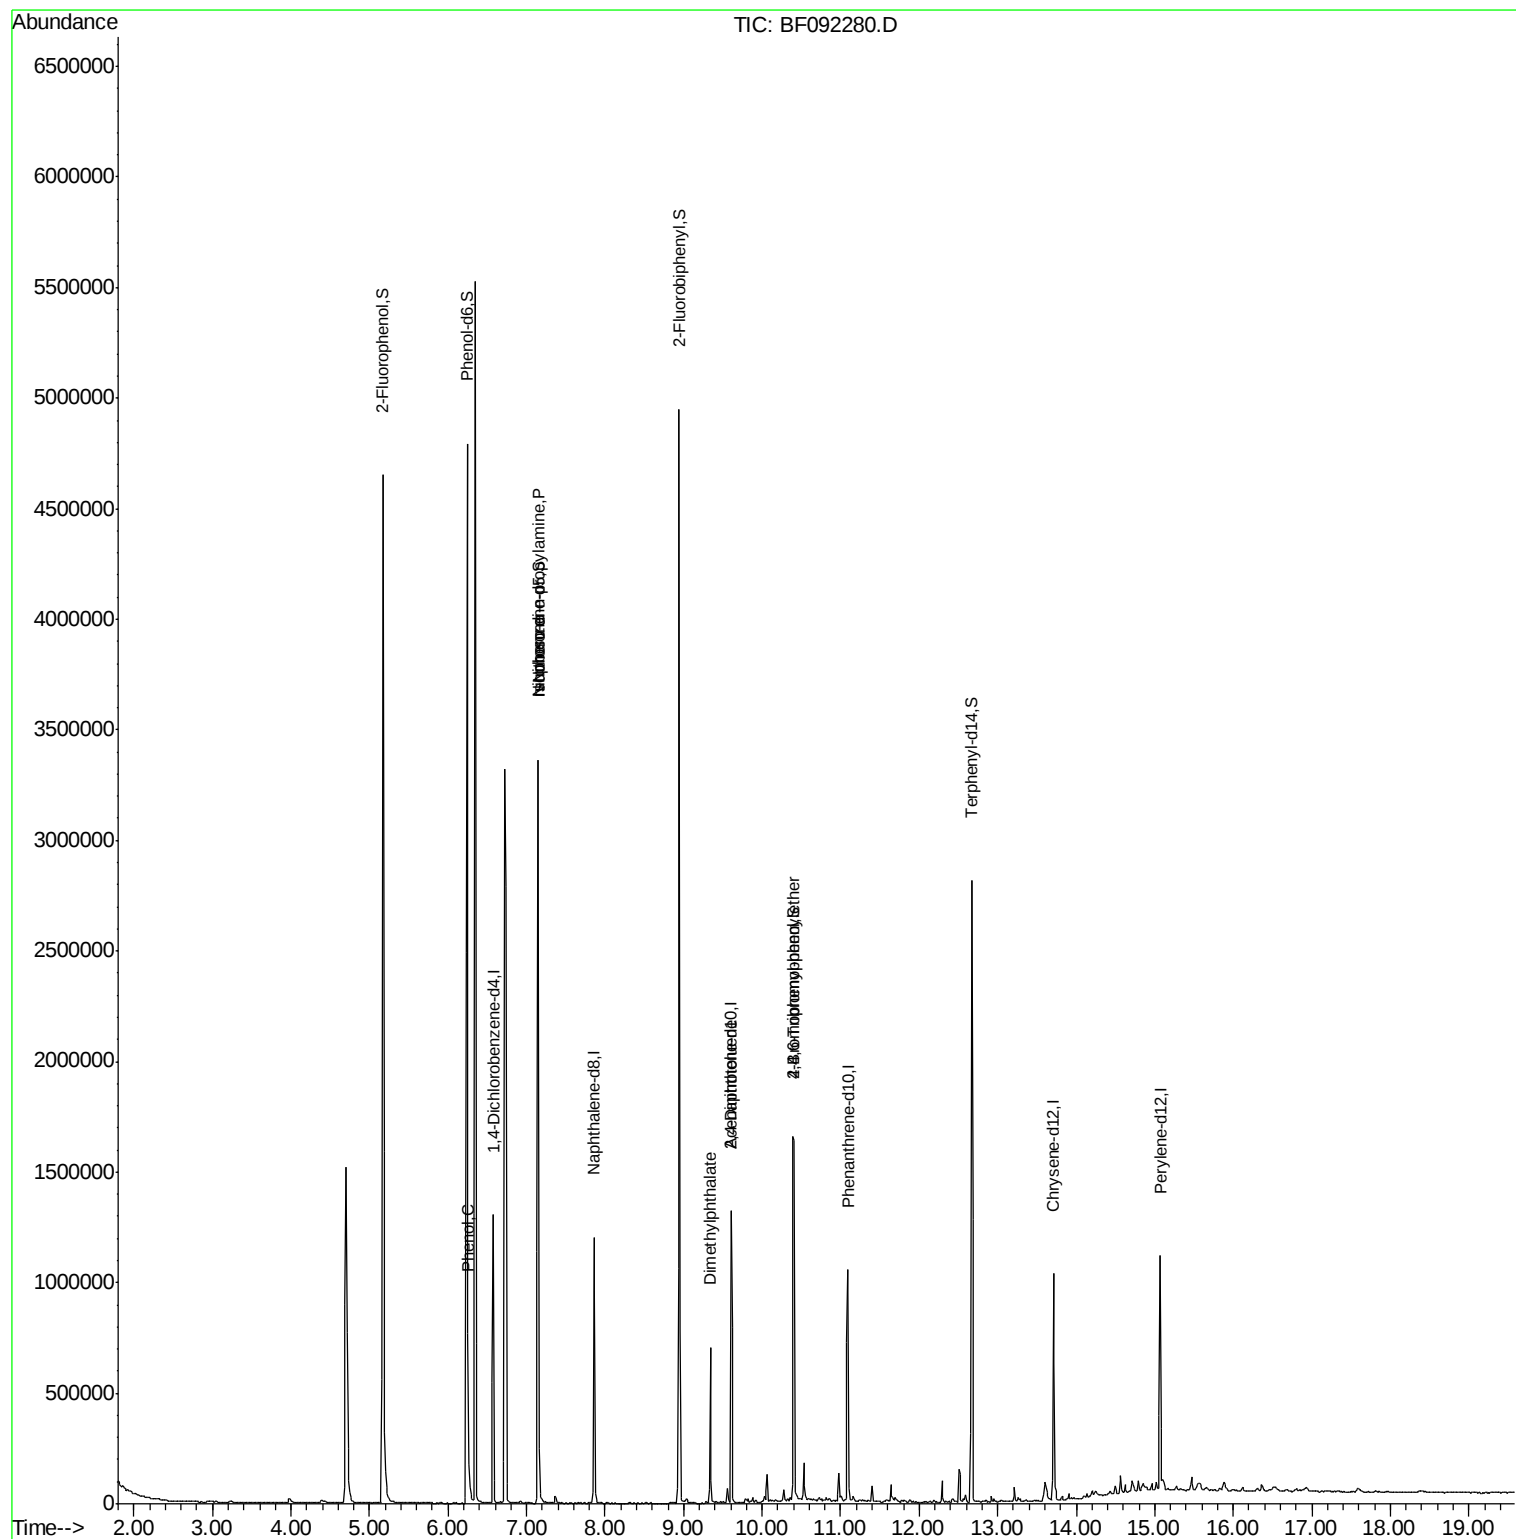



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 419

Delta R.T. -0.01 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55

Instrument :

BNA_F

ClientSampleId :

SB-08-COMP


Tgt Ion:152 Resp: 231361

Ion Ratio Lower Upper

152 100

150 153.9 124.9 187.3




115 54.5 46.0 69.0

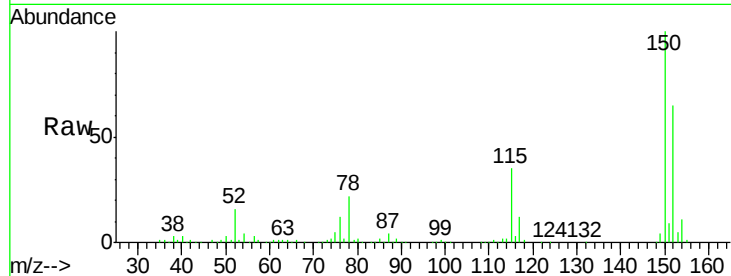

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

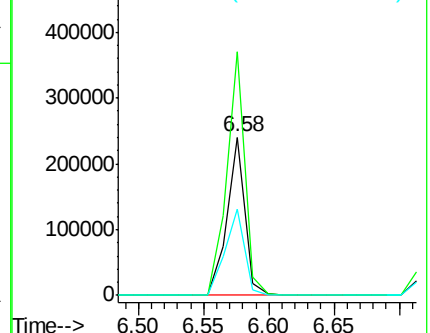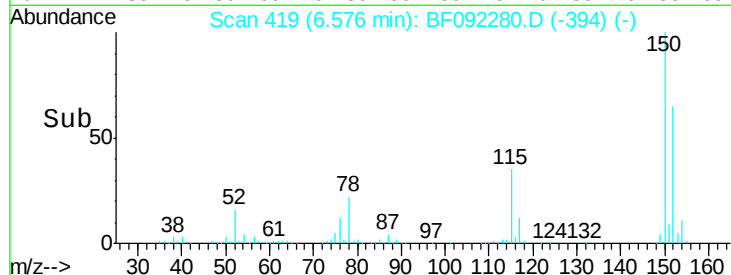

#5

2-Fluorophenol

Concen: 108.76 ng

RT: 5.17 min Scan# 296

Delta R.T. 0.00 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55


Tgt Ion:112 Resp: 1507026

Ion Ratio Lower Upper

112 100

64 63.9 46.1 69.1



63 32.1 23.8 35.6



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

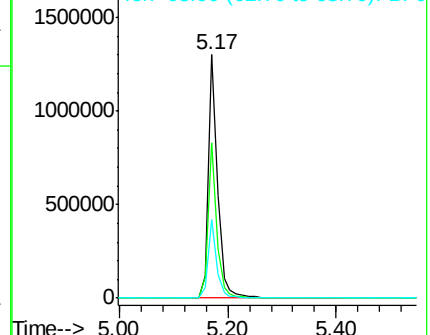



#7

Phenol-d6

Concen: 116.80 ng

RT: 6.24 min Scan# 390

Delta R.T. -0.01 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55

Instrument :

BNA_F

ClientSampleId :

SB-08-COMP


Tgt Ion: 99 Resp: 1975935

Ion Ratio Lower Upper

99 100

42 18.1 15.6 23.4




71 32.4 27.5 41.3

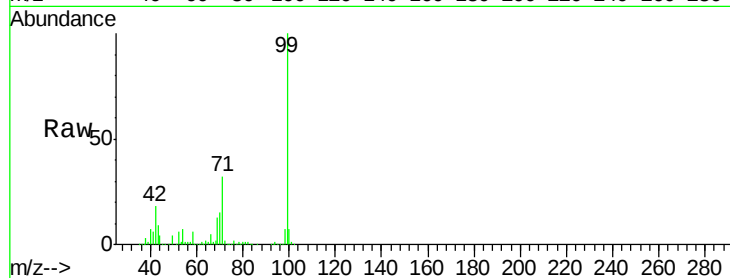

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

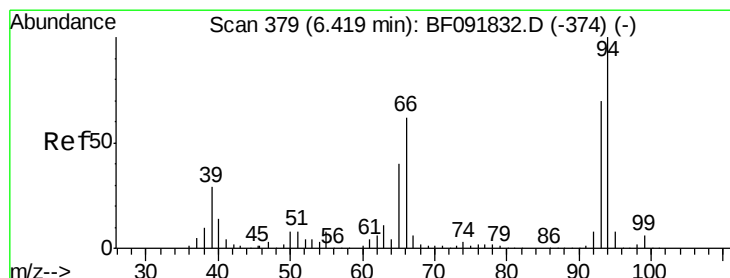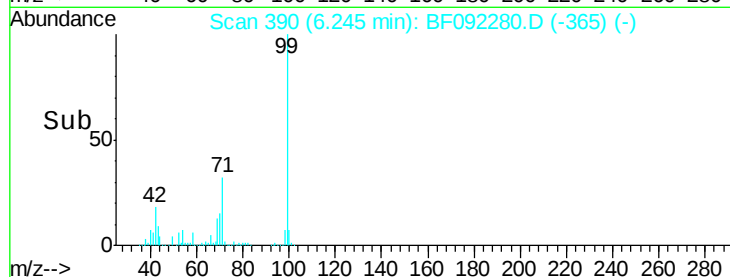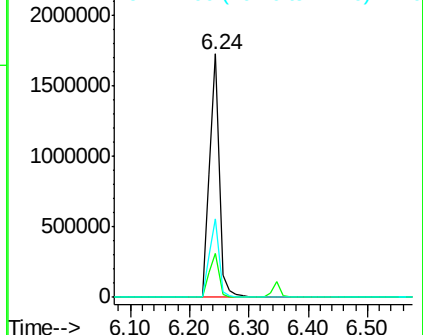

#10

Phenol

Concen: 6.86 ng

RT: 6.26 min Scan# 391

Delta R.T. -0.01 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55


Tgt Ion: 94 Resp: 132226

Ion Ratio Lower Upper

94 100

65 24.4 21.4 61.4



66 33.5 44.0 84.0#



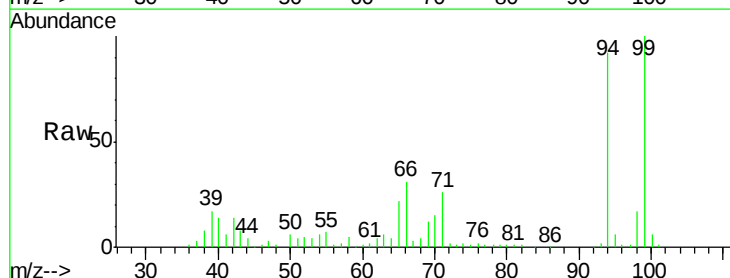


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



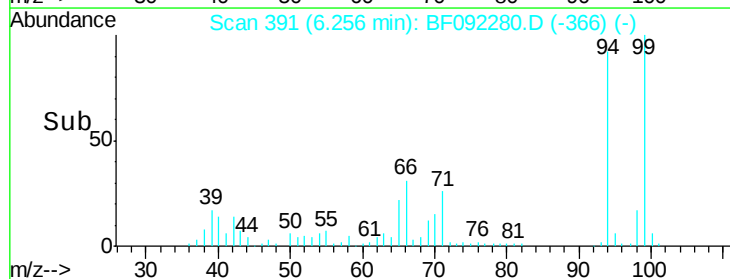
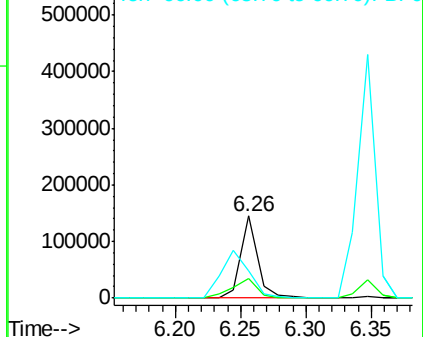


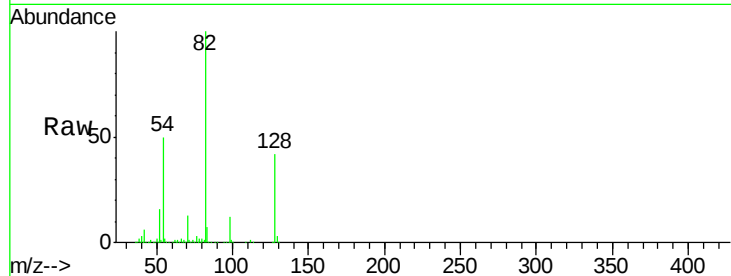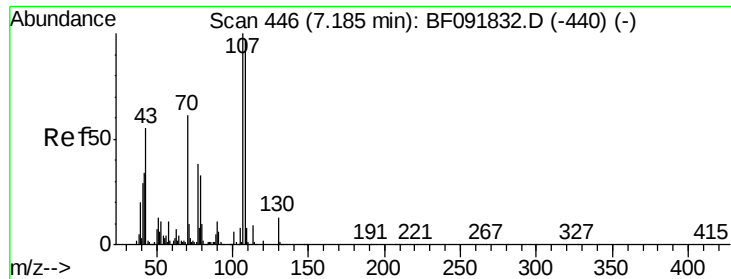

#19
n-Nitroso-di-n-propylamine
Concen: 14.15 ng
RT: 7.15 min Scan# 469
Delta R.T. 0.13 min
Lab File: BF092280.D
Acq: 14 Jan 2017 12:55


Instrument :
BNA_F
ClientSampleId :
SB-08-COMP

Tgt Ion: 70 Resp: 159285
Ion Ratio Lower Upper
70 100
42 46.5 49.4 74.0#
101 0.0 7.4 11.2#
130 2.2 14.2 21.4#

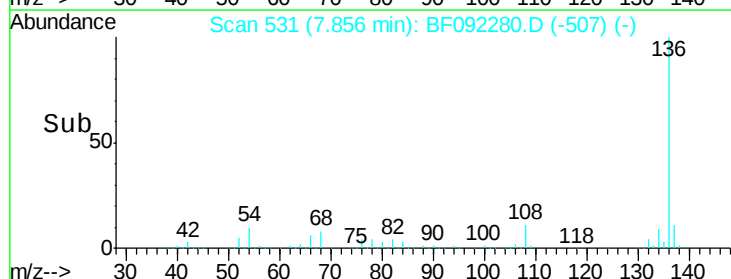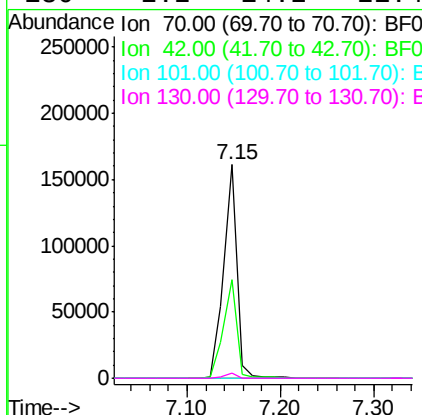

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.86 min Scan# 531
Delta R.T. -0.02 min
Lab File: BF092280.D
Acq: 14 Jan 2017 12:55

Tgt Ion: 136 Resp: 805313
Ion Ratio Lower Upper
136 100
137 11.4 8.4 12.6
54 10.1 4.5 6.7#
68 7.8 3.6 5.4#

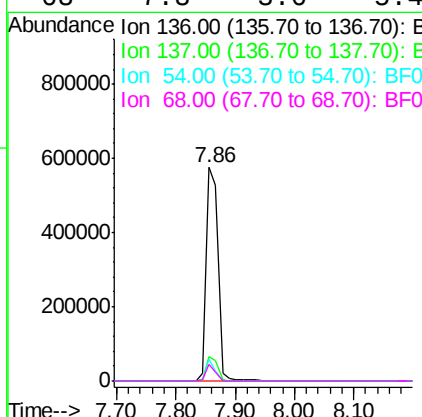







#23
 Nitrobenzene-d5
 Concen: 82.73 ng
 RT: 7.15 min Scan# 469
 Delta R.T. -0.01 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

Tgt Ion: 82 Resp: 1198101
 Ion Ratio Lower Upper
 82 100
 128 42.0 34.6 52.0
 54 49.6 39.5 59.3

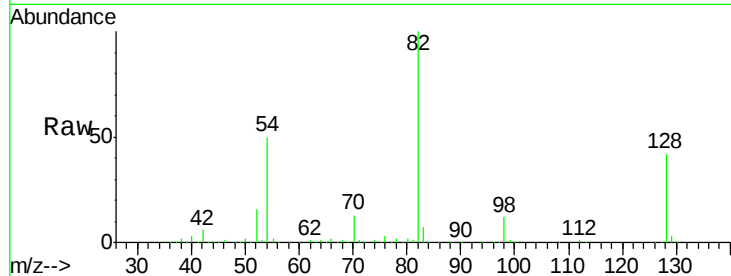


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0


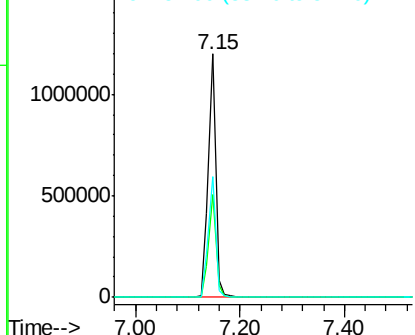



#25
 Isophorone
 Concen: 44.67 ng
 RT: 7.15 min Scan# 469
 Delta R.T. -0.27 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Tgt Ion: 82 Resp: 1193584
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.6 8.4#
 138 0.0 14.6 22.0#



Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0



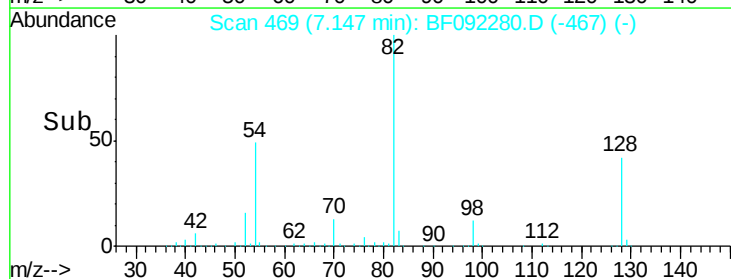
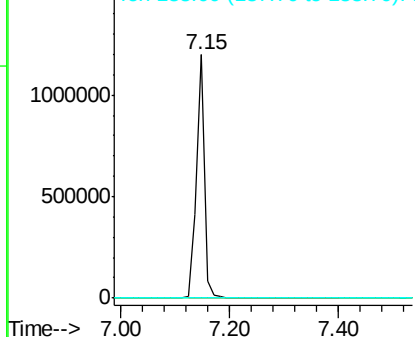


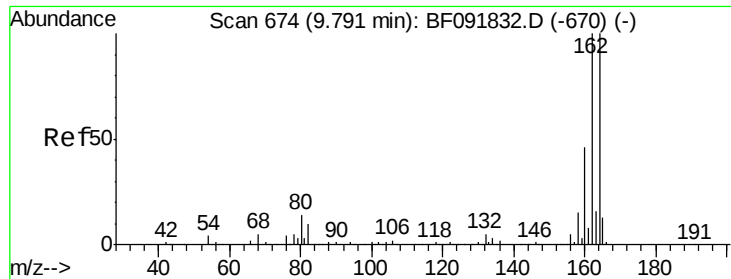

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.60 min Scan# 684
 Delta R.T. -0.02 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55




Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP


Tgt Ion:164 Resp: 360564
 Ion Ratio Lower Upper
 164 100
 162 101.1 80.2 120.2
 160 45.3 36.9 55.3

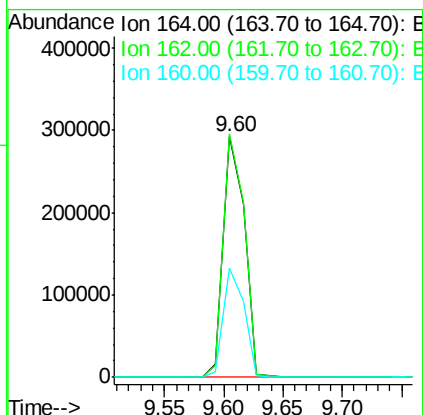

#41
 2,4,6-Tribromophenol
 Concen: 106.04 ng
 RT: 10.40 min Scan# 754
 Delta R.T. -0.01 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Tgt Ion:330 Resp: 316404
 Ion Ratio Lower Upper
 330 100
 332 97.8 77.4 116.2
 141 34.0 34.1 51.1#

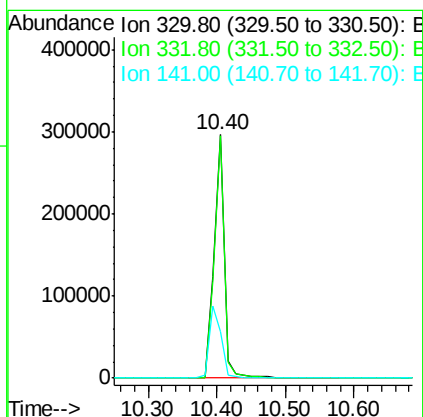


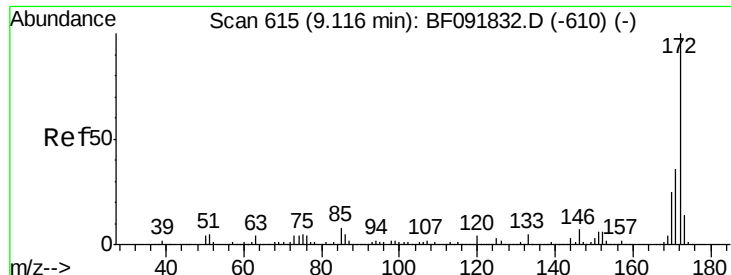




#44
 2-Fluorobiphenyl
 Concen: 91.28 ng
 RT: 8.94 min Scan# 626
 Delta R.T. -0.01 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

Tgt Ion:172 Resp: 1589562
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.4 44.0
 170 24.3 20.2 30.4

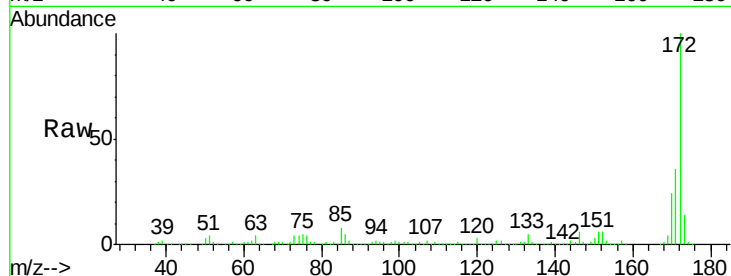


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


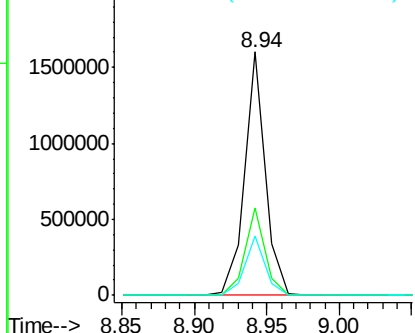


#49
 Dimethylphthalate
 Concen: 12.00 ng
 RT: 9.34 min Scan# 661
 Delta R.T. -0.02 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Tgt Ion:163 Resp: 276778
 Ion Ratio Lower Upper
 163 100
 194 3.3 3.0 4.4
 164 10.1 8.0 12.0

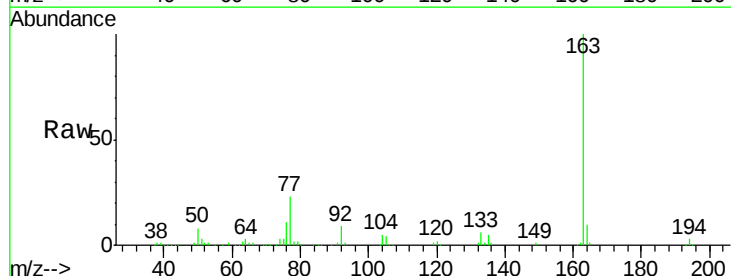

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




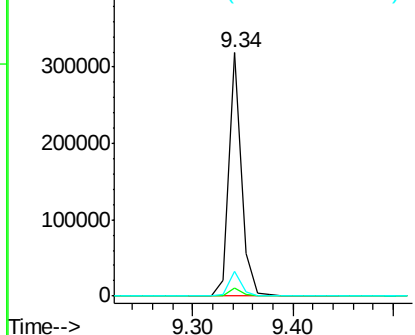




#56
 2,4-Dinitrotoluene
 Concen: 7.42 ng
 RT: 9.60 min Scan# 684
 Delta R.T. -0.23 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55




Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.6	40.2	60.4#
89	1.1	62.5	93.7#
182	0.0	1.8	2.8#

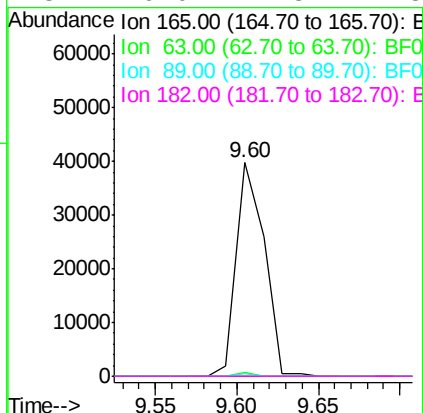

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.09 min Scan# 814
 Delta R.T. -0.01 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.1	10.0	15.0#
80	7.2	11.2	16.8#

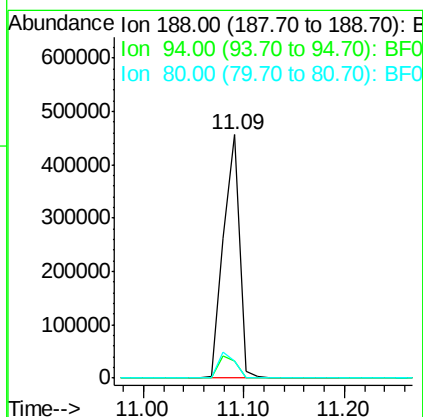

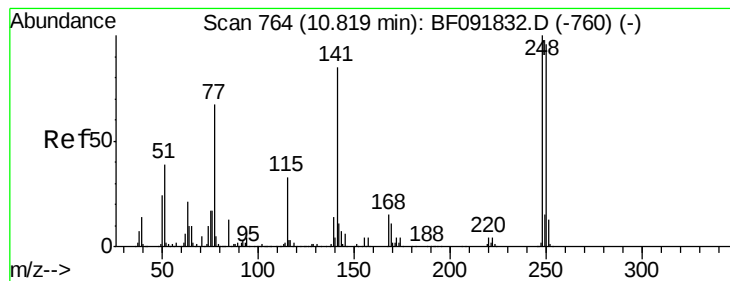

#66

4-Bromophenyl-phenylether

Concen: 3.74 ng

RT: 10.40 min Scan# 754

Delta R.T. -0.25 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55

Instrument :

BNA_F

ClientSampleId :

SB-08-COMP


Tgt Ion:248 Resp: 19825

Ion Ratio Lower Upper

248 100

250 193.3 76.9 115.3#




141 363.1 68.2 102.4#

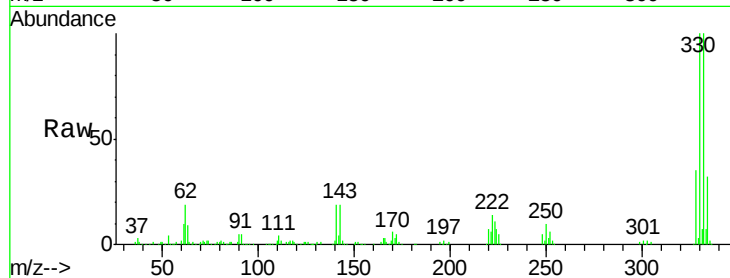

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

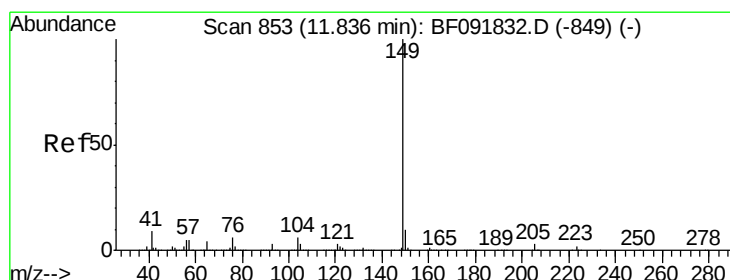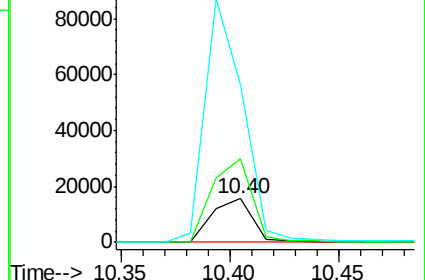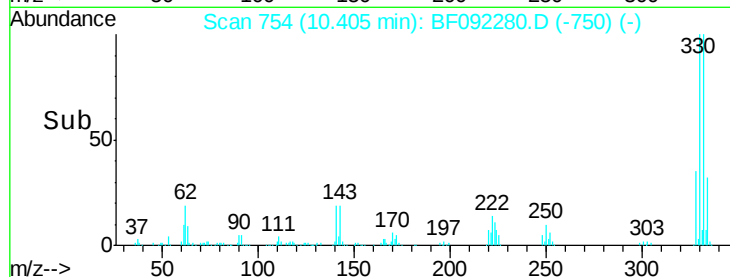

#73

Di-n-butylphthalate

Concen: Below Cal

RT: 11.66 min Scan# 864

Delta R.T. -0.02 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55


Tgt Ion:149 Resp: 3026

Ion Ratio Lower Upper

149 100

150 15.8 8.1 12.1#



104 0.0 4.6 7.0#

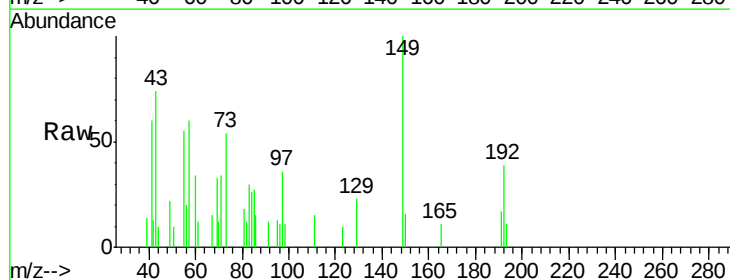


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

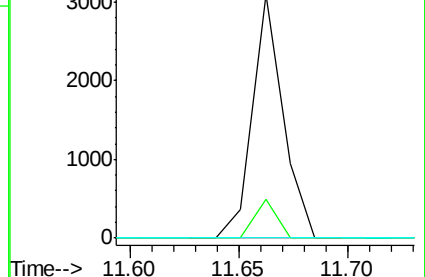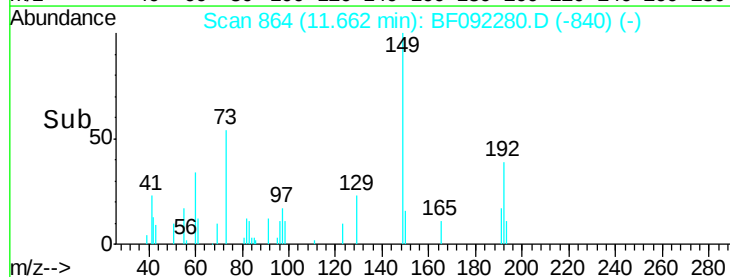



#74

Fluoranthene

Concen: Below Cal

RT: 12.29 min Scan# 919

Delta R.T. -0.01 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55

Instrument :

BNA_F

ClientSampleId :

SB-08-COMP


Tgt Ion:202 Resp: 41708

Ion Ratio Lower Upper

202 100

101 13.6 0.0 34.6




203 17.3 0.0 38.7

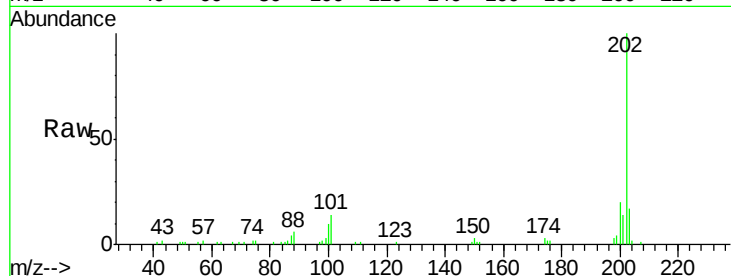

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

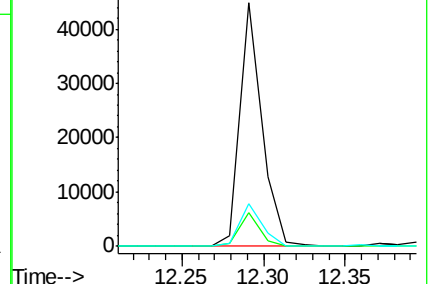

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1043

Delta R.T. -0.02 min

Lab File: BF092280.D

Acq: 14 Jan 2017 12:55


Tgt Ion:240 Resp: 424113

Ion Ratio Lower Upper

240 100

120 16.0 12.9 19.3



236 24.7 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



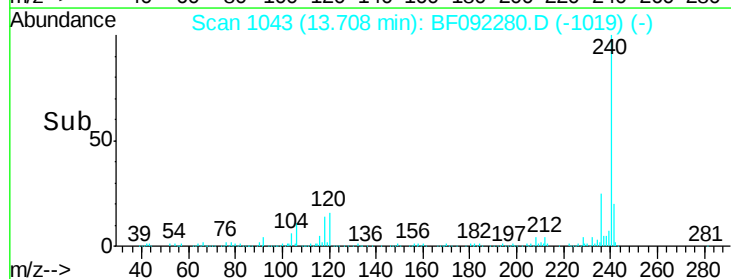
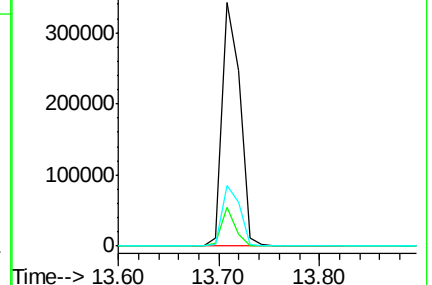




#78
 Terphenyl-d14
 Concen: 58.74 ng
 RT: 12.67 min Scan# 952
 Delta R.T. -0.02 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

Tgt Ion:244 Resp: 1027133
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.2 9.2
 122 15.7 11.4 17.2

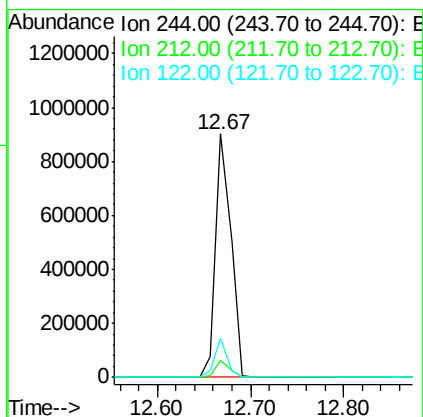

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.07 min Scan# 1162
 Delta R.T. -0.02 min
 Lab File: BF092280.D
 Acq: 14 Jan 2017 12:55

Tgt Ion:264 Resp: 424472
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.2 28.8
 265 22.4 17.4 26.0

