
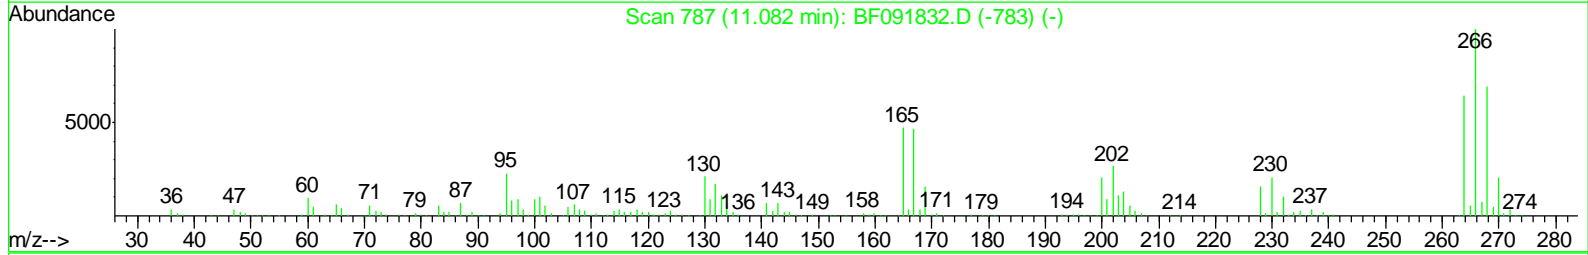
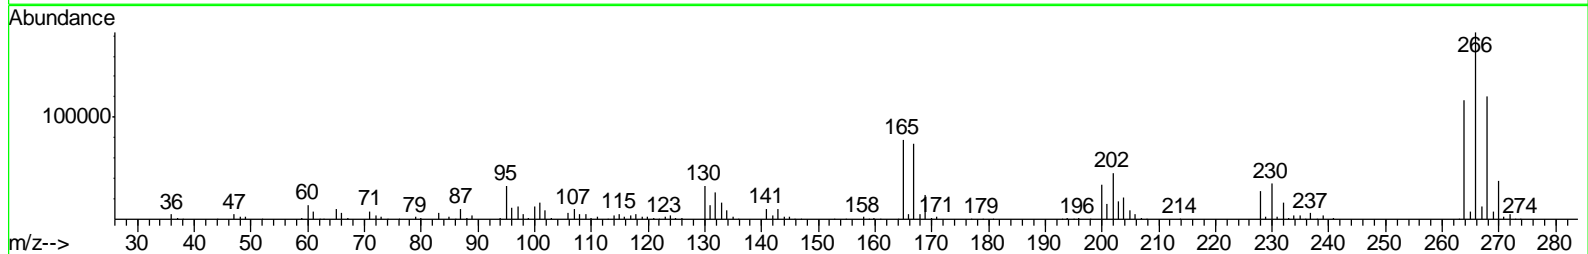


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092238.D
 Acq On : 13 Jan 2017 9:51
 Operator : UM/SJ
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 07:31:48 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 16 01:02:36 2017
 Response via : Initial Calibration

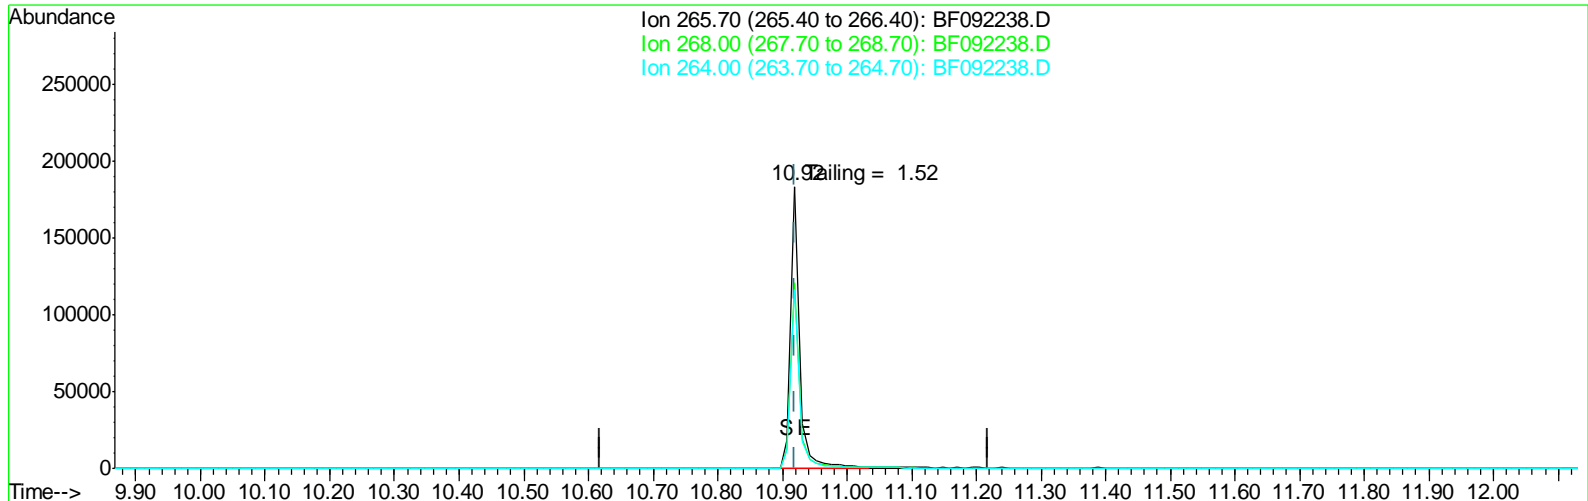

TIC: BF092238.D

(69) Pentachlorophenol (C)




10.919min (-0.000) 0.00ng

response 181211

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.87
264.00	62.90	63.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092238.D
 Acq On : 13 Jan 2017 9:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 07:31:48 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 16 01:02:36 2017
 Response via : Initial Calibration

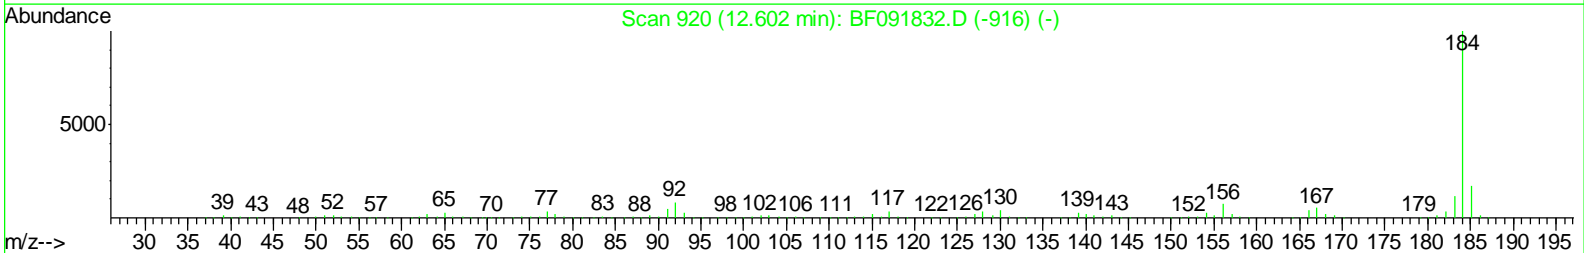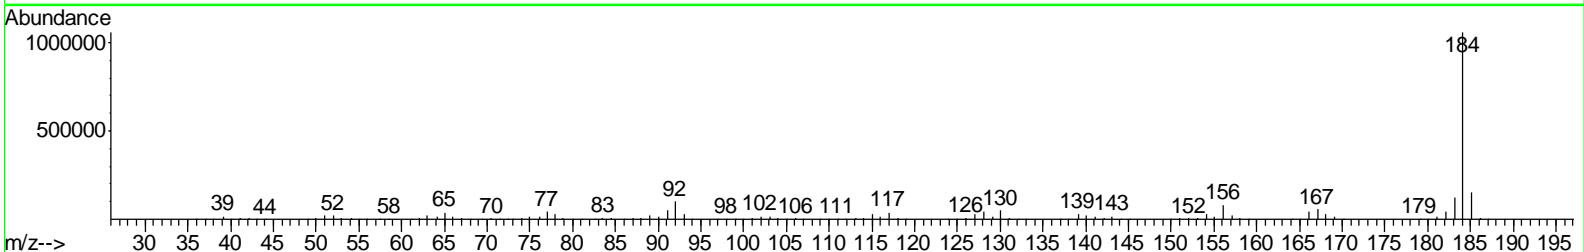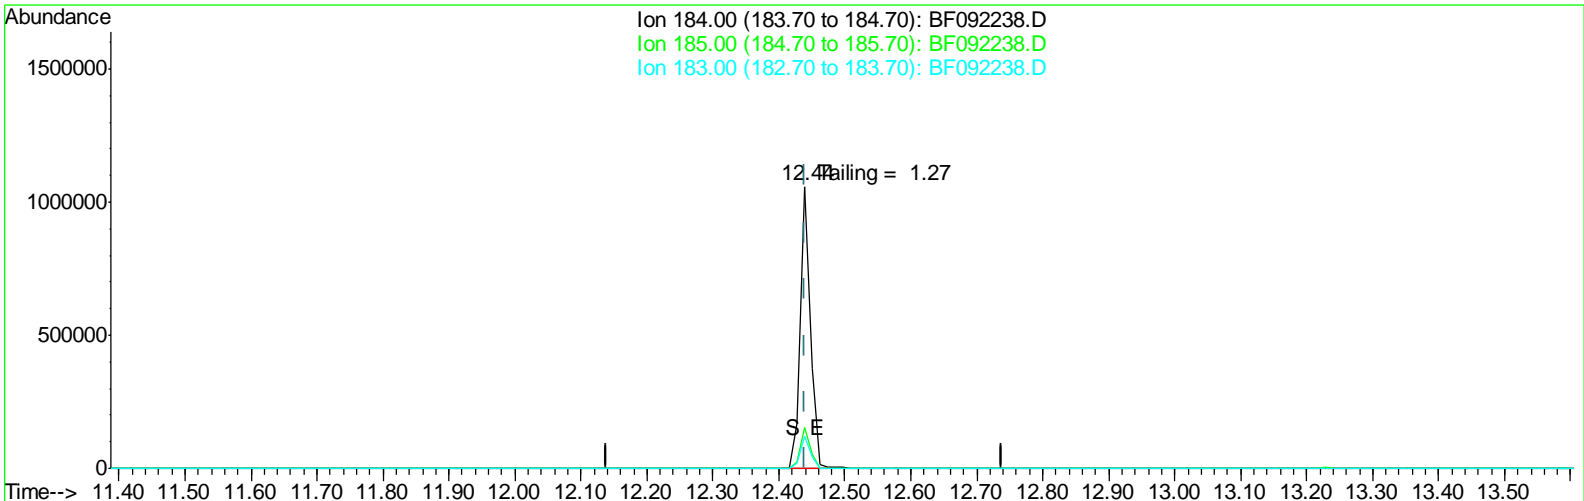

TIC: BF092238.D

(76) Benzidine

12.439min (-0.000) 0.00ng

response 1126998

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.72
183.00	11.50	11.50
0.00	0.00	0.00