

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011317\
 Data File : BF092242.D
 Acq On : 13 Jan 2017 11:52
 Operator : UM/SJ
 Sample : I1131-03MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.072	23	25	32	rVB	374049	492846	5.58%	0.226%
2	2.655	72	76	79	rBV	429490	887027	10.05%	0.407%
3	2.701	79	80	92	rVB	635372	1259692	14.27%	0.578%
4	3.981	190	192	198	rBV	195773	366945	4.16%	0.168%
5	4.667	250	252	254	rBV	112042	151317	1.71%	0.069%
6	4.724	254	257	270	rVB	2078756	3561967	40.36%	1.633%
7	5.193	295	298	300	rBV	4222809	5621068	63.69%	2.578%
8	6.130	378	380	386	rBV	126040	156528	1.77%	0.072%
9	6.267	388	392	395	rBV3	4895497	8825617	100.00%	4.047%
10	6.336	395	398	399	rVV	1681400	2057101	23.31%	0.943%
11	6.359	399	400	404	rVB2	4418774	7606739	86.19%	3.488%
12	6.519	412	414	417	rBV	1514532	2084798	23.62%	0.956%
13	6.599	417	421	424	rVB2	1920613	3422836	38.78%	1.570%
14	6.747	431	434	437	rBV2	4989559	7490541	84.87%	3.435%
15	6.884	443	446	449	rVB	3331397	4263374	48.31%	1.955%
16	7.010	454	457	463	rBV3	3016090	6676121	75.64%	3.061%
17	7.102	463	465	467	rVB	1370769	1566376	17.75%	0.718%
18	7.170	467	471	474	rBV2	2505396	5362339	60.76%	2.459%
19	7.284	478	481	488	rBV	1529273	1470159	16.66%	0.674%
20	7.422	491	493	496	rBV	2026157	2616167	29.64%	1.200%
21	7.502	497	500	502	rBV	1324345	1387071	15.72%	0.636%
22	7.559	502	505	507	rBV	2628031	2417815	27.40%	1.109%
23	7.639	509	512	515	rBV	1381921	1582768	17.93%	0.726%
24	7.753	520	522	525	rBV	2072760	1958695	22.19%	0.898%
25	7.822	525	528	530	rVV	2077303	2080149	23.57%	0.954%
26	7.902	530	535	537	rVB2	2602363	4701617	53.27%	2.156%
27	7.959	537	540	543	rBV	638324	815278	9.24%	0.374%
28	8.016	543	545	548	rVB	1656538	1692397	19.18%	0.776%
29	8.290	566	569	570	rBV	128547	140370	1.59%	0.064%
30	8.336	570	573	575	rVV	501026	734929	8.33%	0.337%
31	8.370	575	576	582	rVB	129473	323409	3.66%	0.148%
32	8.462	582	584	587	rBV	1357532	1940327	21.99%	0.890%
33	8.553	588	592	593	rBV	1364741	1939468	21.98%	0.889%
34	8.587	593	595	598	rVB	3271934	3033642	34.37%	1.391%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092242.D
 Acq On : 13 Jan 2017 11:52
 Operator : UM/SJ
 Sample : I1131-03MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.656	598	601	602	rBV	403996	803051	9.10%	0.368%
36	8.690	602	604	606	rVV	3029225	3327477	37.70%	1.526%
37	8.759	606	610	612	rVB2	2491496	3361388	38.09%	1.541%
38	8.885	618	621	624	rBV2	1719813	3601501	40.81%	1.652%
39	8.953	624	627	630	rVB	3661106	6341777	71.86%	2.908%
40	9.056	632	636	640	rVB2	3515437	5838144	66.15%	2.677%
41	9.182	644	647	650	rVB	1656924	1505564	17.06%	0.690%
42	9.330	658	660	661	rBV	1182242	1138558	12.90%	0.522%
43	9.365	661	663	665	rVV	2321308	2698763	30.58%	1.238%
44	9.410	665	667	670	rVV3	1316857	2541846	28.80%	1.166%
45	9.490	670	674	676	rVB	2997342	3476929	39.40%	1.594%
46	9.593	681	683	684	rVV	1065676	934097	10.58%	0.428%
47	9.628	684	686	687	rVV	1726676	1872666	21.22%	0.859%
48	9.662	687	689	691	rVB	3536855	3561110	40.35%	1.633%
49	9.708	691	693	697	rBV	375106	489603	5.55%	0.225%
50	9.788	697	700	702	rBV	1895836	2330939	26.41%	1.069%
51	9.833	702	704	706	rVV	3987711	3884120	44.01%	1.781%
52	9.913	709	711	713	rVV	1145935	1192223	13.51%	0.547%
53	9.959	713	715	720	rVB	1615383	1477797	16.74%	0.678%
54	10.062	720	724	728	rVB	2541645	2749326	31.15%	1.261%
55	10.165	731	733	735	rBV2	3632568	4505485	51.05%	2.066%
56	10.210	735	737	738	rVB	1045009	1109062	12.57%	0.509%
57	10.245	738	740	742	rBV	627473	677848	7.68%	0.311%
58	10.290	742	744	745	rVV	2914567	2669147	30.24%	1.224%
59	10.325	745	747	750	rVB	2462914	2282383	25.86%	1.047%
60	10.416	752	755	757	rBV	3275699	3293788	37.32%	1.510%
61	10.542	764	766	769	rVB	204597	234029	2.65%	0.107%
62	10.656	773	776	778	rVB	1836266	2052983	23.26%	0.941%
63	10.713	779	781	784	rVB	1493229	1657035	18.78%	0.760%
64	10.828	788	791	793	rVV	1853586	1879181	21.29%	0.862%
65	10.919	797	799	803	rBV	1327696	1519138	17.21%	0.697%
66	10.988	803	805	809	rVV2	228396	328242	3.72%	0.151%
67	11.102	812	815	816	rVV	1392148	1772034	20.08%	0.813%
68	11.125	816	817	819	rVV	3715872	2898615	32.84%	1.329%
69	11.182	819	822	823	rVV	2305732	2895792	32.81%	1.328%
70	11.342	833	836	838	rBV	2371559	2574495	29.17%	1.181%
71	11.411	840	842	844	rVV	196033	213361	2.42%	0.098%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092242.D
 Acq On : 13 Jan 2017 11:52
 Operator : UM/SJ
 Sample : I1131-03MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.593	853	858	860	rBV	90458	175157	1.98%	0.080%
73	11.651	862	863	864	rVV	344805	397716	4.51%	0.182%
74	11.673	864	865	867	rVV	1818547	2242737	25.41%	1.028%
75	11.708	867	868	873	rVB2	256327	307701	3.49%	0.141%
76	11.822	873	878	882	rBV2	108751	197454	2.24%	0.091%
77	11.891	882	884	886	rVV2	93020	141697	1.61%	0.065%
78	12.314	918	921	923	rBV	2847935	3584316	40.61%	1.644%
79	12.439	930	932	937	rVB2	439052	557915	6.32%	0.256%
80	12.531	937	940	943	rBV	2940062	3353818	38.00%	1.538%
81	12.679	951	953	956	rVV	2517840	3429791	38.86%	1.573%
82	12.862	964	969	971	rVB2	201612	340540	3.86%	0.156%
83	12.931	971	975	976	rBV	140098	173922	1.97%	0.080%
84	12.965	976	978	982	rVB2	101677	142979	1.62%	0.066%
85	13.159	993	995	998	rBV	1329689	1790890	20.29%	0.821%
86	13.239	1000	1002	1004	rBV	2533957	2367408	26.82%	1.086%
87	13.605	1030	1034	1039	rVB3	157879	313335	3.55%	0.144%
88	13.685	1039	1041	1042	rBV	691314	779471	8.83%	0.357%
89	13.731	1042	1045	1046	rVV2	3487603	5324591	60.33%	2.442%
90	13.754	1046	1047	1050	rVV	2186197	2021862	22.91%	0.927%
91	13.937	1059	1063	1067	rVB4	215076	368669	4.18%	0.169%
92	14.234	1087	1089	1093	rVV	246661	401900	4.55%	0.184%
93	14.337	1096	1098	1101	rVV	1898839	1927001	21.83%	0.884%
94	14.725	1129	1132	1133	rBV	2064321	2759042	31.26%	1.265%
95	14.817	1136	1140	1141	rVV3	103546	150340	1.70%	0.069%
96	14.977	1152	1154	1157	rBV	319176	384857	4.36%	0.176%
97	15.034	1157	1159	1161	rBV	1810698	2186651	24.78%	1.003%
98	15.091	1161	1164	1165	rBV	657122	846865	9.60%	0.388%
99	16.337	1268	1273	1276	rBV2	1628219	3266899	37.02%	1.498%
100	16.703	1301	1305	1311	rVB	914584	1755028	19.89%	0.805%


Sum of corrected areas: 218067542

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011317\
Data File : BF092242.D
Acq On : 13 Jan 2017 11:52
Operator : UM/SJ
Sample : I1131-03MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-001MS

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

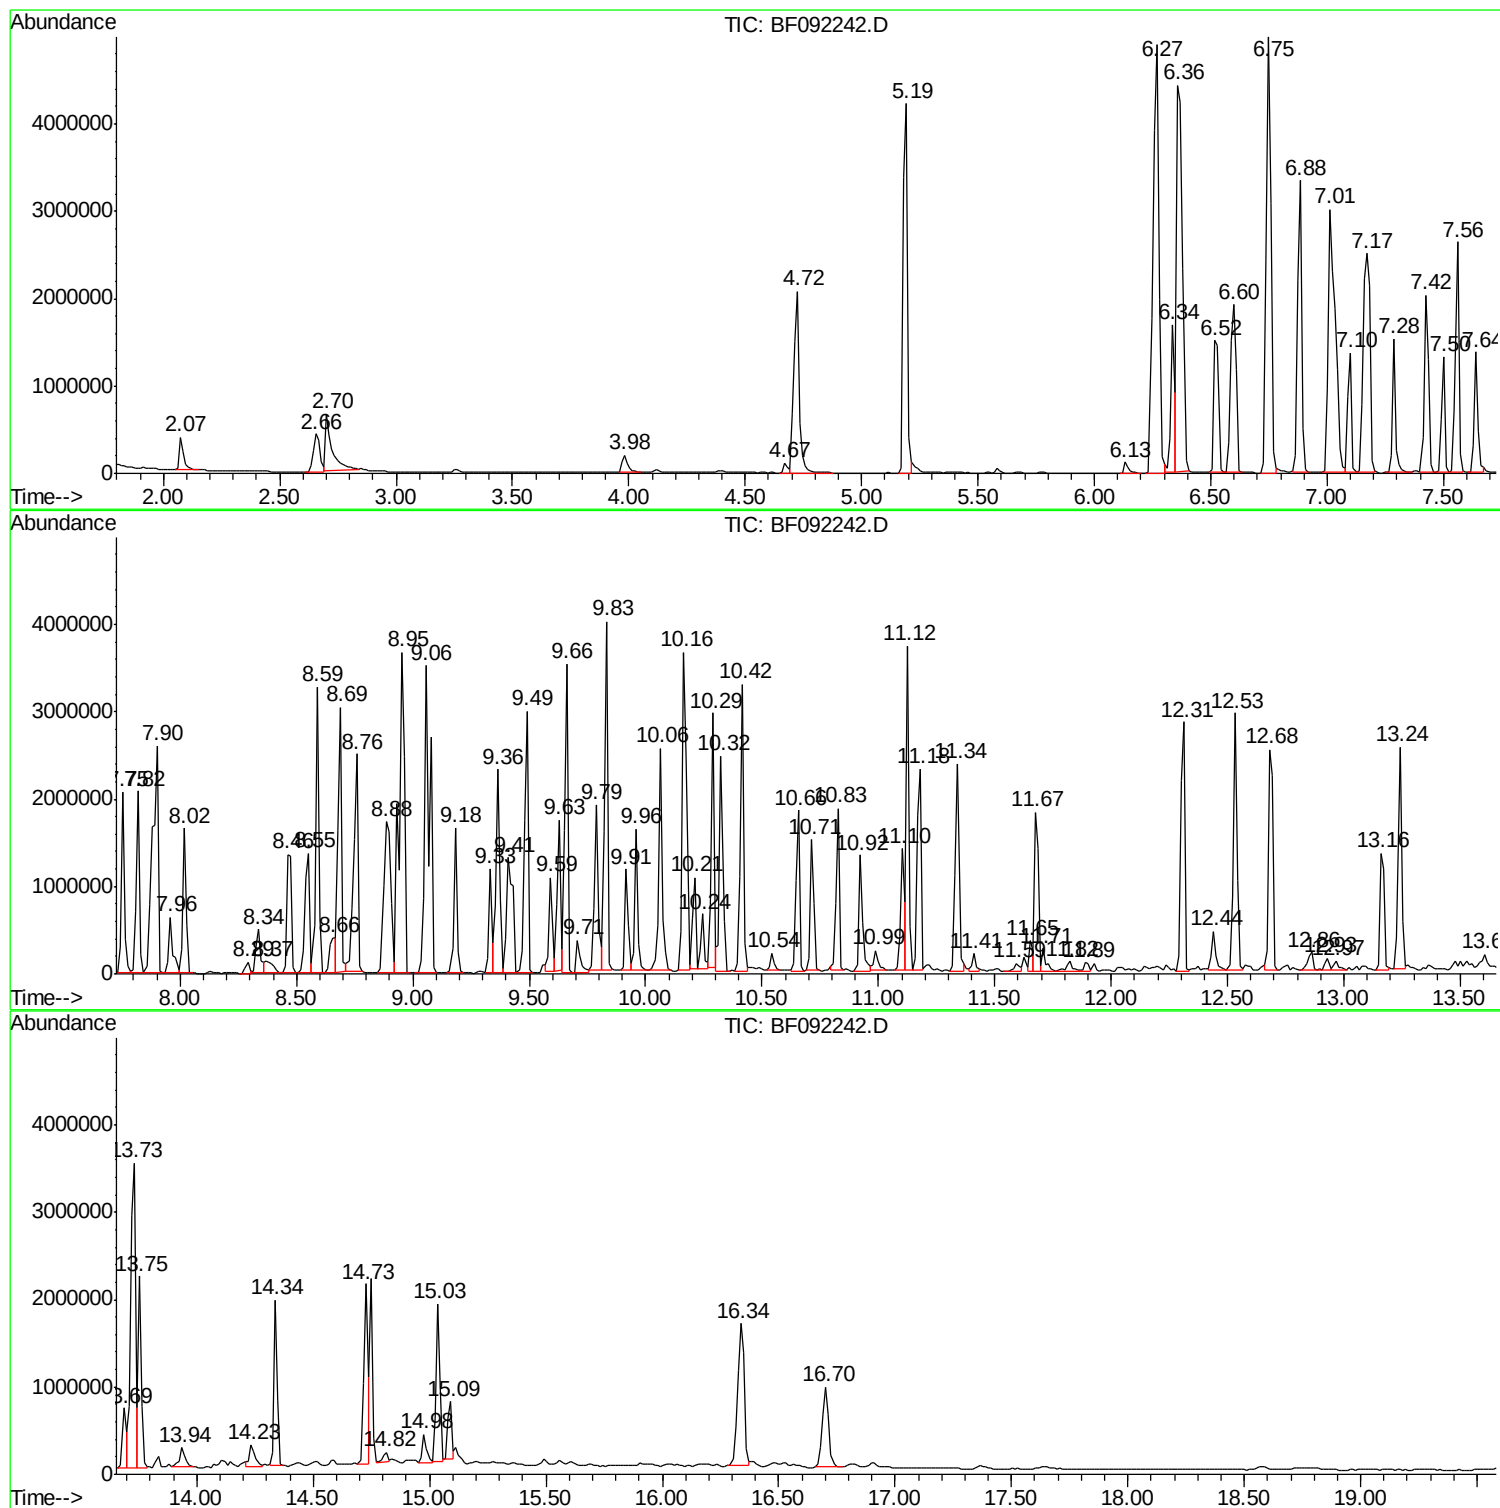

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
Data_File : BF092242.D
Acq_On : 13-Jan-2017 11:522
Operator : UM/SJJ
Sample : I1131-03MSS
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SW-001MS

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
