

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092243.D
 Acq On : 13 Jan 2017 12:21
 Operator : UM/SJ
 Sample : I1131-04MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.084	23	26	33	rBV	402840	595073	6.86%	0.255%
2	2.667	73	77	79	rBV2	509155	1001890	11.55%	0.429%
3	2.701	79	80	93	rVB	776603	1901890	21.92%	0.814%
4	3.981	189	192	202	rBV	162990	338977	3.91%	0.145%
5	4.667	250	252	254	rBV	126061	175433	2.02%	0.075%
6	4.724	254	257	267	rVB	2201623	4036976	46.53%	1.729%
7	5.193	295	298	309	rBV	5365965	6471031	74.59%	2.771%
8	6.130	378	380	388	rVB	180927	205326	2.37%	0.088%
9	6.267	388	392	395	rBV3	4949338	8675352	100.00%	3.715%
10	6.336	395	398	399	rVV	1727694	1971135	22.72%	0.844%
11	6.370	399	401	404	rVB2	4247095	7281330	83.93%	3.118%
12	6.530	412	415	417	rBV	1788584	2283920	26.33%	0.978%
13	6.599	417	421	424	rBV2	1821375	3359926	38.73%	1.439%
14	6.747	431	434	437	rBV2	5320651	8410717	96.95%	3.602%
15	6.884	443	446	449	rVB	3422927	4287456	49.42%	1.836%
16	7.010	454	457	463	rBV3	2871944	7008719	80.79%	3.002%
17	7.102	463	465	467	rVB	1383409	1650910	19.03%	0.707%
18	7.170	467	471	475	rVB2	2800733	5443683	62.75%	2.331%
19	7.285	479	481	488	rBV	1749375	1922713	22.16%	0.823%
20	7.422	491	493	496	rBV	1662817	2566233	29.58%	1.099%
21	7.502	497	500	502	rBV	1657012	1625272	18.73%	0.696%
22	7.559	502	505	507	rVV	3175650	2839073	32.73%	1.216%
23	7.639	509	512	514	rVV	1773669	2148123	24.76%	0.920%
24	7.673	514	515	520	rVB	153238	152581	1.76%	0.065%
25	7.753	520	522	525	rBV	2578911	2442864	28.16%	1.046%
26	7.822	525	528	530	rVV	2441132	2421276	27.91%	1.037%
27	7.902	530	535	537	rVB2	2910791	4680235	53.95%	2.004%
28	7.959	537	540	543	rBV	355893	589847	6.80%	0.253%
29	8.016	543	545	548	rVB	1733418	1892379	21.81%	0.810%
30	8.290	567	569	571	rBV	163824	187106	2.16%	0.080%
31	8.336	571	573	575	rVV	483435	862939	9.95%	0.370%
32	8.393	575	578	582	rVV	134020	418782	4.83%	0.179%
33	8.473	582	585	587	rVV	2213645	2149996	24.78%	0.921%
34	8.553	587	592	593	rVV	1812701	2576720	29.70%	1.103%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092243.D
 Acq On : 13 Jan 2017 12:21
 Operator : UM/SJ
 Sample : I1131-04MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.588	593	595	598 rVB	2939943	2977010	34.32%	1.275%
36	8.656	598	601	602 rBV	507490	865328	9.97%	0.371%
37	8.690	602	604	606 rVV	3251609	3321546	38.29%	1.422%
38	8.759	606	610	612 rVB2	2488043	3264668	37.63%	1.398%
39	8.885	618	621	624 rBV2	2127036	3884043	44.77%	1.663%
40	8.953	624	627	630 rVV	3521179	7020717	80.93%	3.007%
41	9.056	633	636	640 rVB2	3882980	6125876	70.61%	2.623%
42	9.182	642	647	650 rBV	1321181	1471551	16.96%	0.630%
43	9.330	658	660	661 rBV	1150882	1175730	13.55%	0.504%
44	9.365	661	663	665 rVV	2246094	3415612	39.37%	1.463%
45	9.433	665	669	670 rVV2	1813296	2861322	32.98%	1.225%
46	9.490	670	674	676 rVB	3580623	3775382	43.52%	1.617%
47	9.593	681	683	684 rVV	874664	766427	8.83%	0.328%
48	9.628	684	686	687 rVV	1471394	1542662	17.78%	0.661%
49	9.662	687	689	691 rVB	3609155	3402201	39.22%	1.457%
50	9.708	691	693	697 rBV	651655	850274	9.80%	0.364%
51	9.788	697	700	702 rVV2	2037624	2873167	33.12%	1.230%
52	9.833	702	704	706 rVV	4191814	3975373	45.82%	1.702%
53	9.913	709	711	713 rVV	1049457	1350122	15.56%	0.578%
54	9.959	713	715	718 rVV	1602381	1580368	18.22%	0.677%
55	10.062	720	724	731 rVV	2157385	2684430	30.94%	1.150%
56	10.176	731	734	735 rVV2	3382834	4850408	55.91%	2.077%
57	10.211	735	737	738 rVV	1079679	1057767	12.19%	0.453%
58	10.245	738	740	742 rVV	871550	818803	9.44%	0.351%
59	10.291	742	744	746 rVV	2983667	2915726	33.61%	1.249%
60	10.325	746	747	750 rVB	2180636	2066343	23.82%	0.885%
61	10.416	752	755	758 rBV	2925272	2882969	33.23%	1.235%
62	10.542	764	766	769 rVB	143681	153631	1.77%	0.066%
63	10.656	773	776	778 rVB	1875491	1970231	22.71%	0.844%
64	10.713	779	781	784 rBV	1316678	1700498	19.60%	0.728%
65	10.828	788	791	793 rVV	2035475	2021660	23.30%	0.866%
66	10.919	797	799	803 rBV	1376592	1688397	19.46%	0.723%
67	10.988	803	805	809 rVV2	160641	257786	2.97%	0.110%
68	11.125	812	817	819 rVV2	3407059	4455999	51.36%	1.908%
69	11.182	819	822	823 rVV	2699928	3079297	35.49%	1.319%
70	11.342	833	836	838 rBV	2778671	2834110	32.67%	1.214%
71	11.594	853	858	860 rBV	89540	180756	2.08%	0.077%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
 Data File : BF092243.D
 Acq On : 13 Jan 2017 12:21
 Operator : UM/SJ
 Sample : I1131-04MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-001MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.628	860	861	862	rVV	164292	143784	1.66%	0.062%
73	11.674	862	865	867	rVV	1881281	2934194	33.82%	1.257%
74	11.708	867	868	873	rVV2	225161	295301	3.40%	0.126%
75	11.822	873	878	882	rVV4	59774	186307	2.15%	0.080%
76	12.176	907	909	913	rVV3	73194	163277	1.88%	0.070%
77	12.314	918	921	923	rBV	2716639	3514551	40.51%	1.505%
78	12.439	930	932	937	rBV	636705	744106	8.58%	0.319%
79	12.531	937	940	943	rVV	2877961	3305519	38.10%	1.416%
80	12.691	951	954	956	rVV	2852346	3879667	44.72%	1.661%
81	12.851	965	968	971	rVB2	219789	388796	4.48%	0.167%
82	12.931	971	975	976	rBV2	192446	225261	2.60%	0.096%
83	12.965	976	978	982	rVB	123527	175629	2.02%	0.075%
84	13.171	993	996	998	rBV	1667871	2044969	23.57%	0.876%
85	13.239	1000	1002	1004	rBV	2677760	2525437	29.11%	1.082%
86	13.479	1020	1023	1024	rBV	109119	140038	1.61%	0.060%
87	13.605	1030	1034	1039	rVB3	208220	436170	5.03%	0.187%
88	13.685	1039	1041	1042	rBV	750320	887428	10.23%	0.380%
89	13.731	1042	1045	1046	rVV2	3789061	5637385	64.98%	2.414%
90	13.754	1046	1047	1050	rVV	2230168	2314474	26.68%	0.991%
91	13.937	1059	1063	1066	rVB4	267961	424415	4.89%	0.182%
92	14.234	1088	1089	1093	rVB	271025	357774	4.12%	0.153%
93	14.337	1096	1098	1101	rVB	1970198	2193235	25.28%	0.939%
94	14.748	1129	1134	1137	rBV	2180963	4820663	55.57%	2.064%
95	14.817	1137	1140	1141	rBV3	106465	147191	1.70%	0.063%
96	14.977	1152	1154	1157	rBV	244324	342991	3.95%	0.147%
97	15.034	1157	1159	1162	rBV	1676833	2412429	27.81%	1.033%
98	15.091	1162	1164	1165	rBV	664904	814970	9.39%	0.349%
99	16.348	1269	1274	1277	rBV2	1601936	3502376	40.37%	1.500%
100	16.703	1301	1305	1311	rBV	985506	1851908	21.35%	0.793%


Sum of corrected areas: 233504318

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
Data File : BF092243.D
Acq On : 13 Jan 2017 12:21
Operator : UM/SJ
Sample : I1131-04MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-001MSD

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

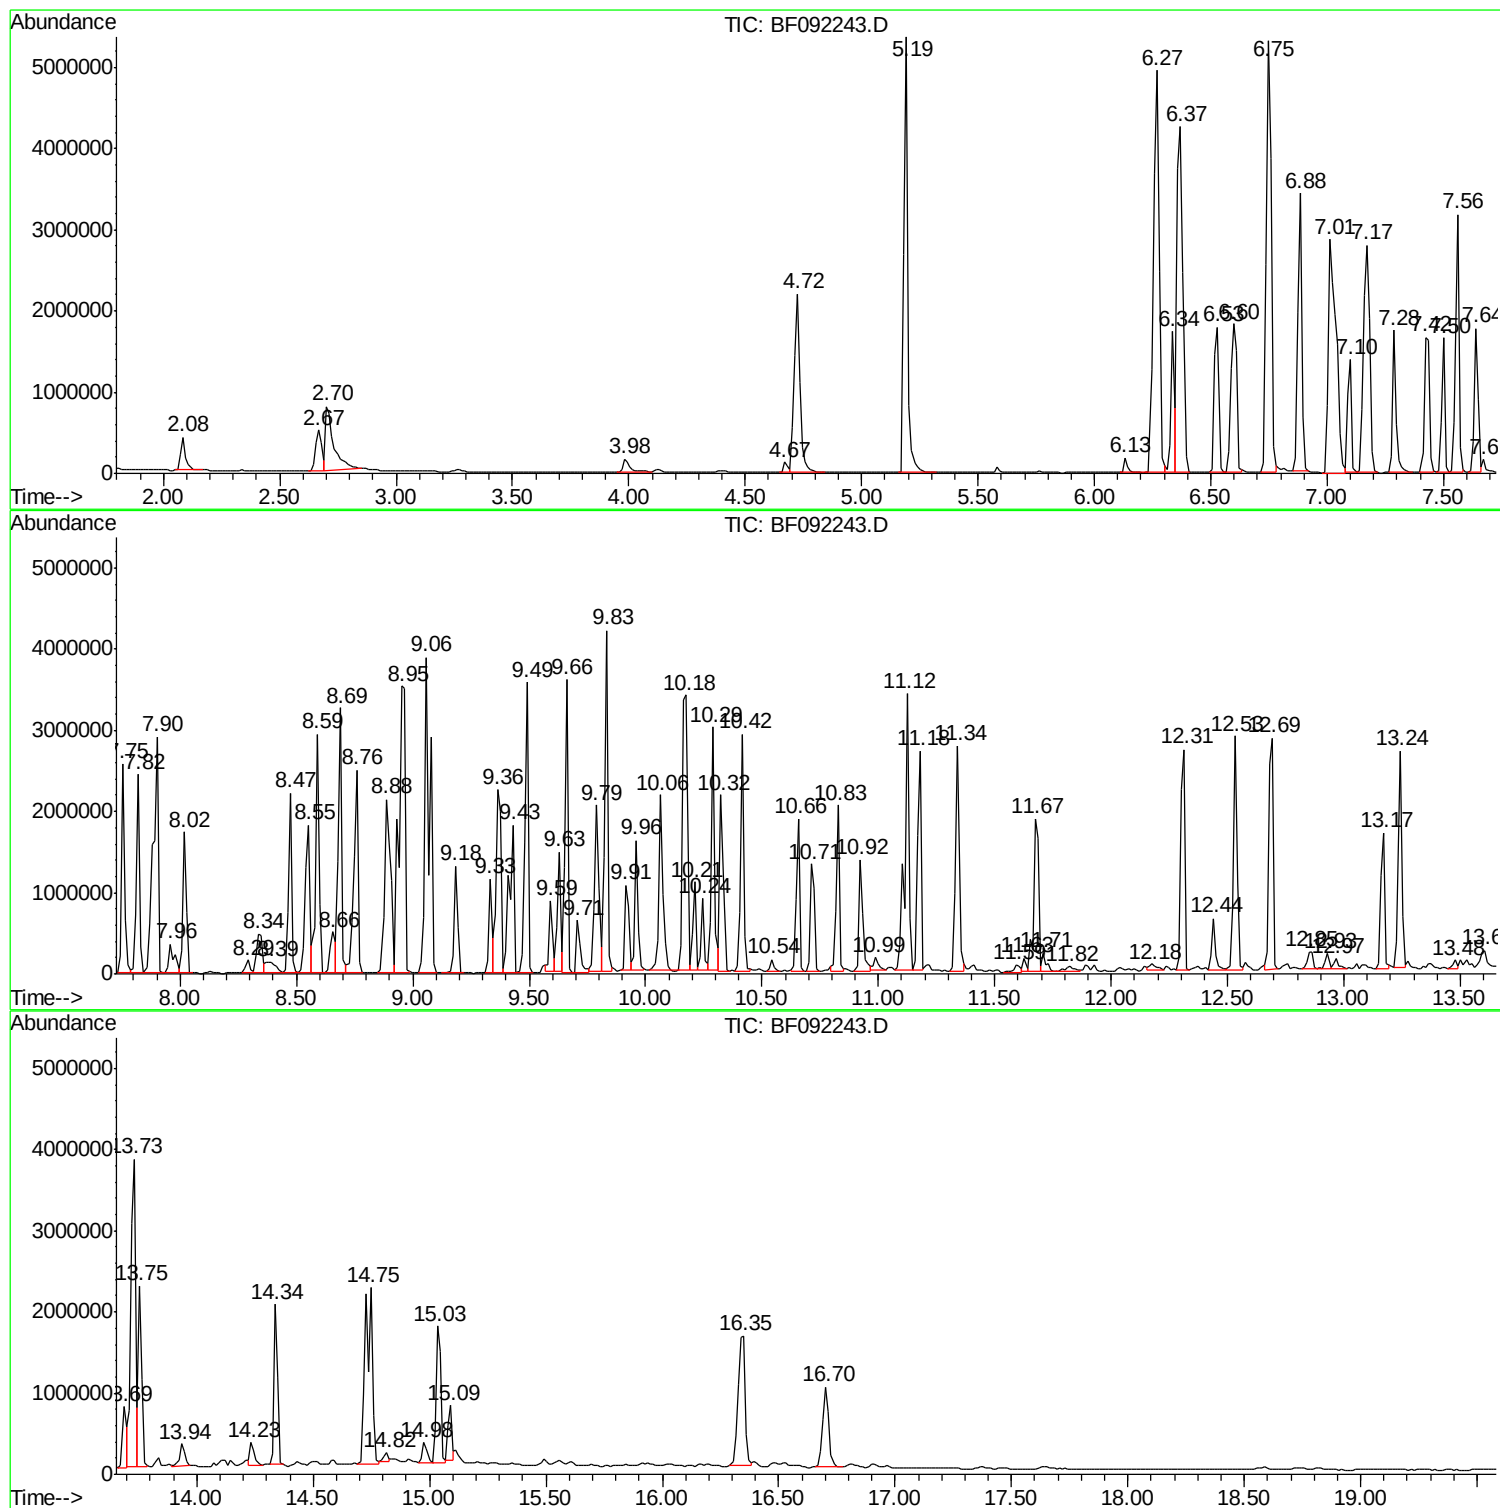

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF011317\
Data_File : BF092243.D
Acq_On : 13-Jan-2017 12:211
Operator : UM/SJJ
Sample : I1131-04MSDD
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SW-001MSD

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
