


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011317\
 Data File : BF092249.D
 Acq On : 13 Jan 2017 17:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

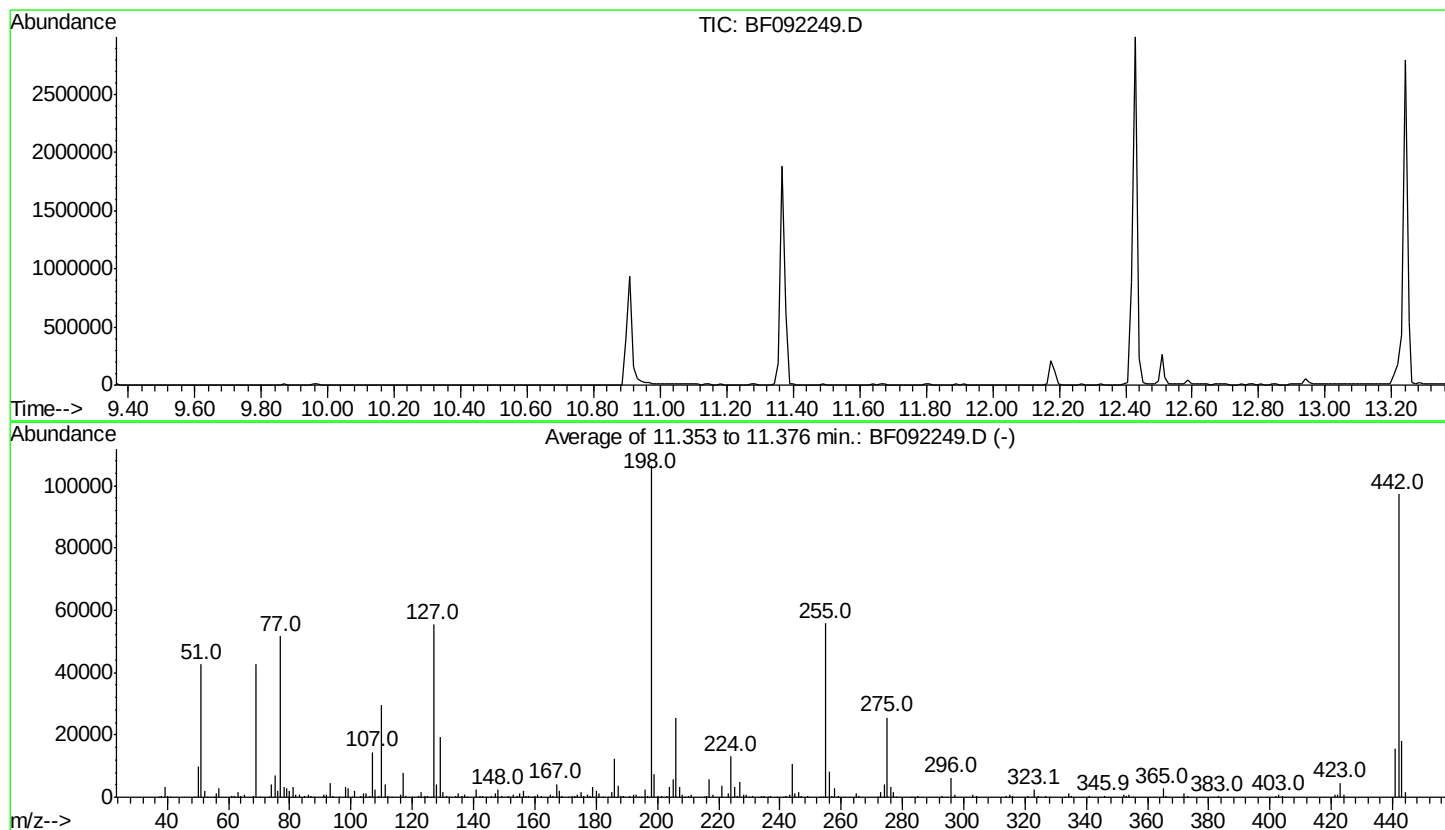

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	42690	PASS
68	69	0.00	2	1.2	526	PASS
69	198	0.00	100	40.2	42808	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	52.1	55397	PASS
197	198	0.00	2	0.5	564	PASS
198	198	100	100	100.0	106418	PASS
199	198	5	9	6.8	7241	PASS
275	198	10	60	24.0	25570	PASS
365	198	1	100	2.7	2829	PASS
441	442	0.01	24	16.0	15599	PASS
442	198	50	100	91.5	97333	PASS
443	442	15	24	18.7	18170	PASS