

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011320\
 Data File : BF118540.D
 Acq On : 13 Jan 2020 19:41
 Operator : JU
 Sample : L1068-02 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SIDE-WALK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.363	383	387	396	rBV	116256	152729	19.20%	1.630%
2	4.998	491	495	510	rBV	154846	163897	20.60%	1.750%
3	5.440	567	570	583	rBV	79075	93147	11.71%	0.994%
4	6.457	741	743	755	rBV	122385	165783	20.84%	1.770%
5	6.592	763	766	775	rVB	157967	158016	19.86%	1.687%
6	6.816	800	804	814	rBV	457323	401591	50.48%	4.287%
7	6.969	827	830	839	rBV	183319	178789	22.47%	1.909%
8	7.381	897	900	917	rBV	113764	120603	15.16%	1.287%
9	8.098	1019	1022	1032	rBV	582832	485758	61.06%	5.185%
10	9.175	1202	1205	1217	rBV	434864	365443	45.93%	3.901%
11	9.292	1222	1225	1228	rBV	11709	9987	1.26%	0.107%
12	9.575	1271	1273	1277	rBV	11763	10481	1.32%	0.112%
13	9.863	1318	1322	1331	rBV	865666	773489	97.22%	8.257%
14	10.657	1454	1457	1464	rBV	64579	64047	8.05%	0.684%
15	11.080	1525	1529	1536	rVB	25001	26071	3.28%	0.278%
16	11.351	1572	1575	1579	rBV	821481	719521	90.44%	7.681%
17	11.516	1600	1603	1607	rBV2	19937	19443	2.44%	0.208%
18	11.933	1670	1674	1678	rVB	25006	24545	3.09%	0.262%
19	12.327	1736	1741	1744	rBV2	21445	22146	2.78%	0.236%
20	12.398	1749	1753	1757	rBV6	18322	27913	3.51%	0.298%
21	12.710	1803	1806	1808	rBV3	11127	11678	1.47%	0.125%
22	12.804	1819	1822	1828	rVV4	13468	17565	2.21%	0.188%
23	12.857	1828	1831	1834	rVB5	9455	11161	1.40%	0.119%
24	12.939	1841	1845	1848	rBV	521339	440745	55.40%	4.705%
25	13.116	1872	1875	1879	rBV5	11673	16199	2.04%	0.173%
26	13.239	1893	1896	1899	rBV2	33474	31142	3.91%	0.332%
27	13.327	1908	1911	1914	rBV	88070	89040	11.19%	0.950%
28	13.363	1914	1917	1920	rVV2	42549	40101	5.04%	0.428%
29	13.421	1924	1927	1930	rVV3	25746	26024	3.27%	0.278%
30	13.533	1944	1946	1947	rBV2	11400	10959	1.38%	0.117%
31	13.580	1952	1954	1956	rBV3	20893	20661	2.60%	0.221%
32	13.639	1962	1964	1970	rVB2	69662	76059	9.56%	0.812%
33	13.704	1972	1975	1979	rBV	244945	210632	26.48%	2.248%
34	13.739	1979	1981	1983	rBV	129395	97616	12.27%	1.042%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011320\
 Data File : BF118540.D
 Acq On : 13 Jan 2020 19:41
 Operator : JU
 Sample : L1068-02 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SIDE-WALK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.763	1983	1985	1988	rVB	79264	61087	7.68%	0.652%
36	13.821	1991	1995	1999	rBV	173543	289807	36.43%	3.094%
37	13.857	1999	2001	2004	rVV	181429	175278	22.03%	1.871%
38	13.886	2004	2006	2009	rVB2	86463	73779	9.27%	0.788%
39	13.921	2009	2012	2014	rBV2	50274	53371	6.71%	0.570%
40	13.951	2014	2017	2018	rBV	42333	41565	5.22%	0.444%
41	14.004	2023	2026	2033	rVB	785508	795566	100.00%	8.493%
42	14.057	2033	2035	2037	rBV3	24343	19361	2.43%	0.207%
43	14.086	2037	2040	2046	rBV	272126	264336	33.23%	2.822%
44	14.174	2049	2055	2057	rVV	107831	188973	23.75%	2.017%
45	14.198	2057	2059	2061	rVB	95497	67922	8.54%	0.725%
46	14.221	2061	2063	2064	rBV	55622	41044	5.16%	0.438%
47	14.239	2064	2066	2069	rVB	149443	123882	15.57%	1.322%
48	14.292	2071	2075	2077	rBV	170799	167755	21.09%	1.791%
49	14.321	2077	2080	2083	rVB	80519	86830	10.91%	0.927%
50	14.357	2083	2086	2088	rBV2	115630	144980	18.22%	1.548%
51	14.380	2088	2090	2094	rVB3	124470	104823	13.18%	1.119%
52	14.439	2098	2100	2102	rBV2	46651	42458	5.34%	0.453%
53	14.510	2109	2112	2115	rBV2	101421	122016	15.34%	1.302%
54	14.615	2128	2130	2133	rVB2	83016	57459	7.22%	0.613%
55	14.727	2146	2149	2153	rBV2	162731	223739	28.12%	2.388%
56	15.098	2208	2212	2217	rVB4	127000	171209	21.52%	1.828%
57	15.357	2254	2256	2260	rVB	90261	98807	12.42%	1.055%
58	15.486	2273	2278	2282	rBV	604203	757621	95.23%	8.087%
59	15.910	2346	2350	2352	rBV2	77799	111187	13.98%	1.187%


Sum of corrected areas: 9367836

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011320\
Data File : BF118540.D
Acq On : 13 Jan 2020 19:41
Operator : JU
Sample : L1068-02 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SIDE-WALK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

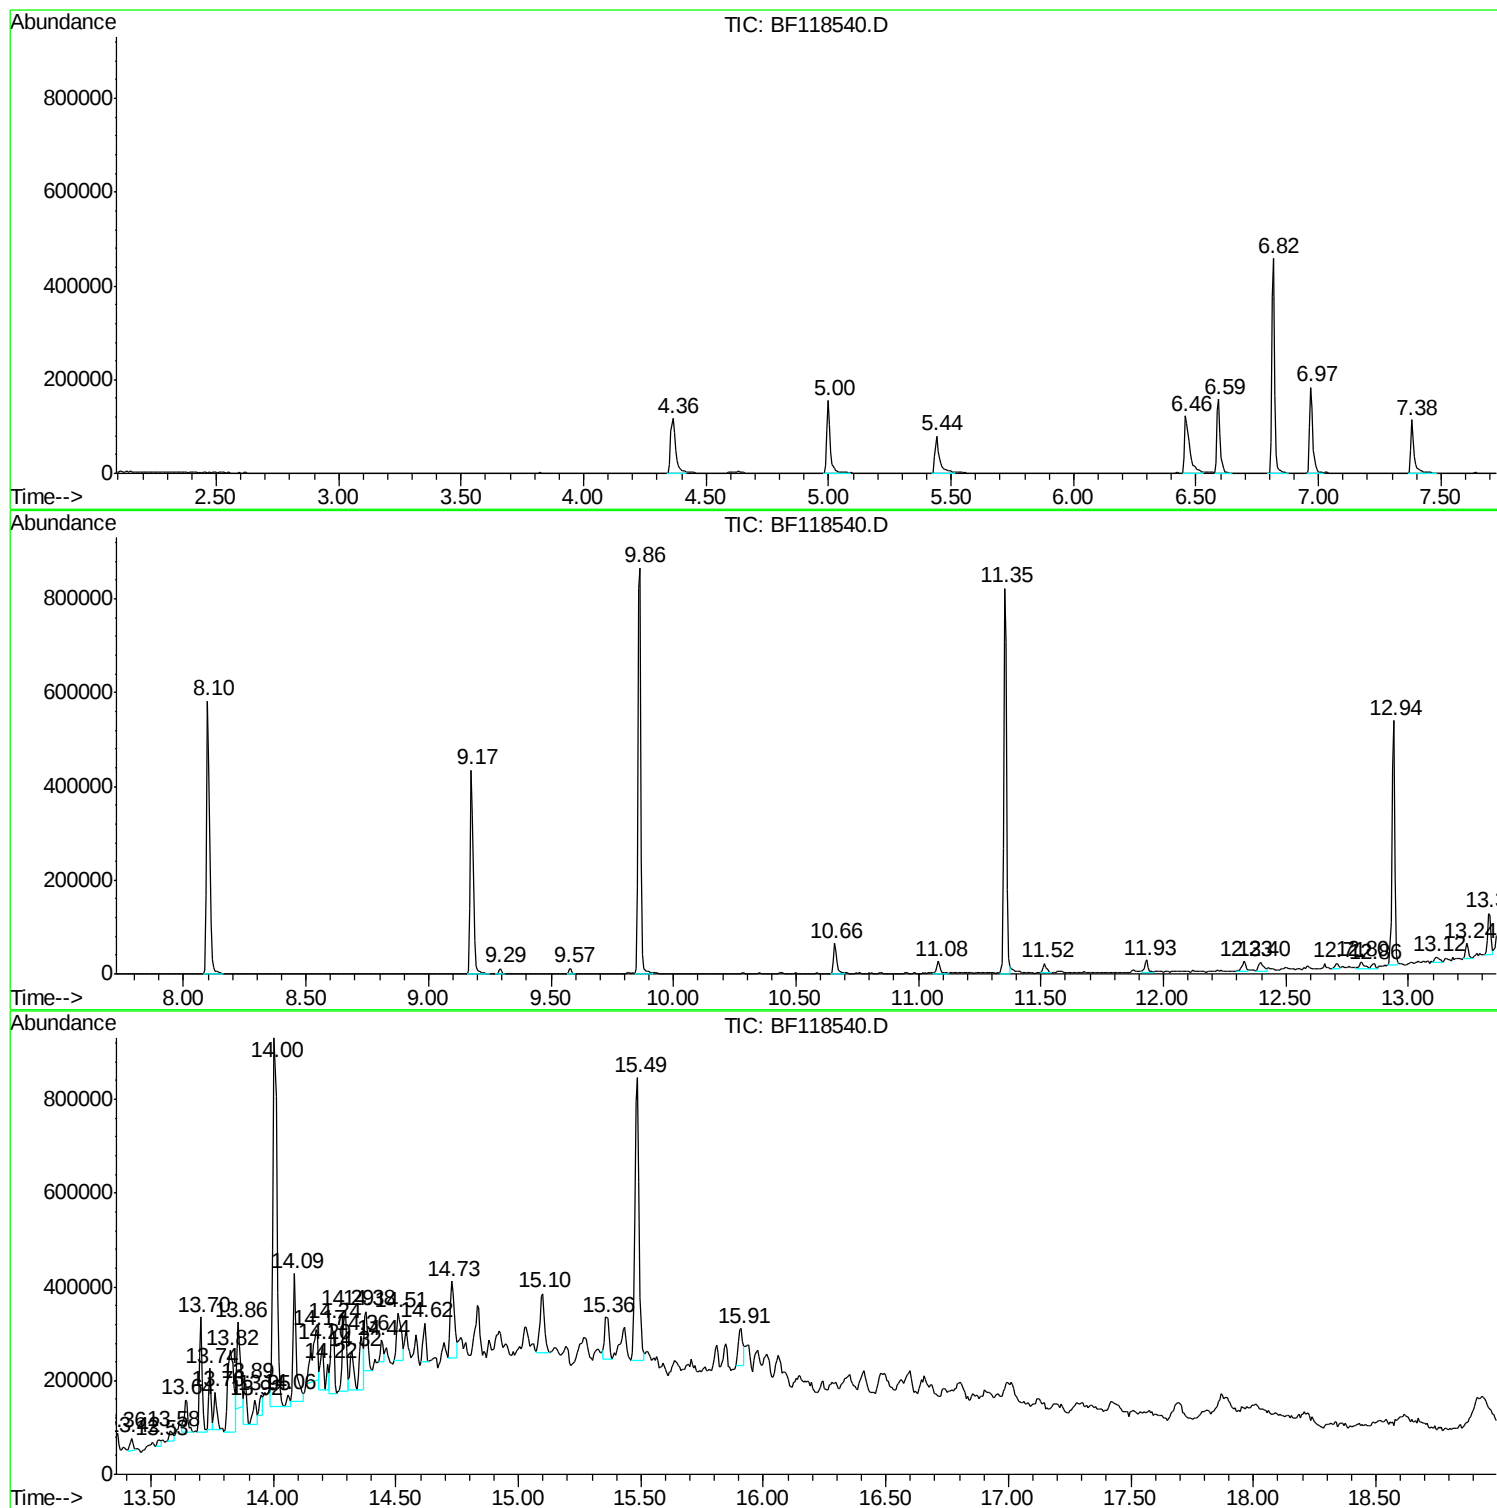

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011320\\
Data_File : BF118540.D
Acq_On : 13-Jan-2020 19:411
Operator : JUJ
Sample : L1068-02_5XX
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SIDE-WALK

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
