


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011320\
 Data File : BF118531.D
 Acq On : 13 Jan 2020 13:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 11:02:16 2020

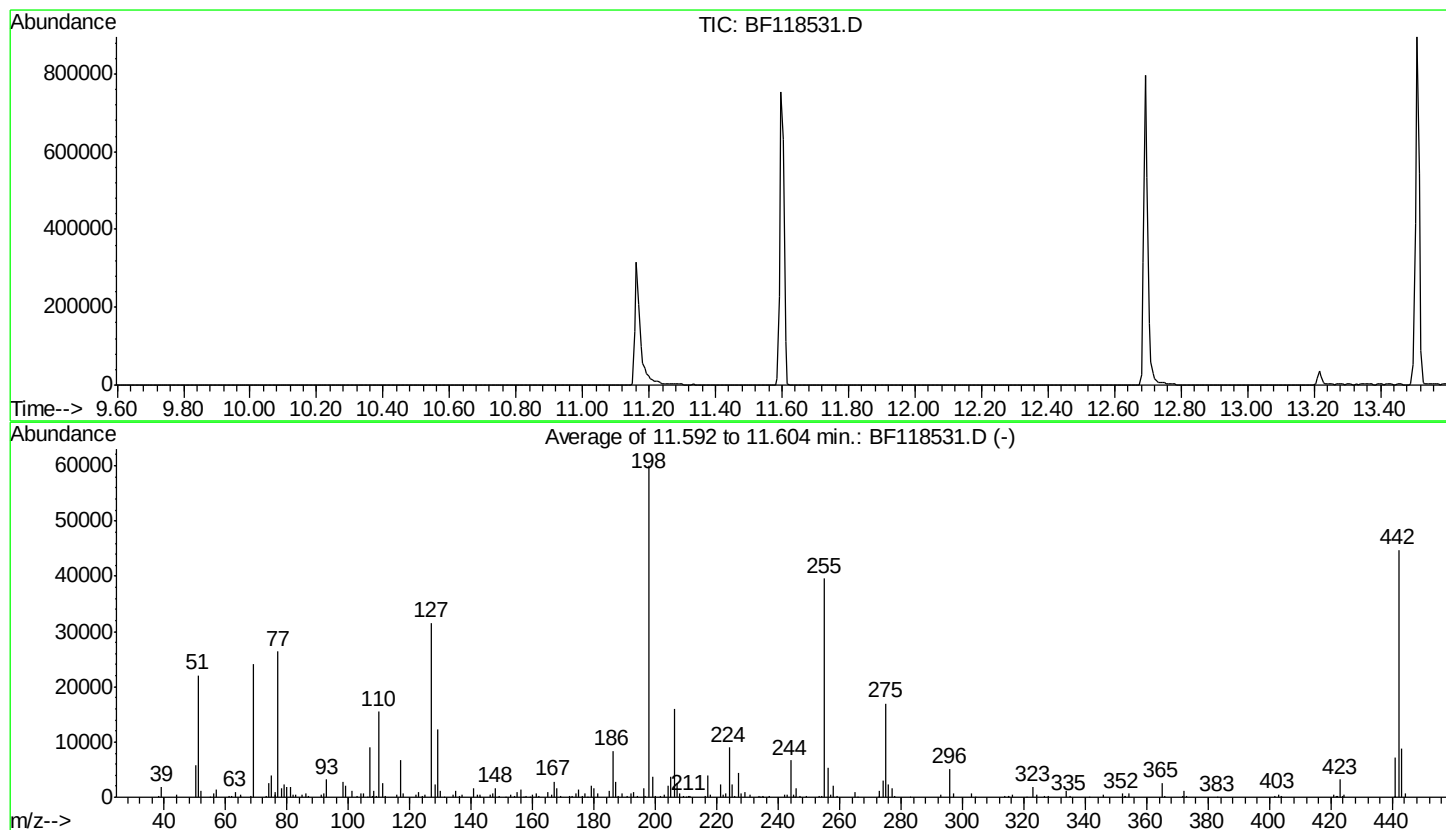

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	22023	PASS
68	69	0.00	2	1.3	320	PASS
69	198	0.00	100	40.0	24016	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	31594	PASS
197	198	0.00	2	0.4	236	PASS
198	198	100	100	100.0	60024	PASS
199	198	5	9	6.3	3791	PASS
275	198	10	60	28.3	17006	PASS
365	198	1	100	4.4	2614	PASS
441	198	0.01	100	11.8	7100	PASS
442	198	50	100	74.6	44794	PASS
443	442	15	24	19.8	8891	PASS