

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011323\
 Data File : BF132069.D
 Acq On : 13 Jan 2023 20:32
 Operator : CG\JU
 Sample : 01140-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-D

Quant Time: Jan 16 01:18:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 23:59:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.769	152	80762	20.000	ng	0.00
21) Naphthalene-d8	8.063	136	299659	20.000	ng	0.00
39) Acenaphthene-d10	9.822	164	170619	20.000	ng	0.00
64) Phenanthrene-d10	11.310	188	315335	20.000	ng	0.00
76) Chrysene-d12	13.957	240	153577	20.000	ng	# 0.00
86) Perylene-d12	15.421	264	180877	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.392	112	415091	84.691	ng	0.01
7) Phenol-d6	6.422	99	543406	83.621	ng	0.00
23) Nitrobenzene-d5	7.345	82	380676	52.724	ng	0.00
42) 2,4,6-Tribromophenol	10.616	330	134633	68.629	ng	0.00
45) 2-Fluorobiphenyl	9.139	172	577206	45.669	ng	0.00
79) Terphenyl-d14	12.904	244	536244	50.046	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.345	70	52690	11.208	ng	# 74
25) Isophorone	7.345	82	377079	27.956	ng	# 69
51) 2,6-Dinitrotoluene	9.822	165	22244	7.952	ng	# 22
57) 2,4-Dinitrotoluene	9.822	165	22244	5.948	ng	# 13
63) Azobenzene	10.539	77	89623	6.460	ng	# 1
67) 4-Bromophenyl-phenylether	10.616	248	9149	2.319	ng	# 1
92) Benzo(g,h,i)perylene	17.321	276	54	3.530	ng	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011323\
Data File : BF132069.D
Acq On : 13 Jan 2023 20:32
Operator : CG\JU
Sample : 01140-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-D

Quant Time: Jan 16 01:18:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 23:59:08 2023
Response via : Initial Calibration




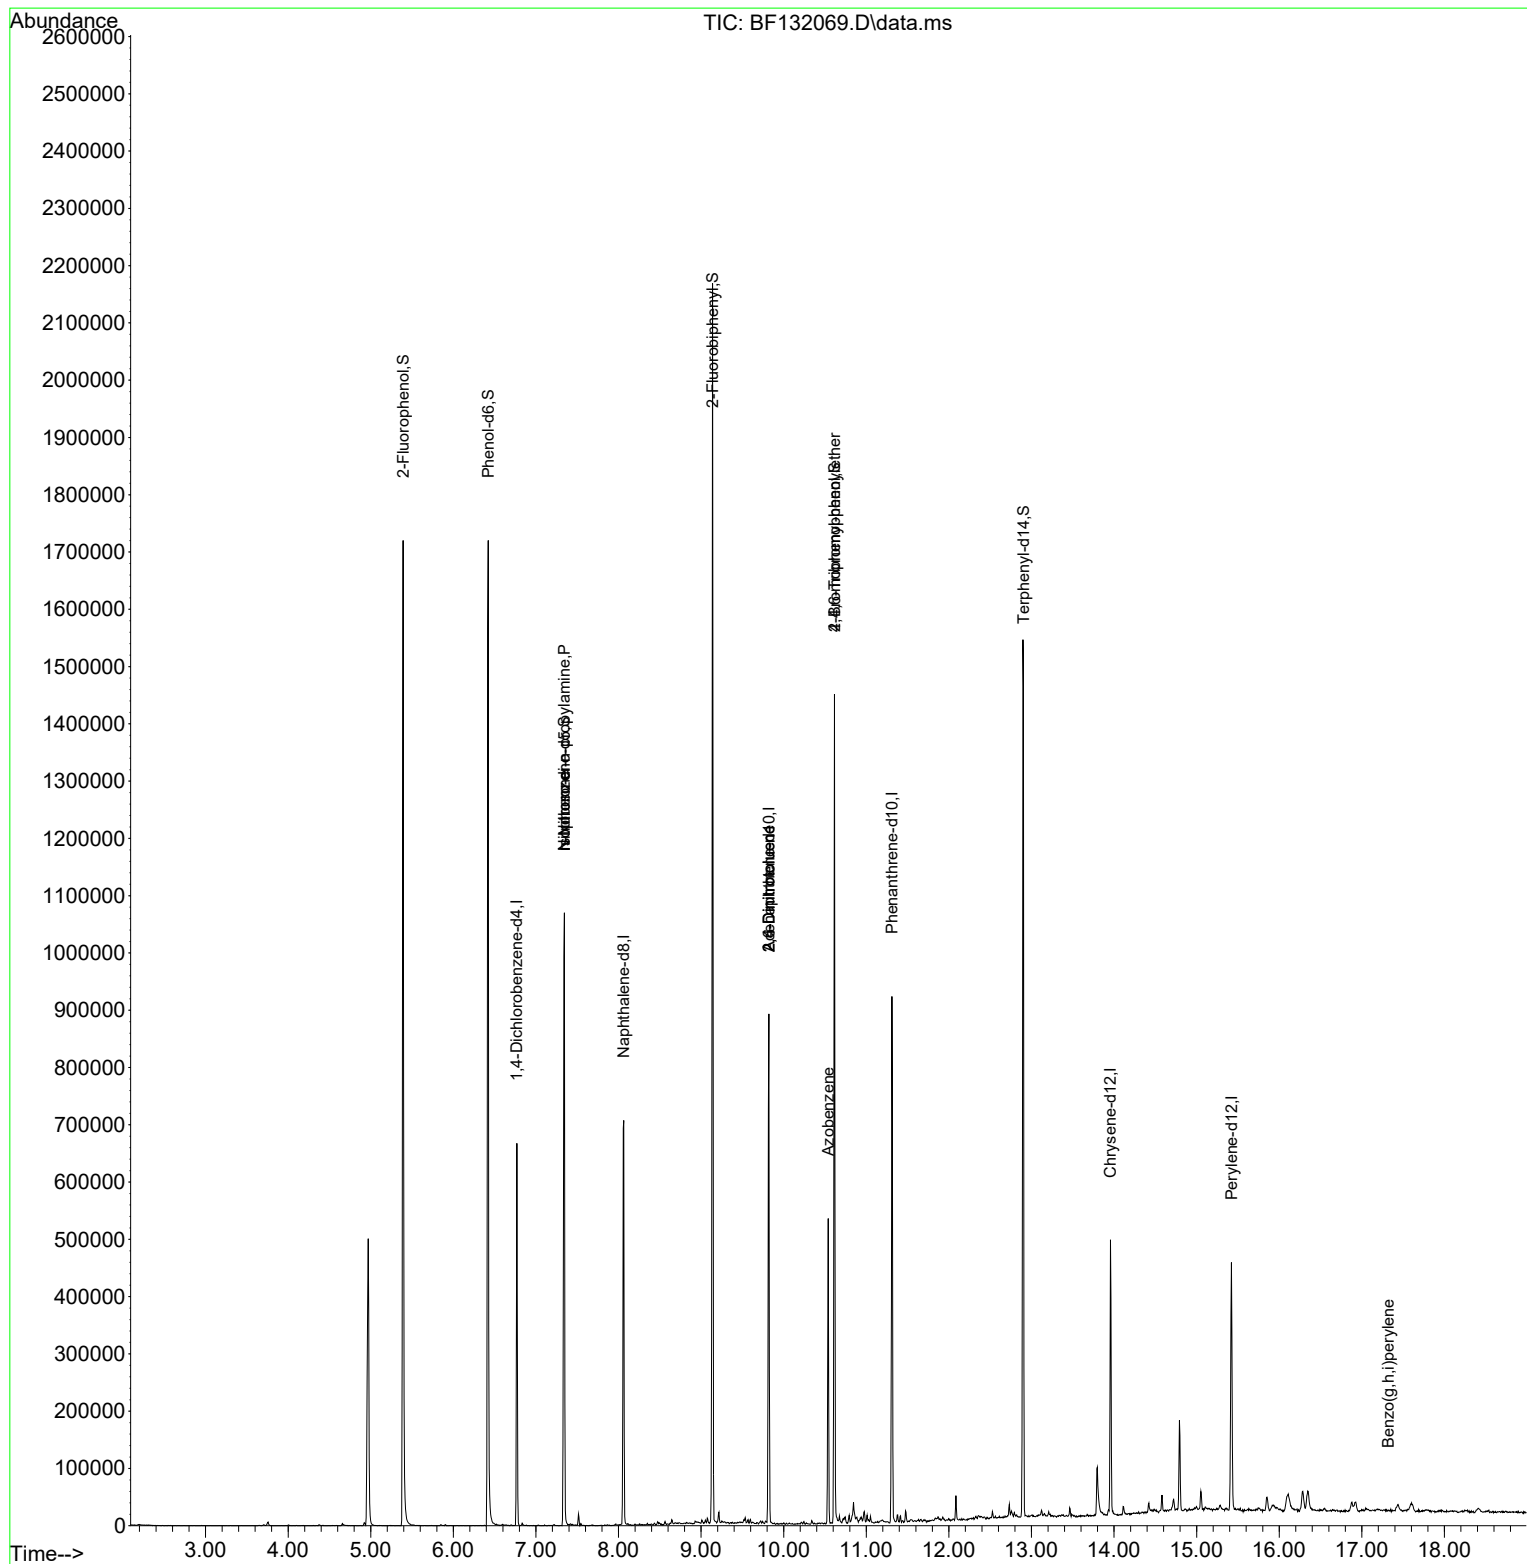


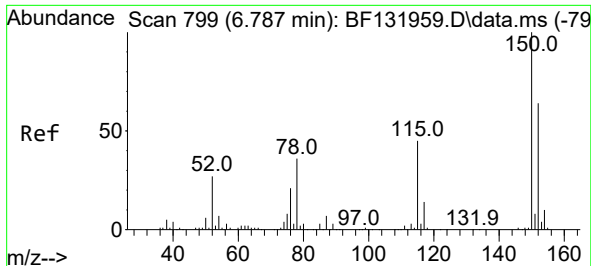

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.769 min Scan# 799
Delta R.T. -0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion:152 Resp: 80762
Ion Ratio Lower Upper
152 100
150 151.2 124.6 186.8
115 69.4 55.6 83.4

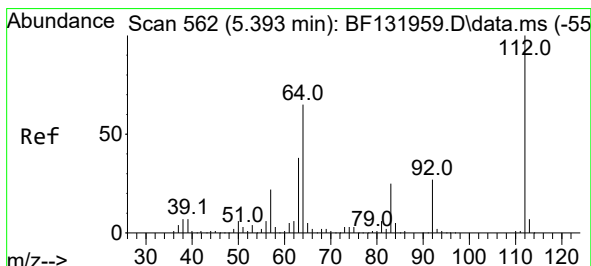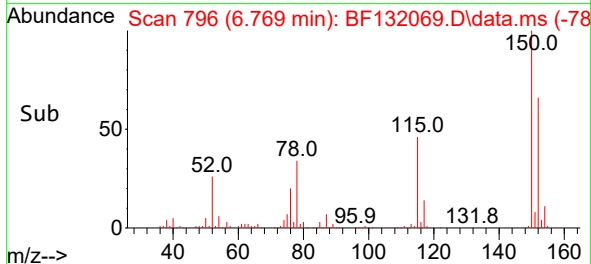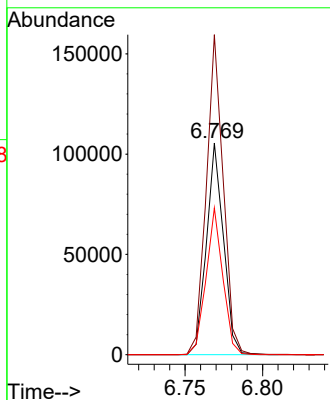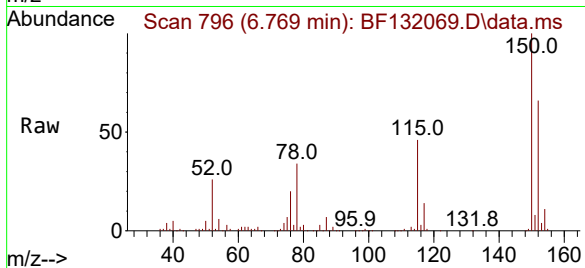

#5
2-Fluorophenol
Concen: 84.691 ng
RT: 5.392 min Scan# 562
Delta R.T. 0.012 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion:112 Resp: 415091
Ion Ratio Lower Upper
112 100
64 64.0 51.9 77.9
63 35.7 30.2 45.2


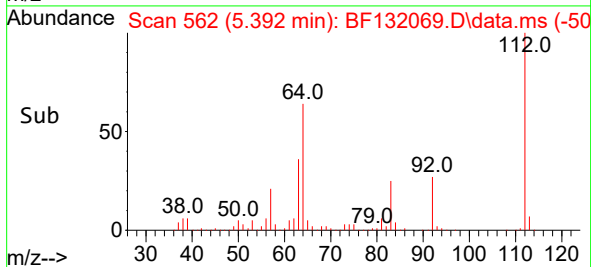
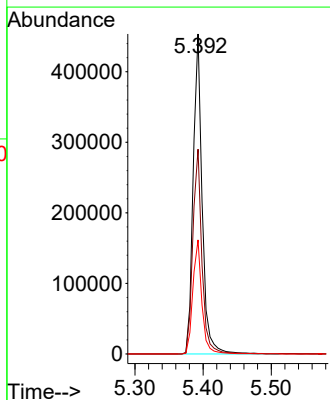
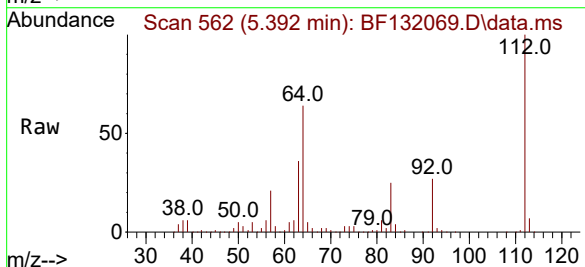


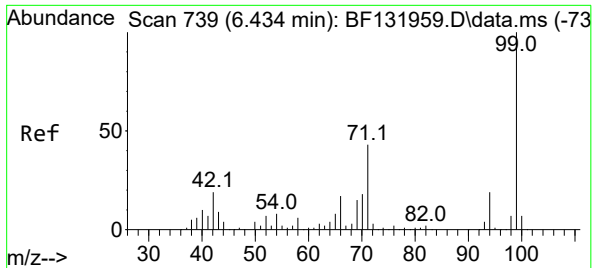

#7
Phenol-d6
Concen: 83.621 ng
RT: 6.422 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion: 99 Resp: 543406
Ion Ratio Lower Upper
99 100
42 18.9 15.4 23.2
71 42.7 34.6 51.8

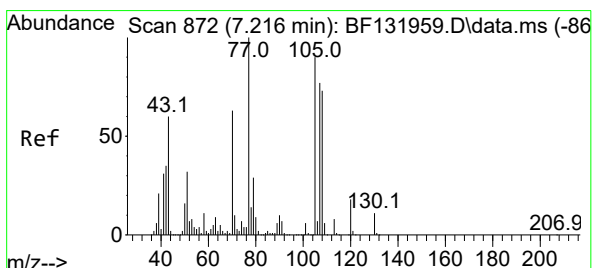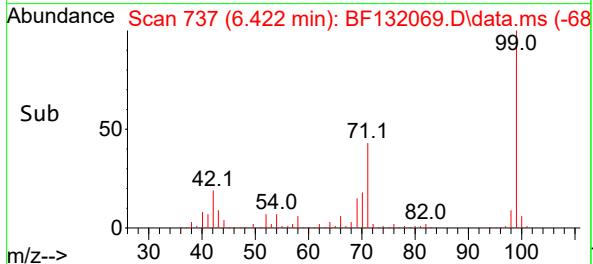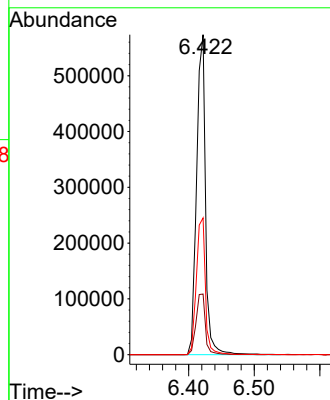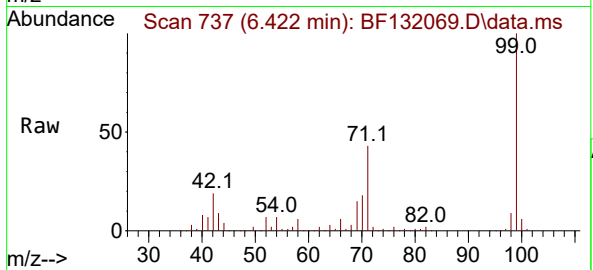

#19
n-Nitroso-di-n-propylamine
Concen: 11.208 ng
RT: 7.345 min Scan# 894
Delta R.T. 0.147 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion: 70 Resp: 52690
Ion Ratio Lower Upper
70 100
42 38.7 44.3 66.5#
101 0.0 7.5 11.3#
130 1.8 14.3 21.5#

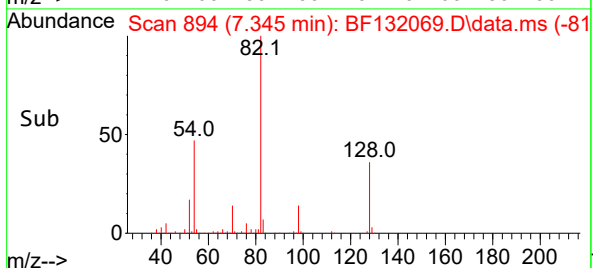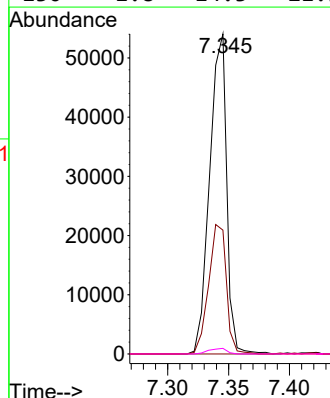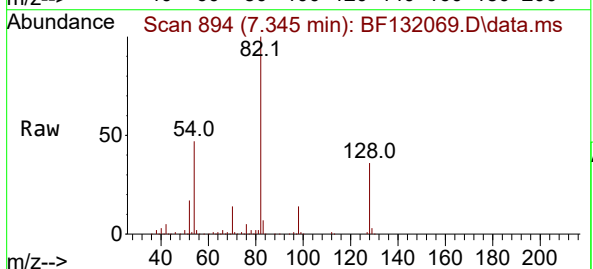

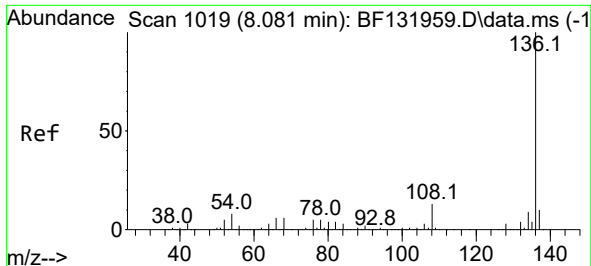

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.063 min Scan# 1016

Delta R.T. -0.000 min

Lab File: BF132069.D

Acq: 13 Jan 2023 20:32

Instrument :

BNA_F

ClientSampleId :

TP-D

Tgt Ion:136 Resp: 299659





Ion Ratio Lower Upper

136 100

137 10.5 8.2 12.2

54 7.3 6.6 9.8

68 5.5 4.5 6.7

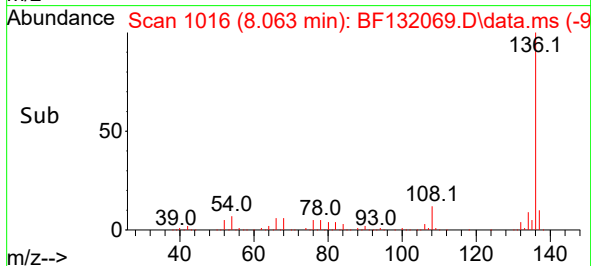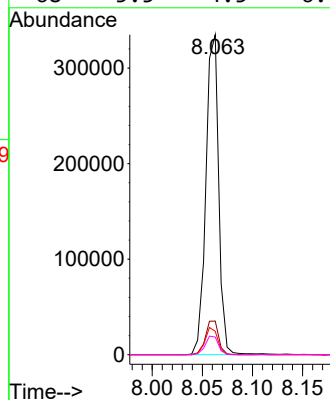

#23

Nitrobenzene-d5

Concen: 52.724 ng

RT: 7.345 min Scan# 894

Delta R.T. -0.006 min

Lab File: BF132069.D

Acq: 13 Jan 2023 20:32




Tgt Ion: 82 Resp: 380676


Ion Ratio Lower Upper

82 100

128 35.5 28.7 43.1

54 46.9 38.1 57.1



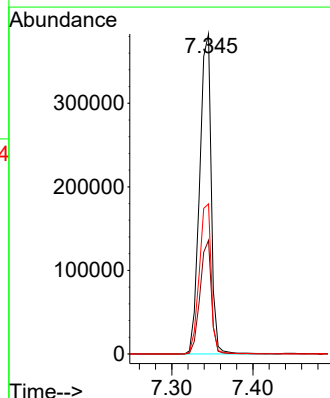
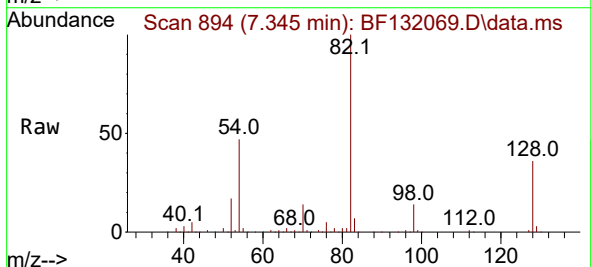


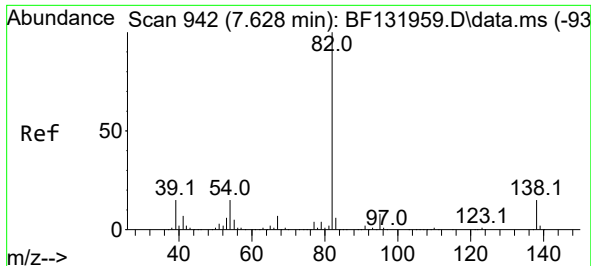

#25
Isophorone
Concen: 27.956 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.265 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion: 82 Resp: 377079
Ion Ratio Lower Upper
82 100
95 0.0 6.5 9.7#
138 0.0 11.9 17.9#

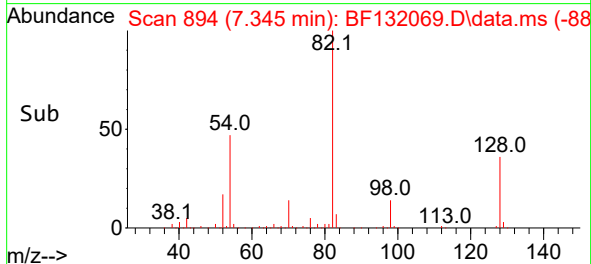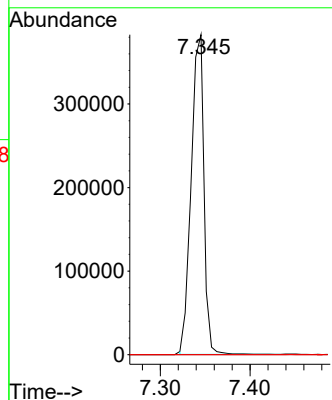

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.822 min Scan# 1315
Delta R.T. -0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion: 164 Resp: 170619
Ion Ratio Lower Upper
164 100
162 102.1 79.4 119.0
160 44.4 33.9 50.9


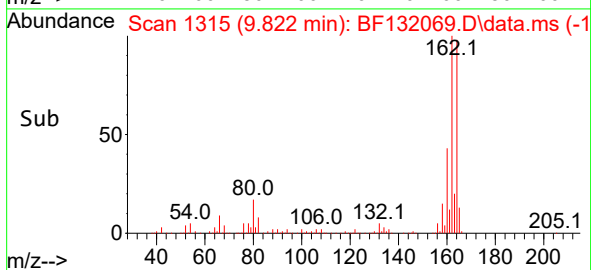
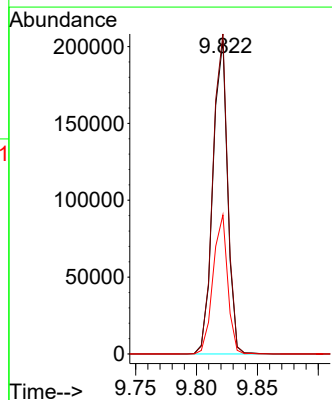
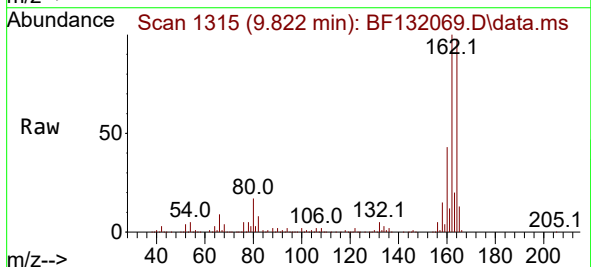


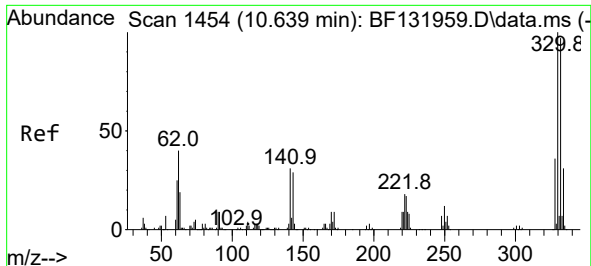

#42
2,4,6-Tribromophenol
Concen: 68.629 ng
RT: 10.616 min Scan# 1454
Delta R.T. -0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion:330 Resp: 134633
Ion Ratio Lower Upper
330 100
332 95.8 76.9 115.3
141 40.1 31.3 46.9

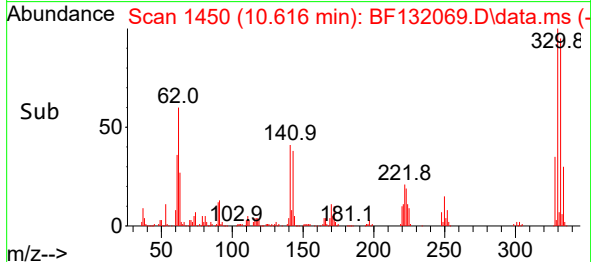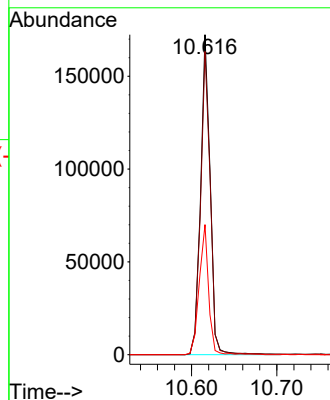

#45
2-Fluorobiphenyl
Concen: 45.669 ng
RT: 9.139 min Scan# 1199
Delta R.T. -0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion:172 Resp: 577206
Ion Ratio Lower Upper
172 100
171 35.1 28.0 42.0
170 23.3 18.9 28.3


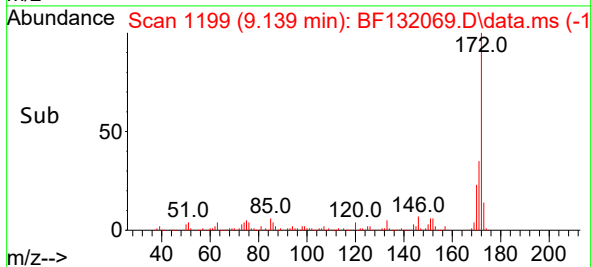
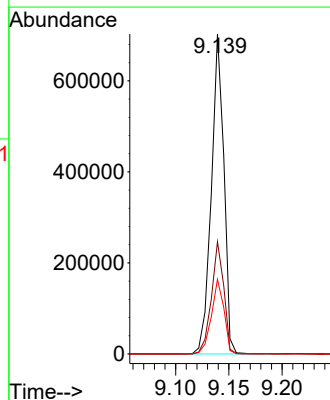
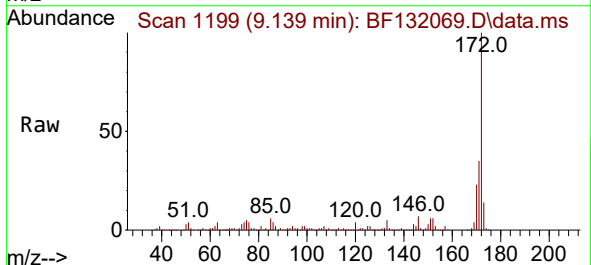


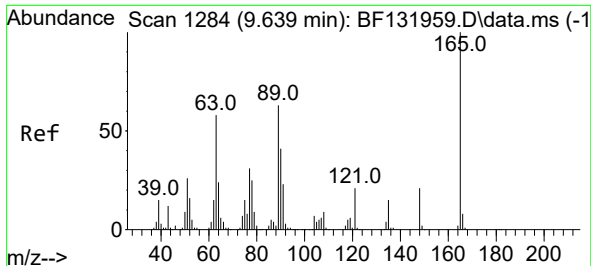

#51
2,6-Dinitrotoluene
Concen: 7.952 ng
RT: 9.822 min Scan# 1315
Delta R.T. 0.200 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion:165 Resp: 22244
Ion Ratio Lower Upper
165 100
63 1.5 47.4 71.0#
89 1.9 50.2 75.2#

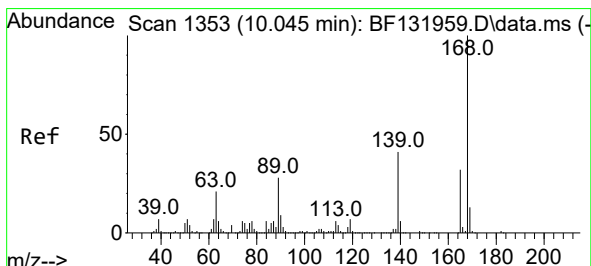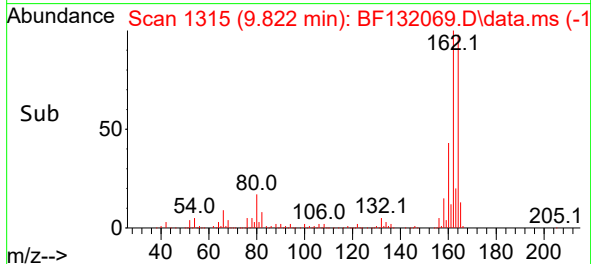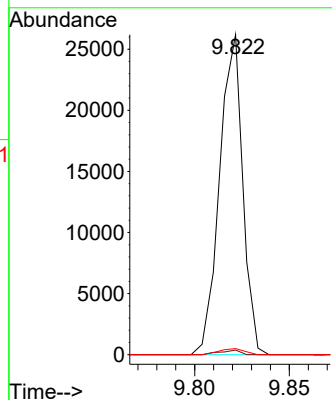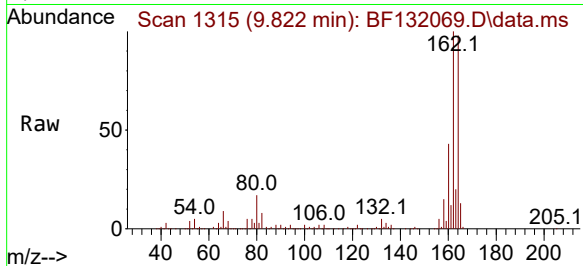

#57
2,4-Dinitrotoluene
Concen: 5.948 ng
RT: 9.822 min Scan# 1315
Delta R.T. -0.206 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion:165 Resp: 22244
Ion Ratio Lower Upper
165 100
63 1.5 53.2 79.8#
89 1.9 71.2 106.8#
182 0.0 2.0 3.0#

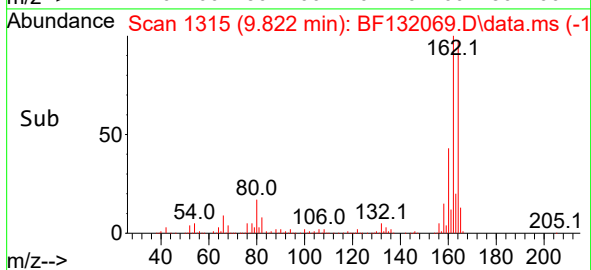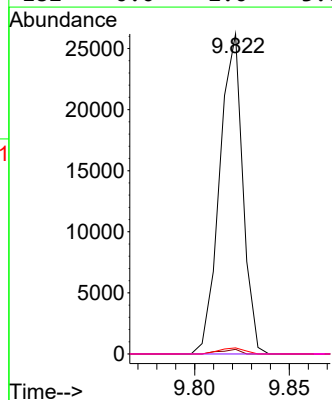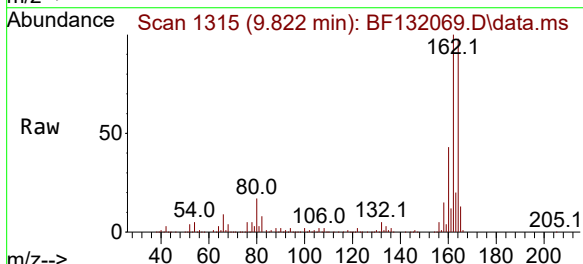

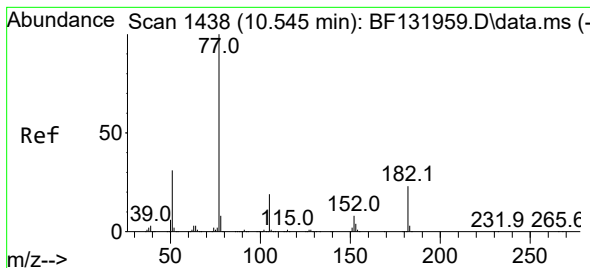

#63

Azobenzene

Concen: 6.460 ng

RT: 10.539 min Scan# 1437

Delta R.T. 0.012 min

Lab File: BF132069.D

Acq: 13 Jan 2023 20:32

Instrument :

BNA_F

ClientSampleId :

TP-D

Tgt Ion: 77 Resp: 89623





Ion Ratio Lower Upper

77 100

182 72.1 2.9 42.9#

105 138.2 0.0 39.3#

51 37.9 10.7 50.7

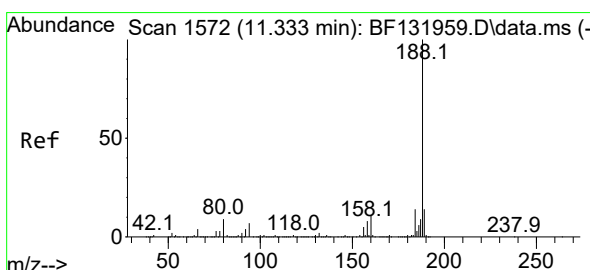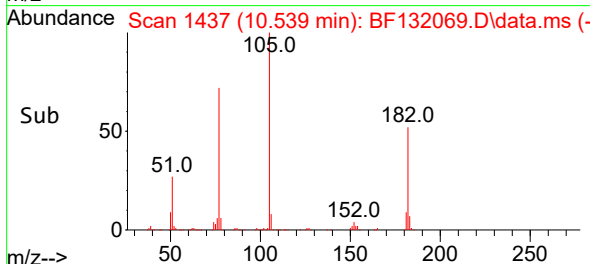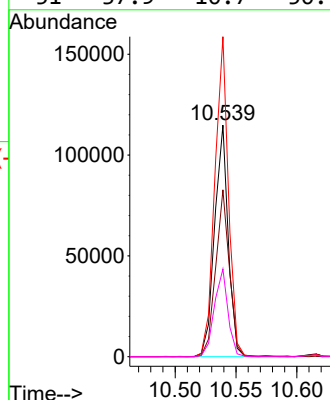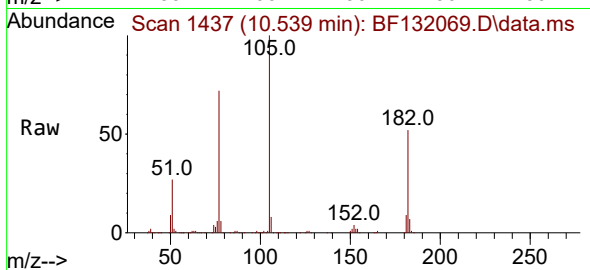

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.310 min Scan# 1568

Delta R.T. -0.006 min

Lab File: BF132069.D

Acq: 13 Jan 2023 20:32




Tgt Ion: 188 Resp: 315335


Ion Ratio Lower Upper

188 100

94 8.4 5.8 8.6

80 9.6 7.4 11.0


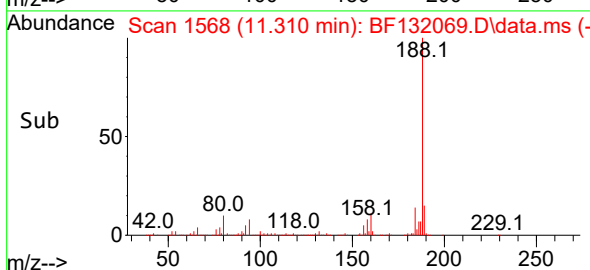
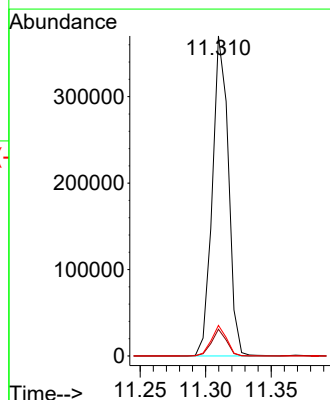
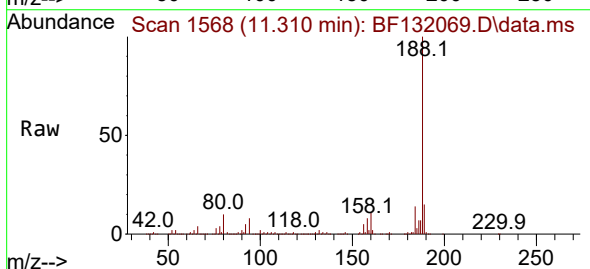




#67
4-Bromophenyl-phenylether
Concen: 2.319 ng
RT: 10.616 min Scan# 1494
Delta R.T. -0.241 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32




Instrument :
BNA_F
ClientSampleId :
TP-D


Tgt Ion:248 Resp: 9149
Ion Ratio Lower Upper
248 100
250 217.9 77.4 116.2#
141 586.4 65.0 97.6#

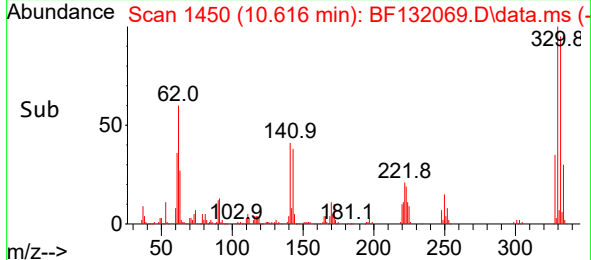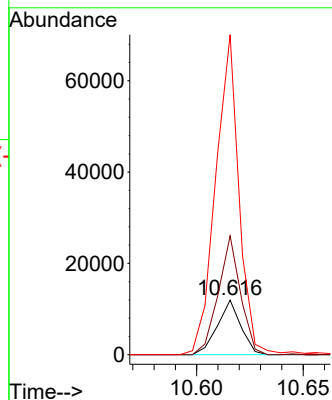

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32


Tgt Ion:240 Resp: 153577
Ion Ratio Lower Upper
240 100
120 8.5 5.4 8.0#
236 25.8 21.1 31.7

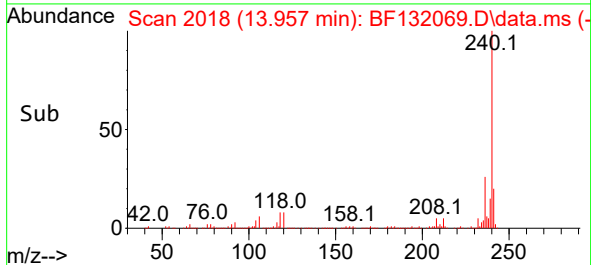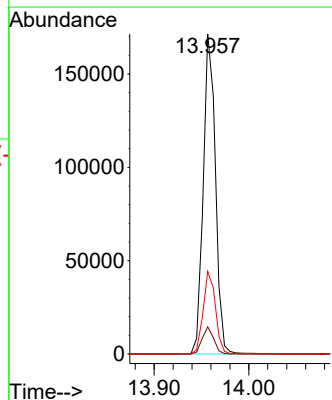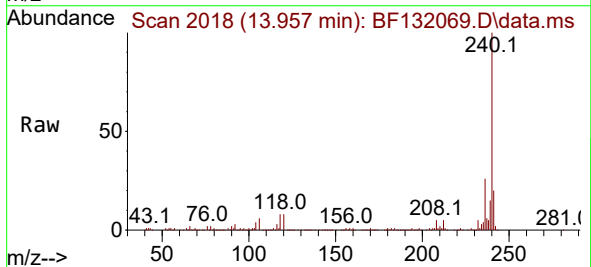



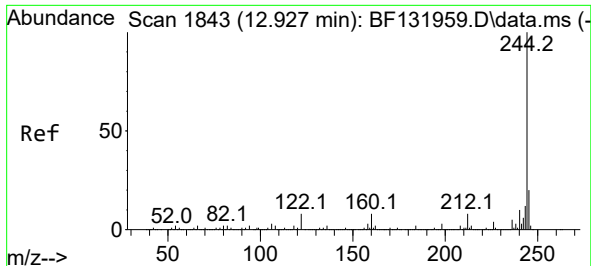


#79
Terphenyl-d14
Concen: 50.046 ng
RT: 12.904 min Scan# 1839
Delta R.T. -0.000 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Instrument :
BNA_F
ClientSampleId :
TP-D



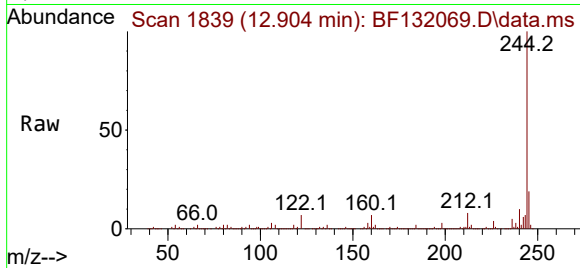



Tgt Ion:244 Resp: 536244
Ion Ratio Lower Upper
244 100
212 7.9 6.3 9.5
122 7.3 6.8 10.2

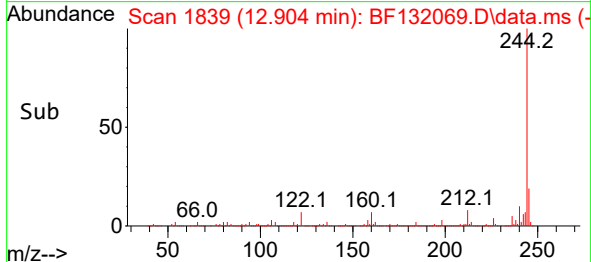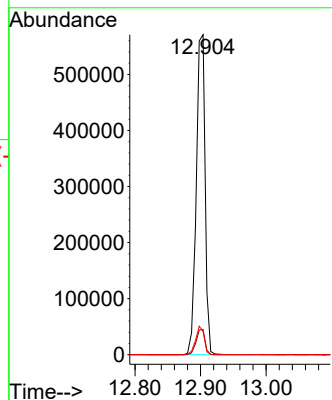

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.421 min Scan# 2267
Delta R.T. 0.006 min
Lab File: BF132069.D
Acq: 13 Jan 2023 20:32

Tgt Ion:264 Resp: 180877
Ion Ratio Lower Upper
264 100
260 24.1 18.3 27.5
265 21.6 16.9 25.3

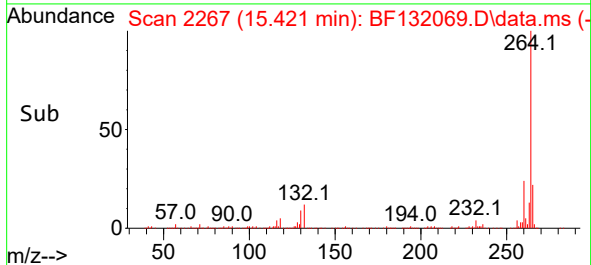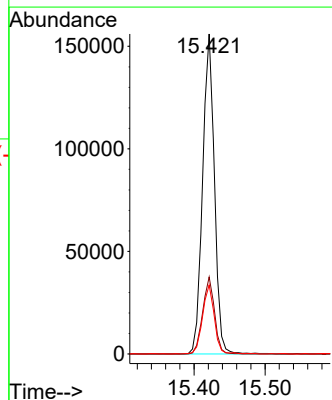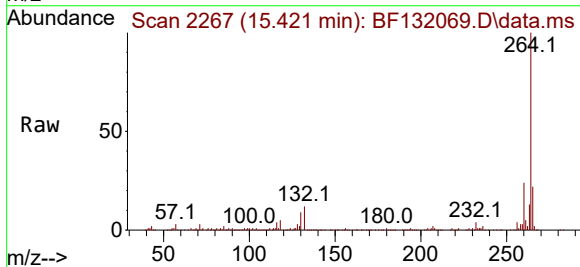

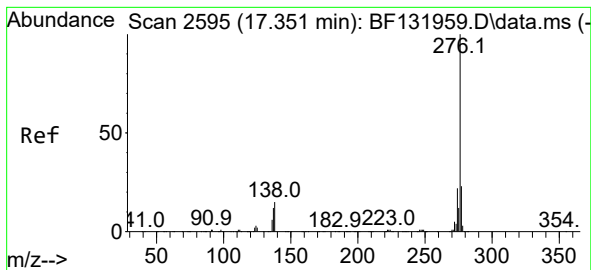

#92

Benzo(g,h,i)perylene

Concen: 3.530 ng

RT: 17.321 min Scan# 21

Delta R.T. 0.006 min

Lab File: BF132069.D


Acq: 13 Jan 2023 20:32

Instrument :

BNA_F

ClientSampleId :

TP-D

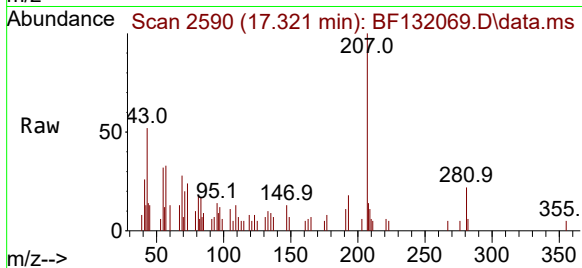

Tgt Ion:276 Resp: 54

Ion Ratio Lower Upper

276 100

277 0.0 18.2 27.2#

138 0.0 11.7 17.5#

