
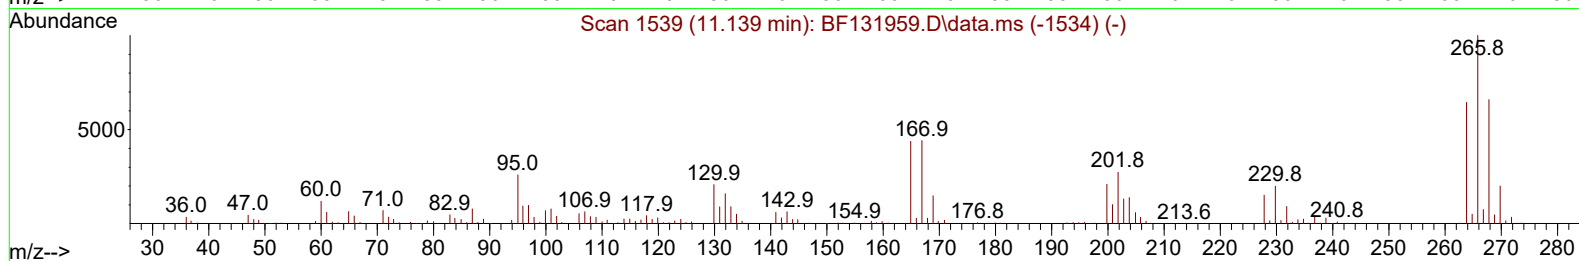
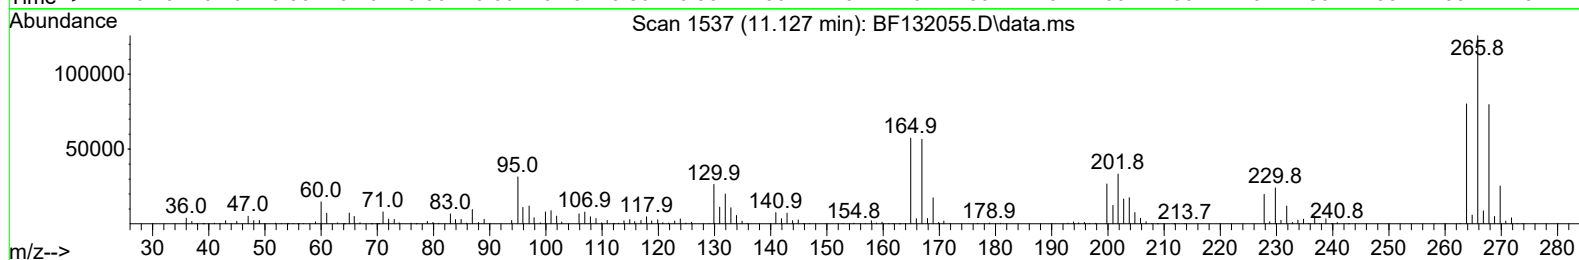


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011323\
Data File : BF132055.D
Acq On : 13 Jan 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:19:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 23:59:08 2023
Response via : Initial Calibration

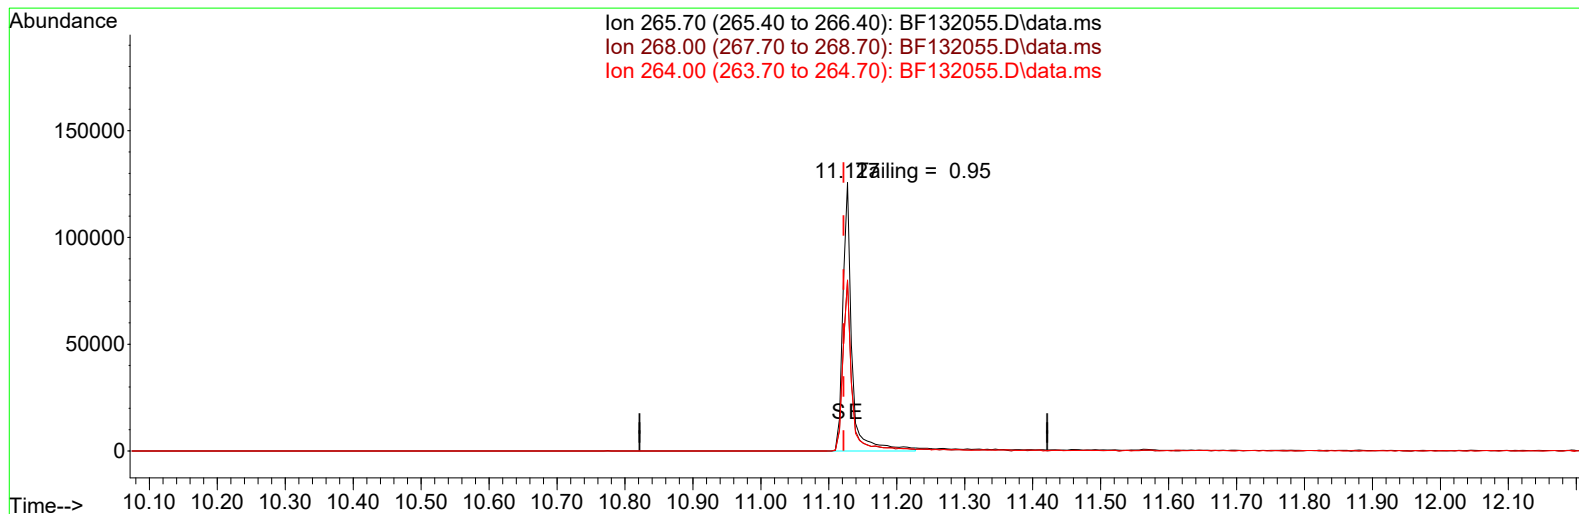

TIC: BF132055.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.006) 21076.81 ng

response 114002

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.47
264.00	64.50	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011323\
Data File : BF132055.D
Acq On : 13 Jan 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:19:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 23:59:08 2023
Response via : Initial Calibration

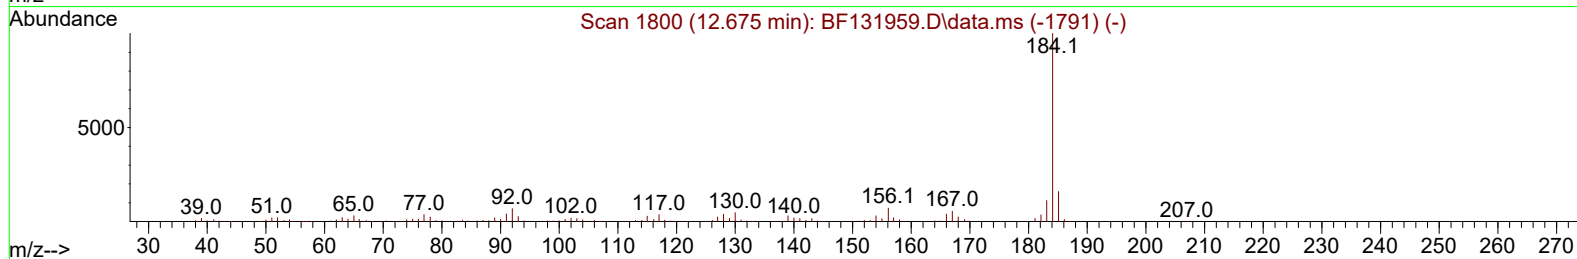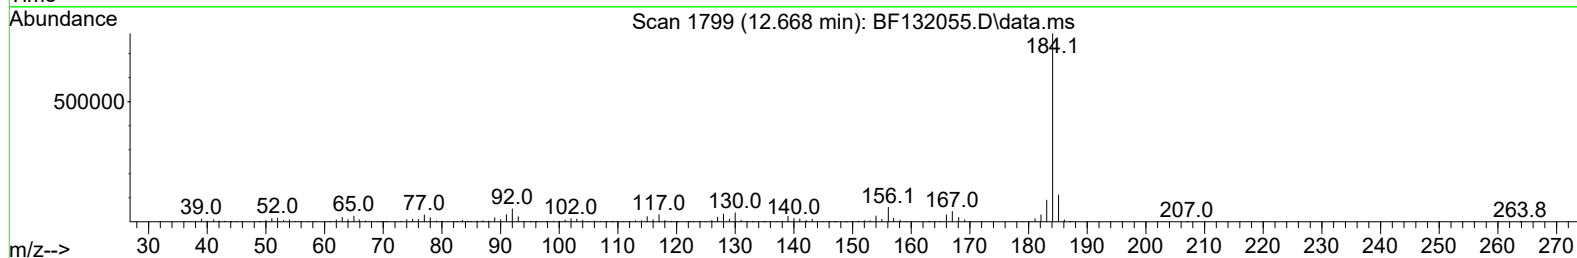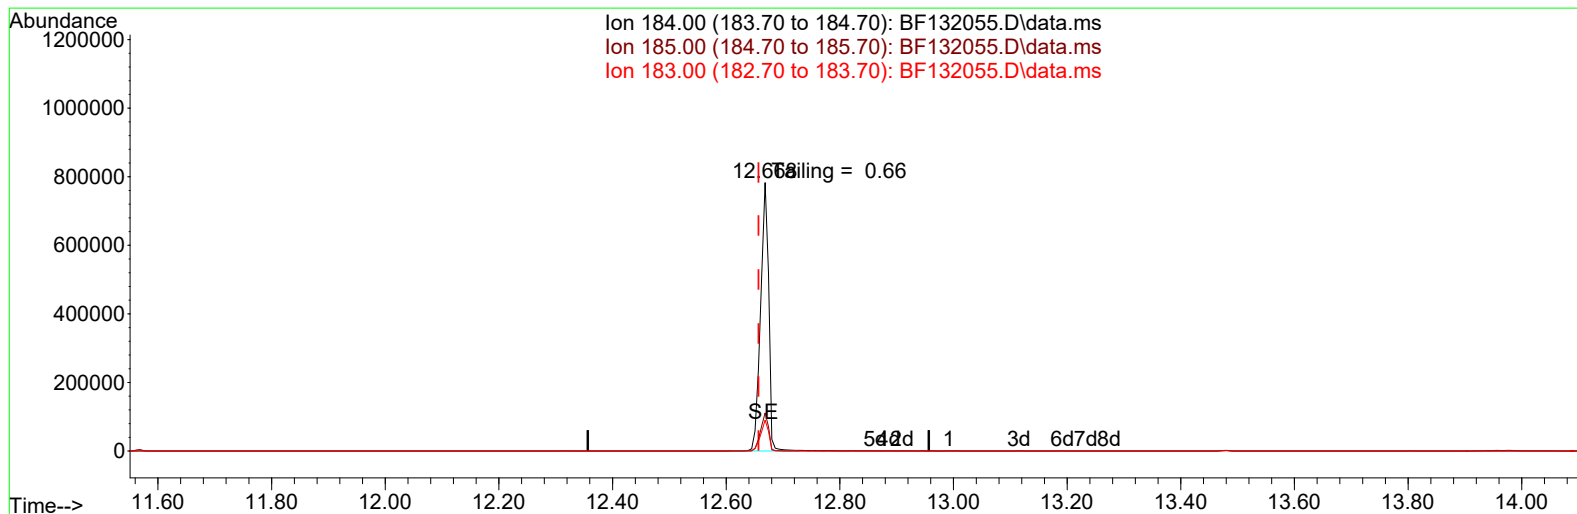

TIC: BF132055.D\data.ms

(77) Benzidine

12.668min (+ 0.012) 446396.20 ng m

response 786003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.22
183.00	11.20	11.53
0.00	0.00	0.00