


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011415\
 Data File : BF076854.D
 Acq On : 14 Jan 2015 11:55
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 14 23:27:58 2015

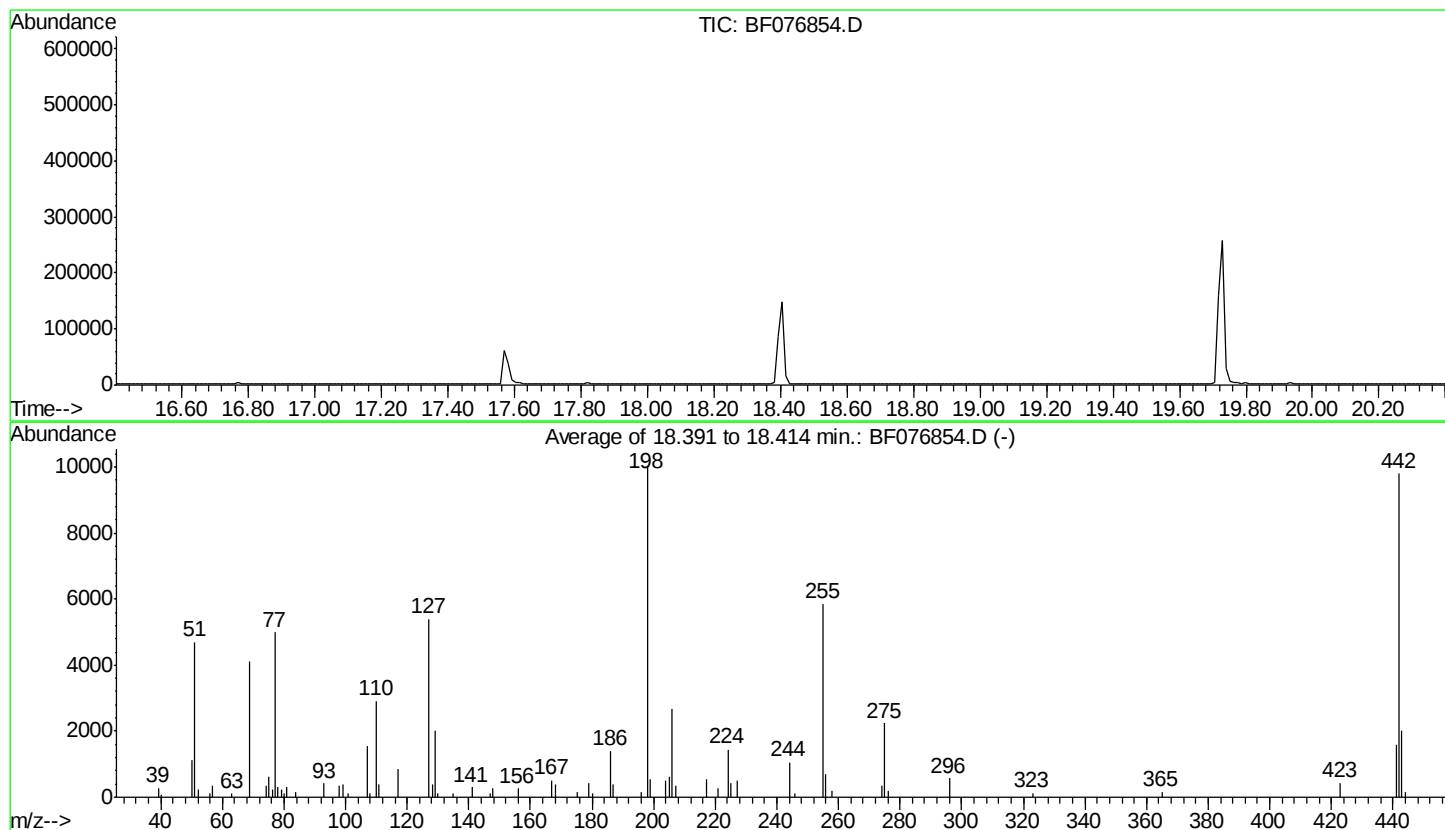

AutoFind: Scans 1514, 1515, 1516; Background Corrected with Scan 1511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	4704	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	4101	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	5393	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10043	PASS
199	198	5	9	5.6	561	PASS
275	198	10	60	22.3	2238	PASS
365	198	1	100	1.6	161	PASS
441	442	0.01	24	16.1	1577	PASS
442	198	50	100	97.6	9797	PASS
443	442	15	24	20.4	1999	PASS