
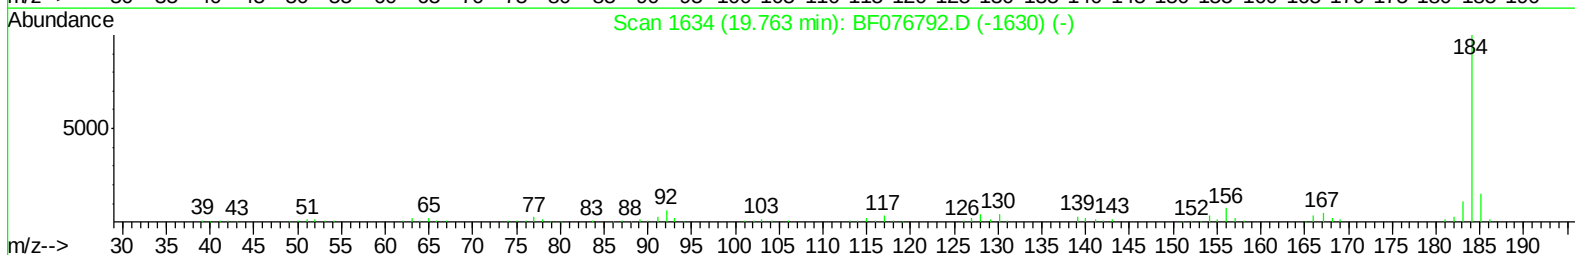
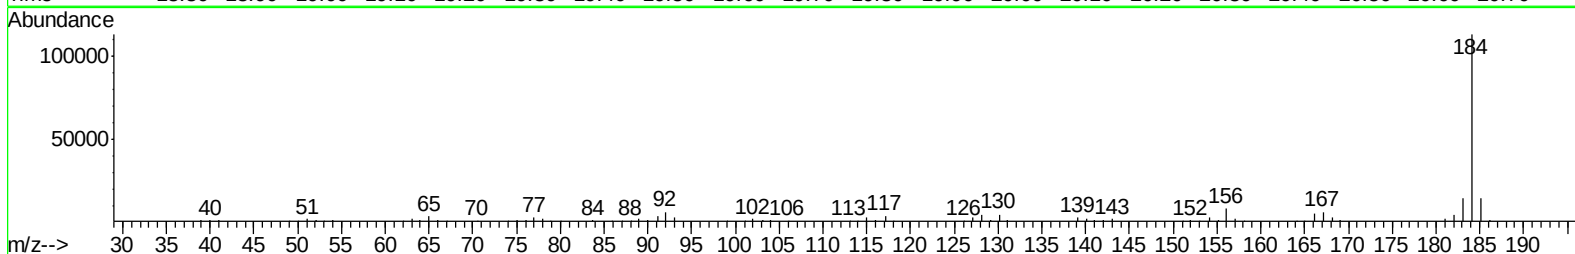


Data Path : Z:\HPCHEM1\BNA F\Data\BF011415\
Data File : BF076854.D
Acq On : 14 Jan 2015 11:55
Operator : IZ / TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 04:40:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 12 10:43:48 2015
Response via : Initial Calibration

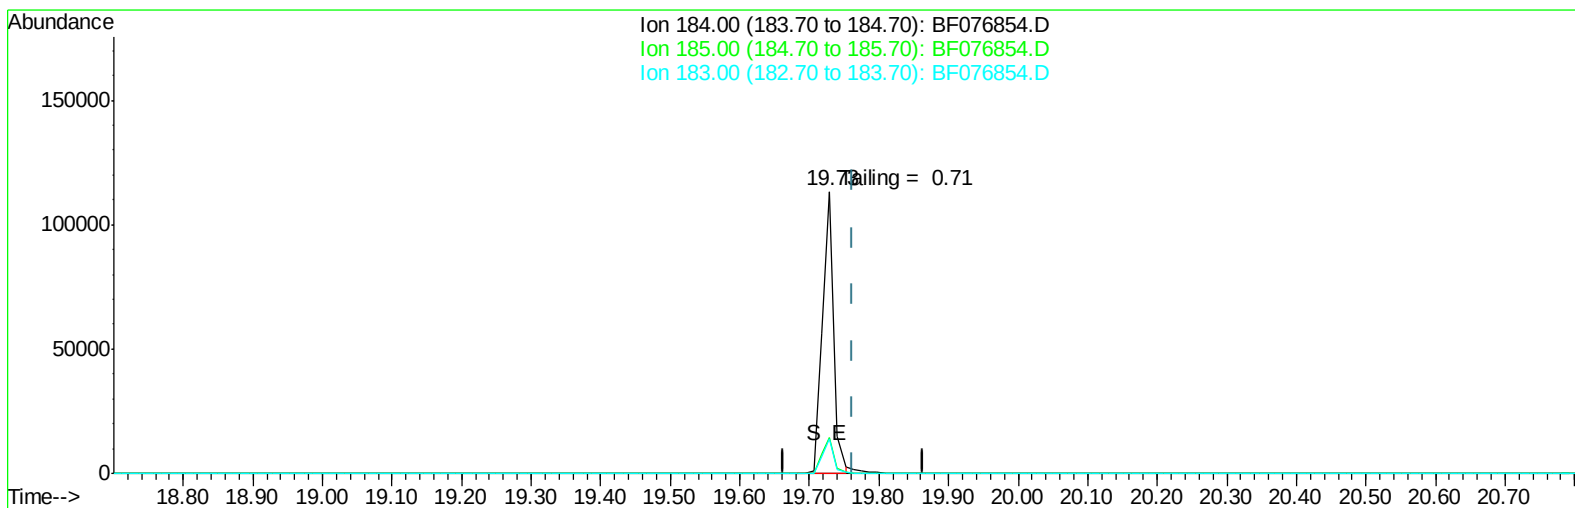

TIC: BF076854.D

(76) Benzidine




19.729min (-0.034) 0.00ng

response 131370

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	12.67
183.00	10.90	12.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF011415\
Data File : BF076854.D
Acq On : 14 Jan 2015 11:55
Operator : IZ / TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 04:40:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 12 10:43:48 2015
Response via : Initial Calibration

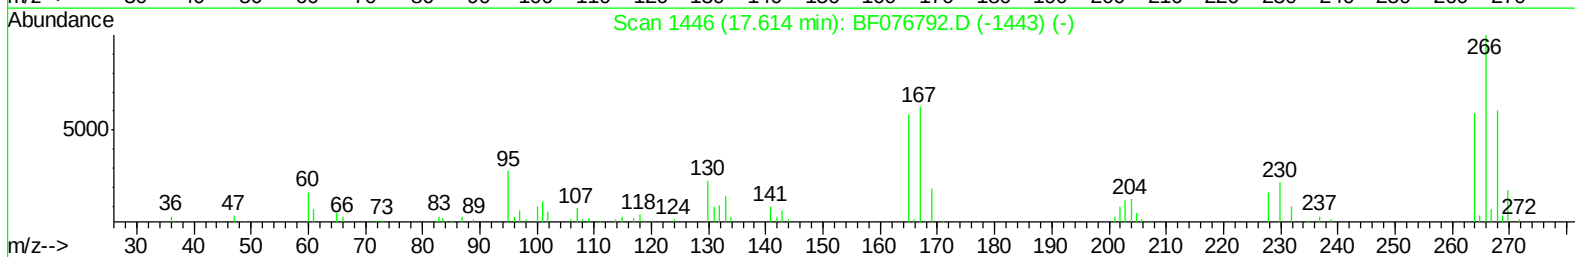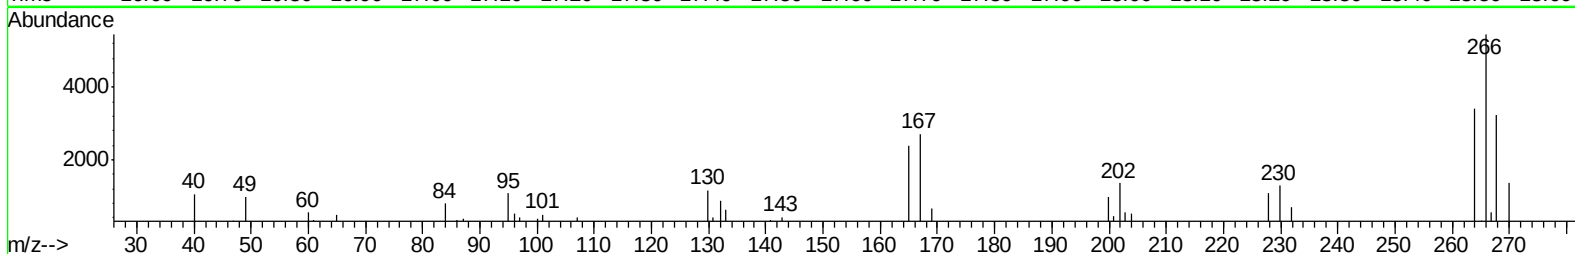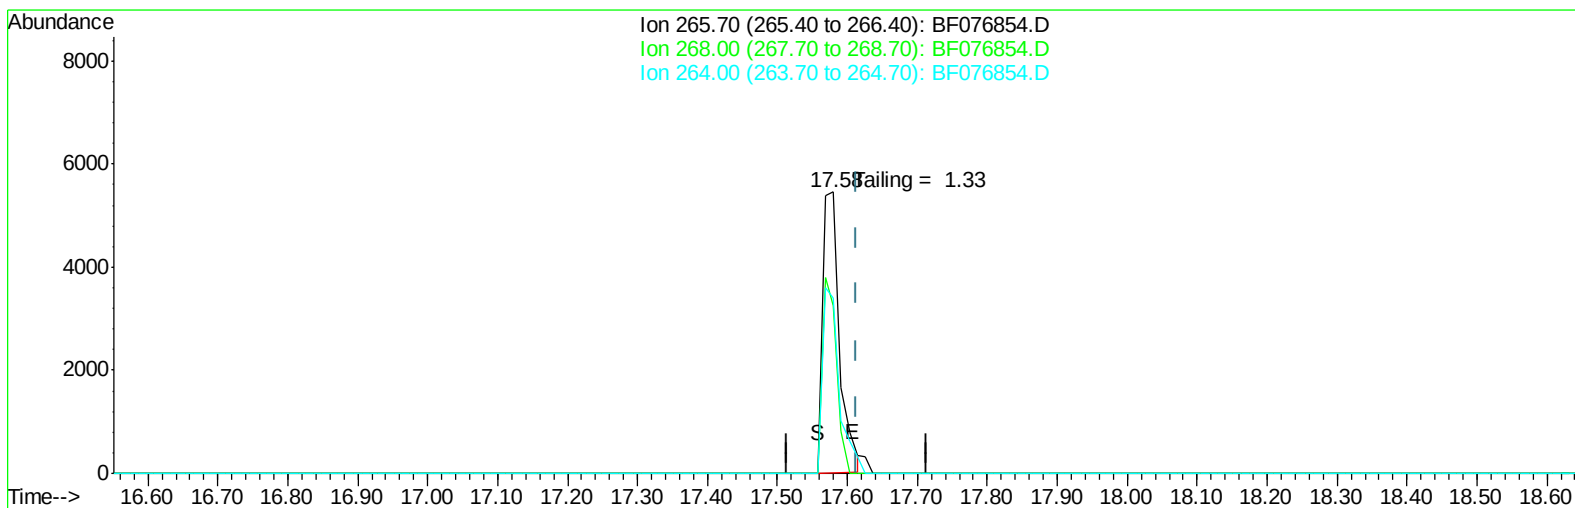

TIC: BF076854.D

(69) Pentachlorophenol (C)

17.580min (-0.034) 0.00ng

response 9606

Ion	Exp%	Act%
265.70	100	100
268.00	60.10	59.48
264.00	58.90	62.50
0.00	0.00	0.00