

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011415\
 Data File : BF076871.D
 Acq On : 14 Jan 2015 21:45
 Operator : IZ / TP
 Sample : PB81324BL
 Misc : S
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81324BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.384	25	26	32	rBV	1293430	2093009	62.72%	15.164%
2	1.475	32	34	59	rVB	1525259	3337257	100.00%	24.178%
3	4.173	267	270	281	rVB	113132	247560	7.42%	1.794%
4	5.099	347	351	359	rBV	440113	856455	25.66%	6.205%
5	7.419	550	554	559	rBV	496659	818727	24.53%	5.932%
6	7.510	559	562	569	rVB	533467	908289	27.22%	6.580%
7	8.025	603	607	611	rBV	114933	188587	5.65%	1.366%
8	8.345	631	635	638	rBV	433496	682184	20.44%	4.942%
9	9.316	716	720	727	rBV	346384	518160	15.53%	3.754%
10	10.928	857	861	864	rBV	168173	253441	7.59%	1.836%
11	13.579	1090	1093	1097	rBV	616729	1029994	30.86%	7.462%
12	15.065	1219	1223	1226	rBV	180754	277310	8.31%	2.009%
13	16.723	1365	1368	1371	rBV	460429	603404	18.08%	4.372%
14	17.808	1461	1463	1466	rBV	219679	280443	8.40%	2.032%
15	20.037	1655	1658	1660	rBV	1038544	1119446	33.54%	8.110%
16	21.306	1766	1769	1772	rVB	249053	286902	8.60%	2.079%
17	22.940	1909	1912	1915	rBV	237255	267603	8.02%	1.939%
18	24.323	2029	2033	2037	rBV2	14386	33982	1.02%	0.246%


Sum of corrected areas: 13802753

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011415\
Data File : BF076871.D
Acq On : 14 Jan 2015 21:45
Operator : IZ / TP
Sample : PB81324BL
Misc : S
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81324BL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

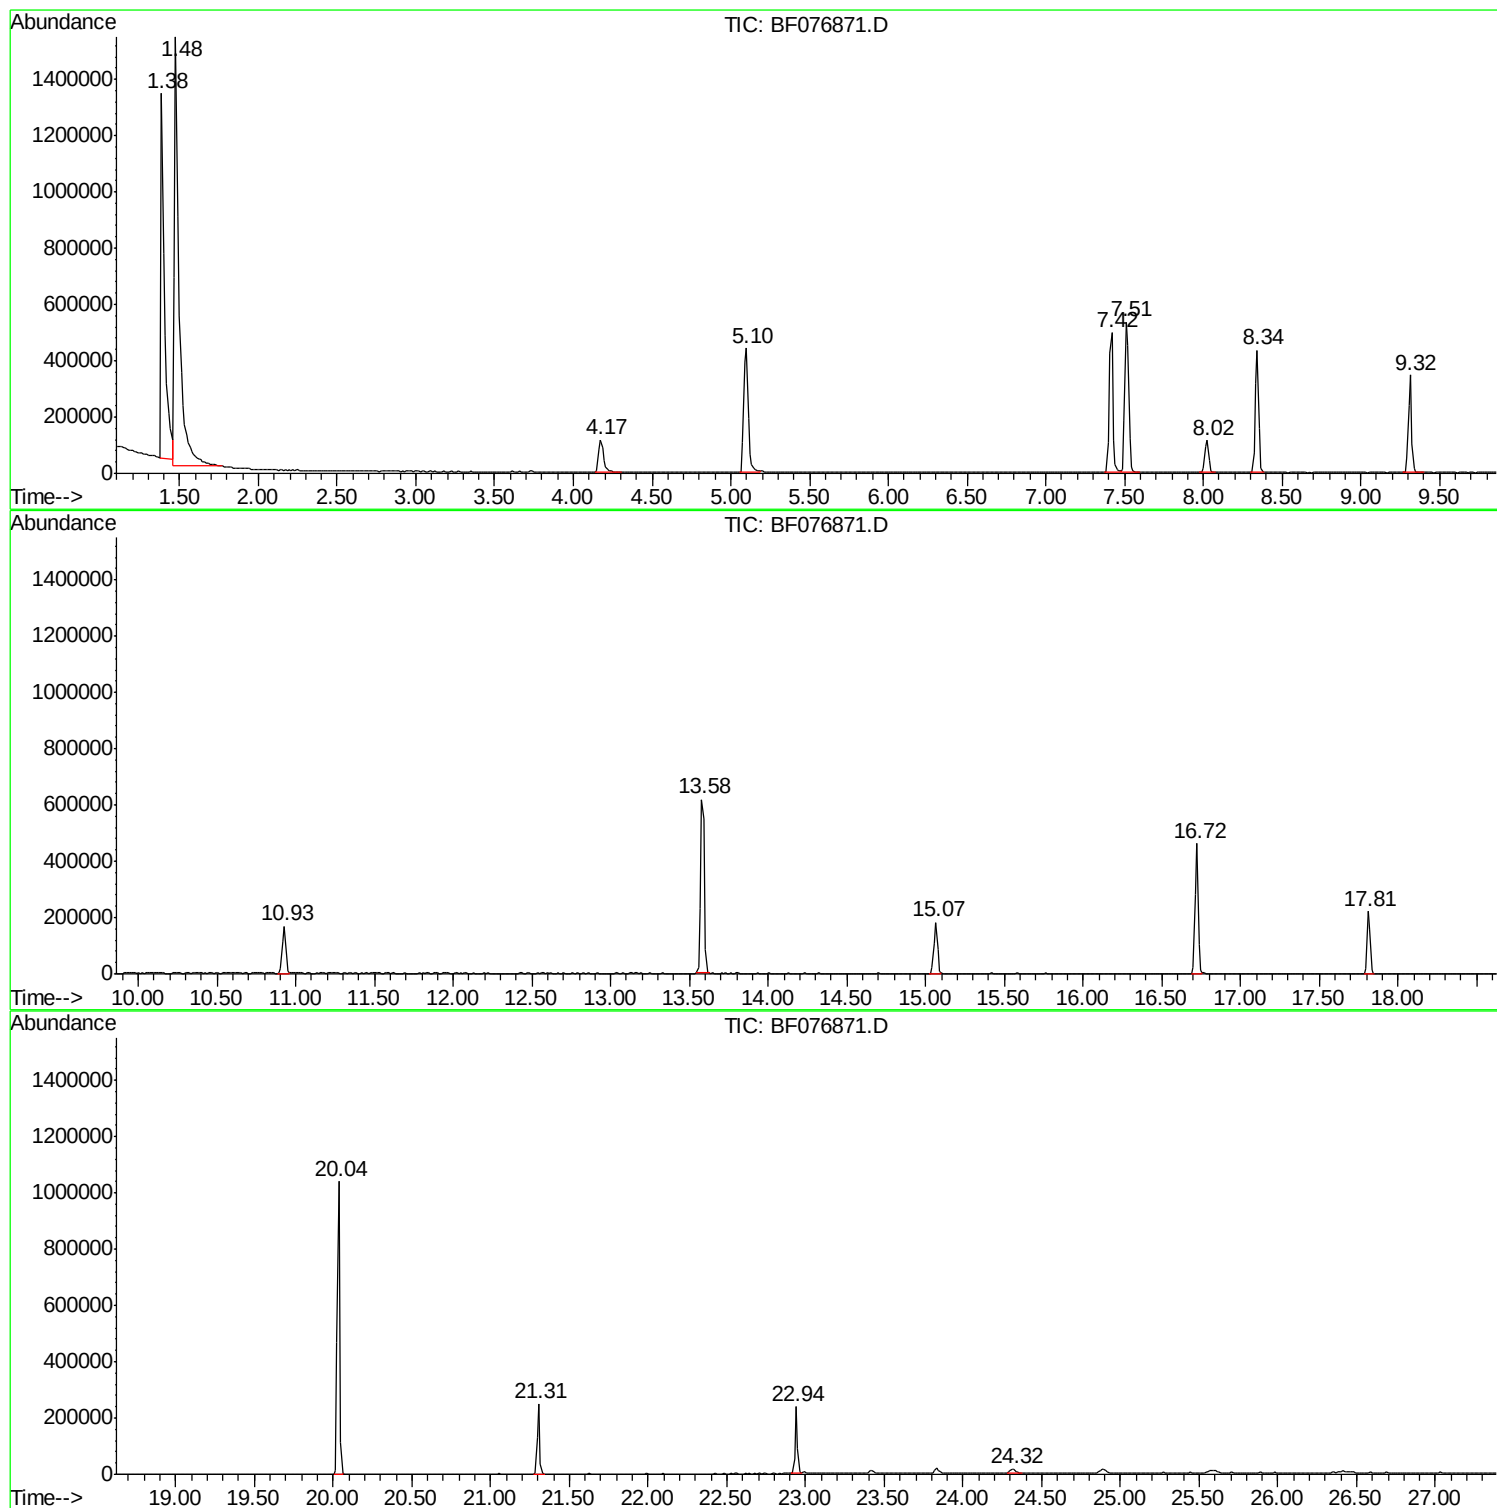

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011415\
Data File : BF076871.D
Acq On : 14 Jan 2015 21:45
Operator : IZ / TP
Sample : PB81324BL
Misc : S
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81324BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.17	26.25 ng	247560	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	32
3		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
4		1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	23
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

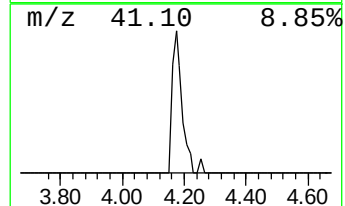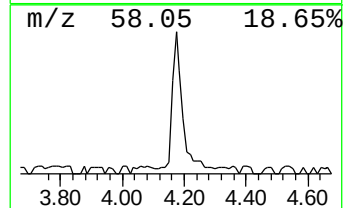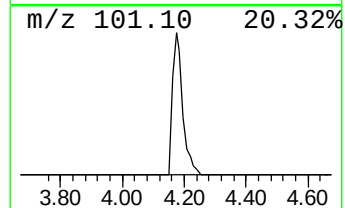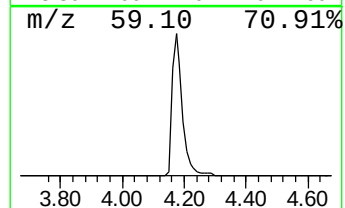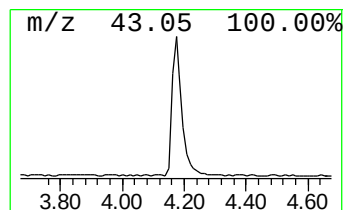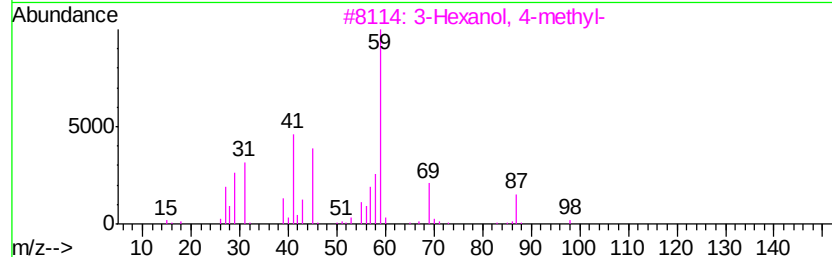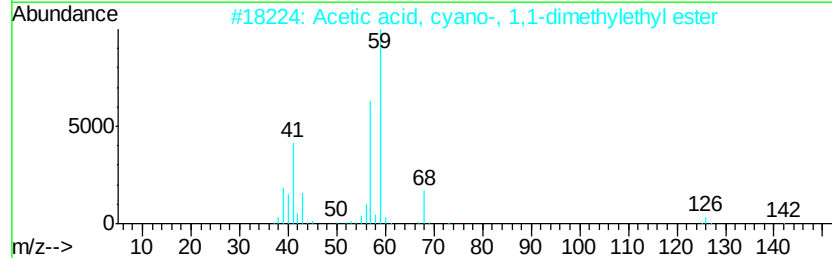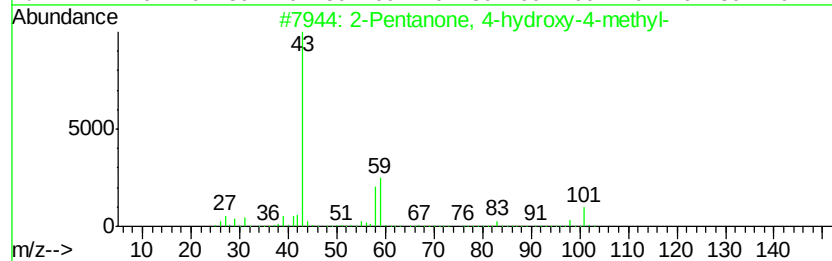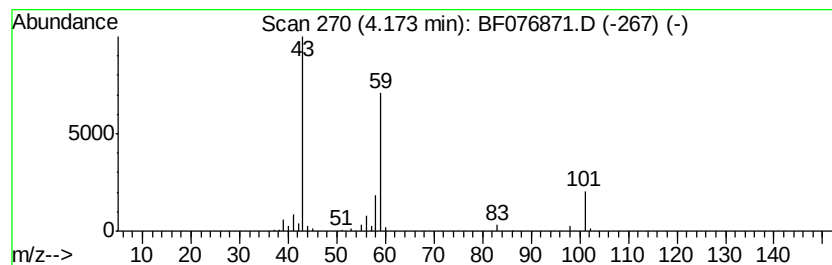

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011415\
Data File : BF076871.D
Acq On : 14 Jan 2015 21:45
Operator : IZ / TP
Sample : PB81324BL
Misc : S
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81324BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 unknown24.32 Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.32	2.54 ng	33982	Perylene-d12	22.94

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3,6-Dioxa-2,4,5,7-tetrasilaoctan...	294	C10H30O2Si4	004342-25-0	38
2			3-Isopropoxy-1,1,1,7,7,7-hexamet...	576	C18H52O7Si7	071579-69-6	32
3			Trisiloxane, 1,1,1,5,5,5-hexamet...	384	C12H36O4Si5	003555-47-3	12
4			Benzo[blselenophene-3-carbonitri...	221	C10H7NSe	037007-54-8	10
5			N-Benzyl-N-ethyl-p-isopropylbenz...	281	C19H23NO	015089-22-2	10

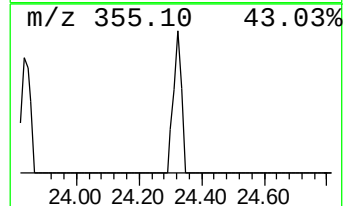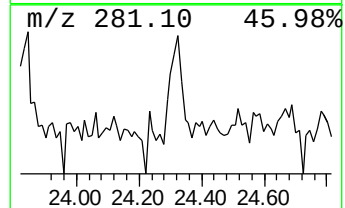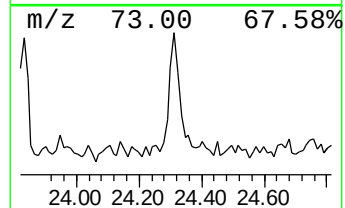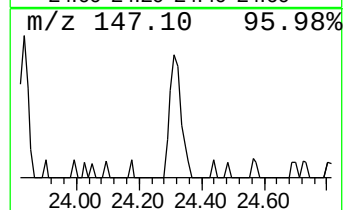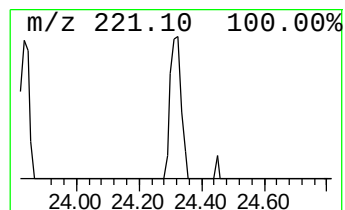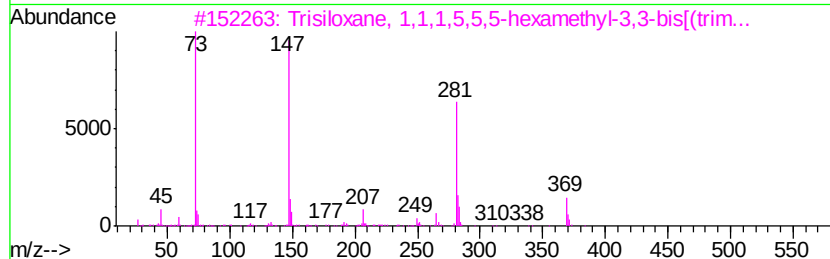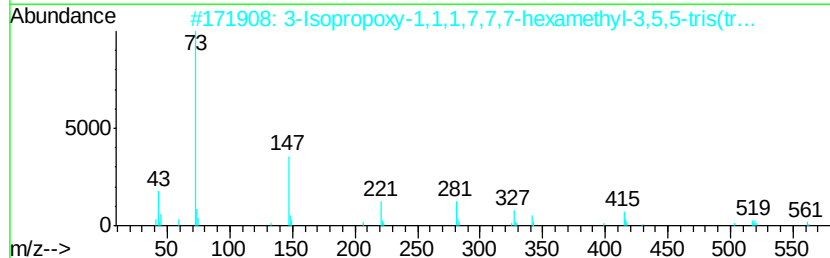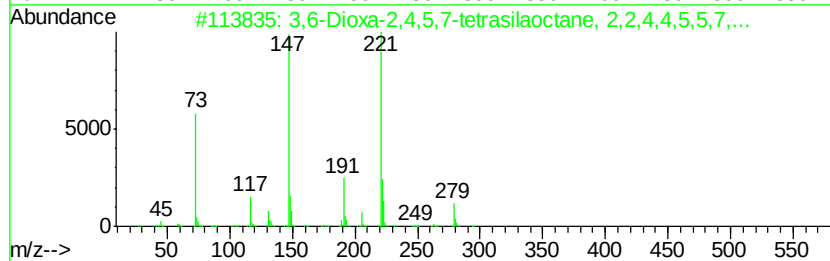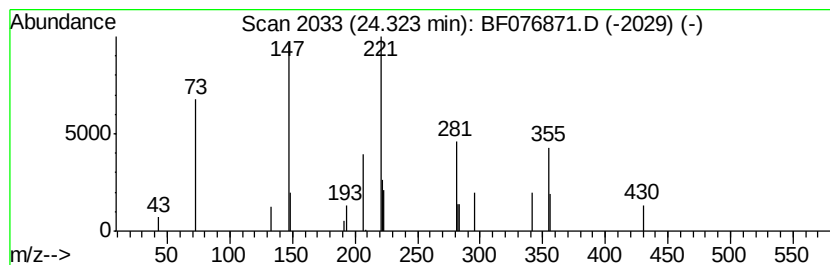

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011415\
Data File : BF076871.D
Acq On : 14 Jan 2015 21:45
Operator : IZ / TP
Sample : PB81324BL
Misc : S
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81324BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.17	26.3	ng	247560	1	8.02	188587	20.0
unknown24.32	24.32	2.5	ng	33982	6	22.94	267603	20.0