
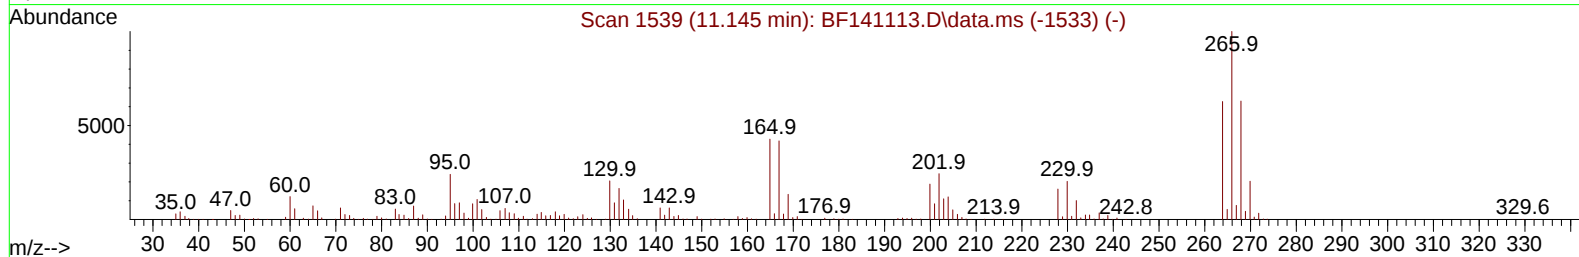
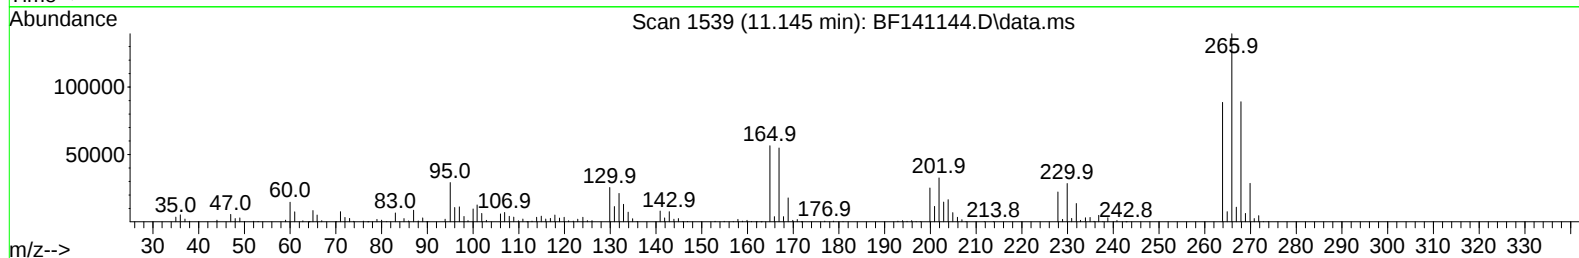


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141144.D
Acq On : 14 Jan 2025 14:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 15:10:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

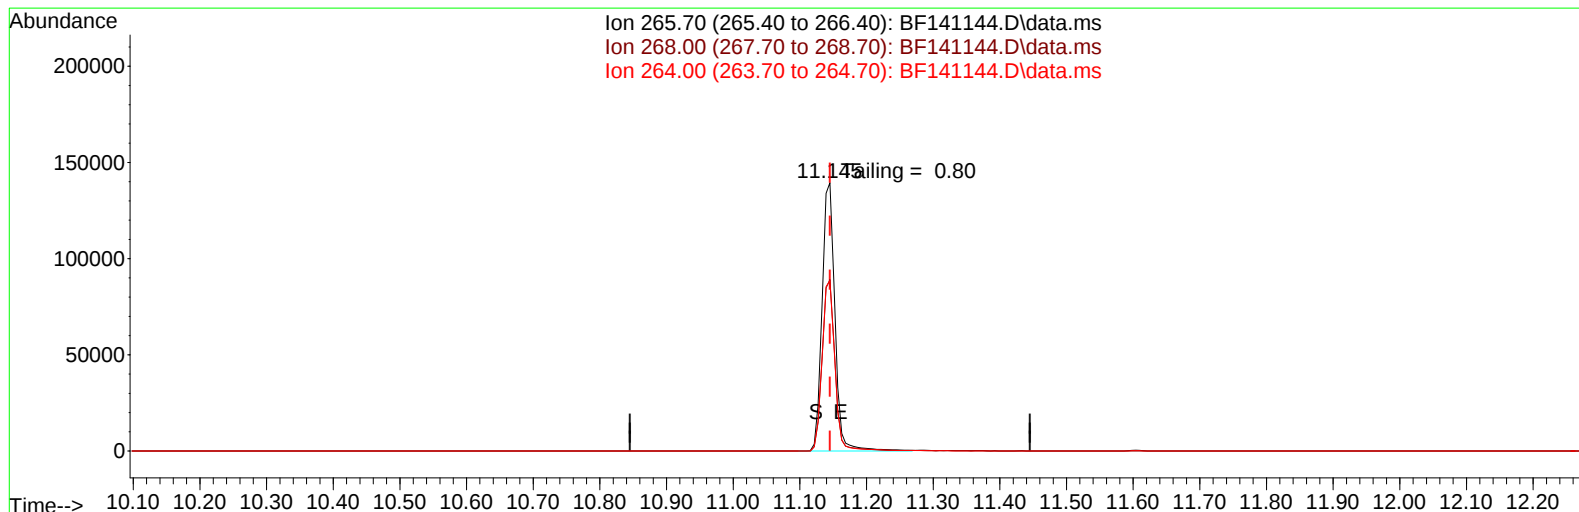

TIC: BF141144.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.000) 18920.76 ng

response 186971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.88
264.00	62.70	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141144.D
Acq On : 14 Jan 2025 14:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 15:10:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

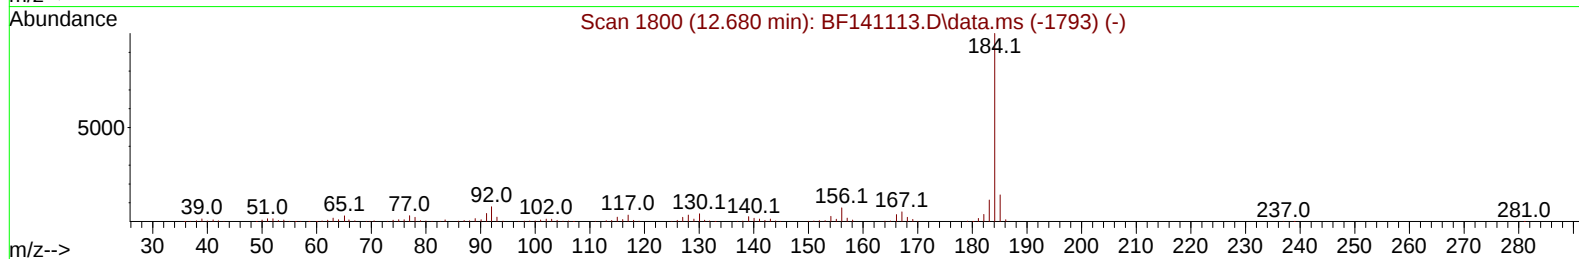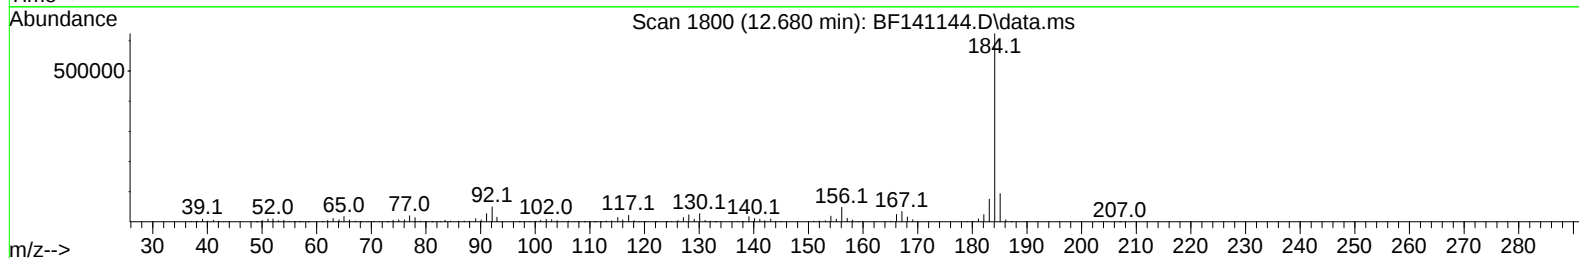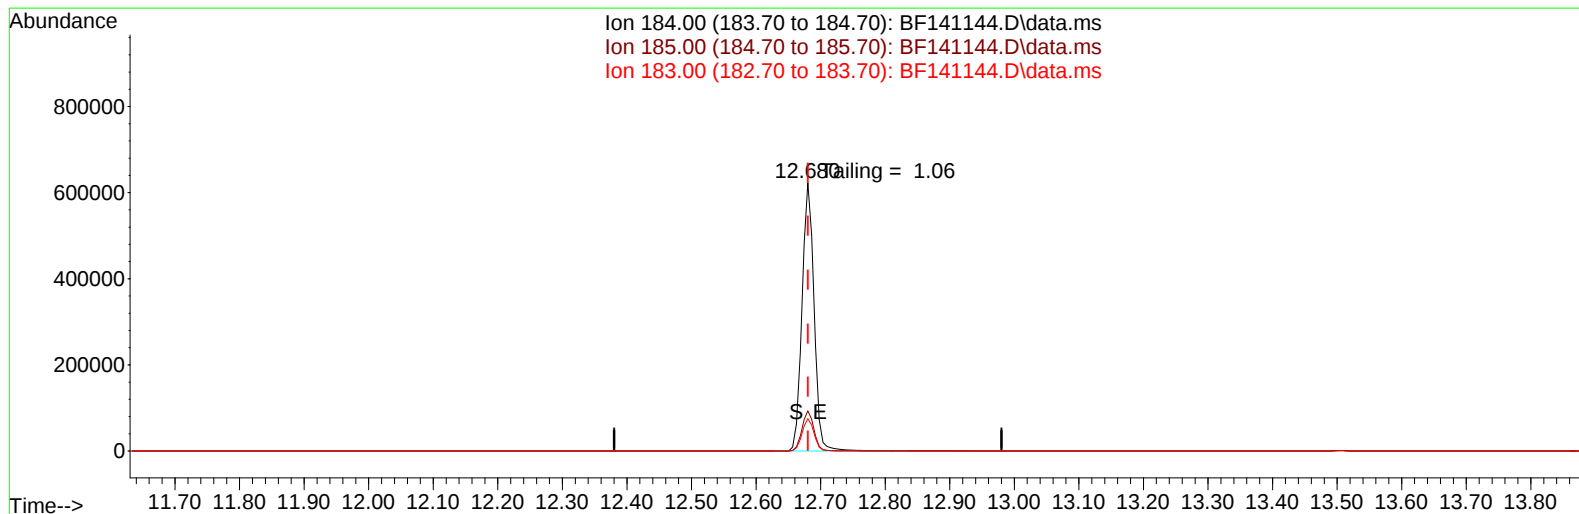

TIC: BF141144.D\data.ms

(77) Benzidine**12.680min (-0.000) 66475.81 ng****response 812384**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.97
183.00	11.50	12.04
0.00	0.00	0.00