
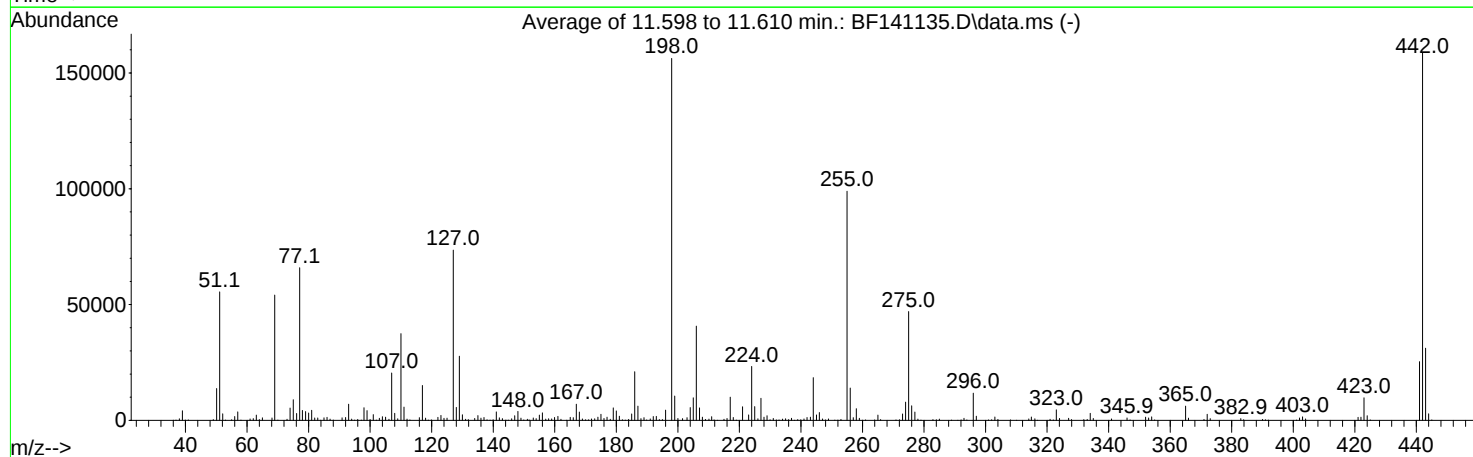


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141135.D
Acq On : 14 Jan 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

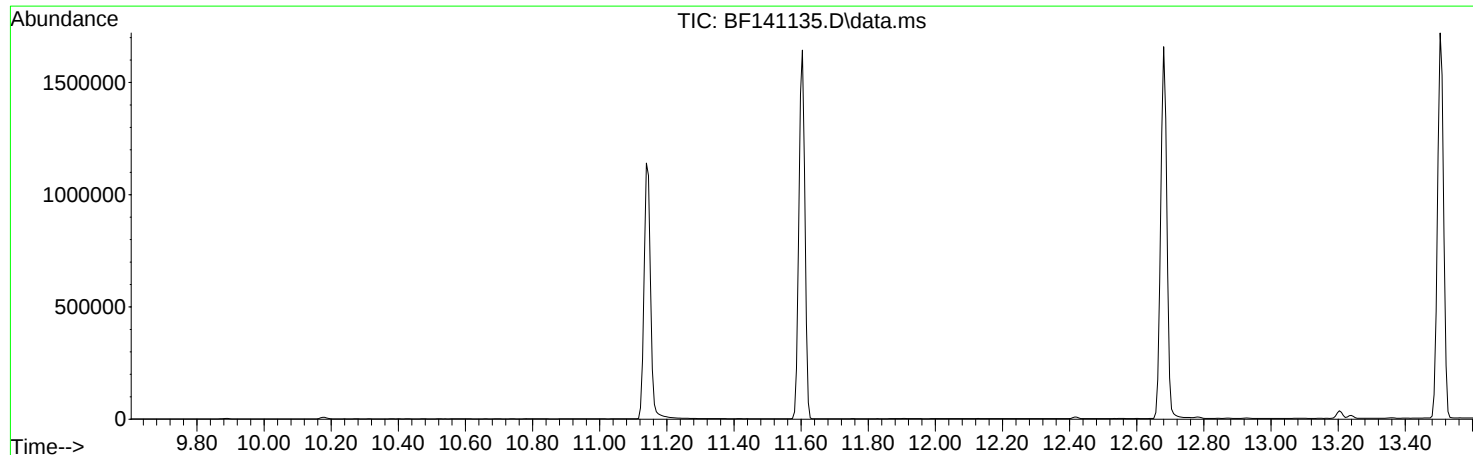

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	55469	PASS
68	69	0.00	2	1.9	1049	PASS
69	198	0.00	100	34.6	54099	PASS
70	69	0.00	2	0.3	158	PASS
127	198	10	80	47.0	73515	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156291	PASS
199	198	5	9	6.7	10482	PASS
275	198	10	60	30.1	46976	PASS
365	198	1	100	3.9	6138	PASS
441	198	0.01	100	16.2	25373	PASS
442	442	50	100	100.0	158829	PASS
443	442	15	24	19.6	31160	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/14/2025	BNA_F	<u>BF141135.D</u>
Compound Name	Response	Retention Time
DDT	428651	13.504
DDD	12314	13.204
DDE	448	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12762	441413	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141135.D
Acq On : 14 Jan 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 14 11:29:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

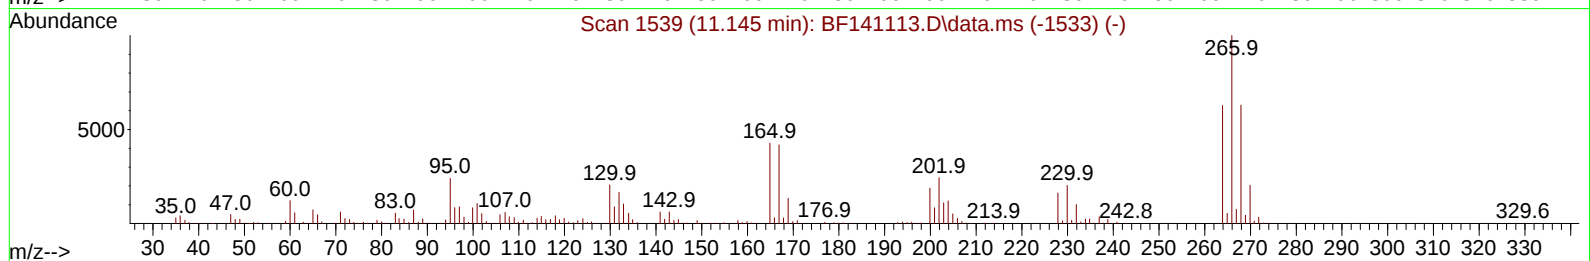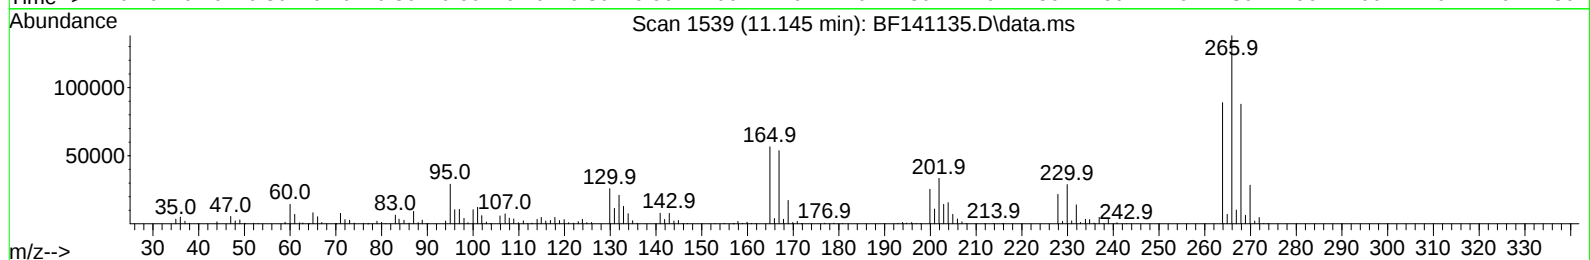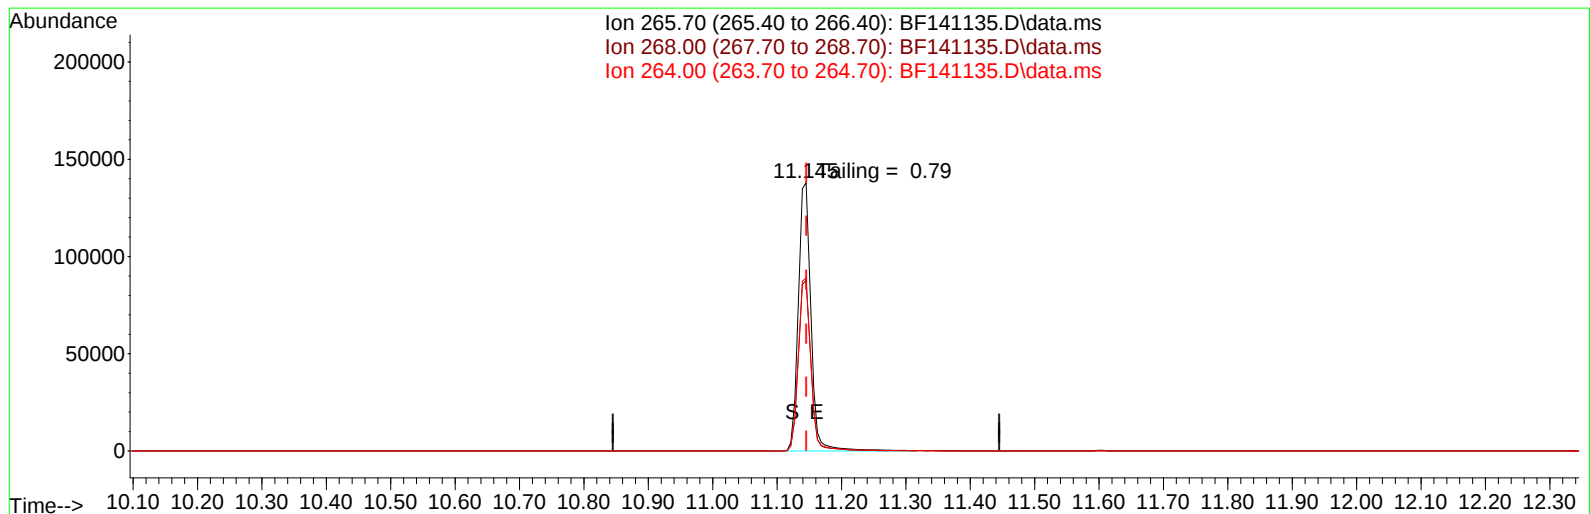

TIC: BF141135.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 45996.99 ng




response 189892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.58
264.00	62.70	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141135.D
Acq On : 14 Jan 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 14 11:29:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

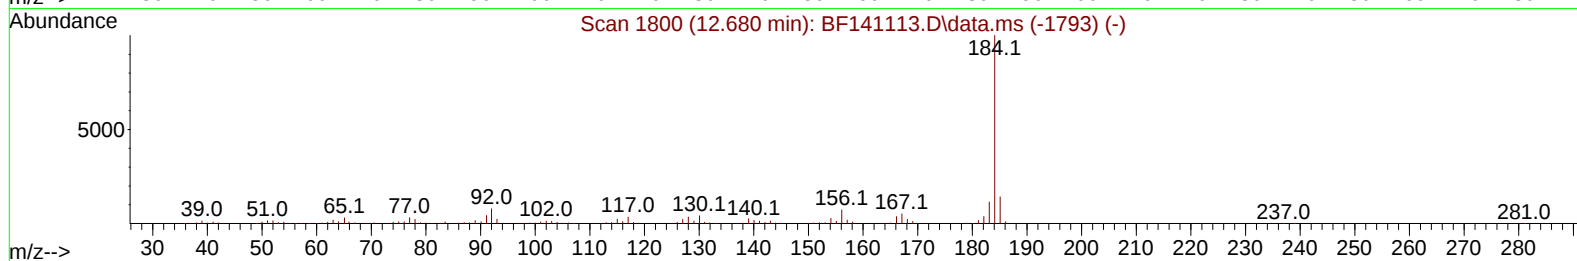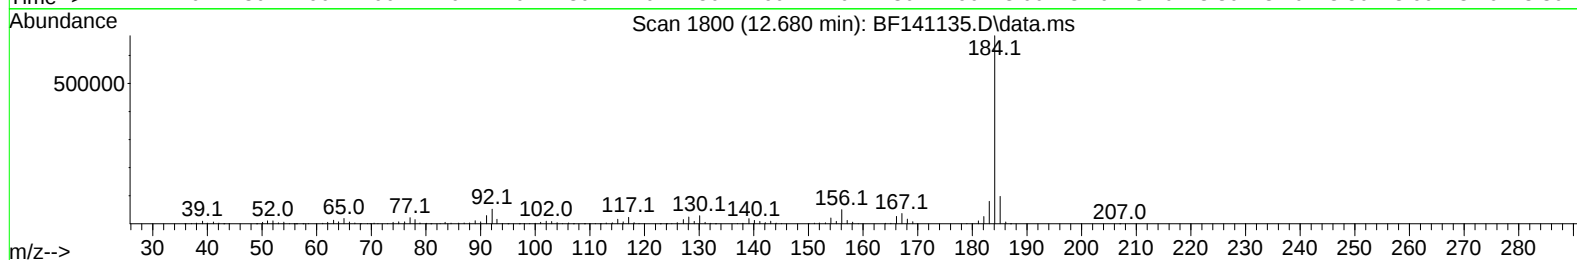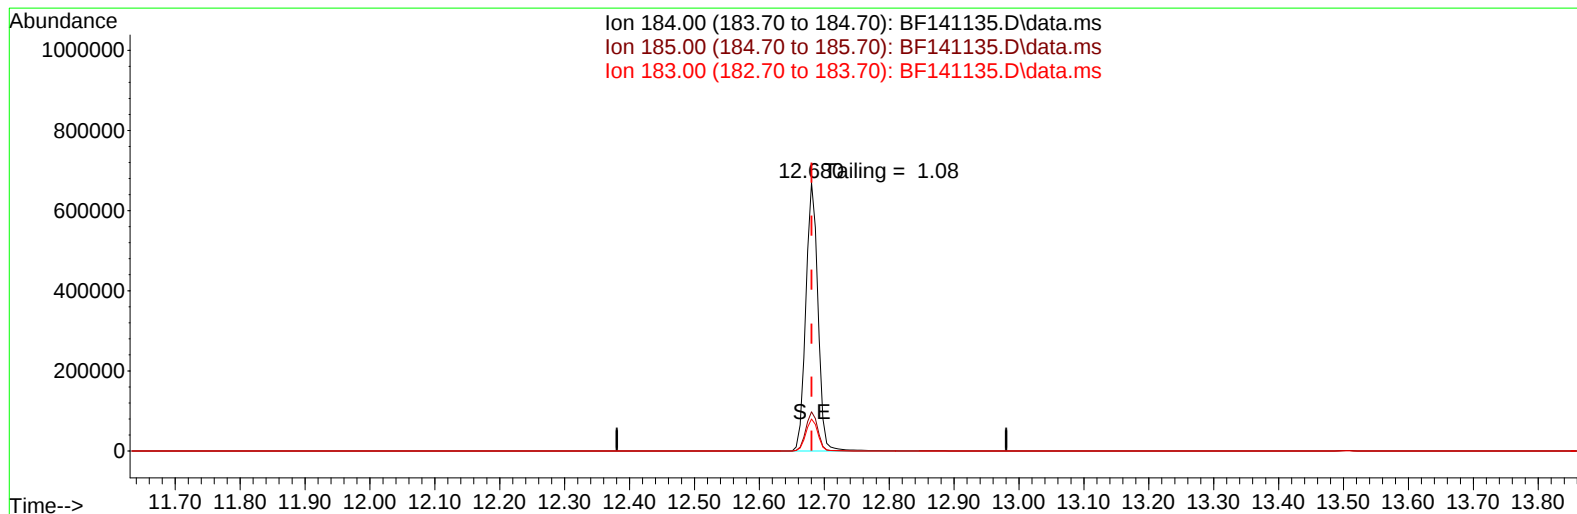

TIC: BF141135.D\data.ms

(77) Benzidine

12.680min (-0.000) 188726.25 ng

response 871453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.62
183.00	11.50	11.95
0.00	0.00	0.00