


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141144.D
Acq On : 14 Jan 2025 14:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

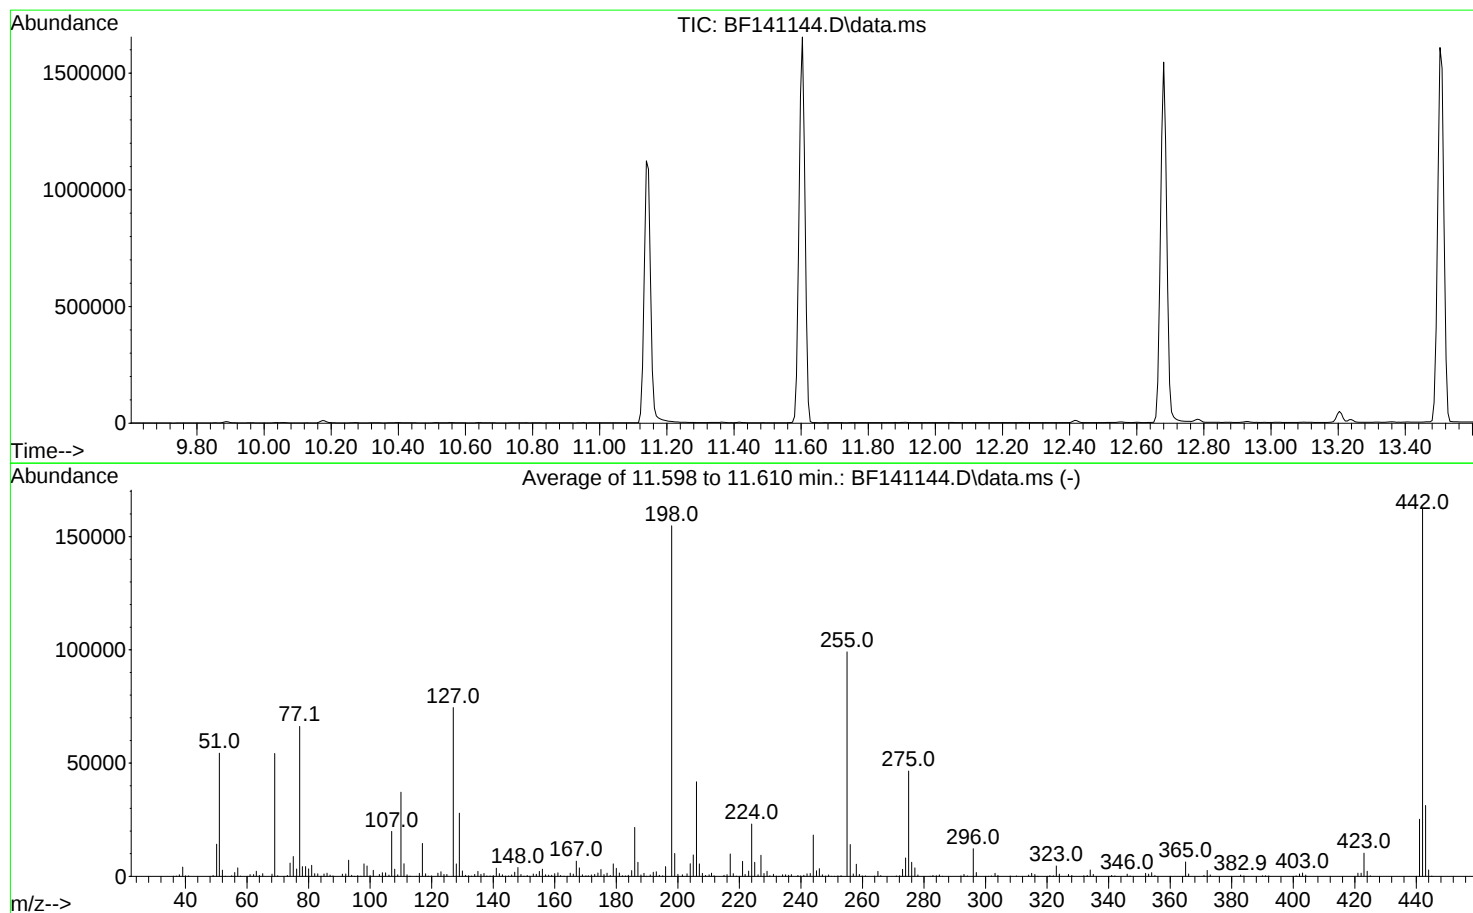

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	54381	PASS
68	69	0.00	2	1.8	988	PASS
69	198	0.00	100	35.1	54269	PASS
70	69	0.00	2	0.6	326	PASS
127	198	10	80	48.2	74544	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	154744	PASS
199	198	5	9	6.5	10098	PASS
275	198	10	60	30.0	46453	PASS
365	198	1	100	4.1	6398	PASS
441	198	0.01	100	16.3	25229	PASS
442	442	50	100	100.0	162400	PASS
443	442	15	24	19.3	31333	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/14/2025	BNA_F	<u>BF141144.D</u>
Compound Name	Response	Retention Time
DDT	410385	13.504
DDD	15889	13.204
DDE	396	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16285	426670	3.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141144.D
Acq On : 14 Jan 2025 14:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 14 15:10:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

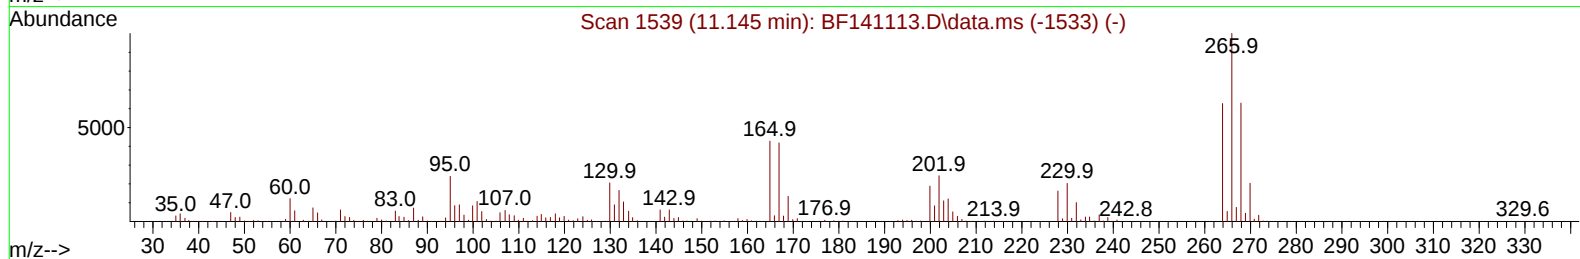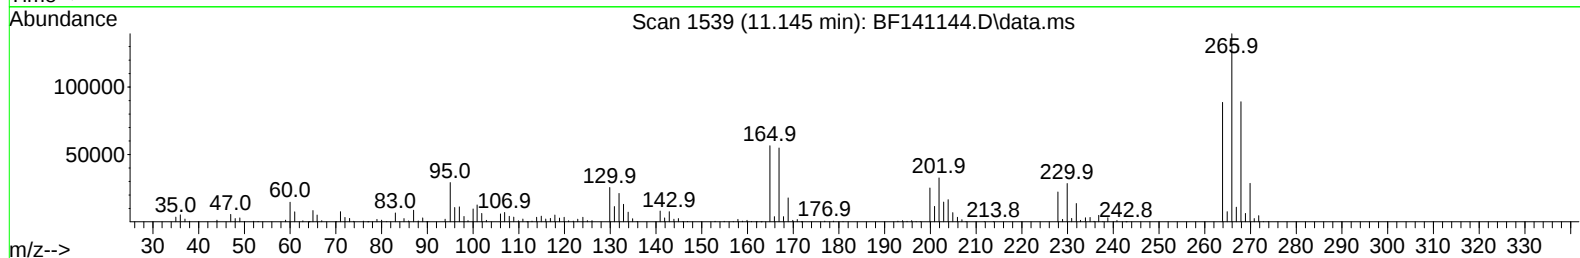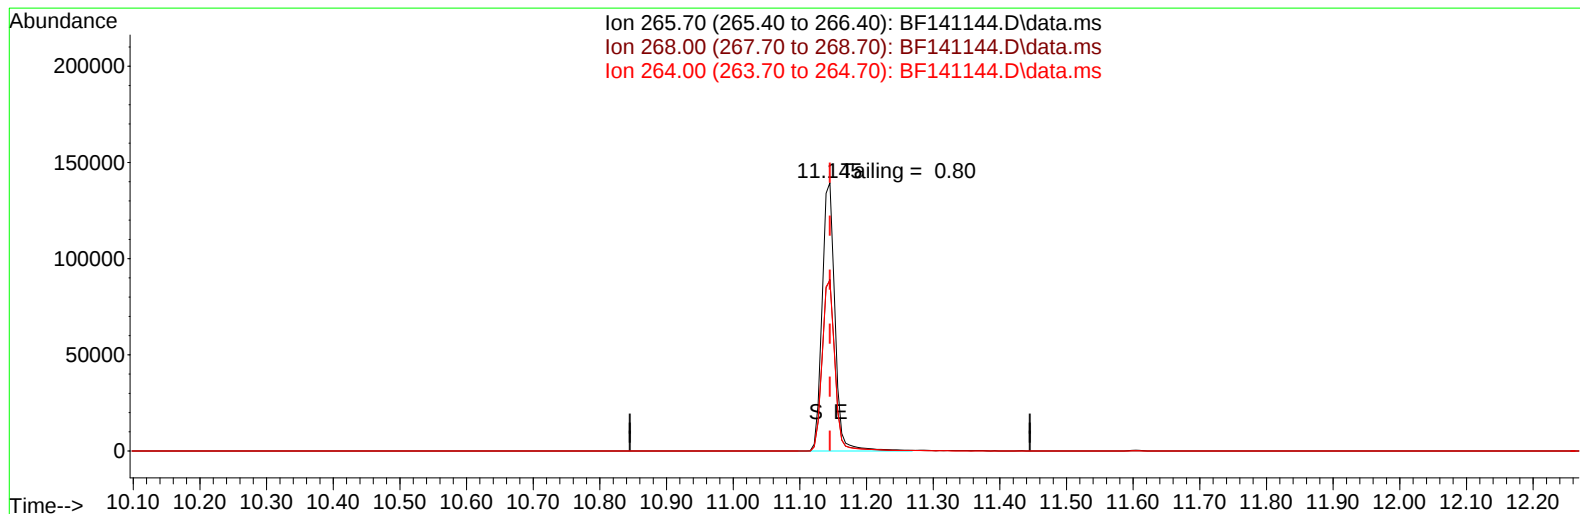

TIC: BF141144.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 18920.76 ng




response 186971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.88
264.00	62.70	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011425\
Data File : BF141144.D
Acq On : 14 Jan 2025 14:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 14 15:10:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

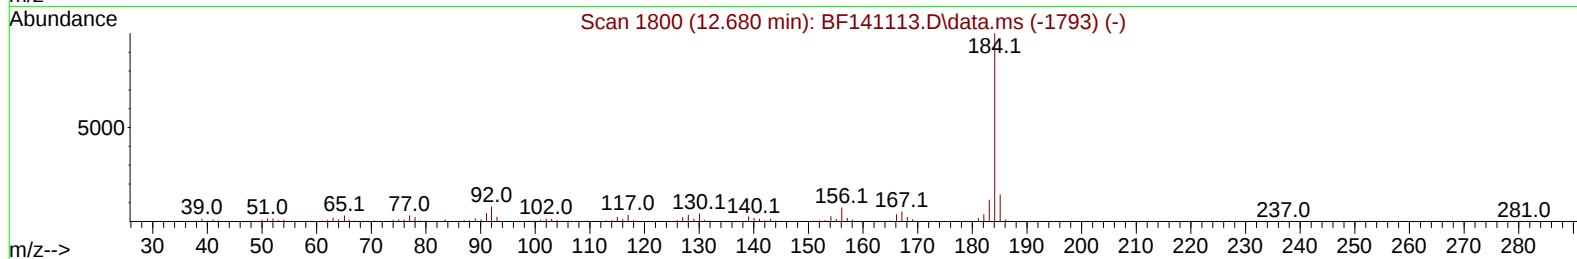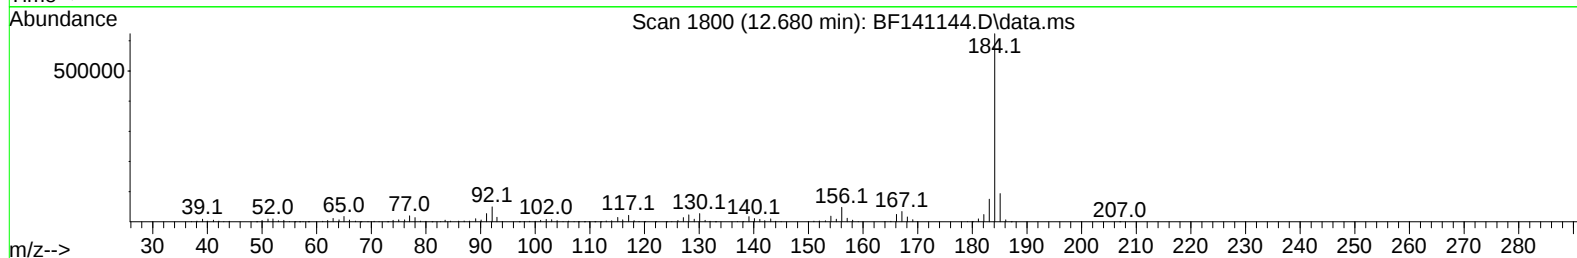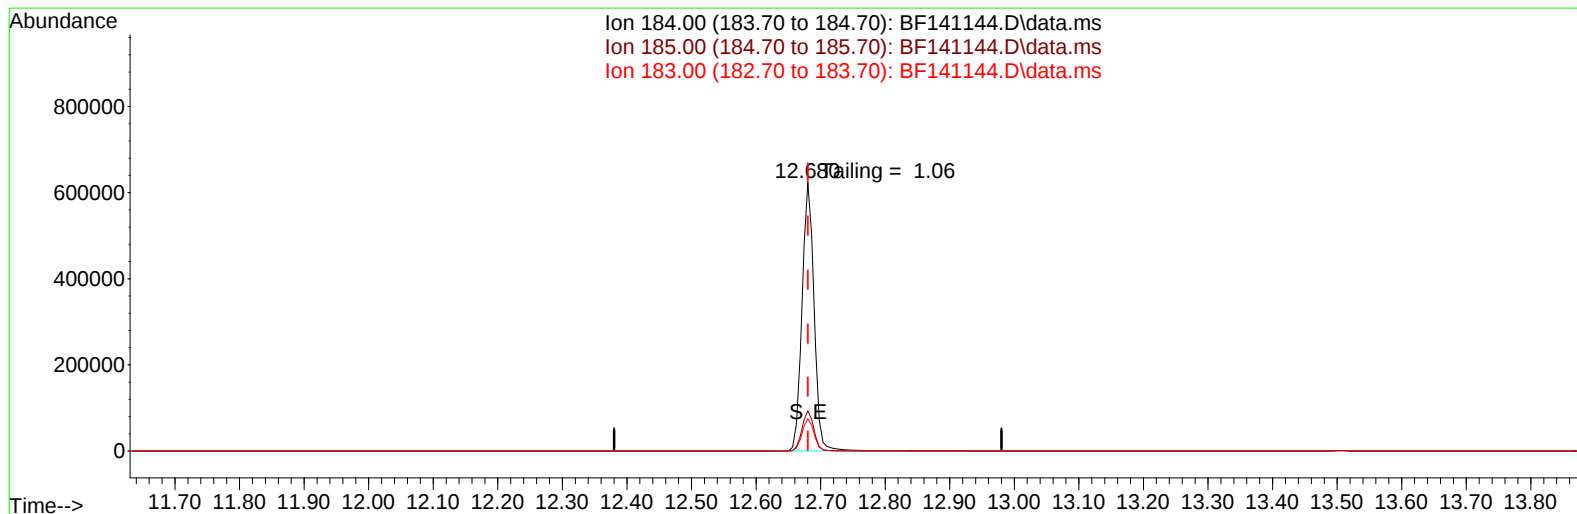

TIC: BF141144.D\data.ms

(77) Benzidine

12.680min (-0.000) 66475.81 ng

response 812384

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.97
183.00	11.50	12.04
0.00	0.00	0.00