

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011515\
 Data File : BF076905.D
 Acq On : 16 Jan 2015 5:17
 Operator : IZ / TP
 Sample : G1086-01
 Misc : W
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-09

Quant Time: Jan 16 06:11:56 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 15 11:52:04 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	35162	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	154542	20.00	ng	0.00
38) Acenaphthene-d10	15.07	164	84335	20.00	ng	-0.01
63) Phenanthrene-d10	17.82	188	141780	20.00	ng	0.00
75) Chrysene-d12	21.31	240	137697	20.00	ng	0.00
86) Perylene-d12	22.95	264	132723	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.10	112	231693	108.34	ng	0.01
7) Phenol-d6	7.42	99	265063	98.25	ng	0.00
23) Nitrobenzene-d5	9.32	82	193004	69.19	ng	0.00
41) 2,4,6-Tribromophenol	16.72	330	69490	101.51	ng	0.00
44) 2-Fluorobiphenyl	13.59	172	383427	69.19	ng	0.00
78) Terphenyl-d14	20.04	244	395954	66.20	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011515\
Data File : BF076905.D
Acq On : 16 Jan 2015 5:17
Operator : IZ / TP
Sample : G1086-01
Misc : W
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-09

Quant Time: Jan 16 06:11:56 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 15 11:52:04 2015
Response via : Initial Calibration

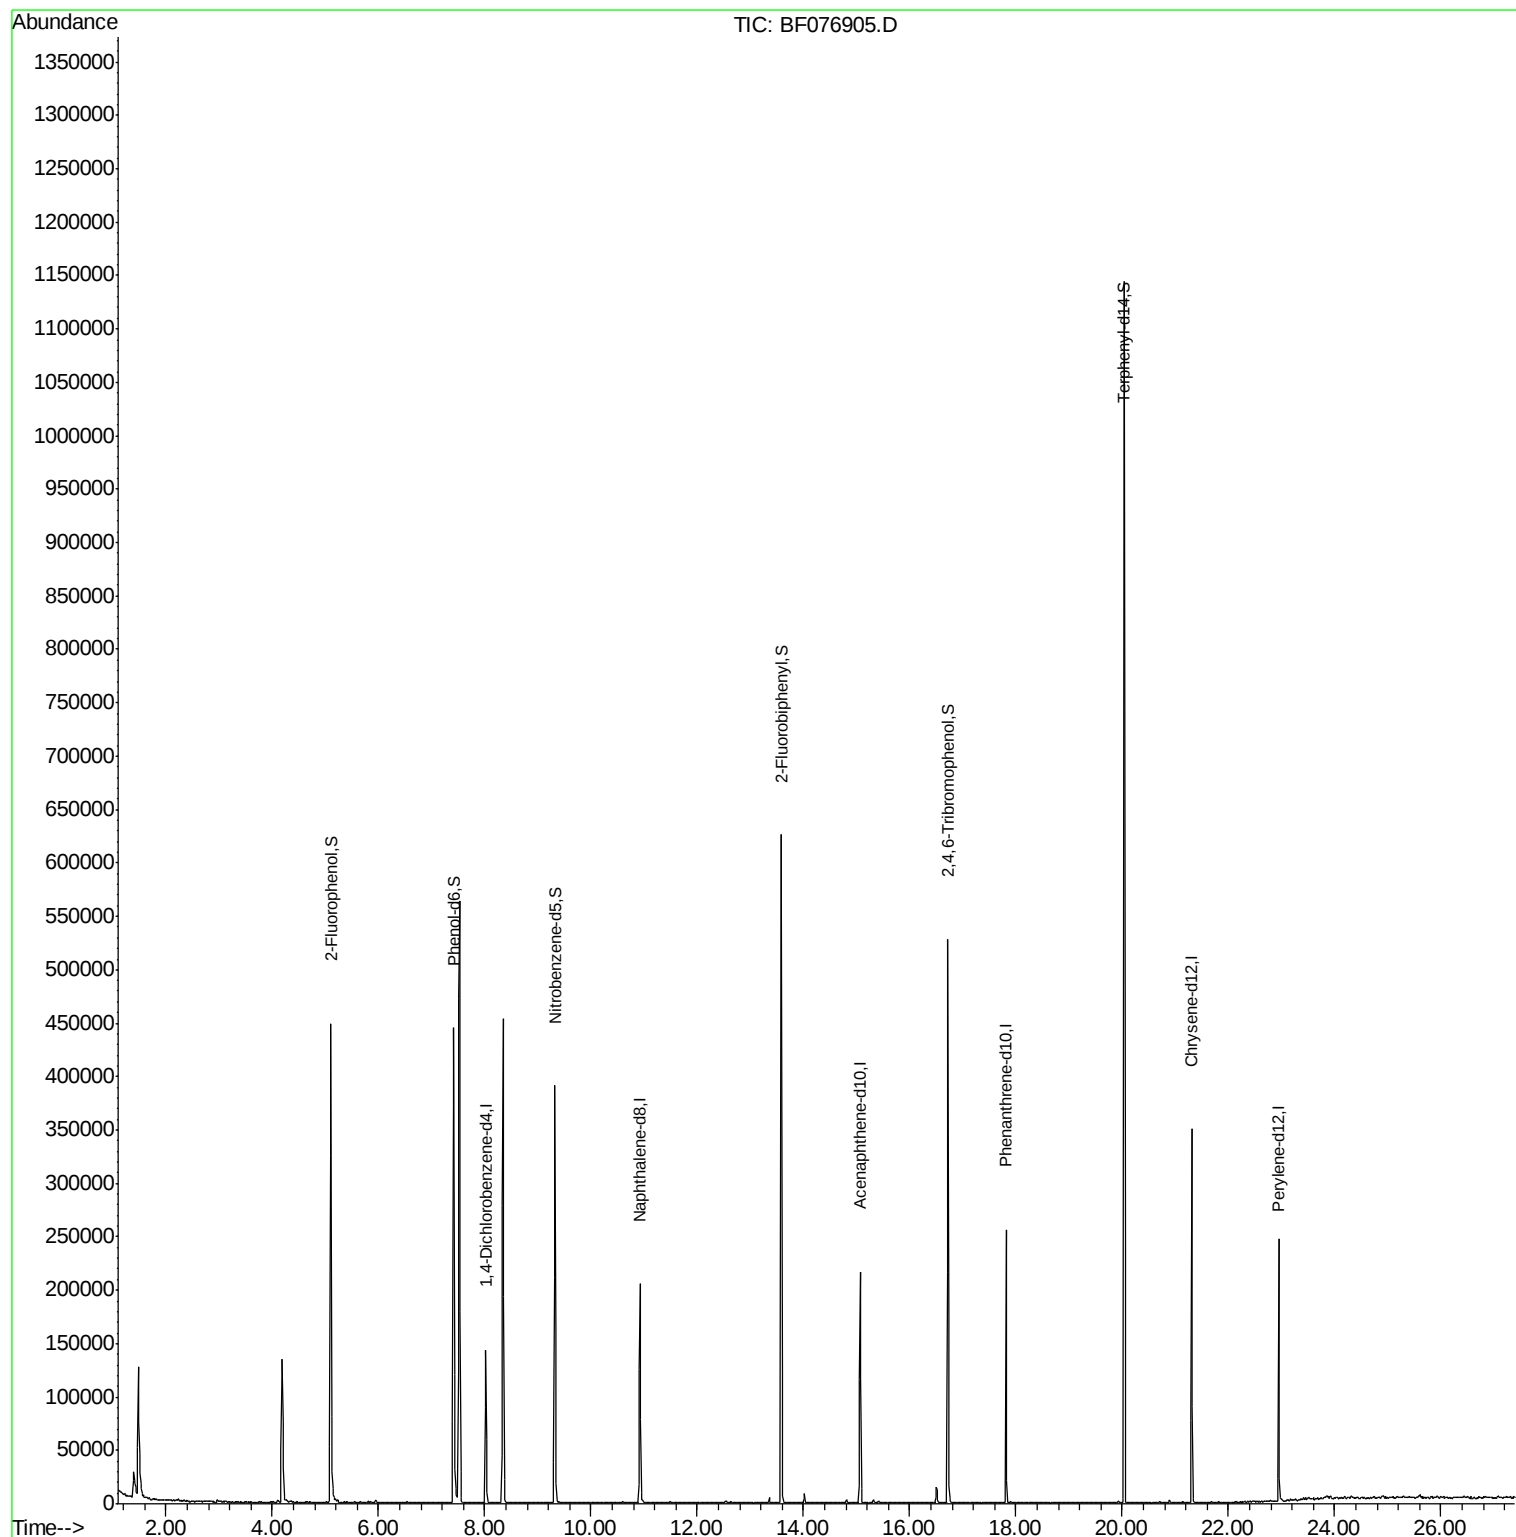

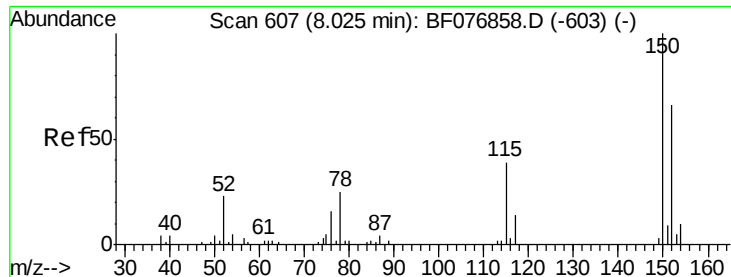


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.02 min Scan# 607
Delta R.T. 0.00 min
Lab File: BF076905.D
Acq: 16 Jan 2015 5:17

Instrument :
BNA_F
ClientSampleId :
TP-09

Tot Ion:152 Resp: 35162
Ion Ratio Lower Upper
152 100
150 159.5 121.7 182.5
115 63.6 47.0 70.6

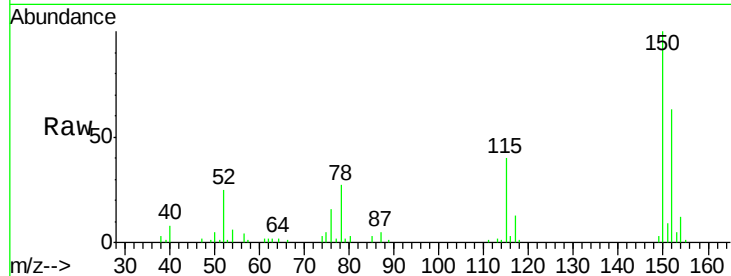


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

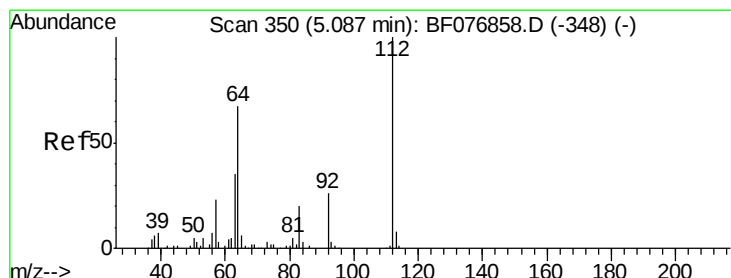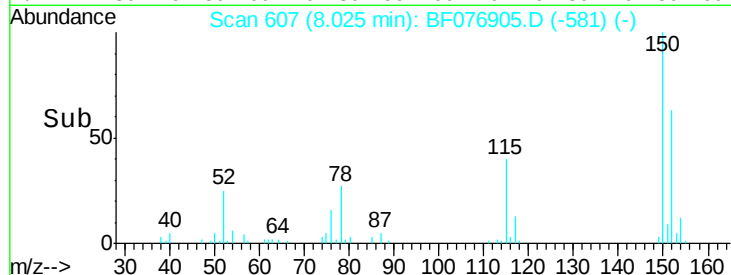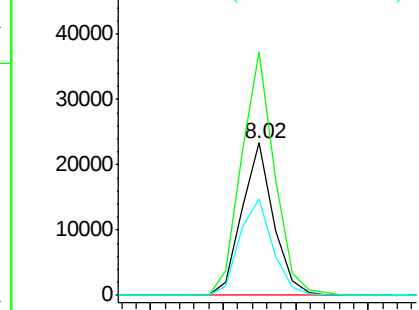



#5


2-Fluorophenol
Concen: 108.34 ng
RT: 5.10 min Scan# 351
Delta R.T. 0.01 min
Lab File: BF076905.D
Acq: 16 Jan 2015 5:17

Tgt Ion:112 Resp: 231693
Ion Ratio Lower Upper
112 100
64 62.2 54.2 81.4
63 34.7 28.4 42.6

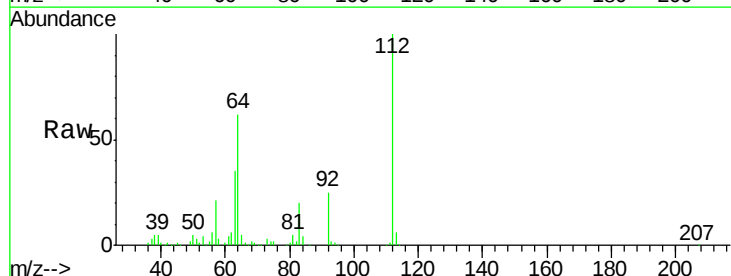

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

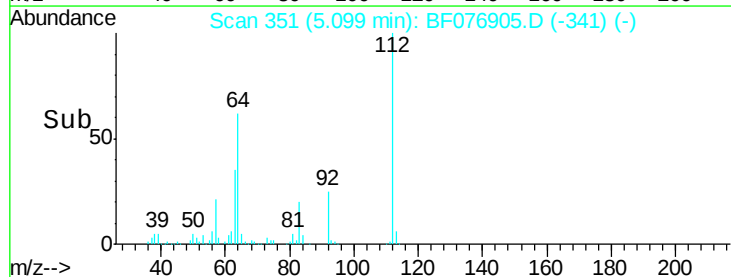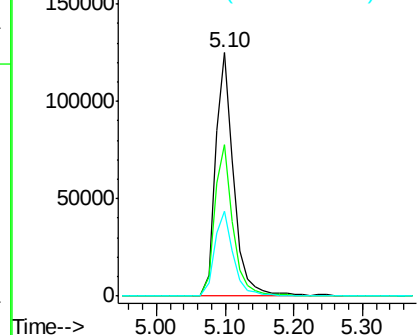

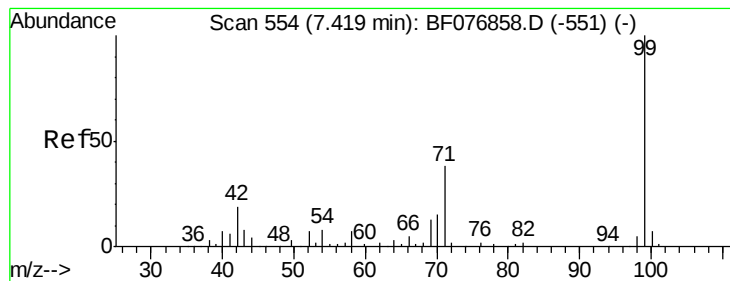

#7

Phenol-d6

Concen: 98.25 ng

RT: 7.42 min Scan# 554

Delta R.T. 0.00 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17

Instrument :

BNA_F

ClientSampleId :

TP-09


Tot Ion: 99 Resp: 265063

Ion Ratio Lower Upper

99 100

42 16.0 15.0 22.4




71 36.9 30.5 45.7

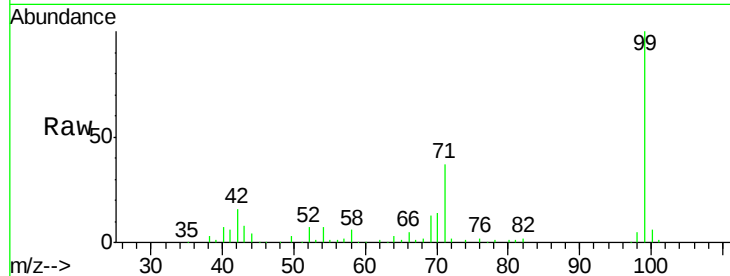

Abundance Ion 99.00 (98.70 to 99.70): BF076858.D (-551) (-)

Ion 42.00 (41.70 to 42.70): BF076858.D (-551) (-)

Ion 71.00 (70.70 to 71.70): BF076858.D (-551) (-)

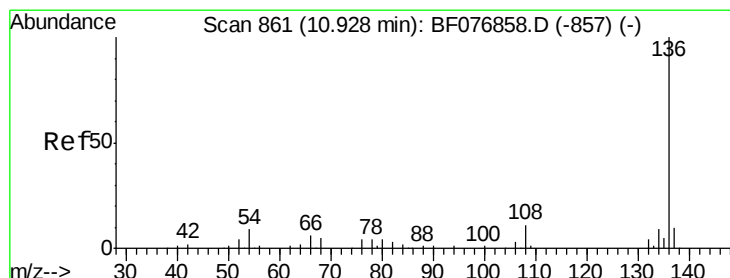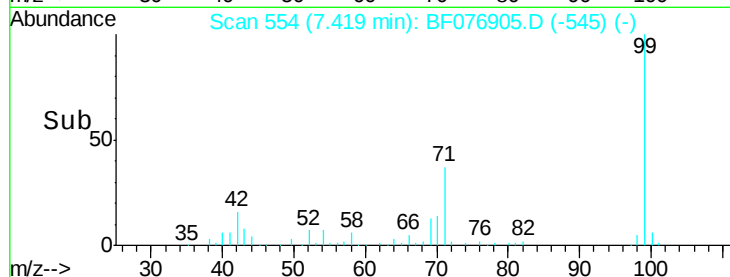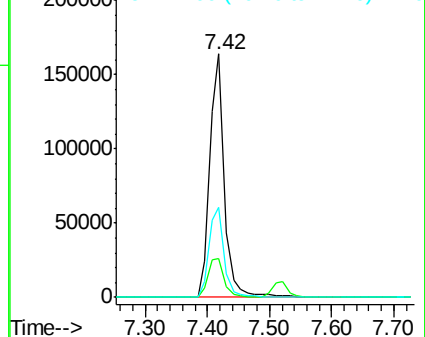

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 861

Delta R.T. 0.00 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17

Tgt Ion: 136 Resp: 154542


Ion Ratio Lower Upper

136 100

137 10.7 8.1 12.1

54 7.4 7.0 10.4

68 3.7 3.7 5.5


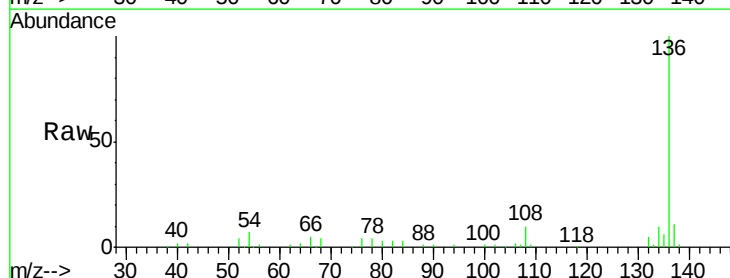


Abundance Ion 136.00 (135.70 to 136.70): BF076858.D (-857) (-)

Ion 137.00 (136.70 to 137.70): BF076858.D (-857) (-)

Ion 54.00 (53.70 to 54.70): BF076858.D (-857) (-)

Ion 68.00 (67.70 to 68.70): BF076858.D (-857) (-)



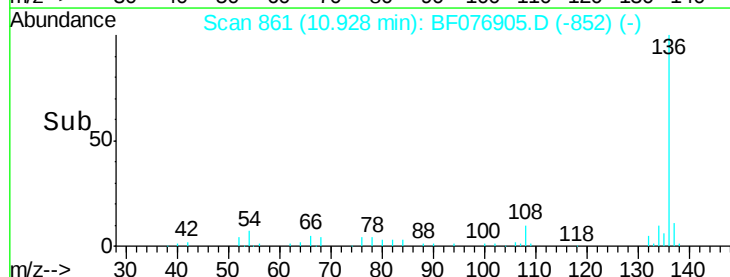
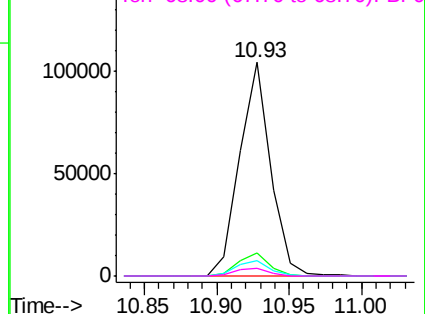




#23
 Nitrobenzene-d5
 Concen: 69.19 ng
 RT: 9.32 min Scan# 720
 Delta R.T. 0.00 min
 Lab File: BF076905.D
 Acq: 16 Jan 2015 5:17




Instrument :
 BNA_F
 ClientSampleId :
 TP-09

Tot Ion	82	Resp	193004
Ion Ratio	Lower	Upper	
82	100		
128	42.5	33.1	49.7
54	58.9	48.3	72.5

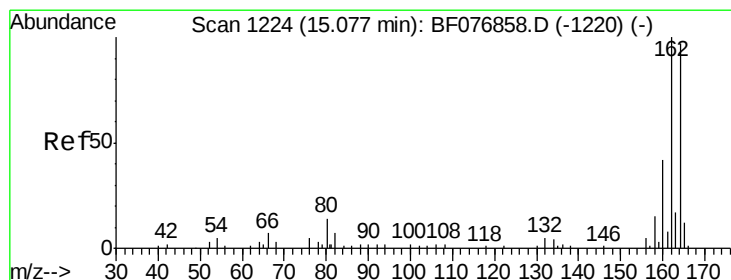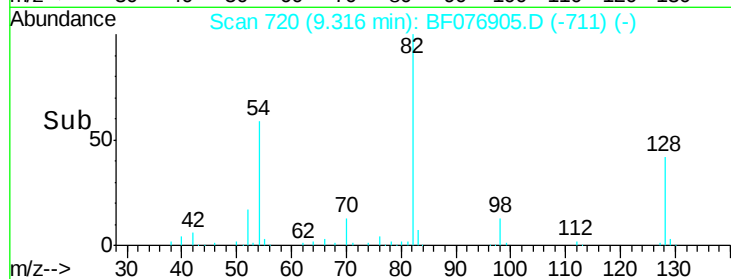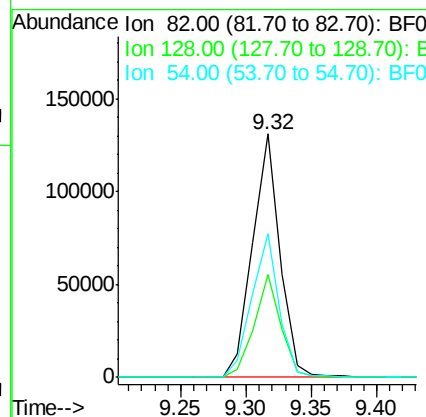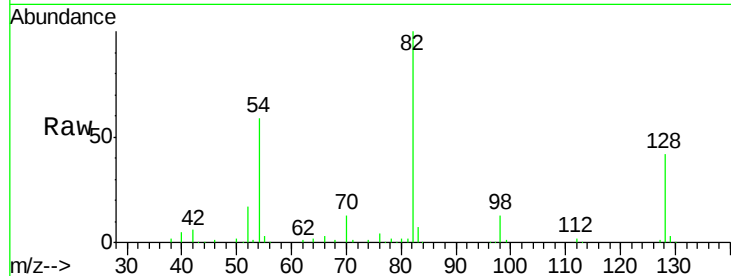

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.07 min Scan# 1223
 Delta R.T. -0.01 min
 Lab File: BF076905.D
 Acq: 16 Jan 2015 5:17

Tgt Ion	164	Resp	84335
Ion Ratio	Lower	Upper	
164	100		
162	98.4	82.4	123.6
160	41.8	34.8	52.2

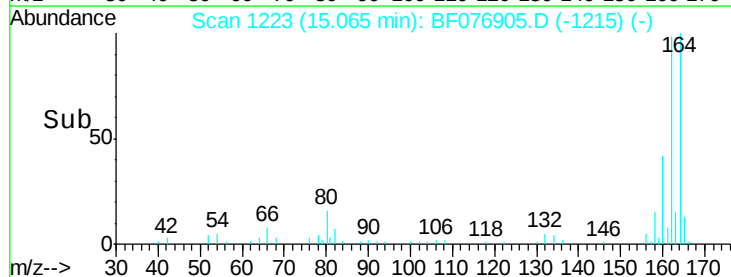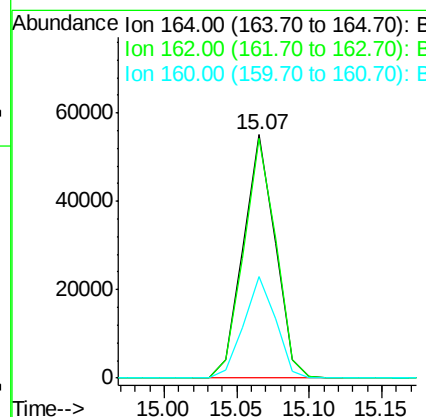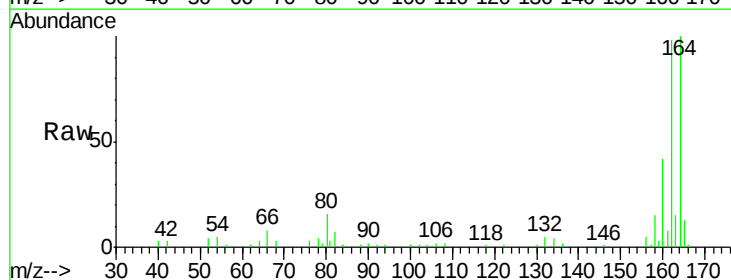



#41

2,4,6-Tribromophenol

Concen: 101.51 ng

RT: 16.72 min Scan# 1368

Delta R.T. 0.00 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17

Instrument :

BNA_F

ClientSampleId :

TP-09


Tot Ion:330 Resp: 69490

Ion Ratio Lower Upper

330 100

332 97.9 77.8 116.6




141 50.3 38.5 57.7

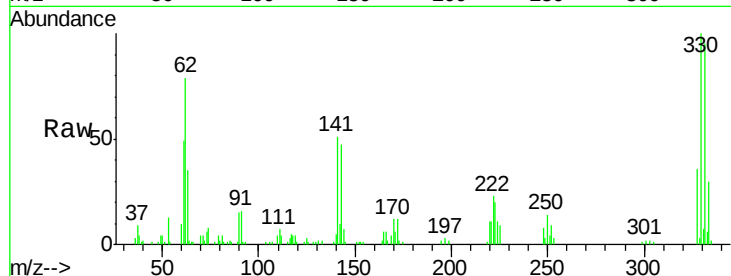

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

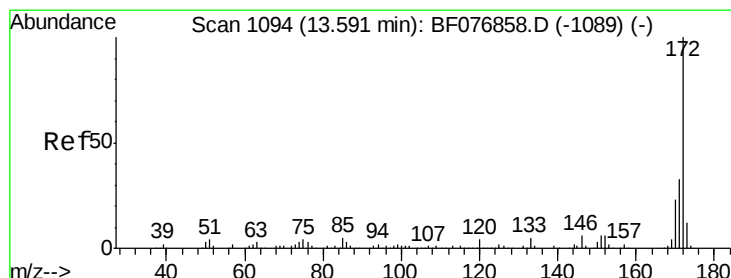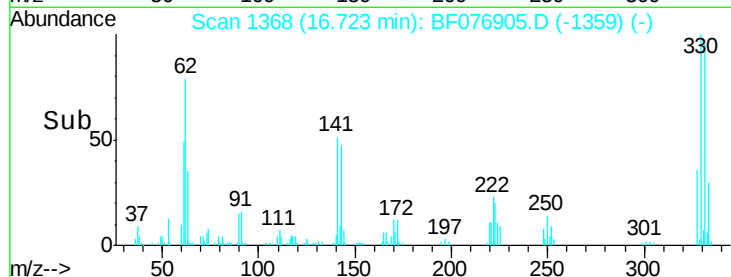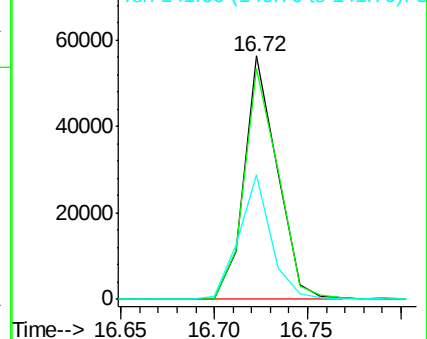

#44

2-Fluorobiphenyl

Concen: 69.19 ng

RT: 13.59 min Scan# 1094

Delta R.T. 0.00 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17


Tgt Ion:172 Resp: 383427

Ion Ratio Lower Upper

172 100

171 33.7 26.6 40.0



170 23.3 18.0 27.0

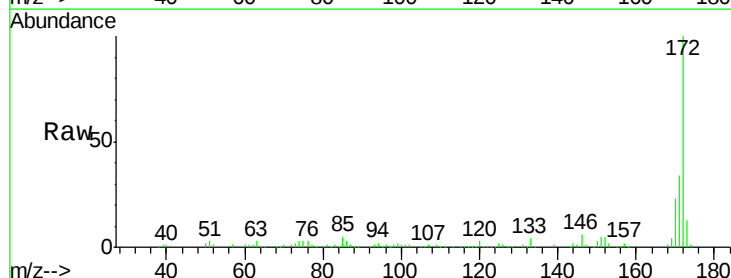

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

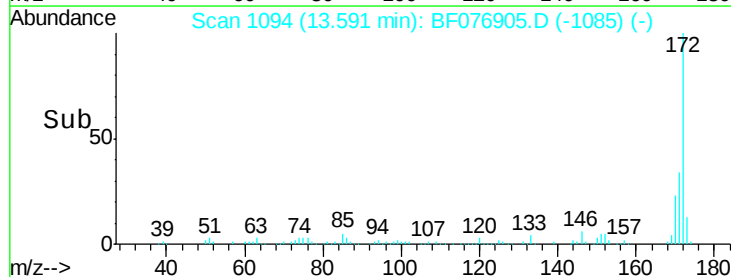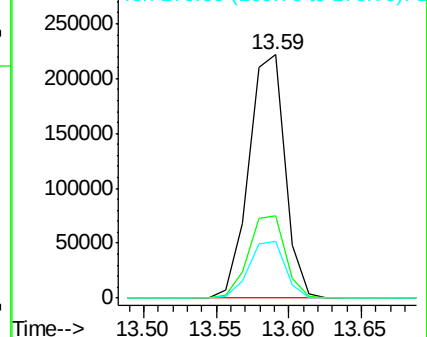






#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.82 min Scan# 1464
Delta R.T. 0.00 min
Lab File: BF076905.D
Acq: 16 Jan 2015 5:17

Instrument :
BNA_F
ClientSampleId :
TP-09

Tot Ion	Ratio	Lower	Upper
188	100		
94	6.2	6.0	9.0
80	7.3	6.9	10.3

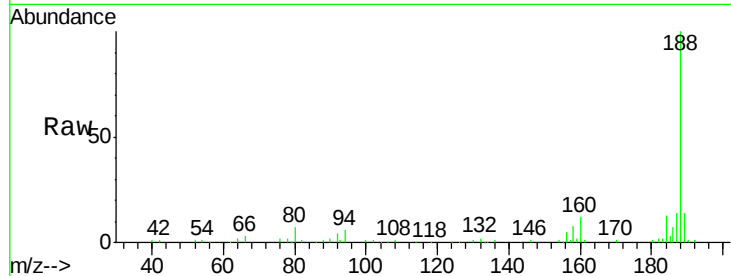


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

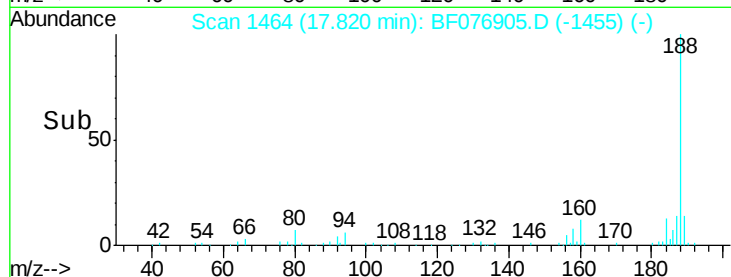
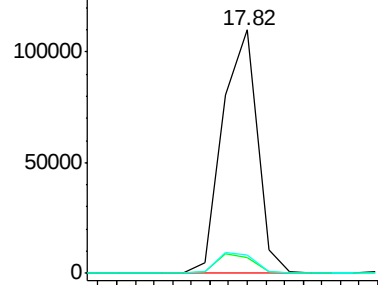


#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.31 min Scan# 1769
Delta R.T. 0.00 min
Lab File: BF076905.D
Acq: 16 Jan 2015 5:17

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.7	10.4	15.6
236	25.8	20.2	30.2

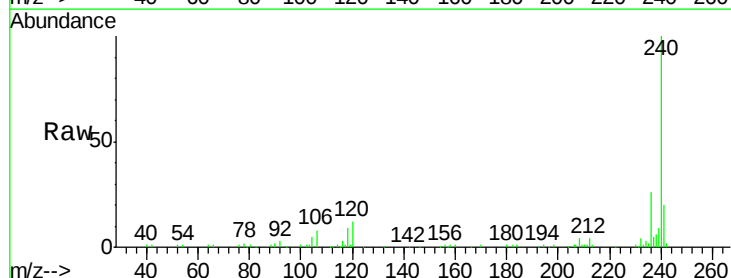

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

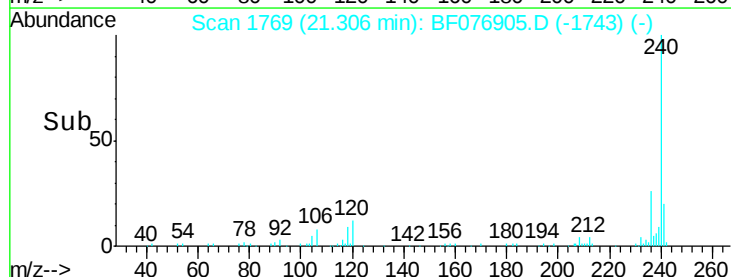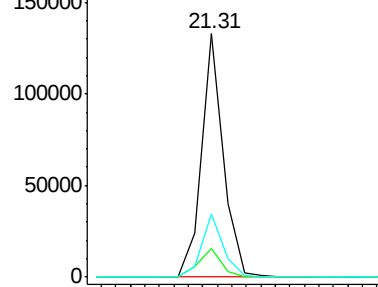



#78

Terphenyl-d14

Concen: 66.20 ng

RT: 20.04 min Scan# 1658

Delta R.T. 0.00 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17

Instrument :

BNA_F

ClientSampleId :

TP-09


Tot Ion:244 Resp: 395954

Ion Ratio Lower Upper

244 100

212 7.4 6.3 9.5




122 12.1 10.1 15.1

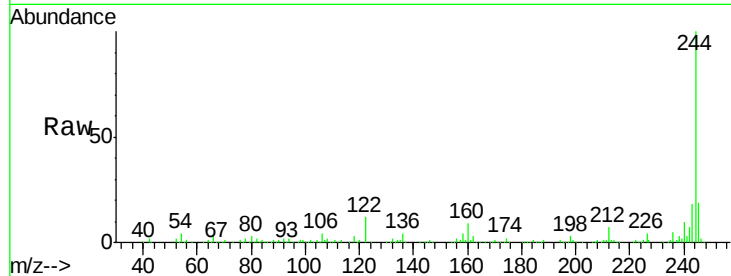

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

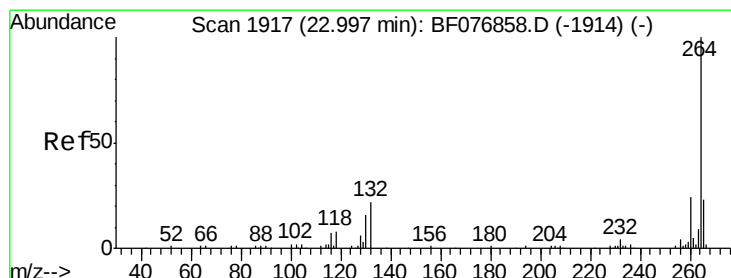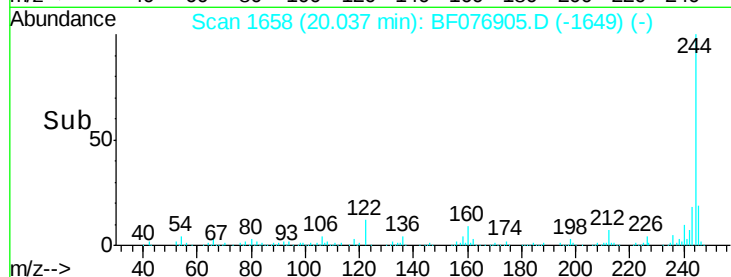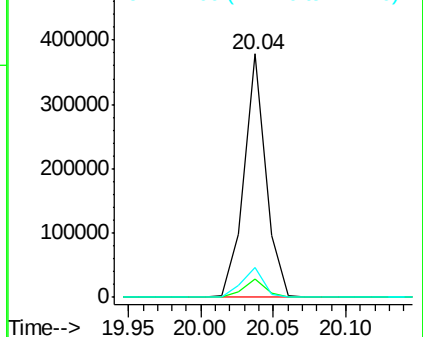

#86

Perylene-d12

Concen: 20.00 ng

RT: 22.95 min Scan# 1913

Delta R.T. -0.05 min

Lab File: BF076905.D

Acq: 16 Jan 2015 5:17


Tgt Ion:264 Resp: 132723

Ion Ratio Lower Upper

264 100

260 22.5 19.0 28.4

265 19.9 18.1 27.1

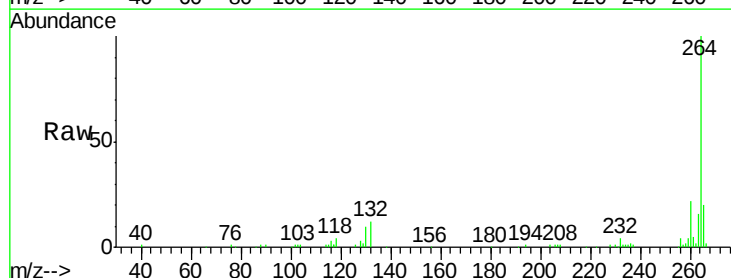

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

