
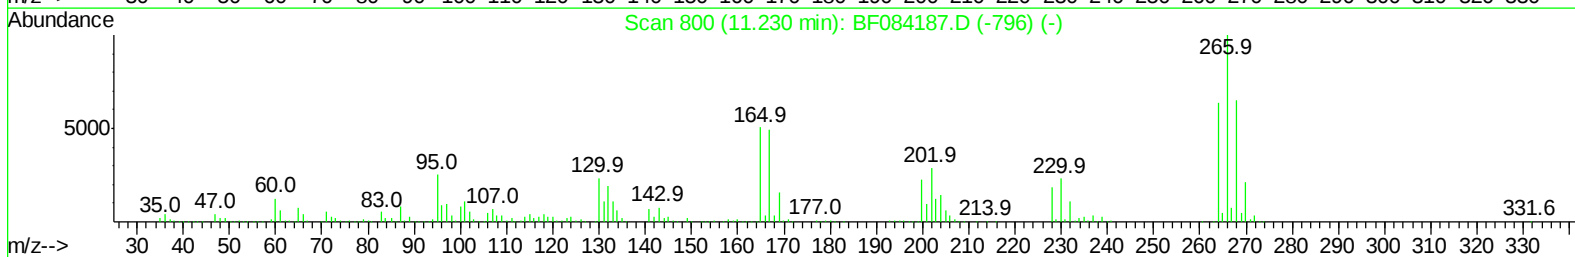
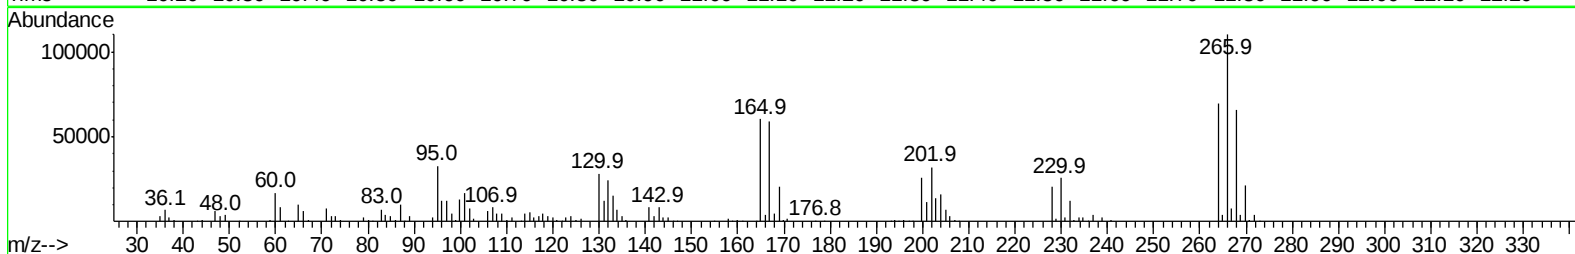


Data Path : U:\HPCHEM1\BNA F\DATA\BF011516\
Data File : BF084485.D
Acq On : 15 Jan 2016 10:41
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 04:53:44 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 16 03:20:07 2016
Response via : Initial Calibration

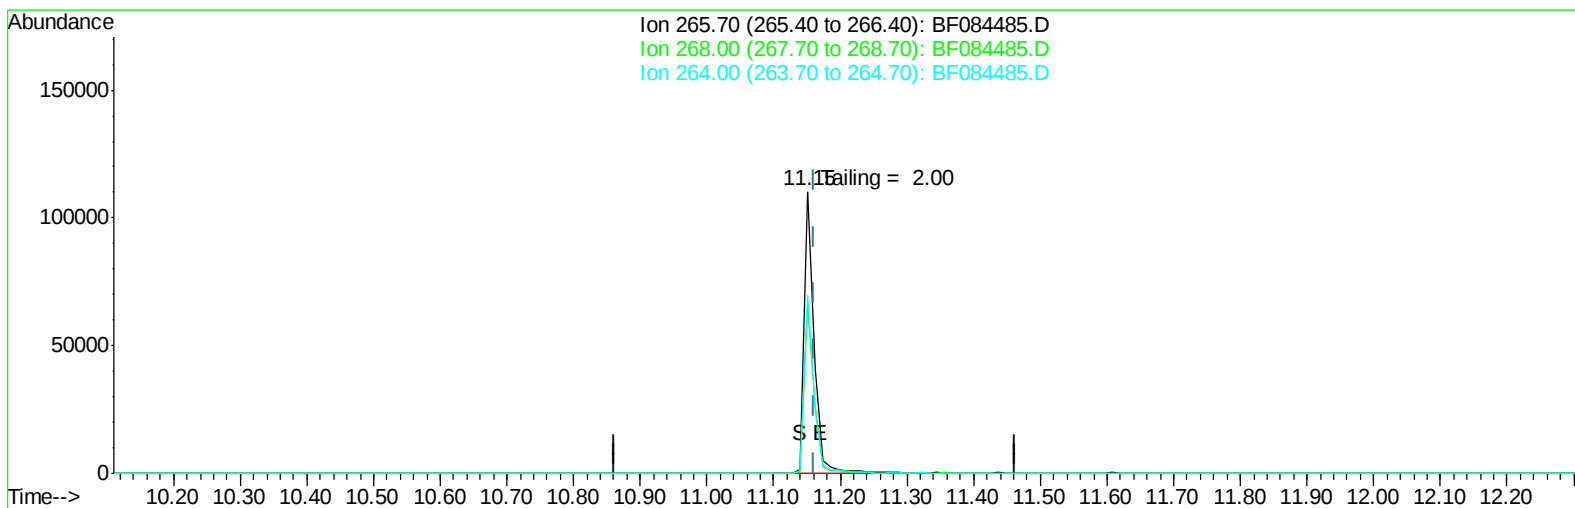

TIC: BF084485.D

(69) Pentachlorophenol (C)

11.150min (-0.012) 0.00ng

response 114336

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	59.80
264.00	62.70	63.17
0.00	0.00	0.00