
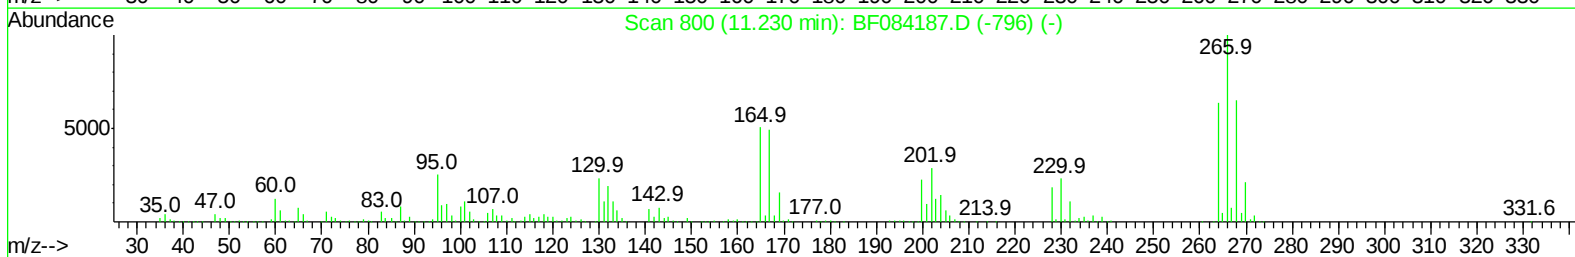
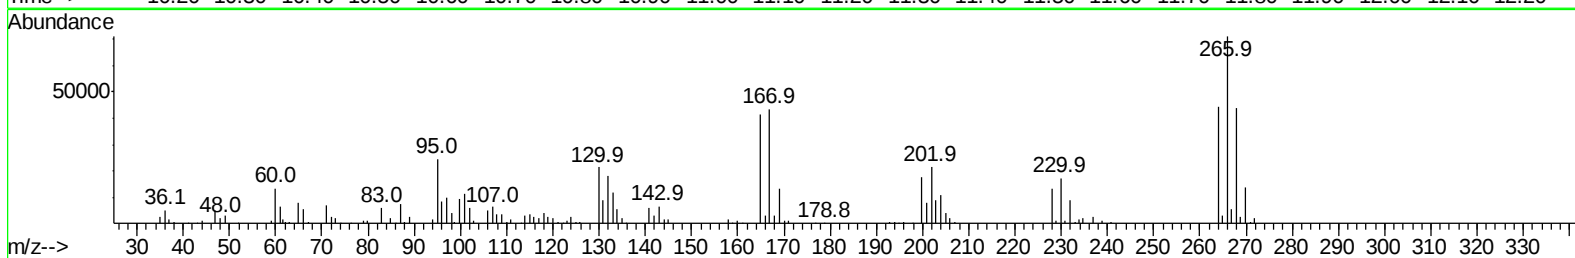


Data Path : U:\HPCHEM1\BNA F\DATA\BF011516\
Data File : BF084508.D
Acq On : 15 Jan 2016 23:18
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 04:54:38 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 16 03:20:07 2016
Response via : Initial Calibration

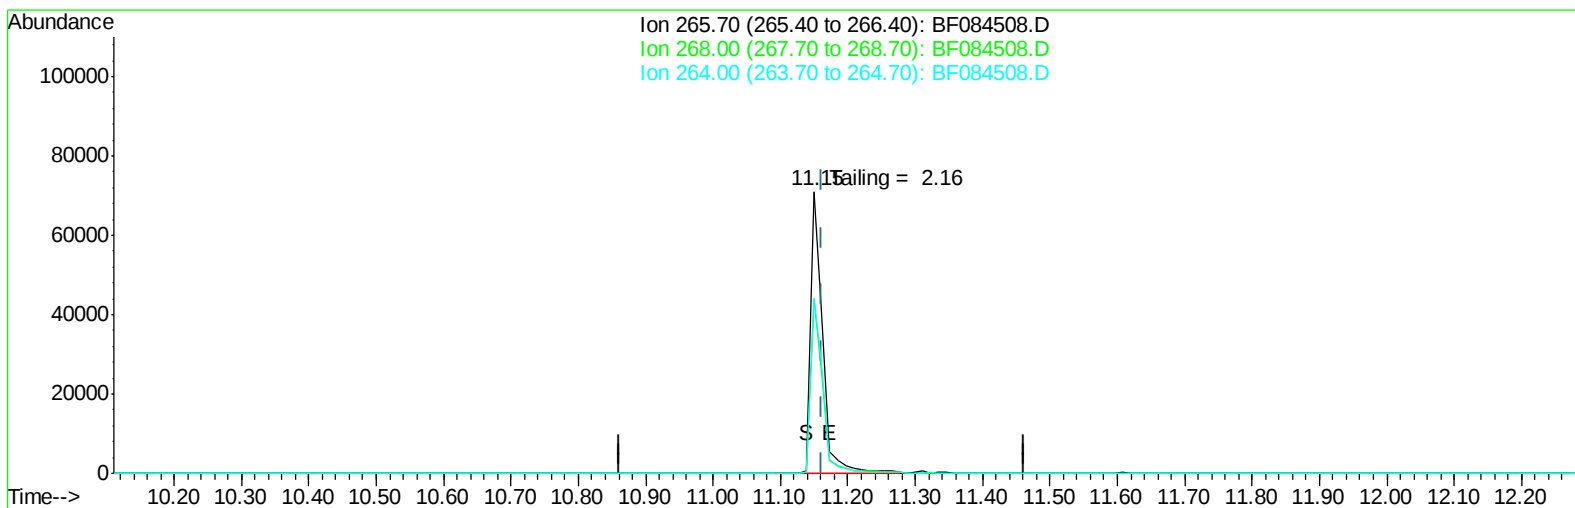

TIC: BF084508.D

(69) Pentachlorophenol (C)




11.151min (-0.012) 0.00ng

response 87258

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.83
264.00	62.70	62.43
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011516\
Data File : BF084508.D
Acq On : 15 Jan 2016 23:18
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 04:54:38 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 16 03:20:07 2016
Response via : Initial Calibration

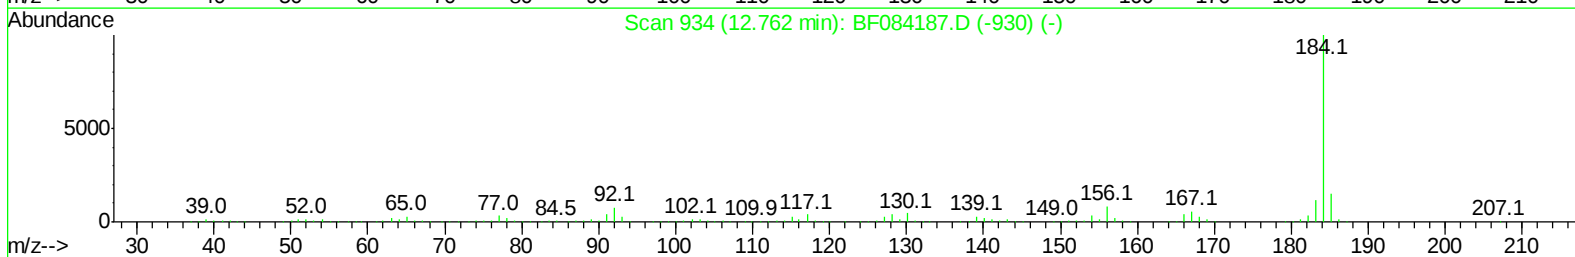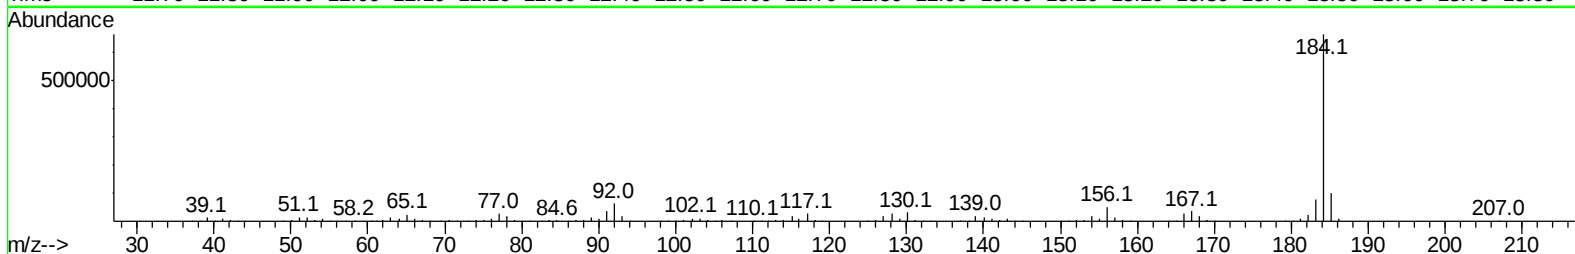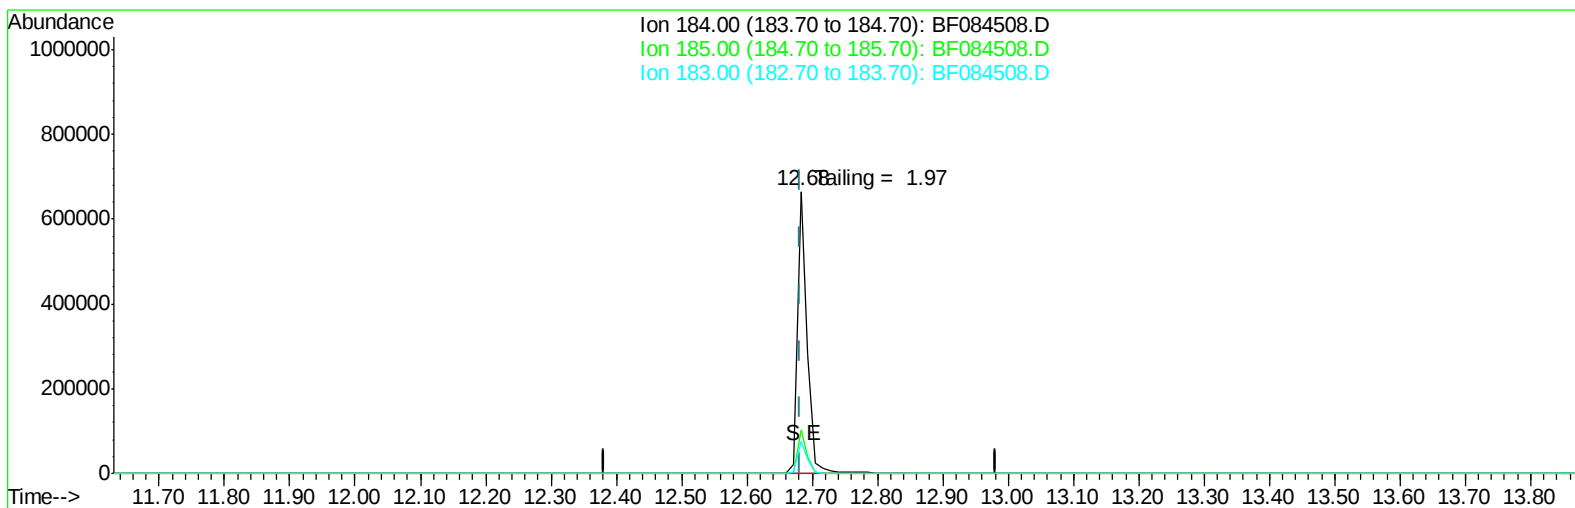

TIC: BF084508.D

(76) Benzidine

12.682min (-0.000) 62868.15ng

response 705546

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.26
183.00	12.30	11.59
0.00	0.00	0.00