


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011516\
Data File : BF084485.D
Acq On : 15 Jan 2016 10:41
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 14 14:15:52 2016

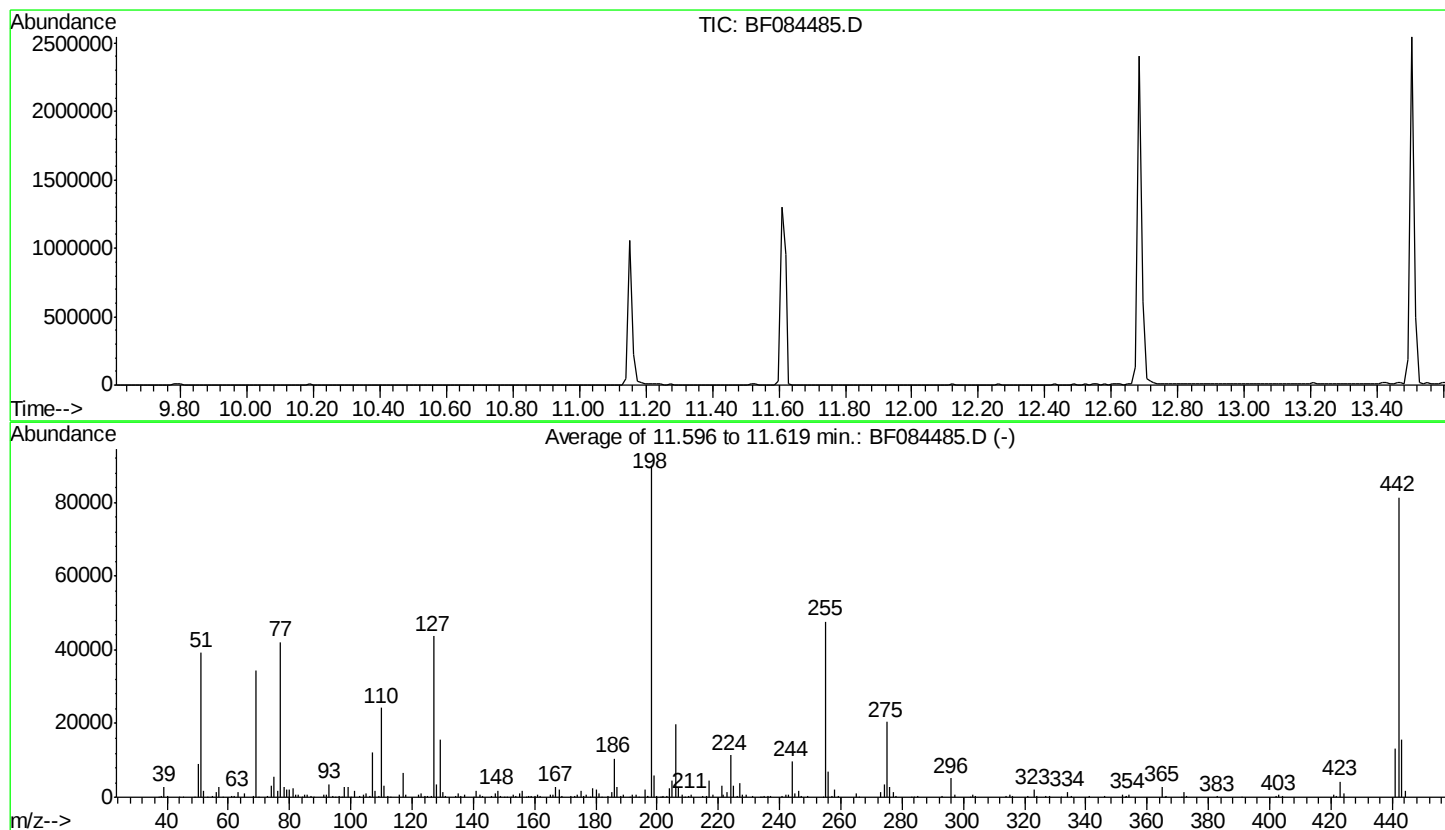

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	39208	PASS
68	69	0.00	2	1.3	458	PASS
69	198	0.00	100	38.3	34477	PASS
70	69	0.00	2	0.5	177	PASS
127	198	10	80	48.5	43631	PASS
197	198	0.00	2	0.2	212	PASS
198	198	100	100	100.0	90027	PASS
199	198	5	9	6.6	5897	PASS
275	198	10	60	22.6	20362	PASS
365	198	1	100	3.2	2868	PASS
441	442	0.01	24	16.4	13315	PASS
442	198	50	100	90.4	81418	PASS
443	442	15	24	19.2	15642	PASS