


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011516\
 Data File : BF084508.D
 Acq On : 15 Jan 2016 23:18
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

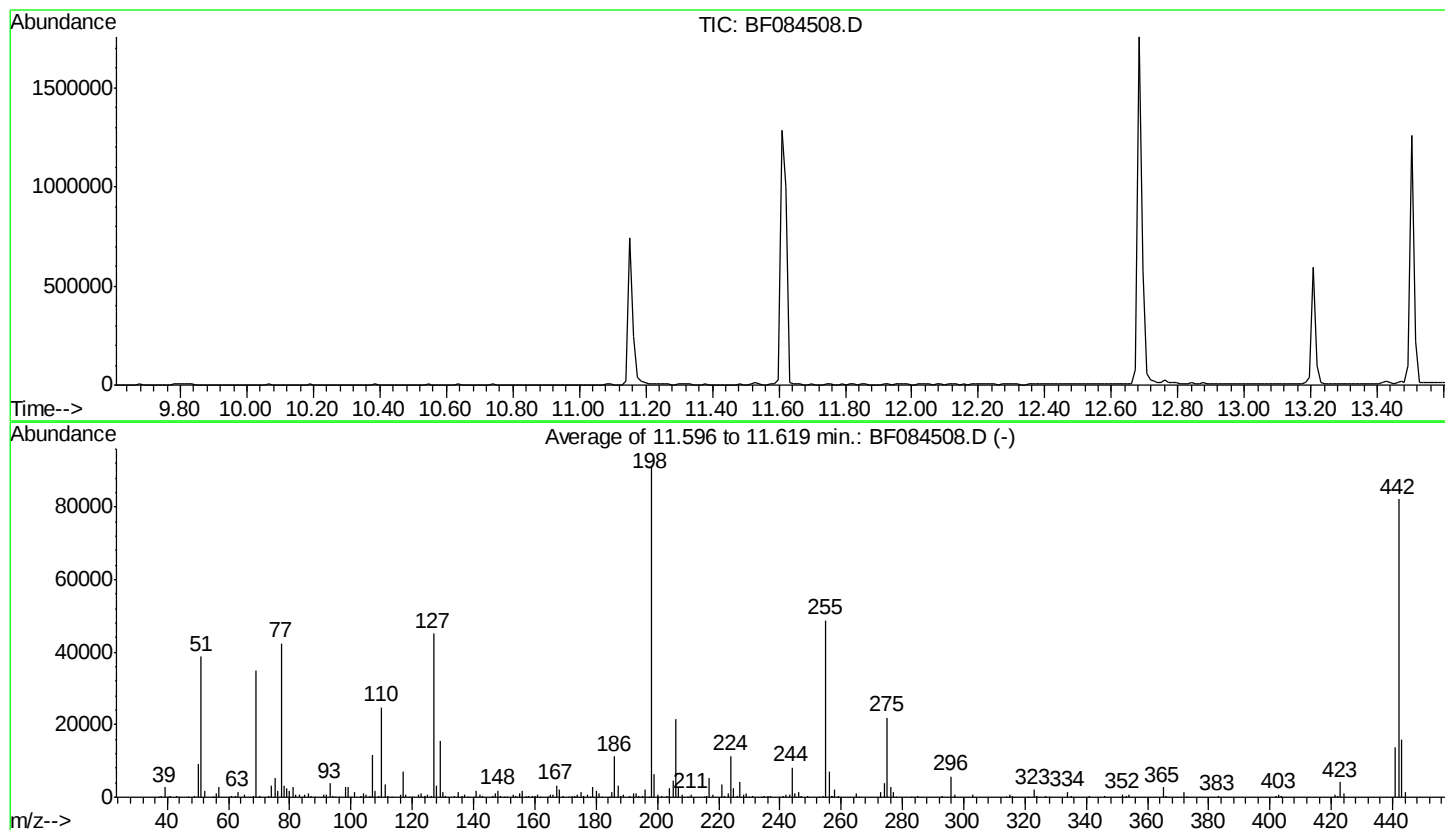

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	38726	PASS
68	69	0.00	2	1.1	385	PASS
69	198	0.00	100	38.3	35061	PASS
70	69	0.00	2	0.6	217	PASS
127	198	10	80	49.3	45074	PASS
197	198	0.00	2	0.1	123	PASS
198	198	100	100	100.0	91449	PASS
199	198	5	9	6.9	6279	PASS
275	198	10	60	24.0	21968	PASS
365	198	1	100	3.0	2735	PASS
441	442	0.01	24	16.7	13739	PASS
442	198	50	100	89.8	82093	PASS
443	442	15	24	19.4	15885	PASS