
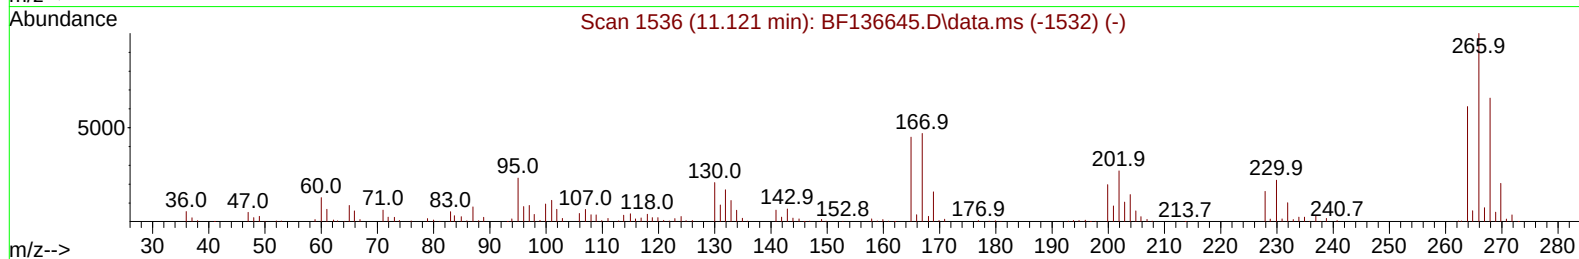
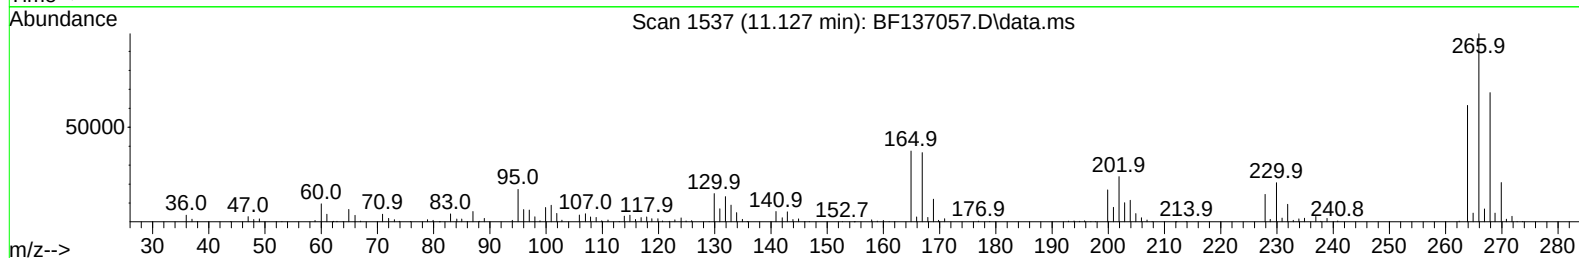


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011524\
Data File : BF137057.D
Acq On : 15 Jan 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 16:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

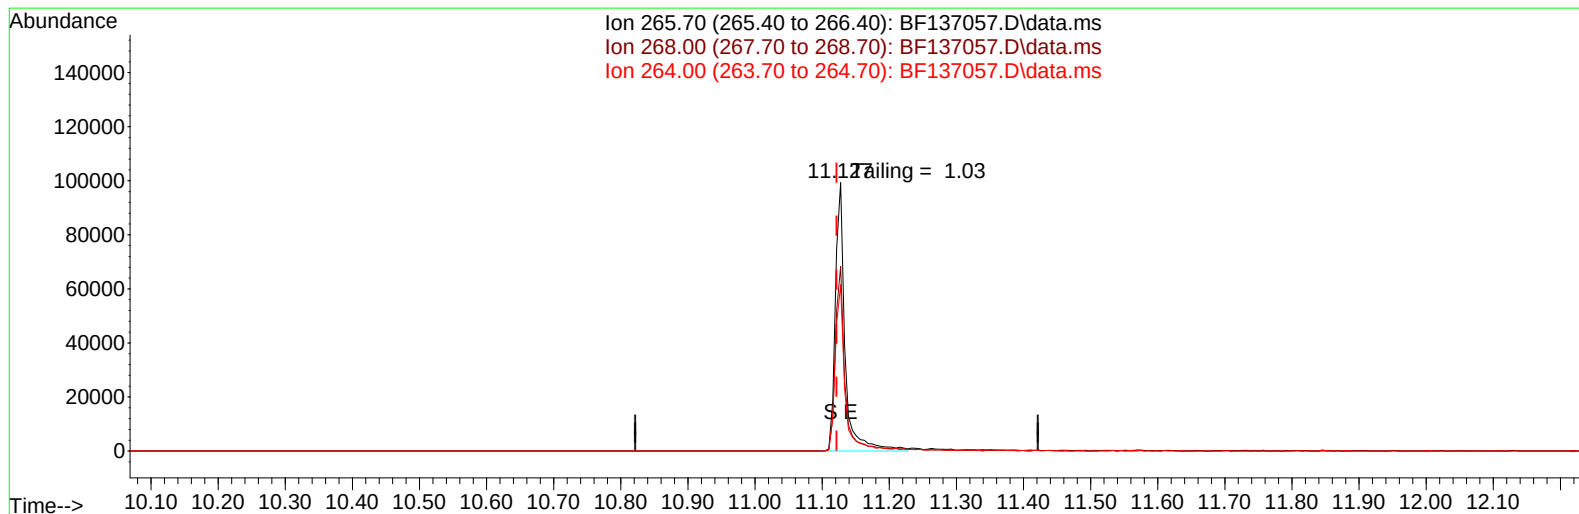

TIC: BF137057.D\data.ms




(70) Pentachlorophenol (C)

11.127min (+ 0.006) 29690.29 ng

response 100368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.77
264.00	61.20	61.94
0.00	0.00	0.00

Quant Time: Jan 15 16:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

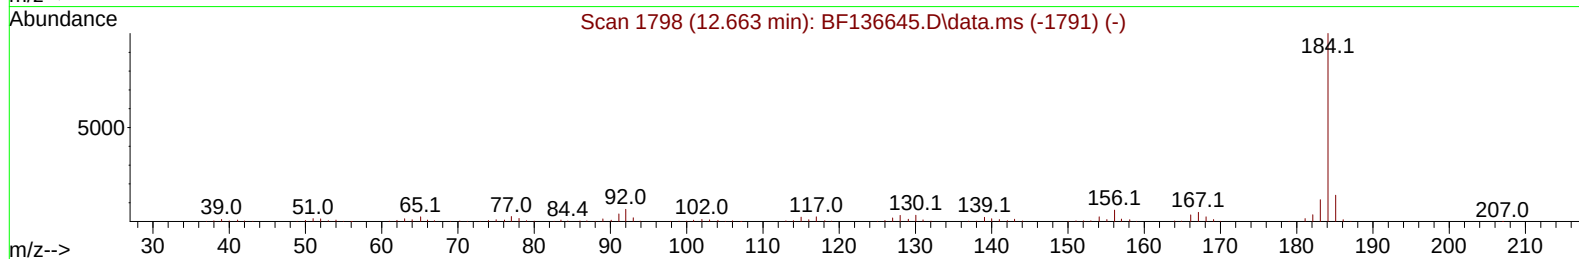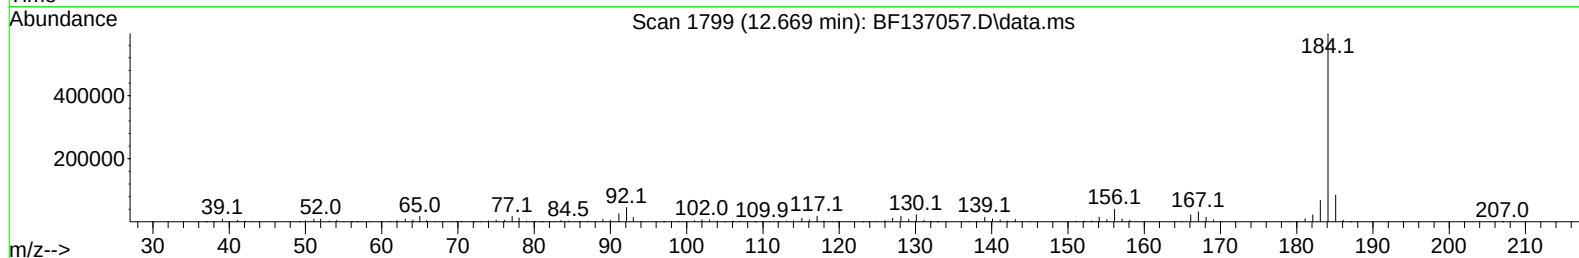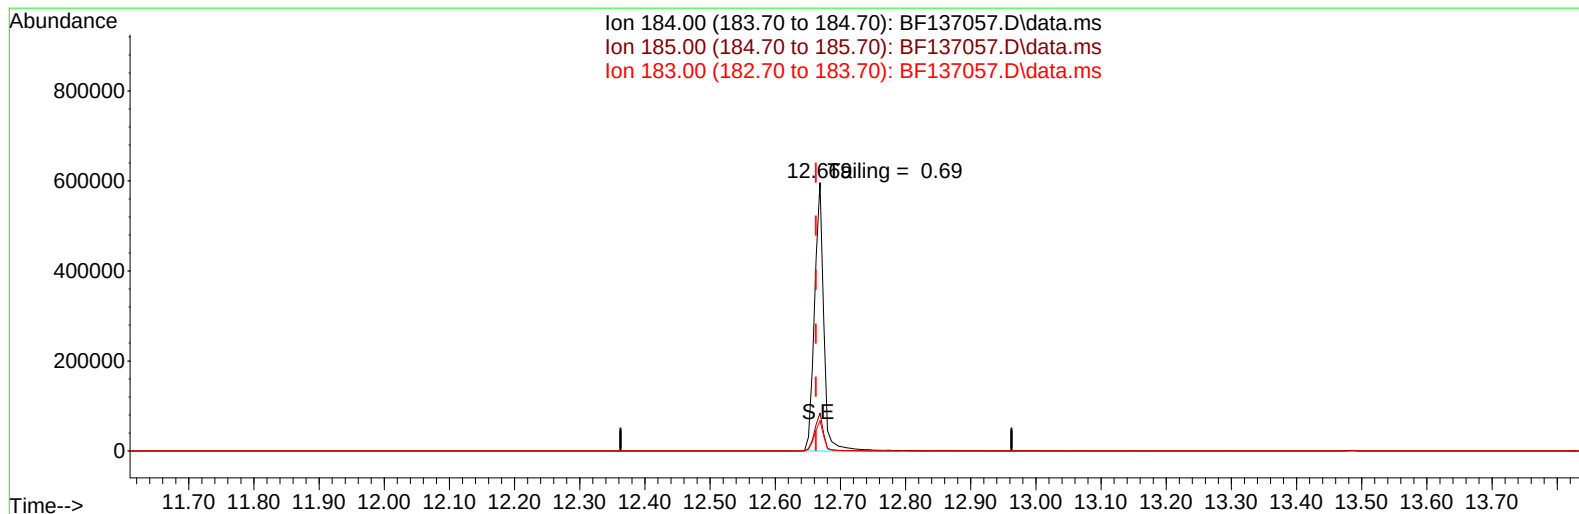

TIC: BF137057.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response **591864**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	11.60	11.34
0.00	0.00	0.00