


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011524\
Data File : BF137057.D
Acq On : 15 Jan 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

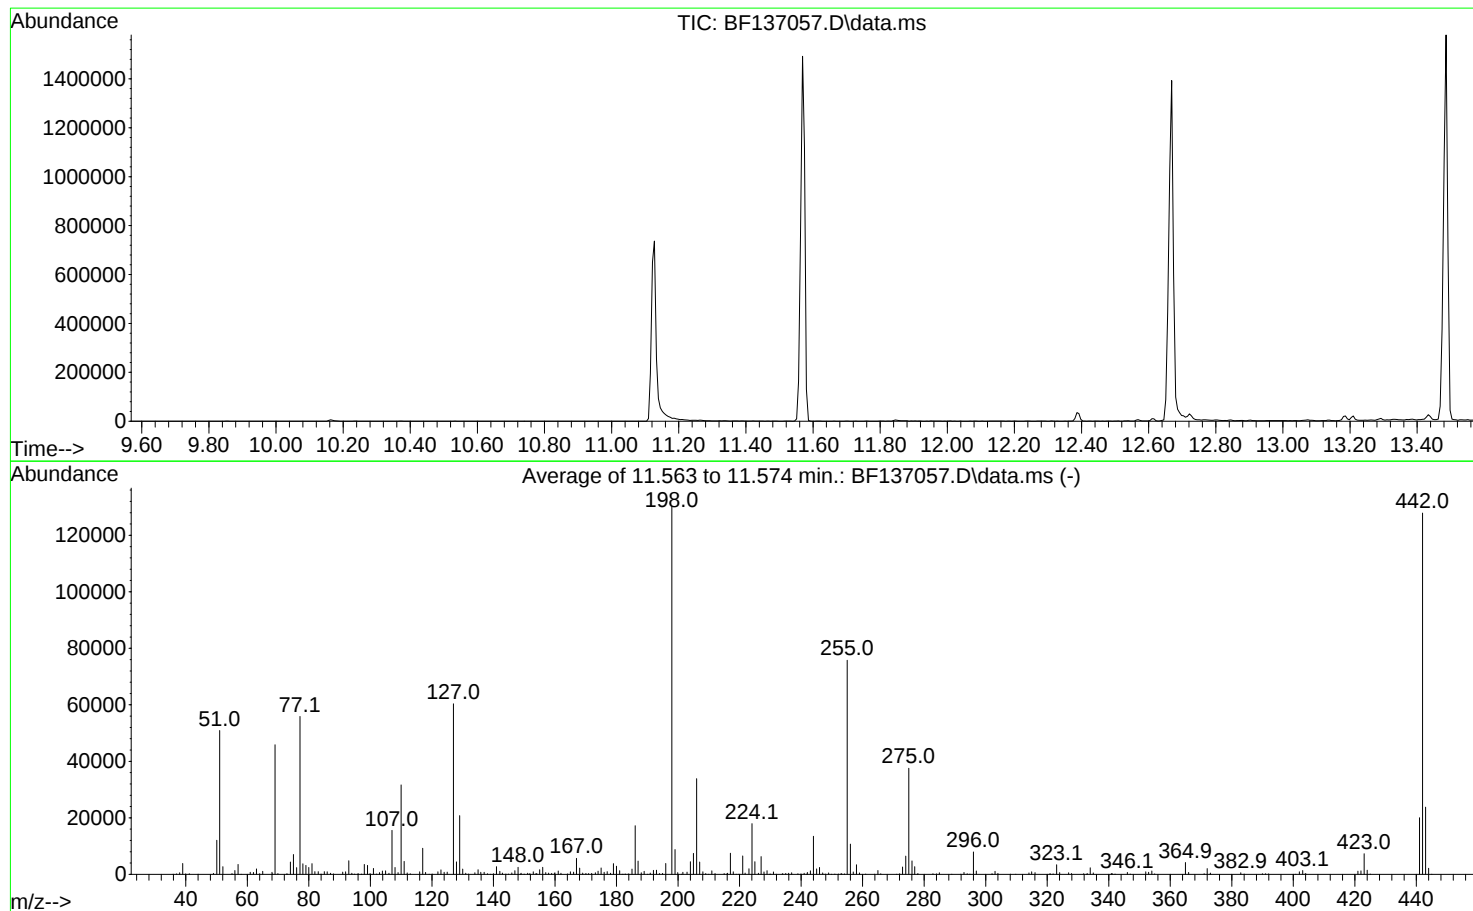




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	50925	PASS
68	69	0.00	2	1.6	754	PASS
69	198	0.00	100	35.3	45896	PASS
70	69	0.00	2	0.7	316	PASS
127	198	10	80	46.4	60392	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	130187	PASS
199	198	5	9	6.7	8760	PASS
275	198	10	60	28.9	37568	PASS
365	198	1	100	3.2	4222	PASS
441	198	0.01	100	15.4	20062	PASS
442	442	50	100	100.0	127861	PASS
443	442	15	24	18.6	23794	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011524\
Data File : BF137057.D
Acq On : 15 Jan 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 15 16:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

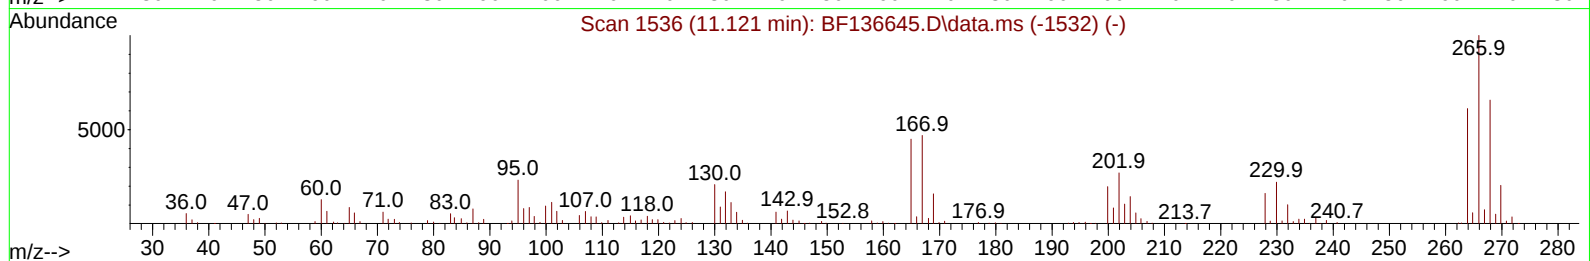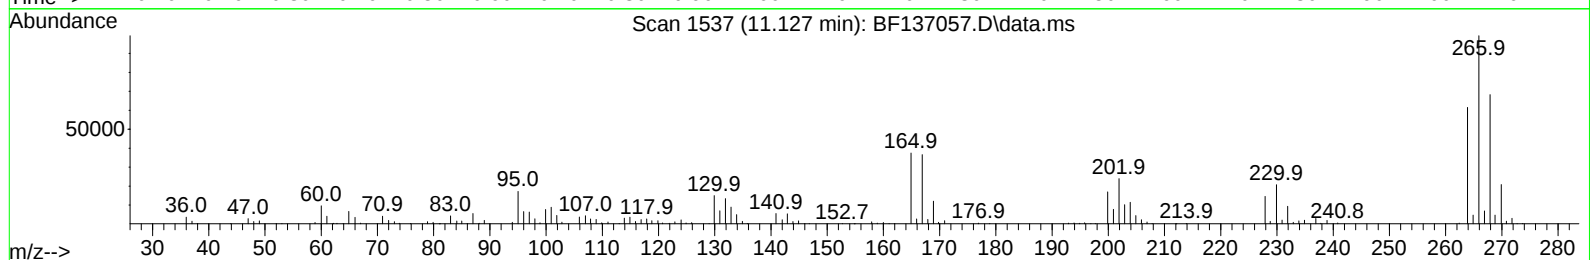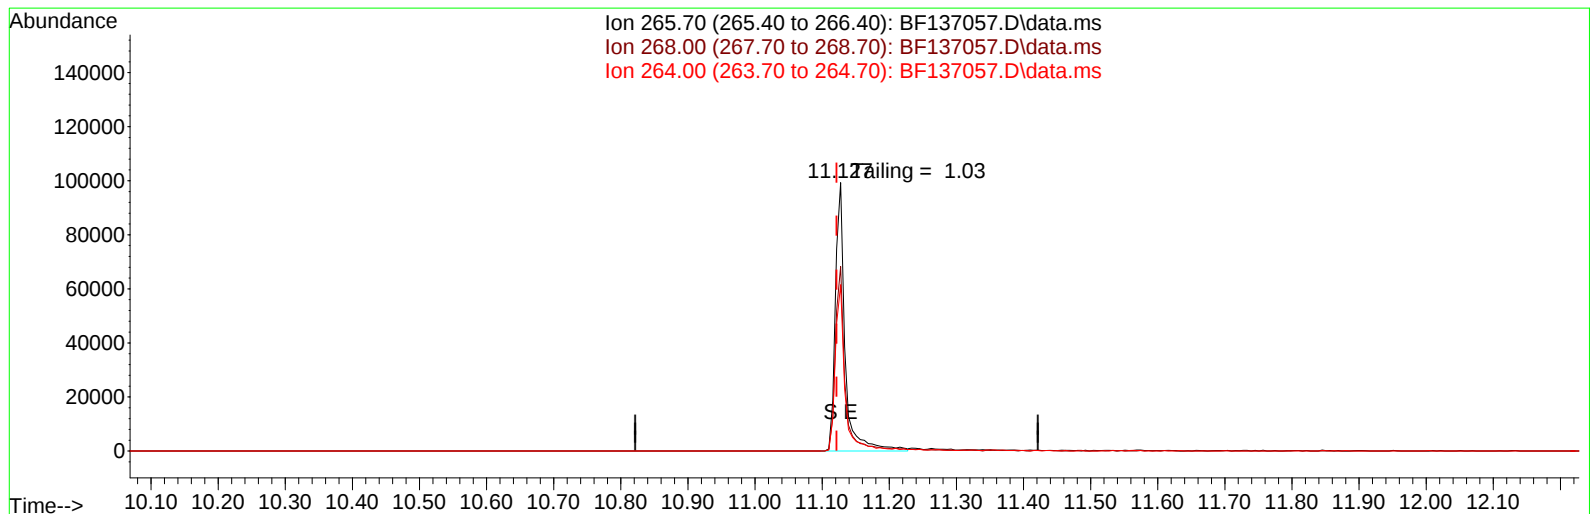

TIC: BF137057.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.006) 29690.29 ng




response 100368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.77
264.00	61.20	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011524\
Data File : BF137057.D
Acq On : 15 Jan 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 15 16:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

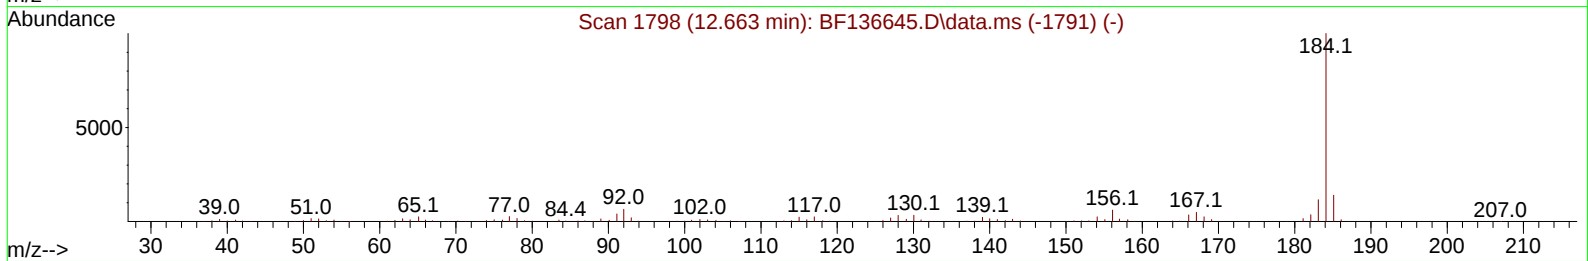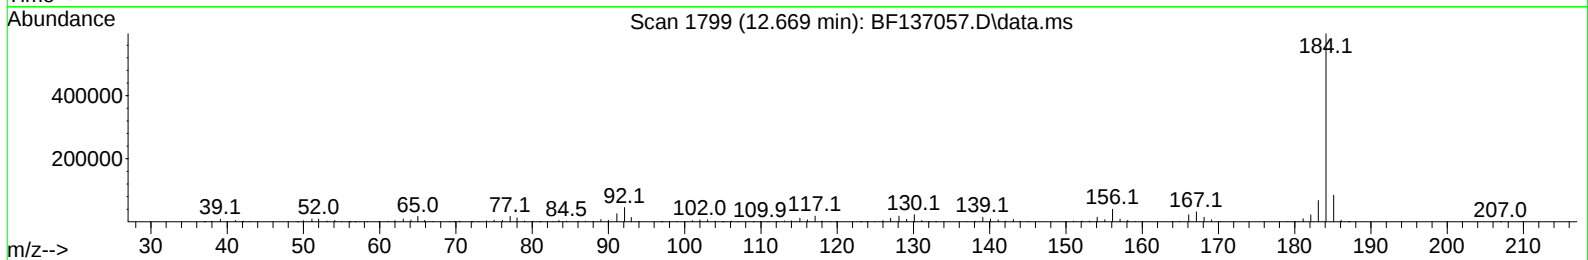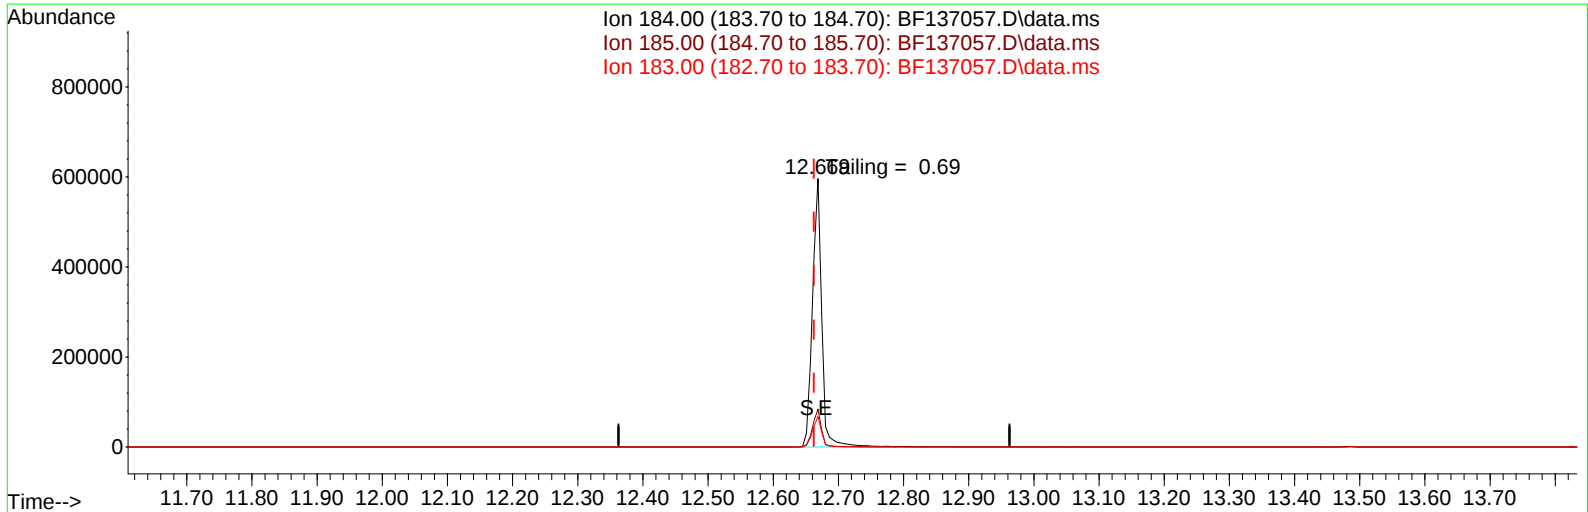

TIC: BF137057.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response 591864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	11.60	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/15/2024	BNA_F	<u>BF137057.D</u>
Compound Name	Response	Retention Time
DDT	287721	13.486
DDD	8020	13.186
DDE	554	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8574	296295	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP