
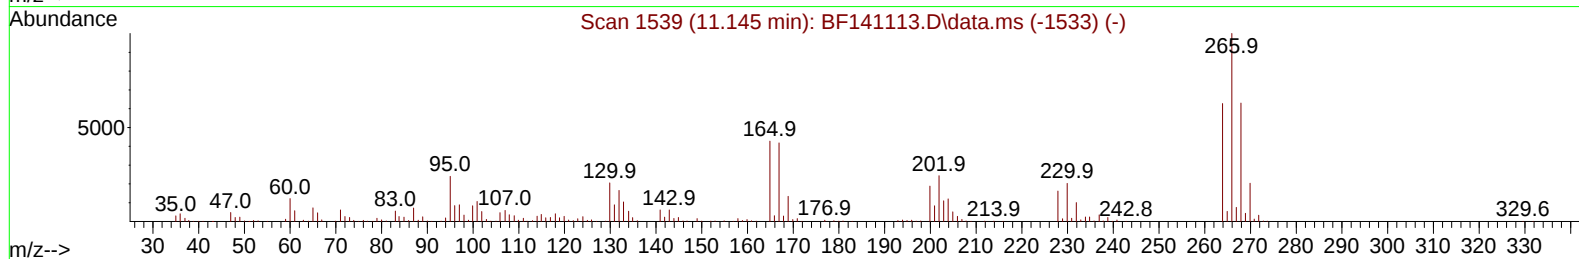
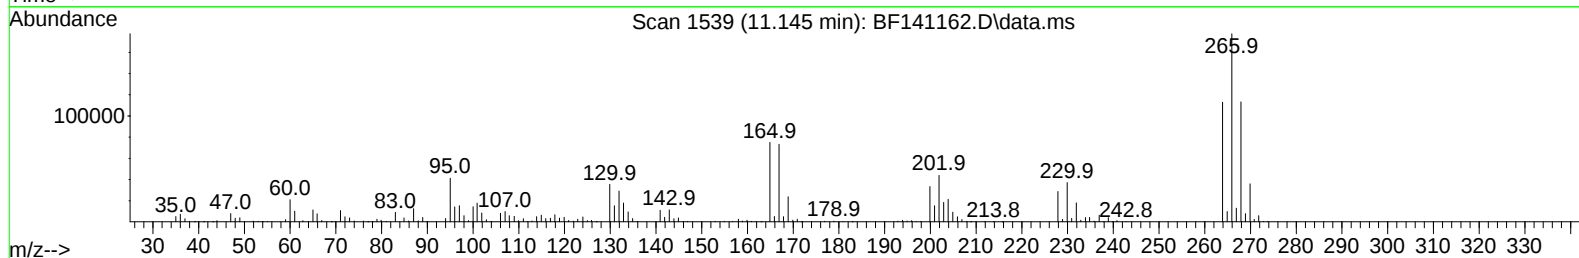


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011525\
Data File : BF141162.D
Acq On : 15 Jan 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 10:11:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

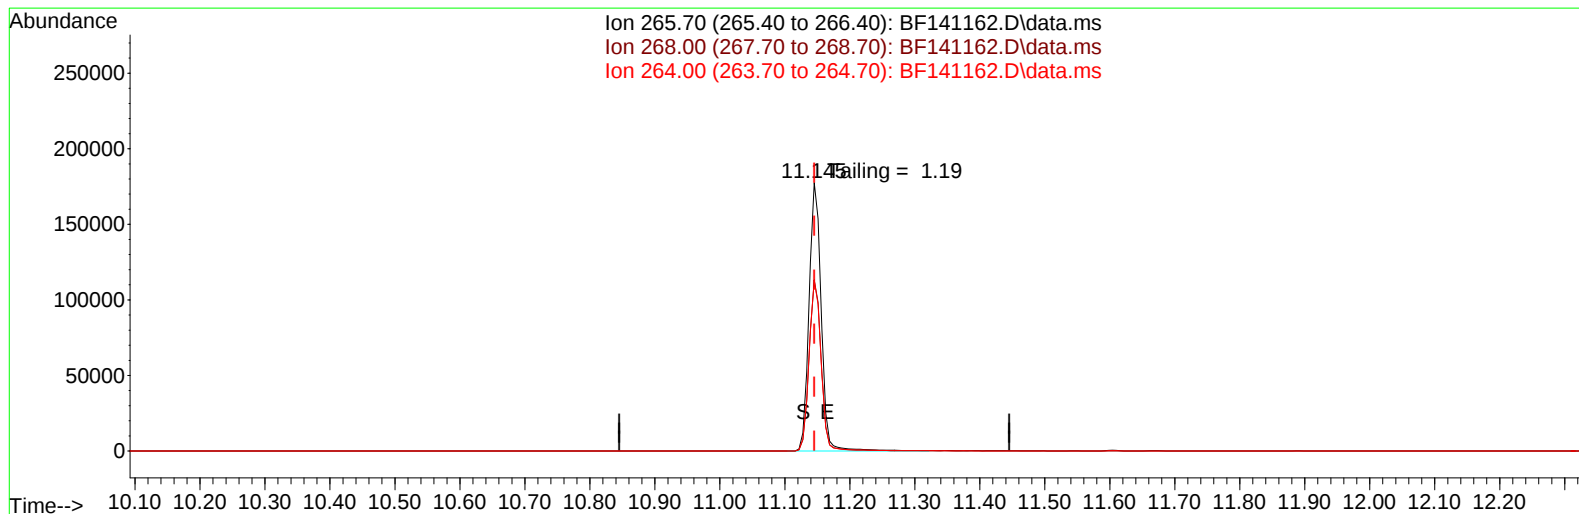

TIC: BF141162.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.000) 17848.17 ng

response 232184

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.76
264.00	62.70	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011525\
Data File : BF141162.D
Acq On : 15 Jan 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 10:11:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

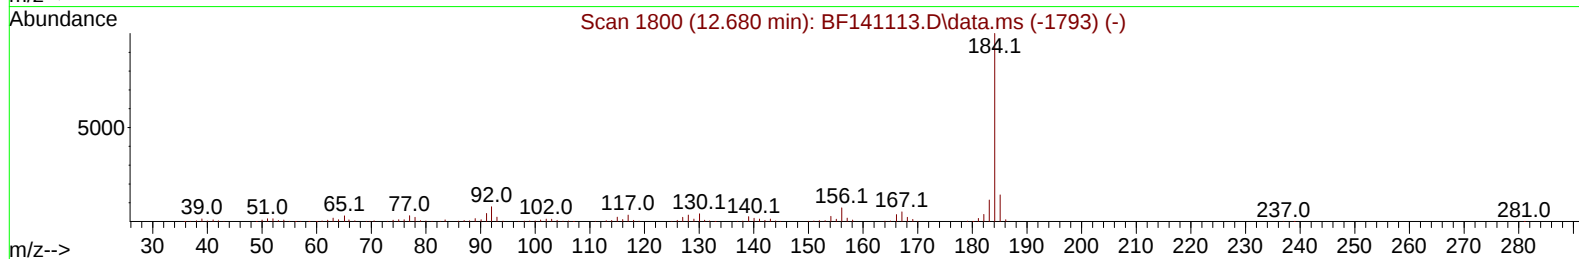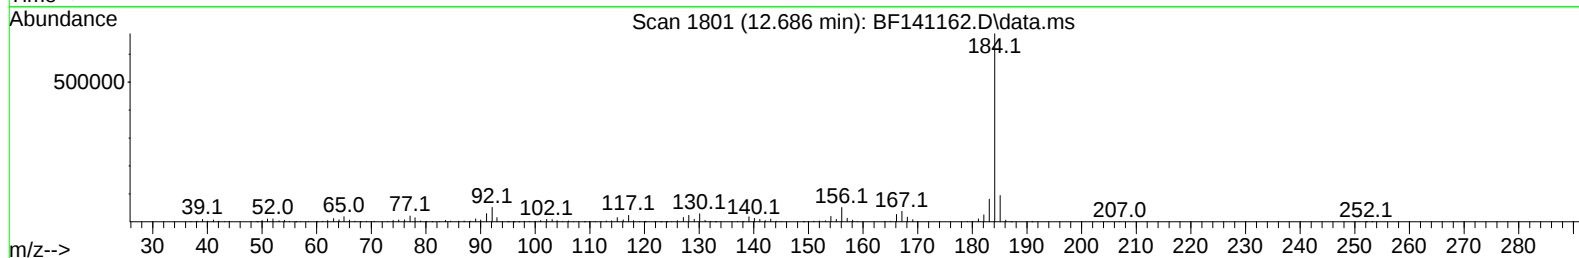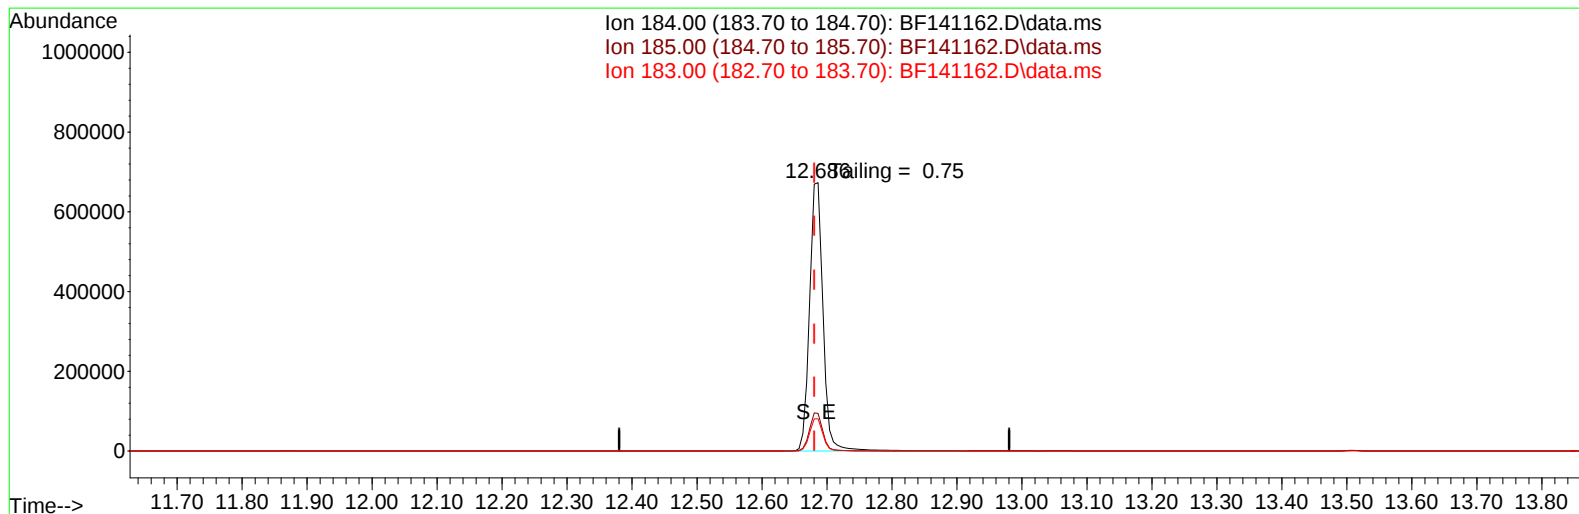

TIC: BF141162.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 34812.04 ng****response 973516**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.00
183.00	11.50	12.01
0.00	0.00	0.00