

Data Path : Z:\HPCHEM1\BNA F\Data\BF011615\
 Data File : BF076915.D
 Acq On : 16 Jan 2015 19:04
 Operator : IZ / TP
 Sample : G1091-05
 Misc : W
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jan 16 22:48:21 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 16 21:57:04 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	40284	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	175042	20.00	ng	0.00
38) Acenaphthene-d10	15.01	164	99936	20.00	ng	-0.01
63) Phenanthrene-d10	17.77	188	173260	20.00	ng	0.00
75) Chrysene-d12	21.27	240	155526	20.00	ng	0.00
86) Perylene-d12	22.94	264	136696	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.03	112	100992	41.22	ng	-0.01
7) Phenol-d6	7.37	99	74806	24.20	ng	0.00
23) Nitrobenzene-d5	9.27	82	207009	65.52	ng	-0.01
41) 2,4,6-Tribromophenol	16.68	330	85432	105.31	ng	-0.01
44) 2-Fluorobiphenyl	13.53	172	430466	65.55	ng	0.00
78) Terphenyl-d14	20.00	244	444053	65.73	ng	0.00
Target Compounds						
2) 1,4-Dioxane	1.45	88	5267	5.02	ng	Qvalue # 12
49) Dimethylphthalate	14.60	163	31045	4.38	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF011615\
Data File : BF076915.D
Acq On : 16 Jan 2015 19:04
Operator : IZ / TP
Sample : G1091-05
Misc : W
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jan 16 22:48:21 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 16 21:57:04 2015
Response via : Initial Calibration

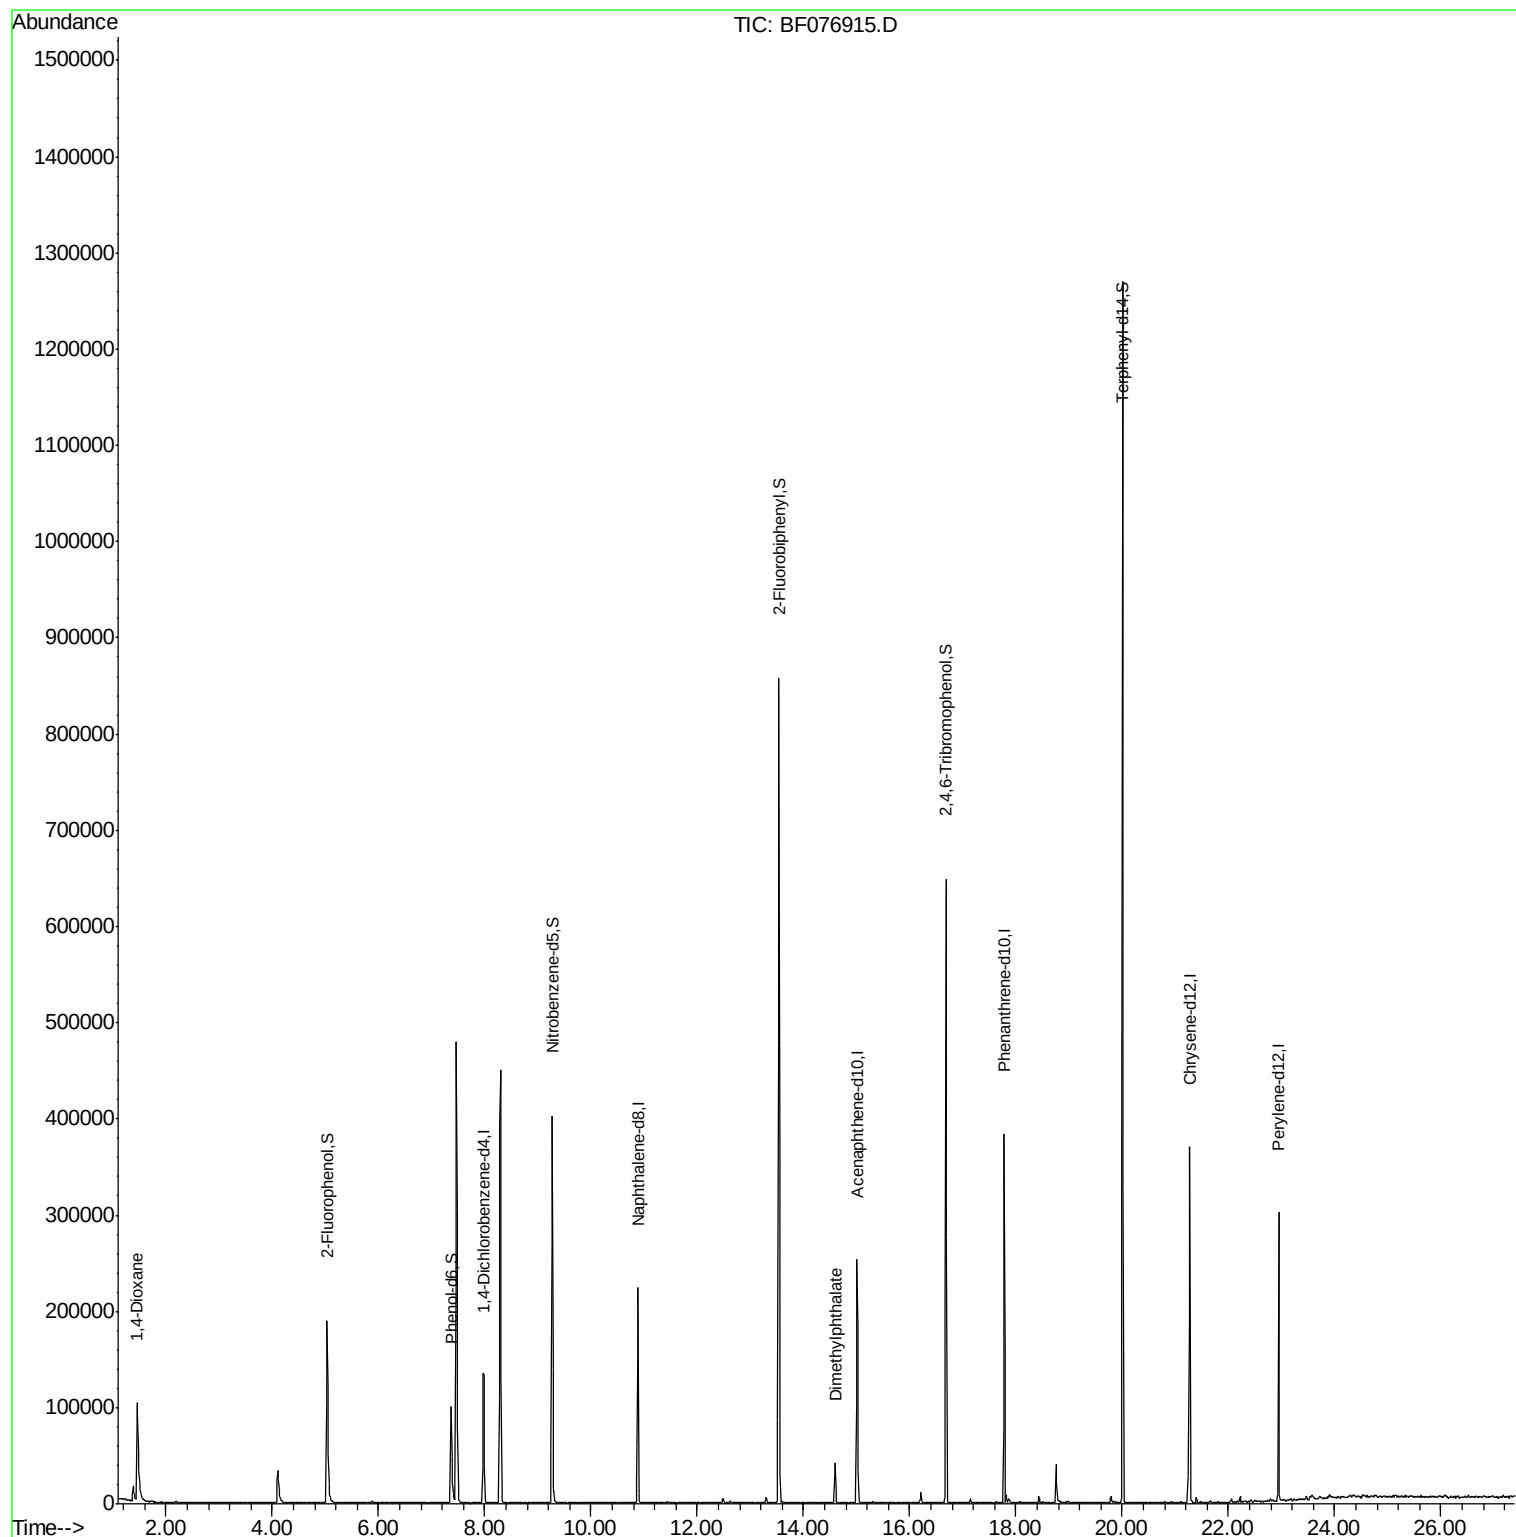

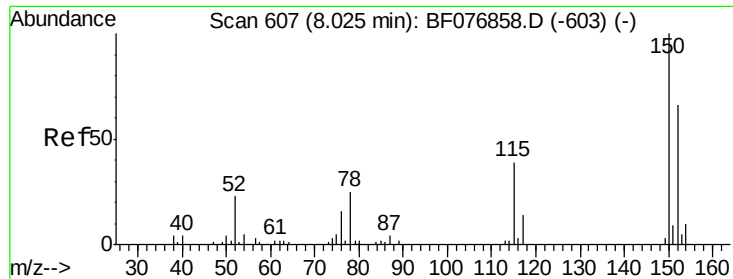


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.98 min Scan# 603
Delta R.T. 0.00 min
Lab File: BF076915.D
Acq: 16 Jan 2015 19:04

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 40284
Ion Ratio Lower Upper
152 100
150 152.2 121.7 182.5
115 62.6 47.0 70.6

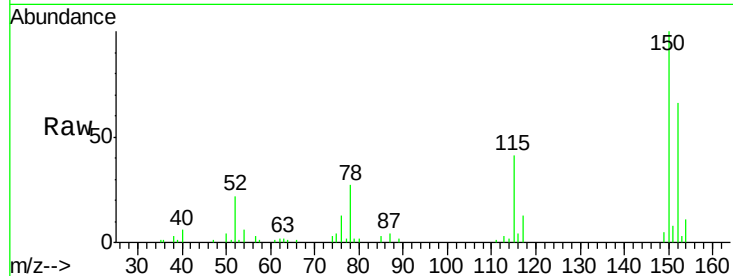


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

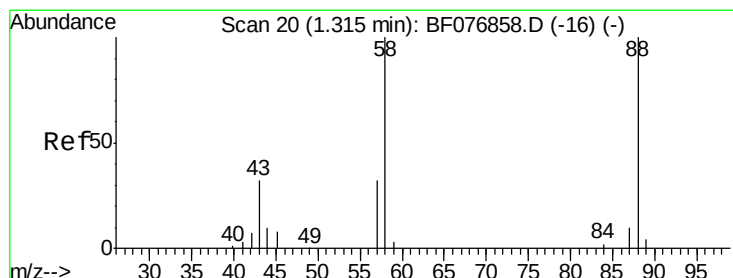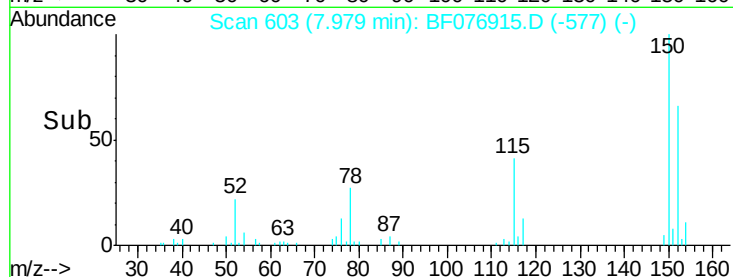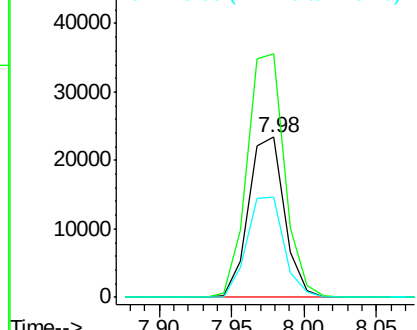



#2


1,4-Dioxane
Concen: 5.02 ng
RT: 1.45 min Scan# 32
Delta R.T. 0.17 min
Lab File: BF076915.D
Acq: 16 Jan 2015 19:04

Tgt Ion: 88 Resp: 5267
Ion Ratio Lower Upper
88 100
58 0.0 77.0 115.4#
43 0.0 25.6 38.4#

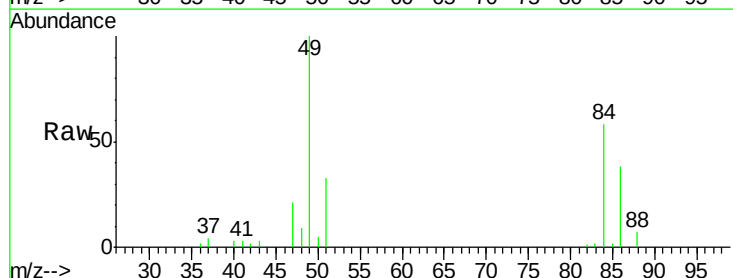

Abundance Ion 88.00 (87.70 to 88.70): BF0
Ion 58.00 (57.70 to 58.70): BF0
Ion 43.00 (42.70 to 43.70): BF0

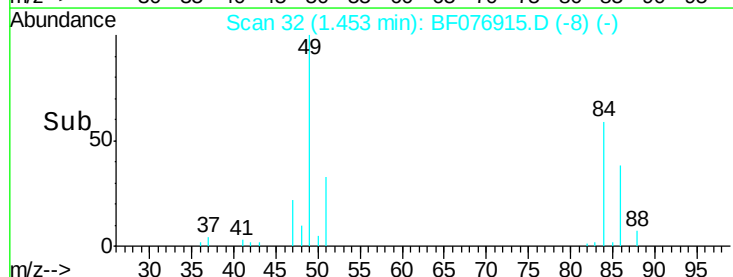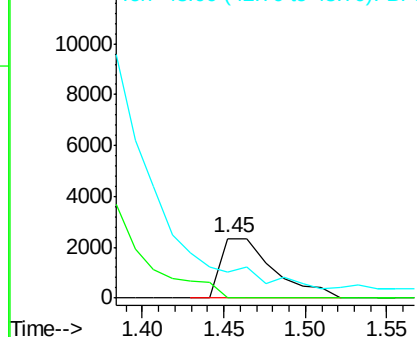

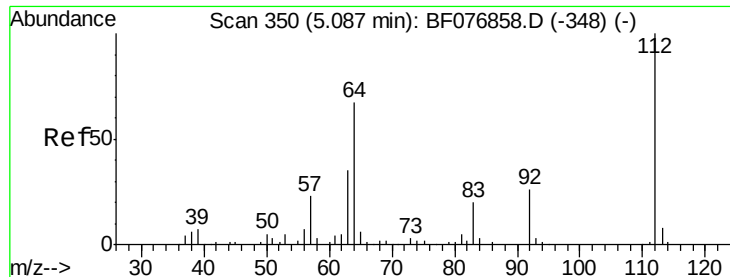

#5

2-Fluorophenol

Concen: 41.22 ng

RT: 5.03 min Scan# 345

Delta R.T. -0.01 min

Lab File: BF076915.D


Acq: 16 Jan 2015 19:04

Instrument :




BNA_F

ClientSampleId :

Tot Ion:	112	Resp:	100992
Ion	Ratio	Lower	Upper
112	100		
64	62.9	54.2	81.4
63	39.4	28.4	42.6

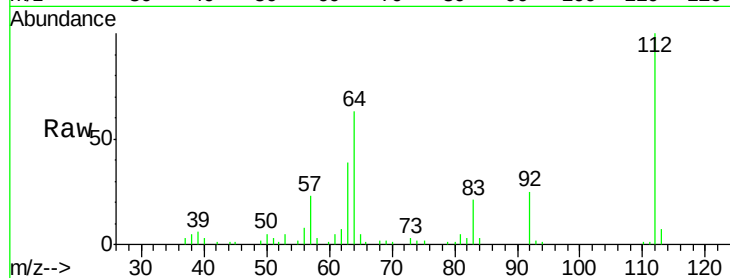

Abundance Ion 112.00 (111.70 to 112.70): E

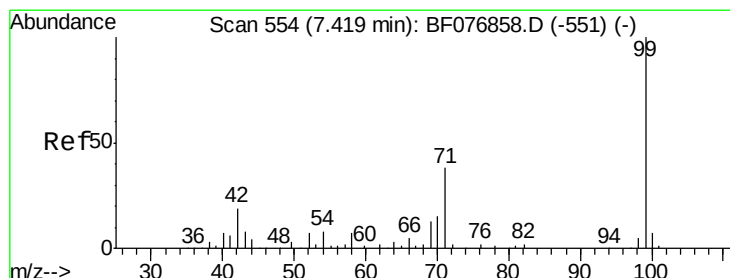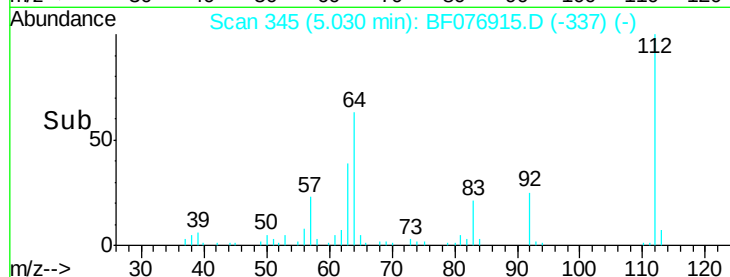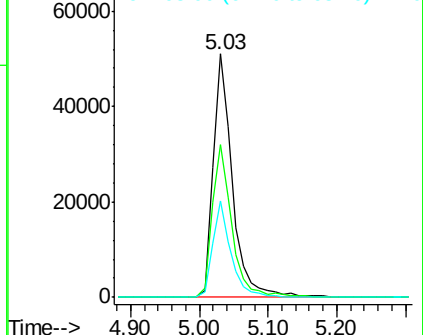

#7

Phenol-d6

Concen: 24.20 ng


RT: 7.37 min Scan# 550

Delta R.T. 0.00 min



Lab File: BF076915.D


Acq: 16 Jan 2015 19:04

Tgt Ion:	99	Resp:	74806
Ion	Ratio	Lower	Upper
99	100		
42	19.5	15.0	22.4
71	34.4	30.5	45.7

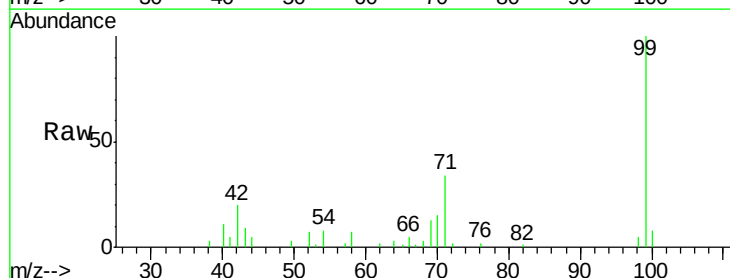

Abundance Ion 99.00 (98.70 to 99.70): BF0

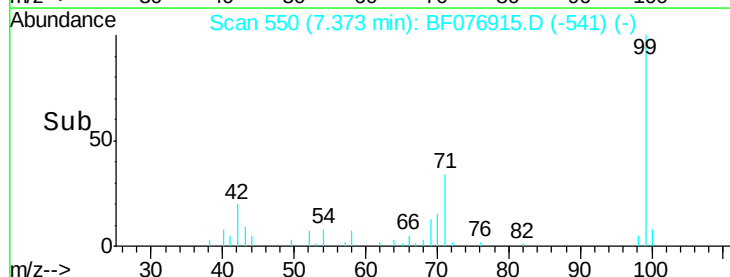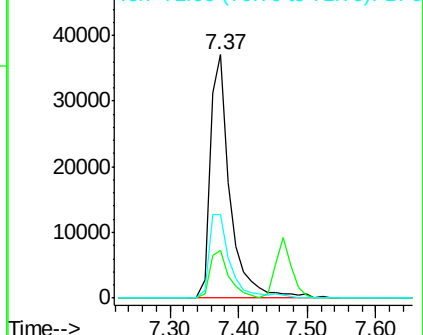

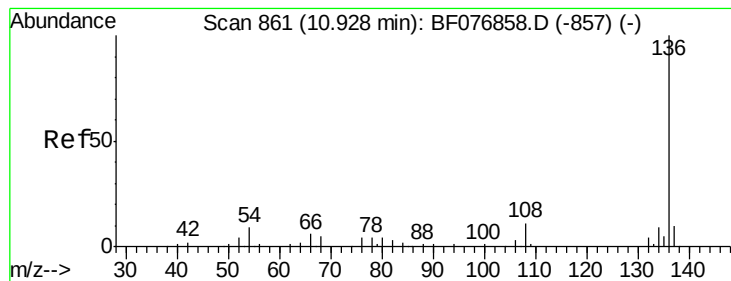

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 857

Delta R.T. 0.00 min

Lab File: BF076915.D

Acq: 16 Jan 2015 19:04

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 175042


Ion Ratio Lower Upper

136 100

137 10.5 8.1 12.1

54 8.0 7.0 10.4

68 4.2 3.7 5.5



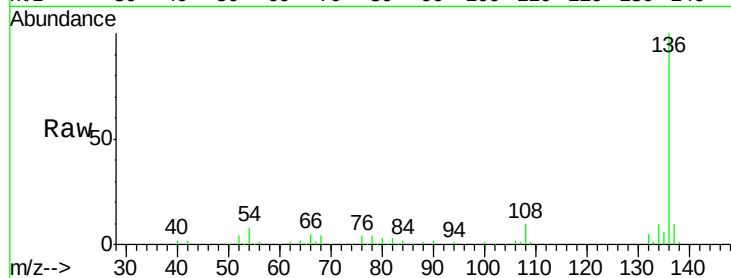


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

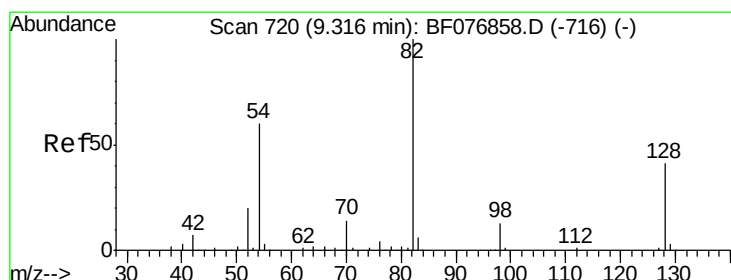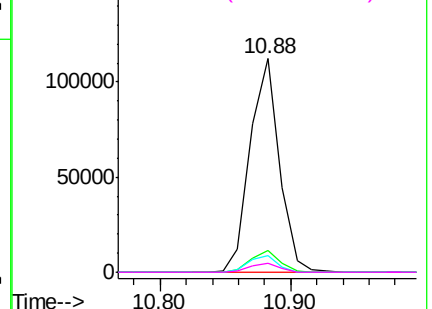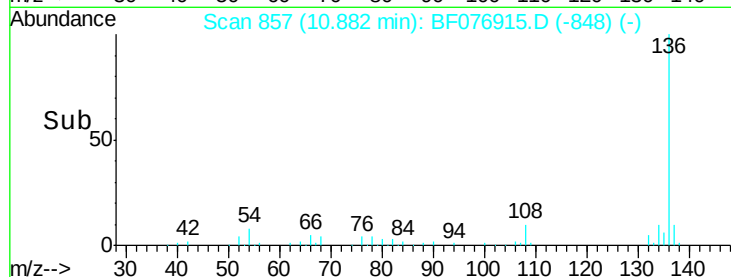

#23

Nitrobenzene-d5

Concen: 65.52 ng

RT: 9.27 min Scan# 716

Delta R.T. -0.01 min

Lab File: BF076915.D

Acq: 16 Jan 2015 19:04


Tgt Ion: 82 Resp: 207009

Ion Ratio Lower Upper

82 100

128 43.6 33.1 49.7



54 56.9 48.3 72.5

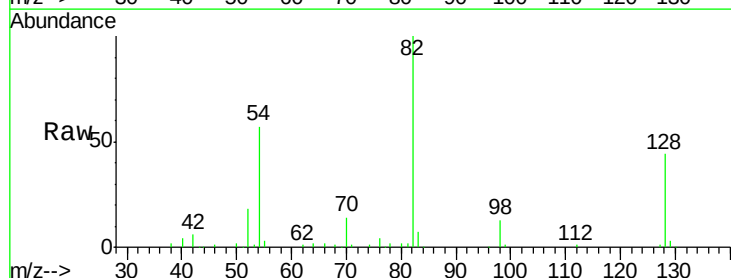


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

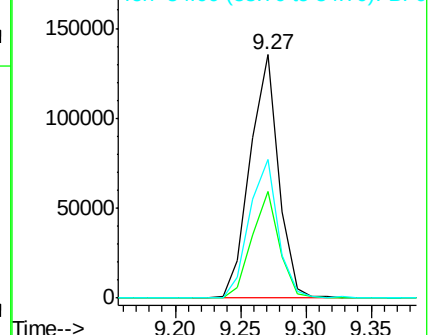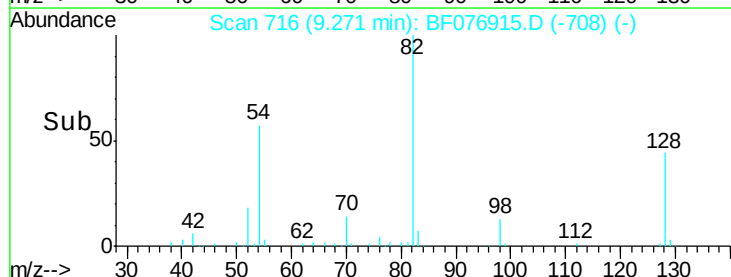

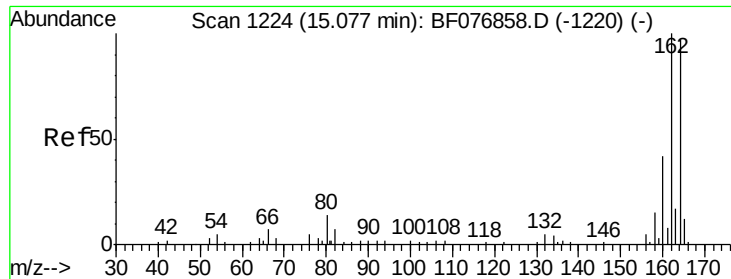

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 15.01 min Scan# 1218

Delta R.T. -0.01 min

Lab File: BF076915.D

Acq: 16 Jan 2015 19:04

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 99936

Ion Ratio Lower Upper

164 100

162 104.1 82.4 123.6




160 44.9 34.8 52.2

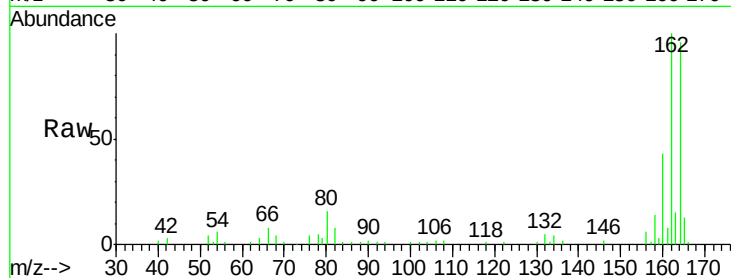

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

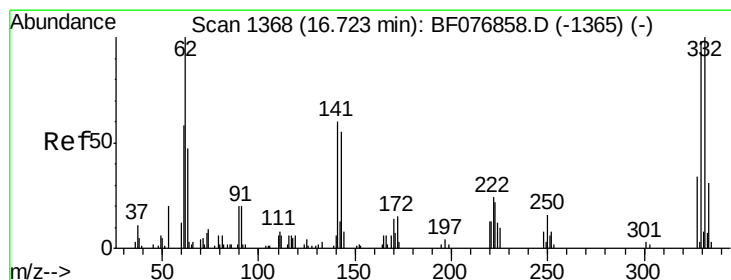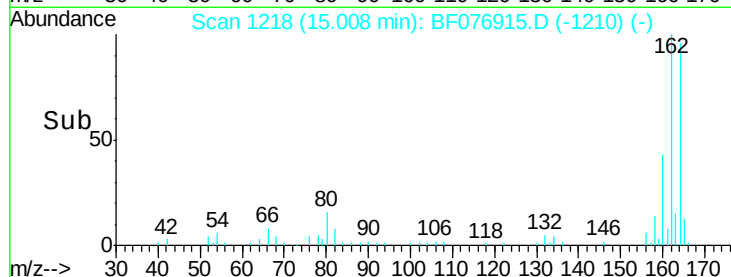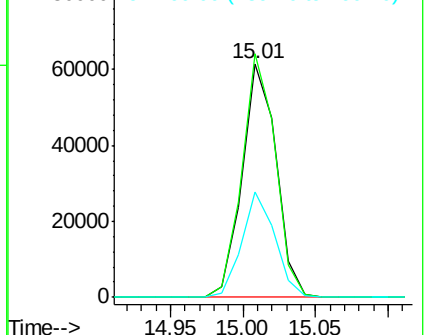

#41

2,4,6-Tribromophenol

Concen: 105.31 ng

RT: 16.68 min Scan# 1364

Delta R.T. -0.01 min

Lab File: BF076915.D

Acq: 16 Jan 2015 19:04


Tgt Ion:330 Resp: 85432

Ion Ratio Lower Upper

330 100

332 96.9 77.8 116.6



141 47.8 38.5 57.7

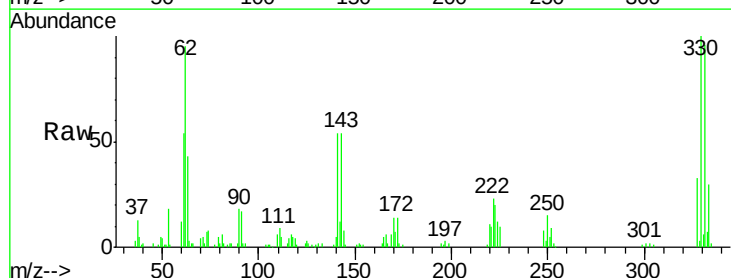


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



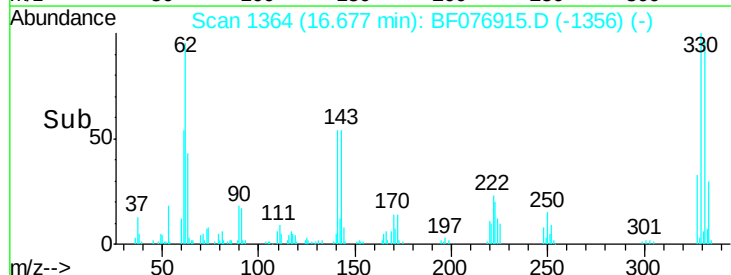
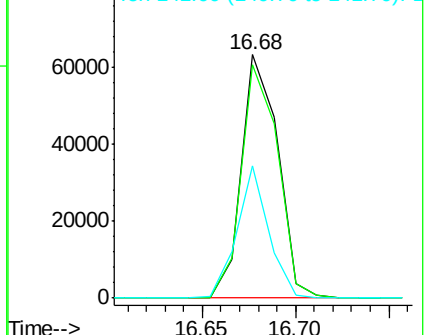


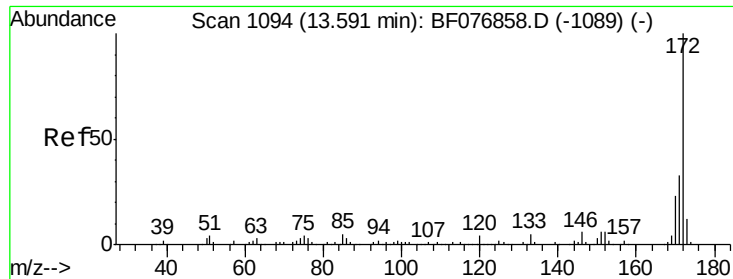

#44
2-Fluorobiphenyl
Concen: 65.55 ng
RT: 13.53 min Scan# 1089
Delta R.T. 0.00 min
Lab File: BF076915.D
Acq: 16 Jan 2015 19:04




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 430466
Ion Ratio Lower Upper
172 100
171 35.0 26.6 40.0
170 23.6 18.0 27.0

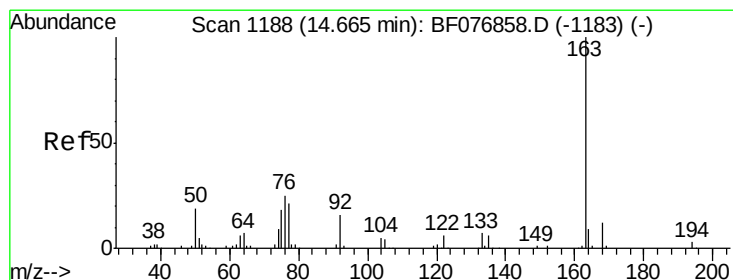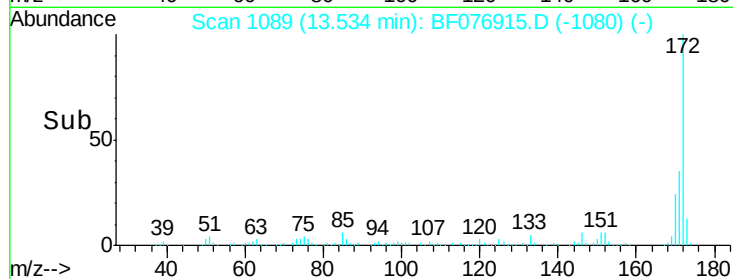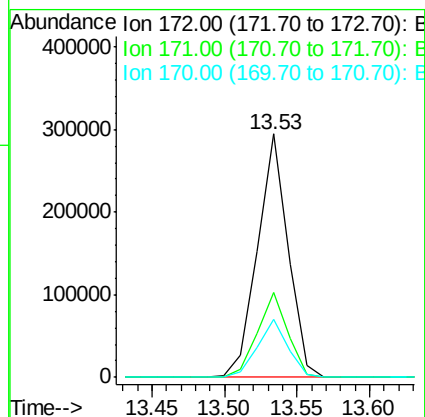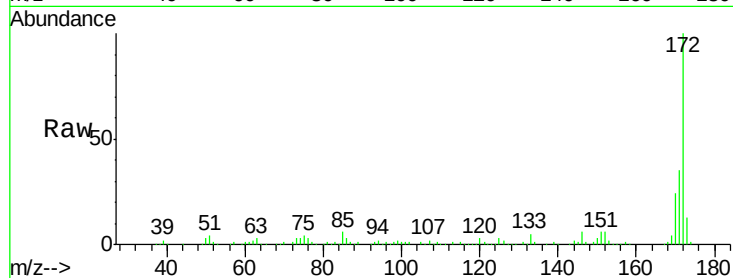

#49
Dimethylphthalate
Concen: 4.38 ng
RT: 14.60 min Scan# 1182
Delta R.T. -0.01 min
Lab File: BF076915.D
Acq: 16 Jan 2015 19:04

Tgt Ion:163 Resp: 31045
Ion Ratio Lower Upper
163 100
194 2.9 2.6 4.0
164 9.3 7.5 11.3

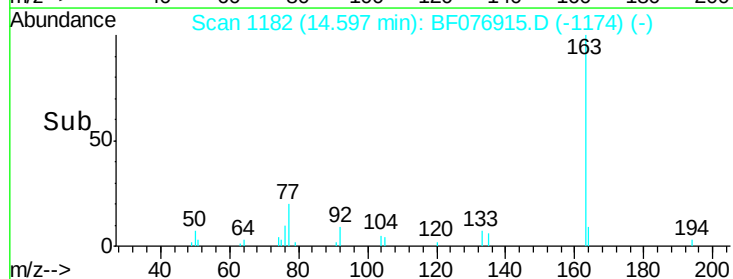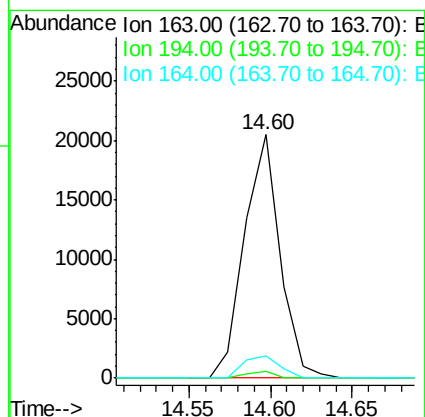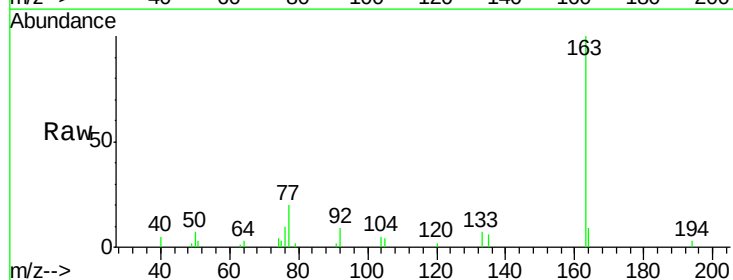


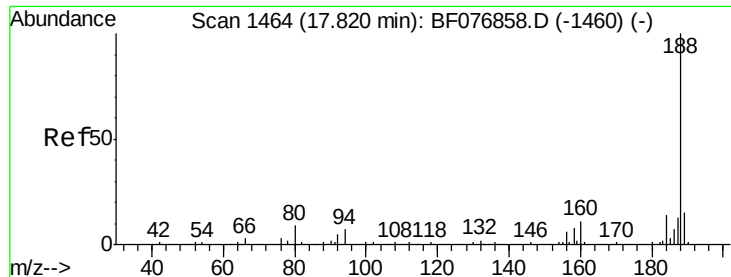




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.77 min Scan# 1460
 Delta R.T. 0.00 min
 Lab File: BF076915.D
 Acq: 16 Jan 2015 19:04

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:188 Resp: 173260
 Ion Ratio Lower Upper
 188 100
 94 9.5 6.0 9.0#
 80 10.1 6.9 10.3

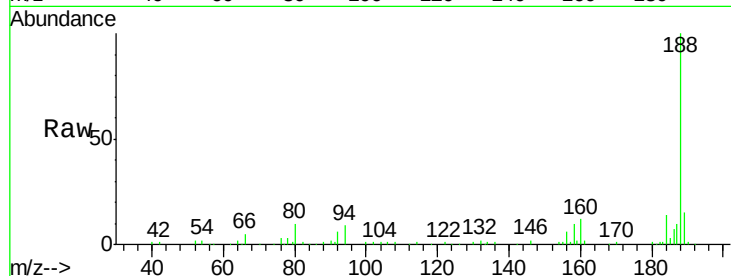


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

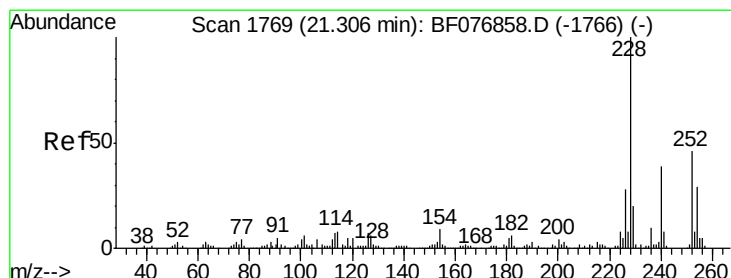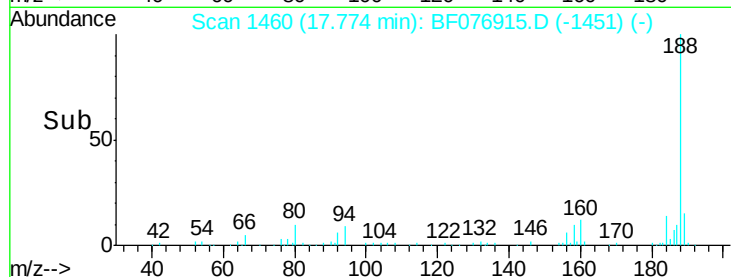
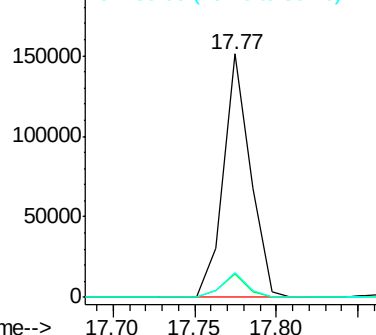



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.27 min Scan# 1766
 Delta R.T. 0.00 min
 Lab File: BF076915.D
 Acq: 16 Jan 2015 19:04

Tgt Ion:240 Resp: 155526
 Ion Ratio Lower Upper
 240 100
 120 10.0 10.4 15.6#
 236 25.3 20.2 30.2

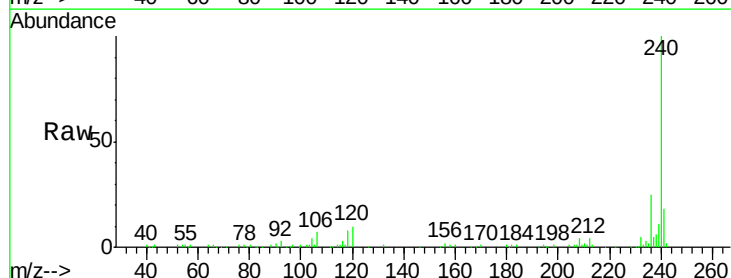

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



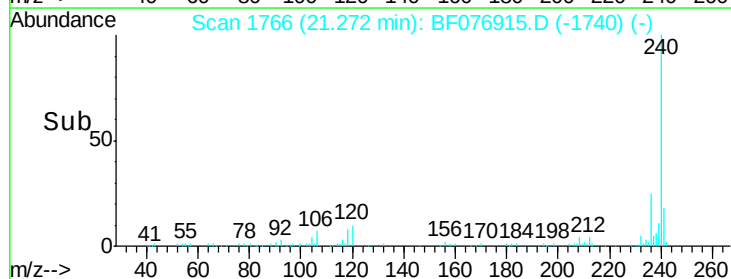
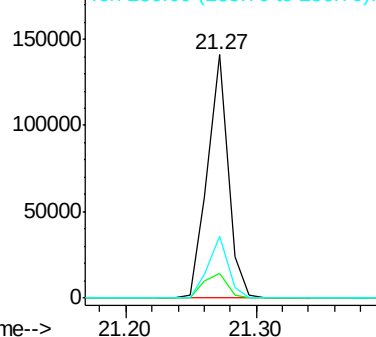


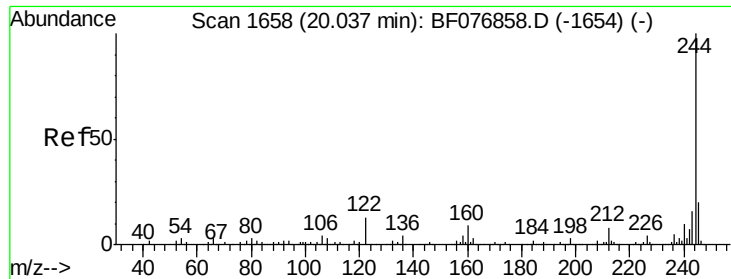

#78
 Terphenyl-d14
 Concen: 65.73 ng
 RT: 20.00 min Scan# 1655
 Delta R.T. 0.00 min
 Lab File: BF076915.D
 Acq: 16 Jan 2015 19:04

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:244 Resp: 444053
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.3 9.5
 122 11.8 10.1 15.1

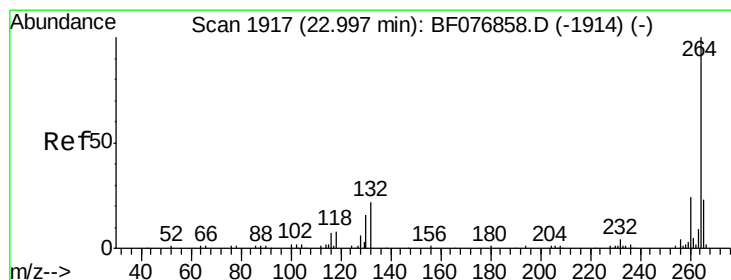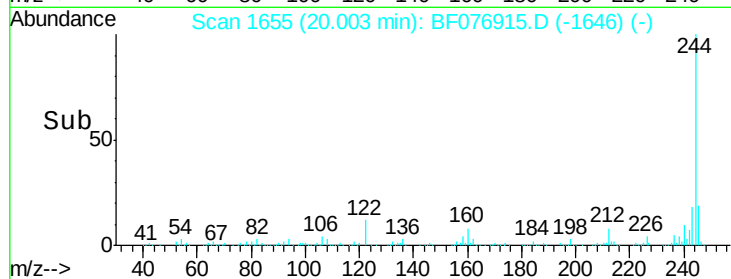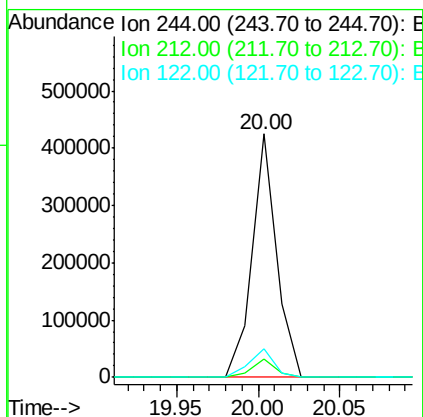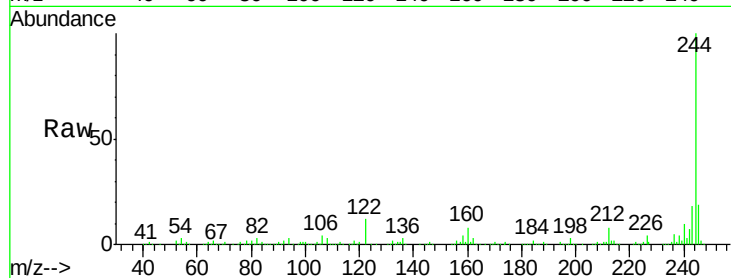

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 22.94 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BF076915.D
 Acq: 16 Jan 2015 19:04

Tgt Ion:264 Resp: 136696
 Ion Ratio Lower Upper
 264 100
 260 22.2 19.0 28.4
 265 22.0 18.1 27.1

