
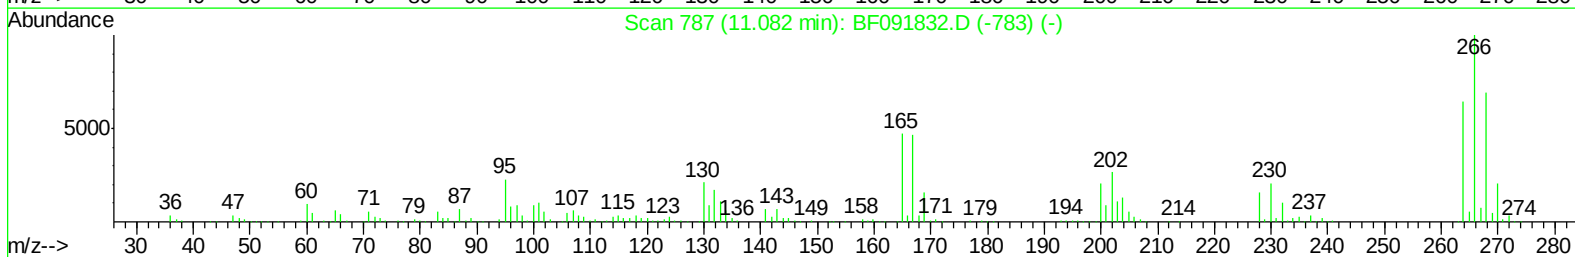
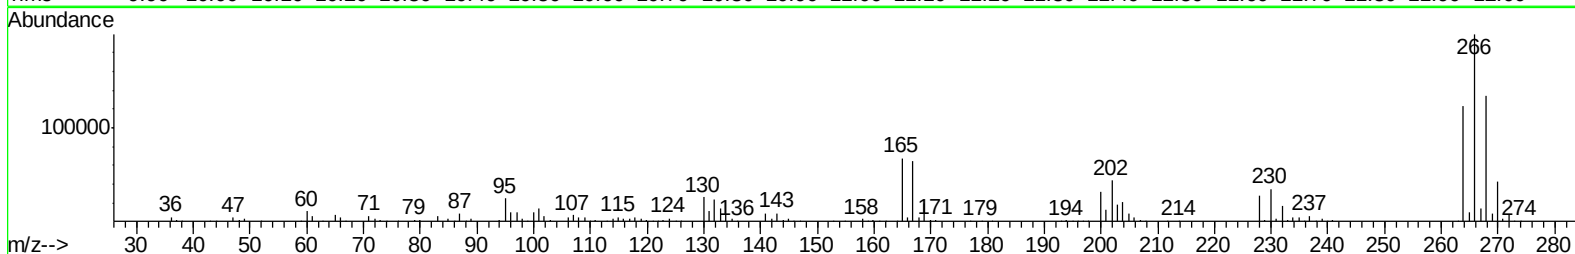


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011617\
Data File : BF092305.D
Acq On : 17 Jan 2017 1:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:42:54 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 00:52:12 2017
Response via : Initial Calibration

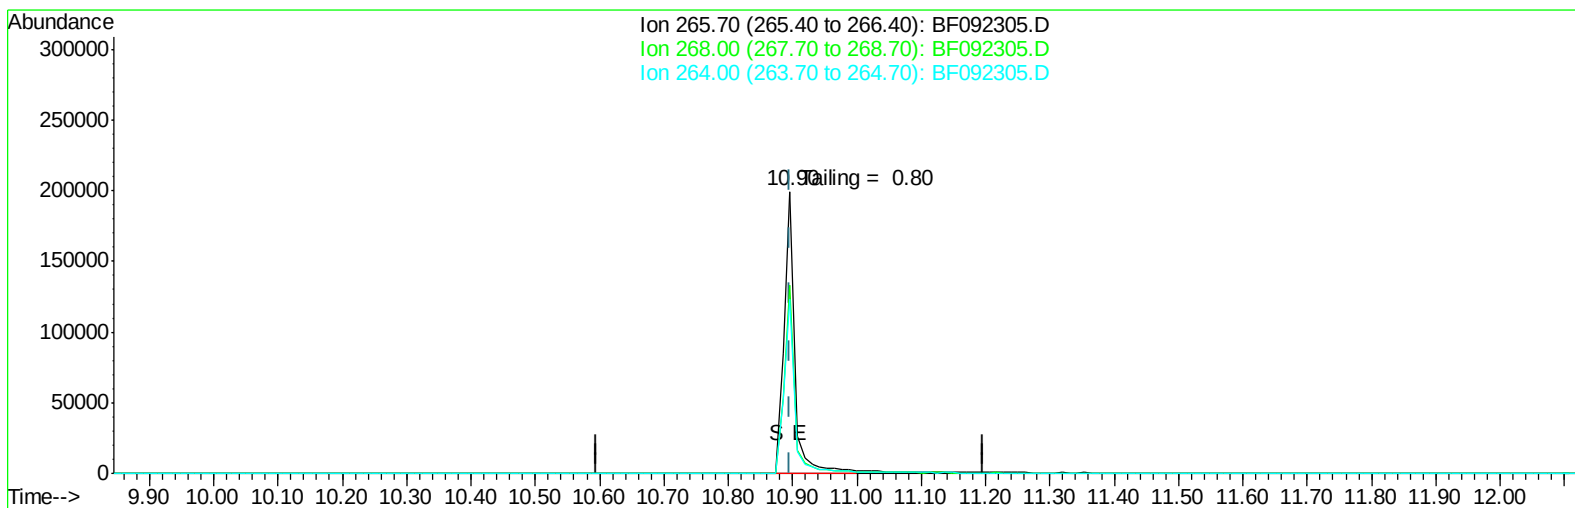

TIC: BF092305.D

(69) Pentachlorophenol (C)




10.896min (-0.000) 0.00ng

response 246854

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.98
264.00	62.90	62.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011617\
Data File : BF092305.D
Acq On : 17 Jan 2017 1:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:42:54 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 00:52:12 2017
Response via : Initial Calibration

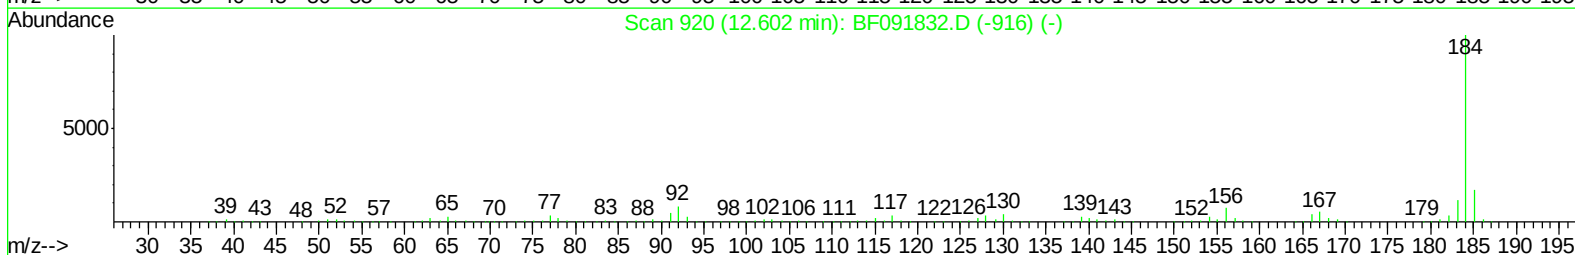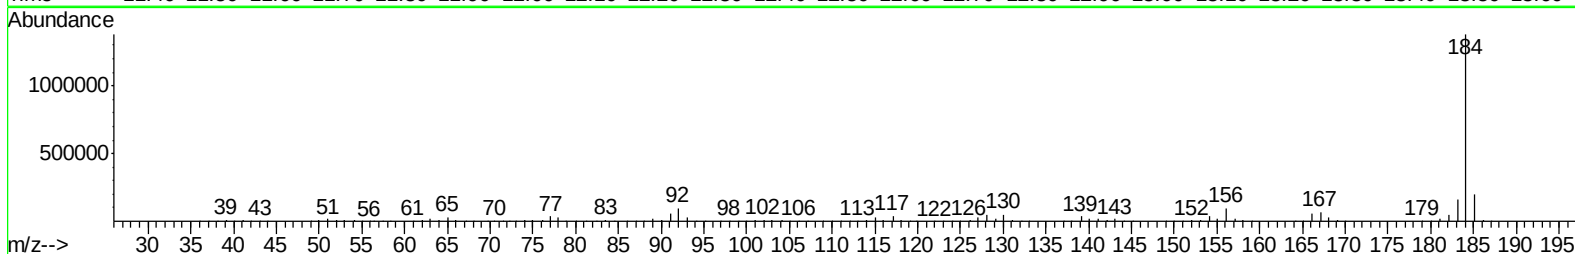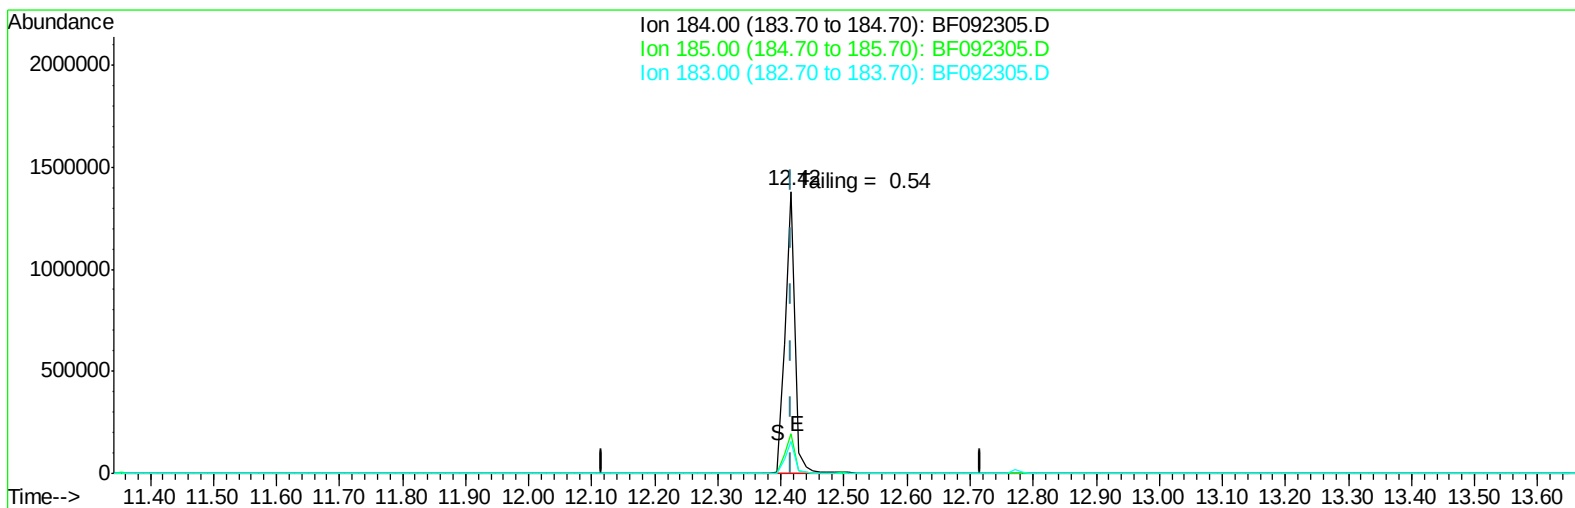

TIC: BF092305.D

(76) Benzidine

12.416min (-0.000) 0.00ng m

response 1499906

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.33
183.00	11.50	11.52
0.00	0.00	0.00