


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011617\
 Data File : BF092282.D
 Acq On : 16 Jan 2017 13:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

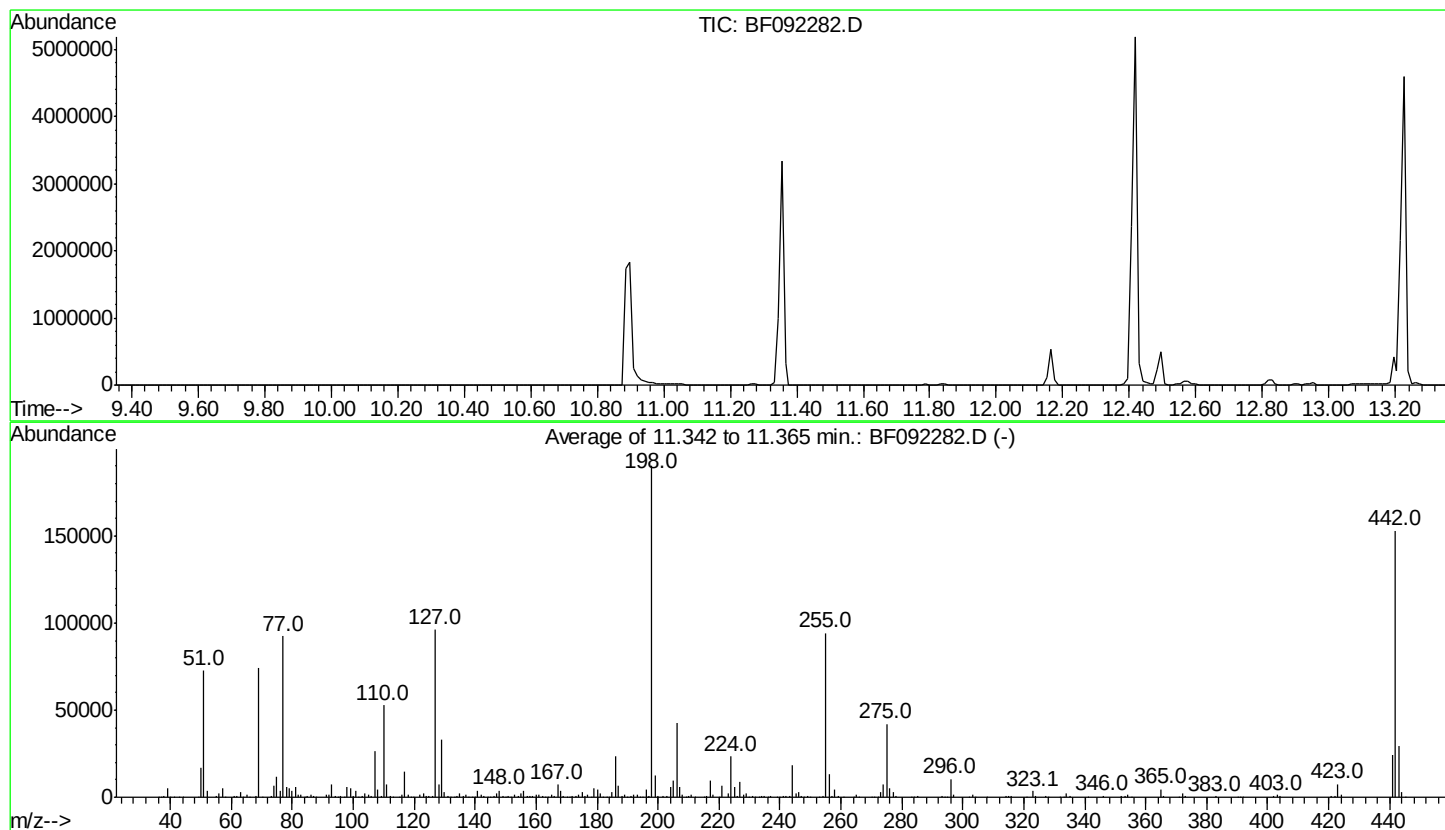

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	72718	PASS
68	69	0.00	2	1.5	1095	PASS
69	198	0.00	100	39.1	74350	PASS
70	69	0.00	2	0.5	382	PASS
127	198	10	80	50.5	96168	PASS
197	198	0.00	2	0.5	867	PASS
198	198	100	100	100.0	190338	PASS
199	198	5	9	6.7	12817	PASS
275	198	10	60	22.1	42029	PASS
365	198	1	100	2.4	4544	PASS
441	442	0.01	24	16.0	24470	PASS
442	198	50	100	80.3	152834	PASS
443	442	15	24	19.2	29353	PASS