


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011617\
 Data File : BF092305.D
 Acq On : 17 Jan 2017 1:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

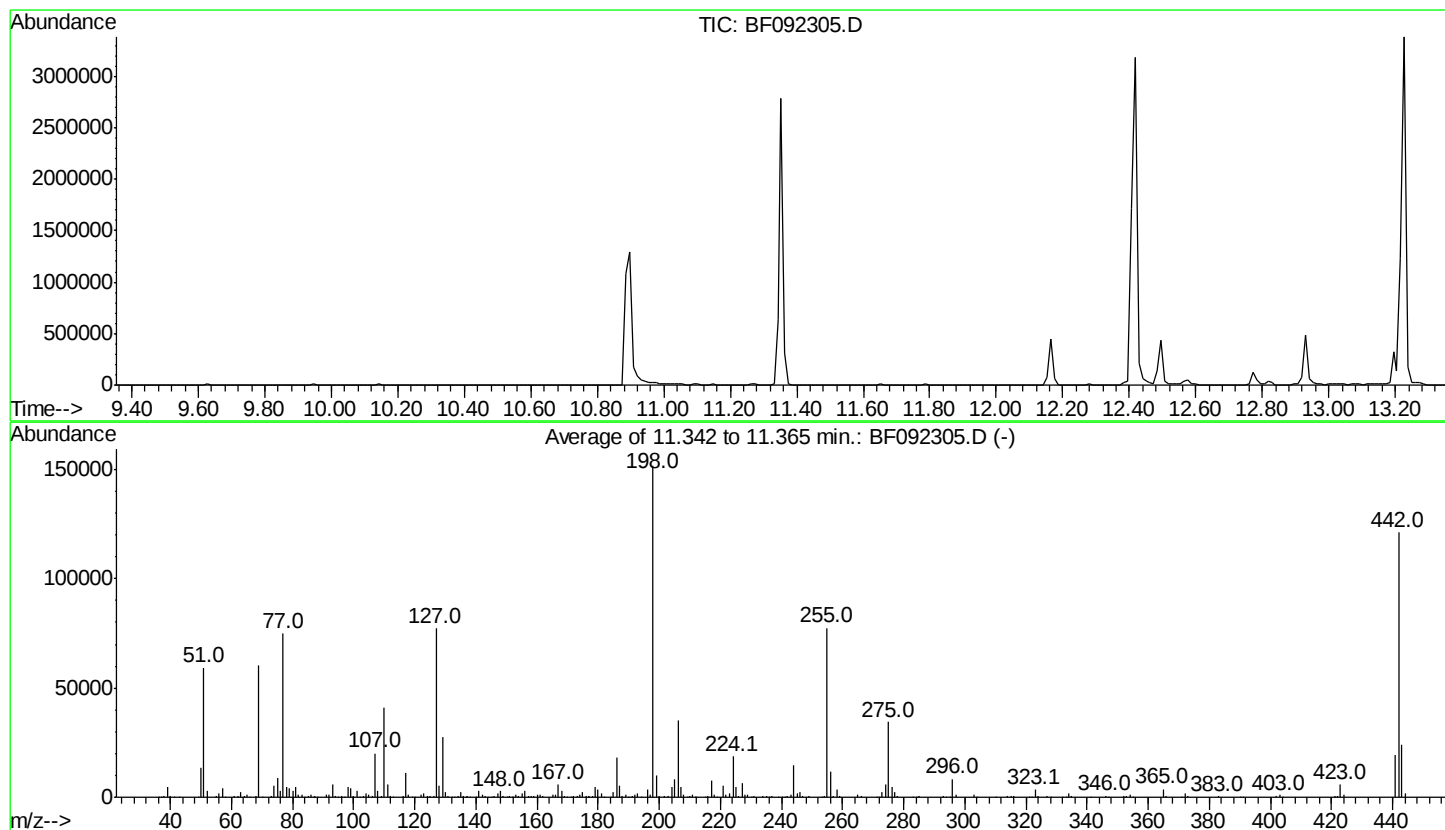

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	59241	PASS
68	69	0.00	2	1.4	842	PASS
69	198	0.00	100	39.8	60349	PASS
70	69	0.00	2	0.4	222	PASS
127	198	10	80	50.8	77169	PASS
197	198	0.00	2	0.6	907	PASS
198	198	100	100	100.0	151781	PASS
199	198	5	9	6.5	9917	PASS
275	198	10	60	22.8	34552	PASS
365	198	1	100	2.5	3739	PASS
441	442	0.01	24	15.8	19150	PASS
442	198	50	100	79.9	121218	PASS
443	442	15	24	19.9	24075	PASS