

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
 Data File : BF102127.D
 Acq On : 16 Jan 2018 23:16
 Operator : SJ/JU
 Sample : J1131-04 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jan 17 02:29:11 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 11 12:53:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	133452	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	525966	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	221437	20.00	ng	-0.01
63) Phenanthrene-d10	11.23	188	337552	20.00	ng	-0.01
75) Chrysene-d12	13.86	240	231911	20.00	ng	-0.02
86) Perylene-d12	15.28	264	240549	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	253854	26.86	ng	0.00
7) Phenol-d6	6.35	99	274092	24.31	ng	-0.02
23) Nitrobenzene-d5	7.28	82	194797	21.76	ng	-0.02
41) 2,4,6-Tribromophenol	10.54	330	67958	35.17	ng	-0.01
44) 2-Fluorobiphenyl	9.07	172	374475	26.42	ng	-0.02
78) Terphenyl-d14	12.82	244	235919	21.12	ng	-0.02
Target Compounds						Qvalue
15) Benzyl Alcohol	6.87	79	438037	53.109	ng	96
17) 2-Methylphenol	6.87	107	243883	28.523	ng	# 11
20) 3+4-Methylphenols	7.12	107	37260	3.629	ng	87
25) Isophorone	7.28	82	194793	11.014	ng	# 64
27) 2,4-Dimethylphenol	7.82	122	429620	57.146	ng	# 4
31) Naphthalene	8.02	128	69300	2.637	ng	98
32) Benzoic acid	7.82	122	429620	75.361	ng	97
50) 2,6-Dinitrotoluene	9.75	165	29232	8.238	ng	# 26
56) 2,4-Dinitrotoluene	9.75	165	29232	6.573	ng	# 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102127.D
Acq On : 16 Jan 2018 23:16
Operator : SJ/JU
Sample : J1131-04 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jan 17 02:29:11 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

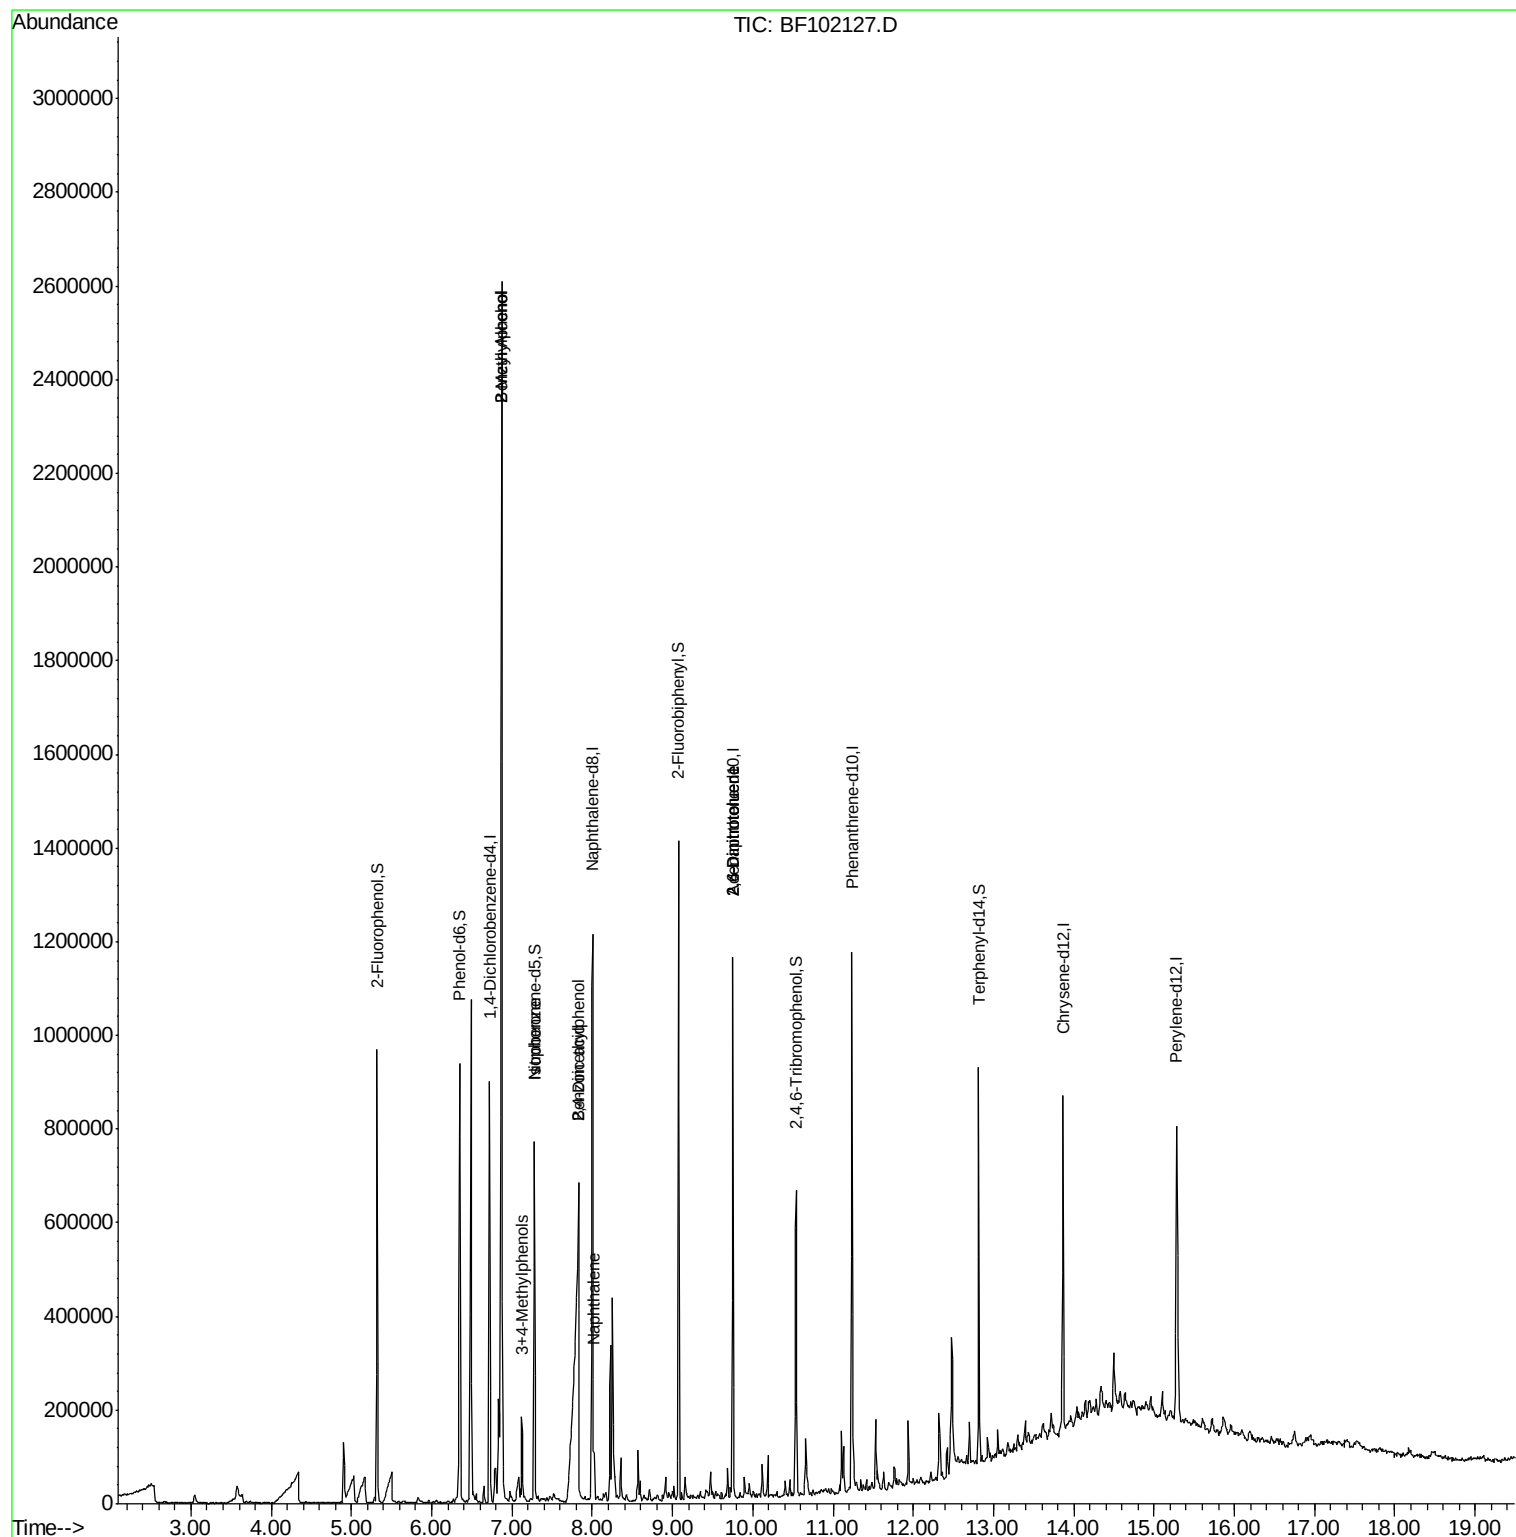

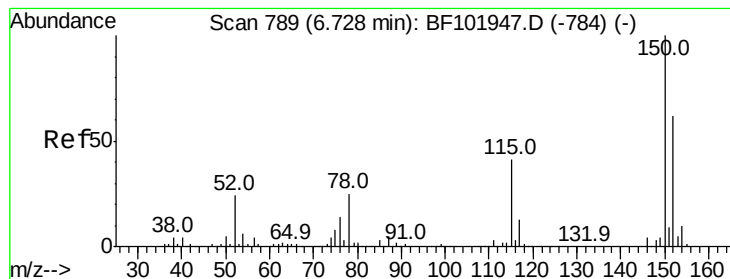


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 788
Delta R.T. -0.01 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.1	124.6	186.8
115	56.9	50.1	75.1

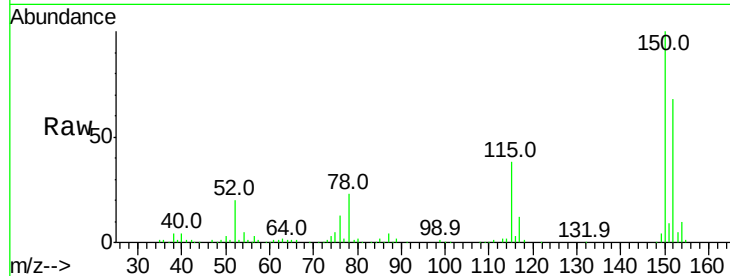


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

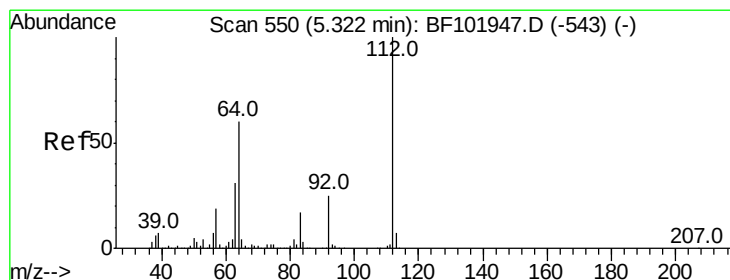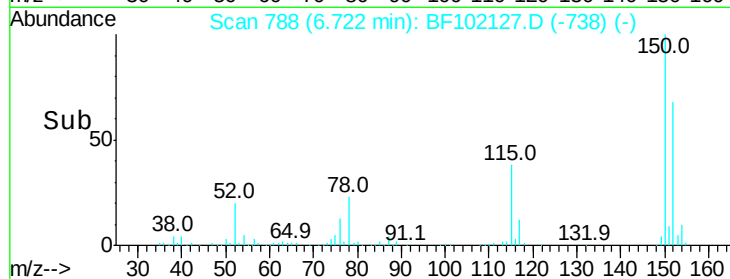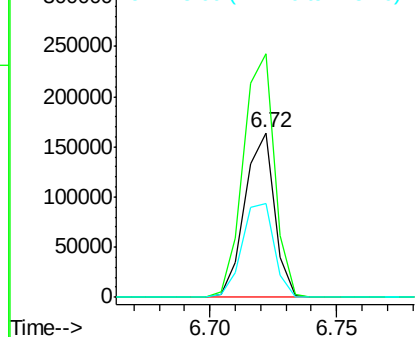



#5


2-Fluorophenol
Concen: 26.861 ng
RT: 5.32 min Scan# 550
Delta R.T. -0.01 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.8	47.9	71.9
63	29.2	23.7	35.5

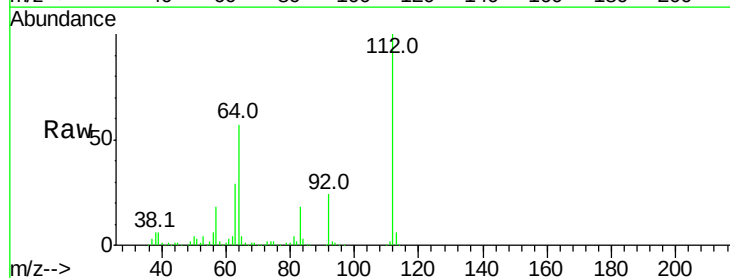

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

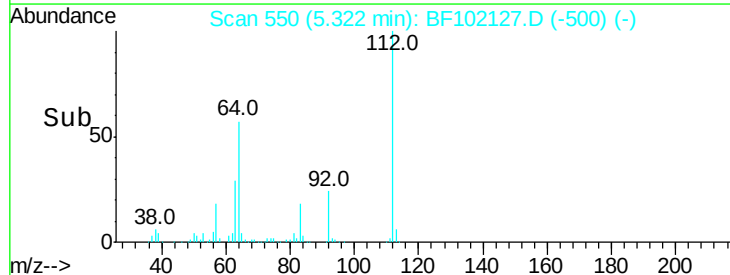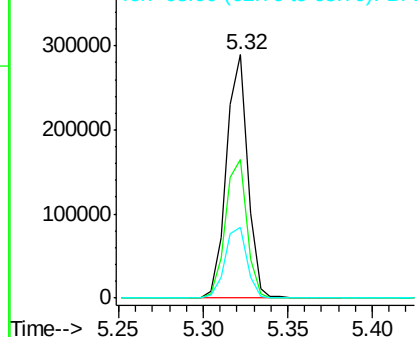

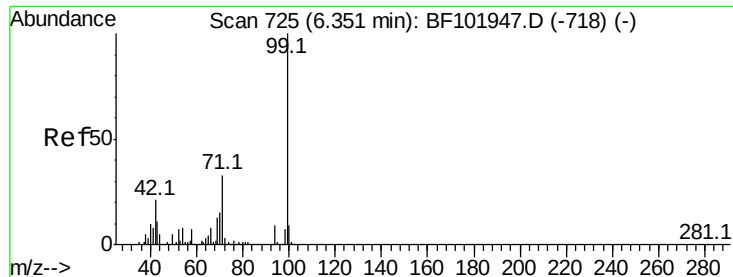

#7

Phenol-d6

Concen: 24.308 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 274092

Ion Ratio Lower Upper

99 100

42 20.1 14.5 21.7

71 35.4 25.4 38.0

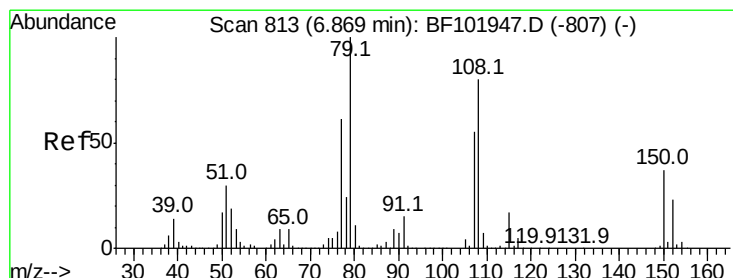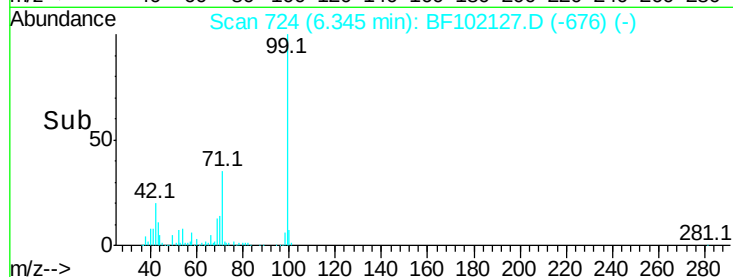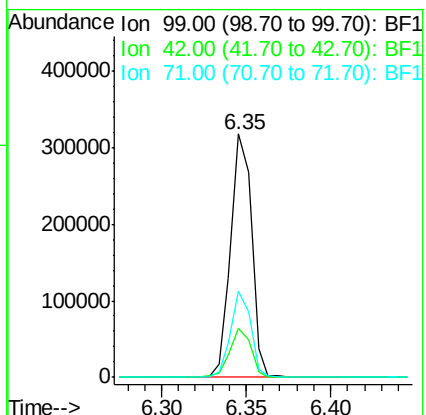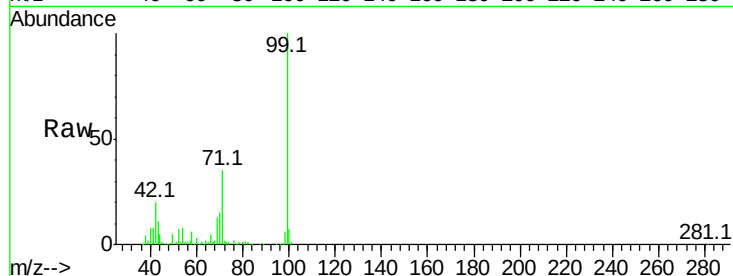

#15

Benzyl Alcohol

Concen: 53.109 ng

RT: 6.87 min Scan# 813

Delta R.T. 0.00 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16




Tgt Ion: 79 Resp: 438037


Ion Ratio Lower Upper

79 100

108 78.3 65.1 97.7

77 60.4 50.6 75.8


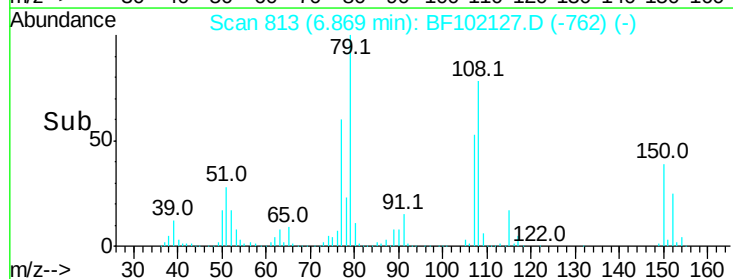
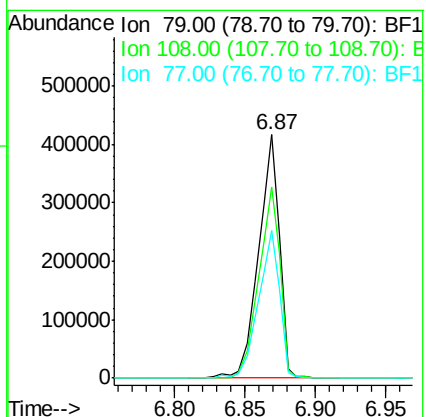
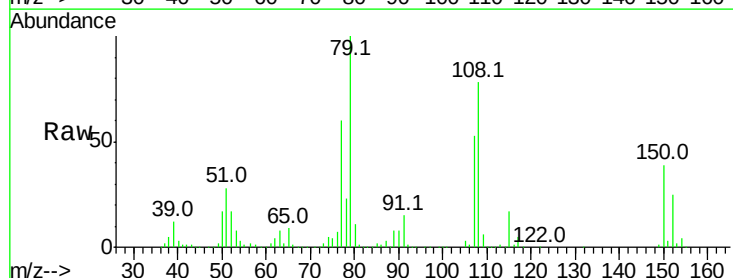


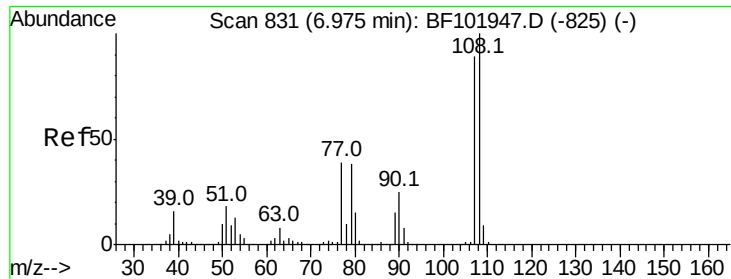

#17
2-Methylphenol
Concen: 28.523 ng
RT: 6.87 min Scan# 813
Delta R.T. -0.11 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16




Instrument :
BNA_F
ClientSampled :


Tot Ion	Ratio	Lower	Upper
107	100		
108	146.7	91.7	137.5#
77	113.2	33.8	50.8#
79	187.3	33.8	50.8#

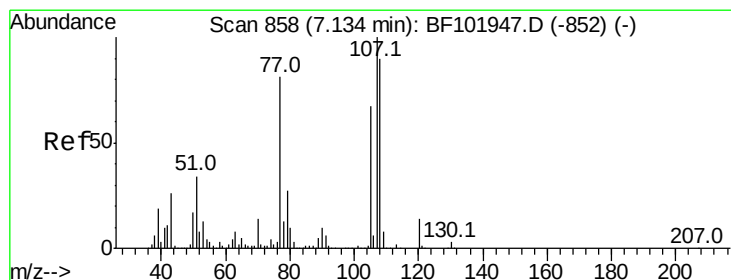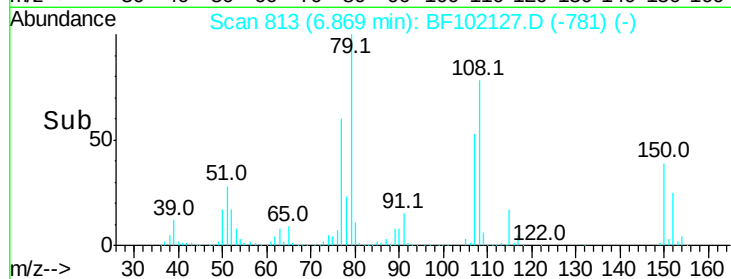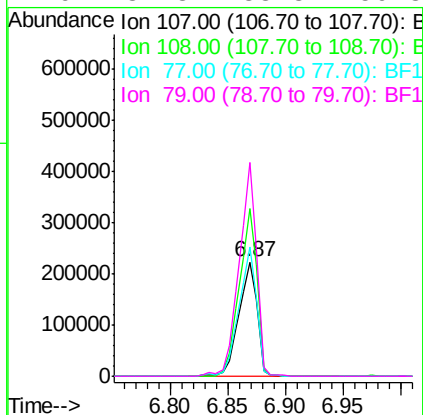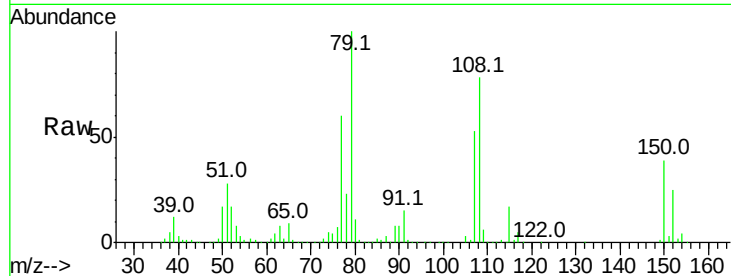

#20
3+4-Methylphenols
Concen: 3.629 ng
RT: 7.12 min Scan# 856
Delta R.T. -0.02 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Tgt Ion	Ratio	Lower	Upper
107	100		
108	79.9	68.2	108.2
77	32.2	26.7	66.7
79	21.7	6.3	46.3


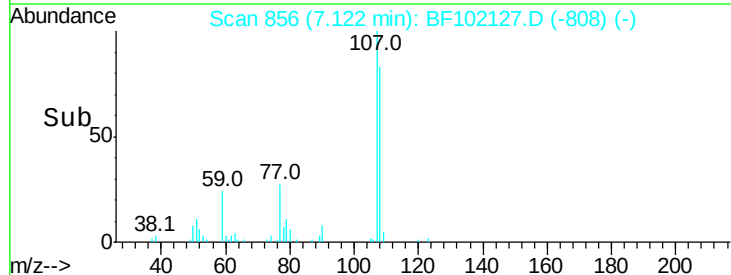
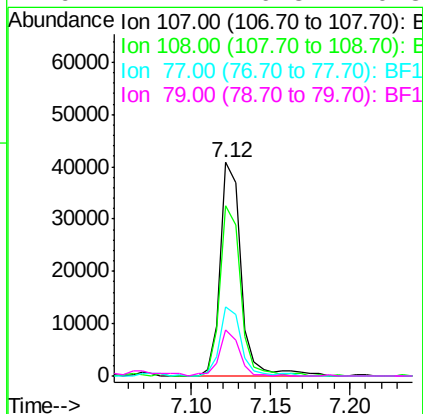



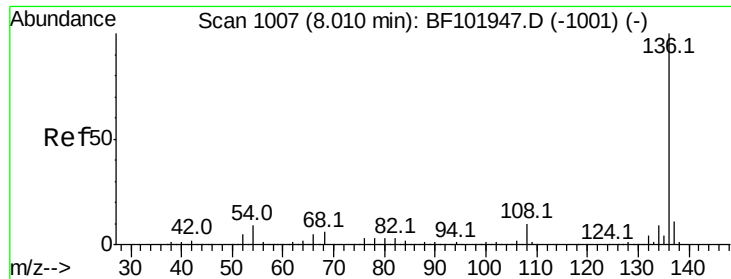

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.00 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16




Instrument :
BNA_F
ClientSampled :


Tot Ion:	136	Resp:	525966
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.9	13.3
54	7.0	6.6	9.8
68	4.9	5.0	7.4#

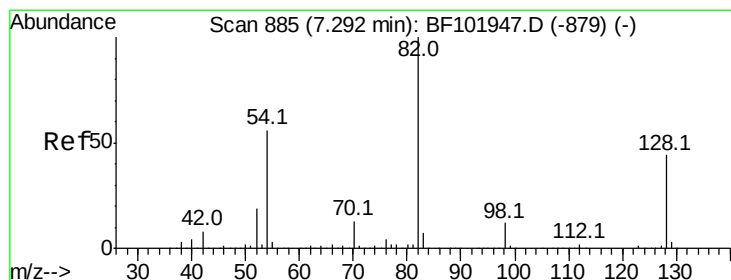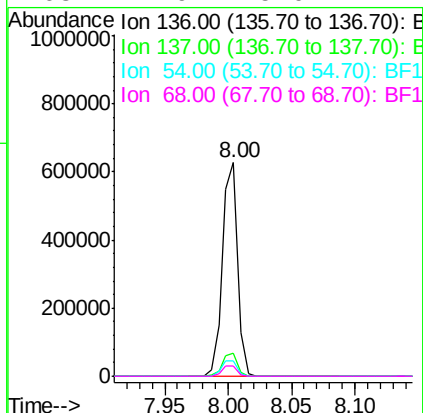

#23
Nitrobenzene-d5
Concen: 21.764 ng
RT: 7.28 min Scan# 883
Delta R.T. -0.02 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Tgt Ion:	82	Resp:	194797
Ion	Ratio	Lower	Upper
82	100		
128	46.0	36.1	54.1
54	53.2	41.4	62.2

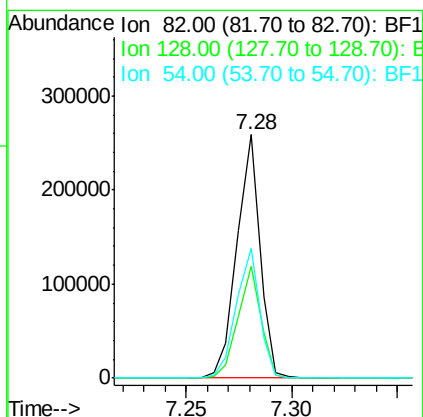

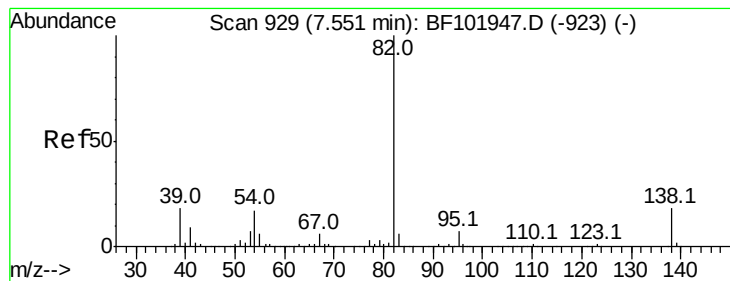

#25

Isophorone

Concen: 11.014 ng

RT: 7.28 min Scan# 883

Delta R.T. -0.27 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 194793

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

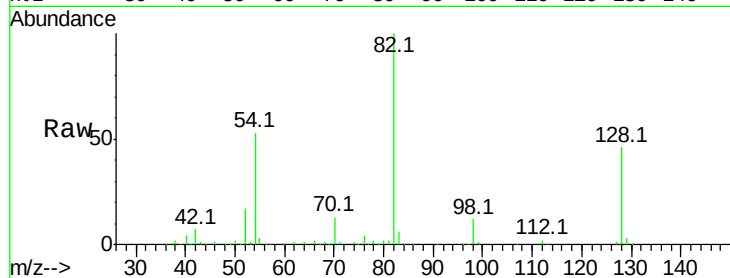

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

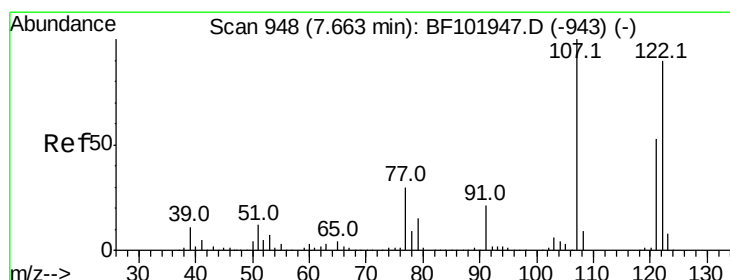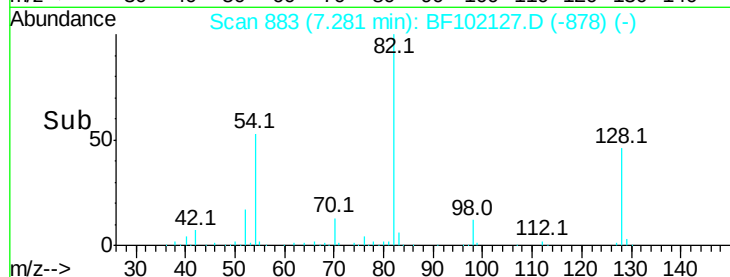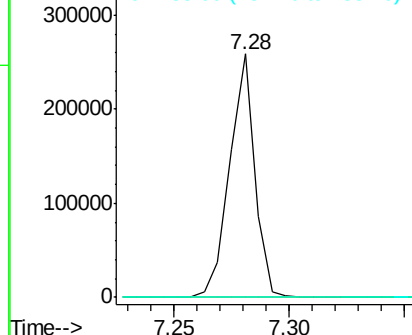

#27

2,4-Dimethylphenol

Concen: 57.146 ng

RT: 7.82 min Scan# 975

Delta R.T. 0.15 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16


Tgt Ion:122 Resp: 429620

Ion Ratio Lower Upper



122 100


107 0.6 91.2 136.8#

121 1.2 47.2 70.8#

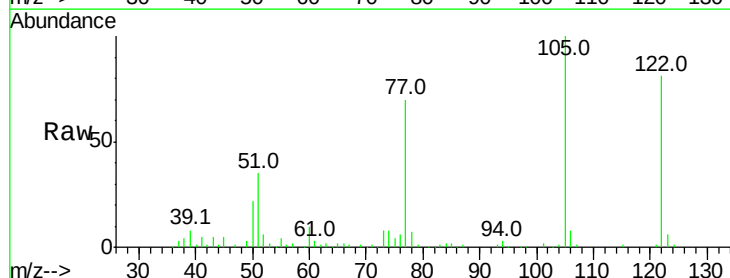

Abundance Ion 122.00 (121.70 to 122.70): E
Ion 107.00 (106.70 to 107.70): E
Ion 121.00 (120.70 to 121.70): E

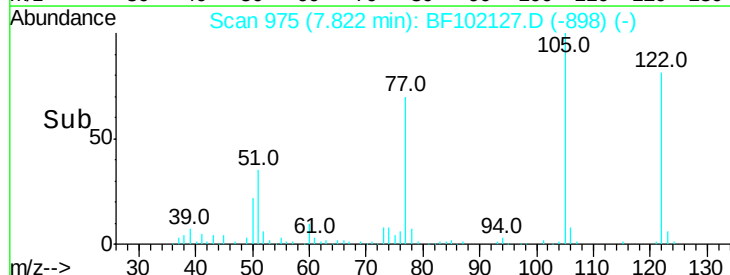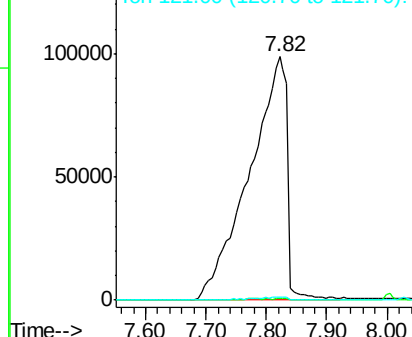

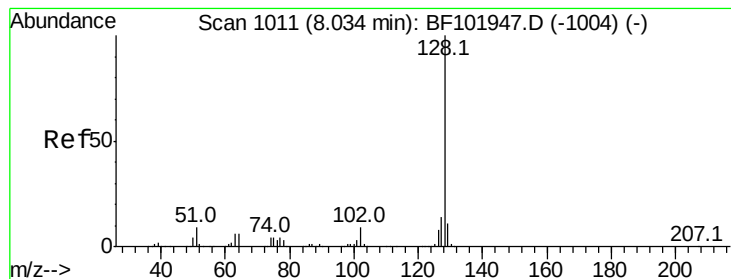

#31

Naphthalene

Concen: 2.637 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.01 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16

Instrument :

BNA_F

ClientSampleId :


Tot Ion:128 Resp: 69300

Ion Ratio Lower Upper

128 100

129 10.6 8.8 13.2




127 12.2 10.9 16.3



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

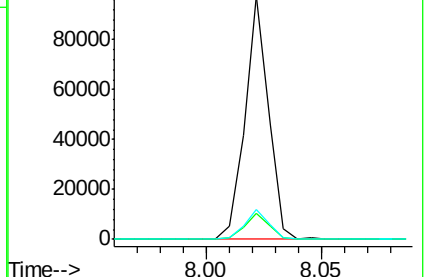

#32

Benzoic acid

Concen: 75.361 ng

RT: 7.82 min Scan# 975

Delta R.T. 0.04 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16


Tgt Ion:122 Resp: 429620

Ion Ratio Lower Upper

122 100

105 123.1 101.1 141.1



77 86.7 70.7 110.7




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1



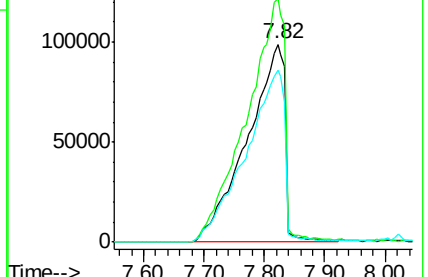





#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1303
 Delta R.T. -0.01 min
 Lab File: BF102127.D
 Acq: 16 Jan 2018 23:16




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	105.5	86.1	129.1
160	45.7	38.3	57.5

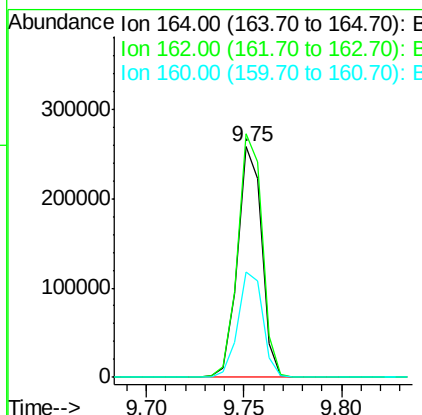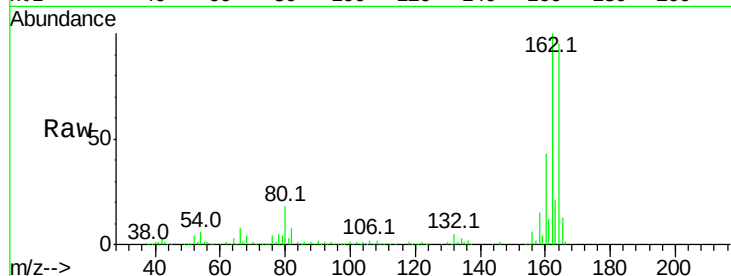

#41
 2,4,6-Tribromophenol
 Concen: 35.167 ng
 RT: 10.54 min Scan# 1437
 Delta R.T. -0.01 min
 Lab File: BF102127.D
 Acq: 16 Jan 2018 23:16

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.0	115.6
141	39.6	29.9	44.9

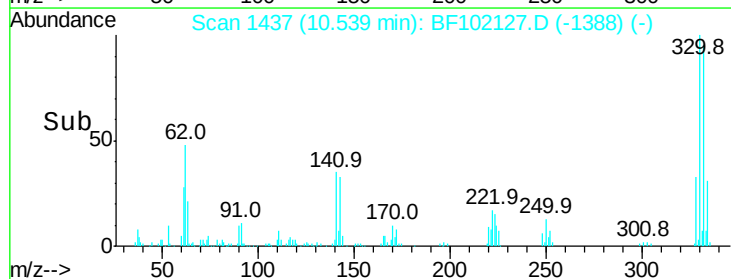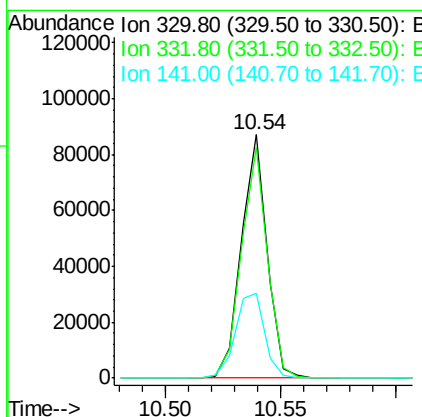


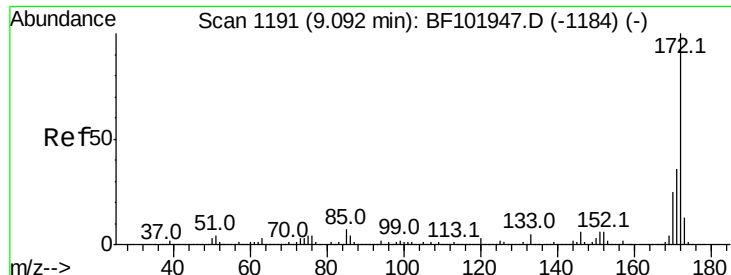




#44
 2-Fluorobiphenyl
 Concen: 26.420 ng
 RT: 9.07 min Scan# 1188
 Delta R.T. -0.02 min
 Lab File: BF102127.D
 Acq: 16 Jan 2018 23:16

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 374475
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.7 44.5
 170 23.9 19.6 29.4

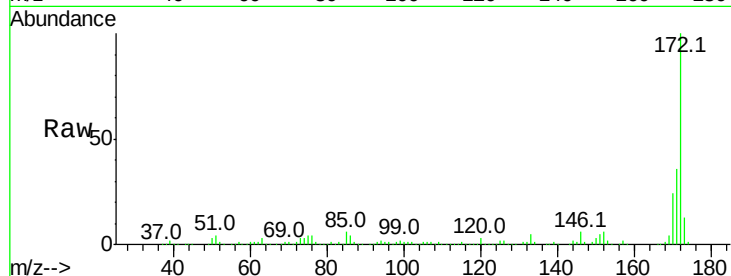


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

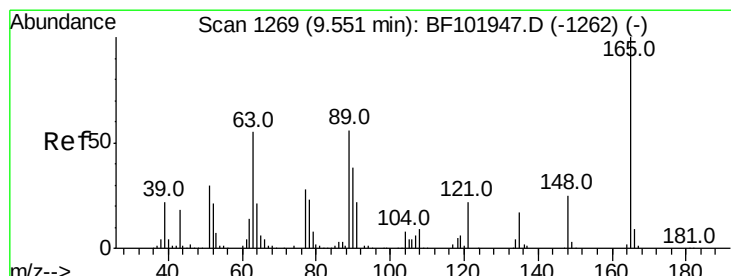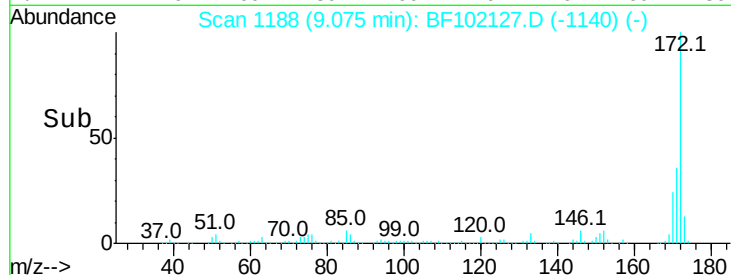
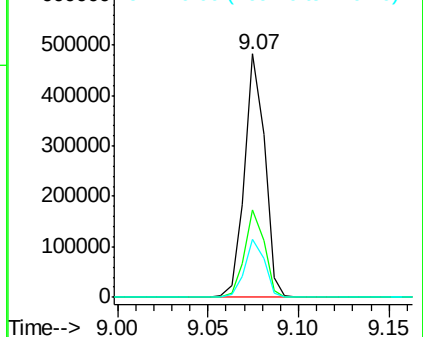



#50
 2,6-Dinitrotoluene
 Concen: 8.238 ng
 RT: 9.75 min Scan# 1303
 Delta R.T. 0.20 min
 Lab File: BF102127.D
 Acq: 16 Jan 2018 23:16

Tgt Ion:165 Resp: 29232
 Ion Ratio Lower Upper
 165 100
 63 1.2 44.7 67.1#
 89 1.6 44.0 66.0#

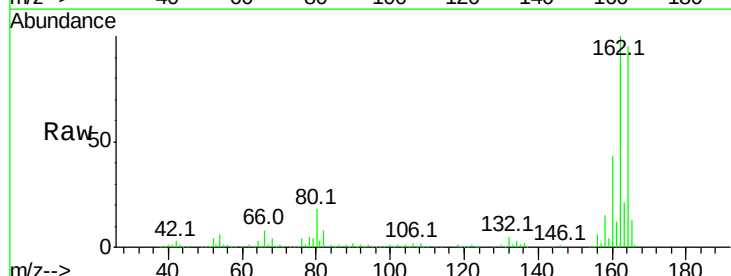

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1




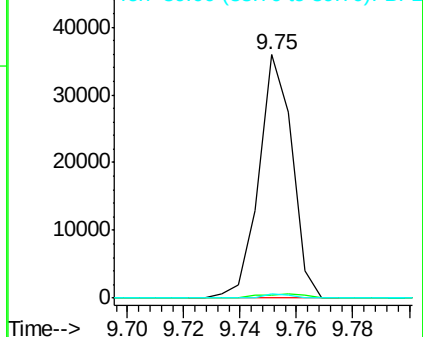




#56
2,4-Dinitrotoluene
Concen: 6.573 ng
RT: 9.75 min Scan# 1303
Delta R.T. -0.20 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16




Instrument :
BNA_F
ClientSampled :


Tot Ion:	165	Resp:	29232
Ion	Ratio	Lower	Upper
165	100		
63	1.2	36.4	54.6#
89	1.6	57.8	86.6#
182	0.0	1.6	2.4#

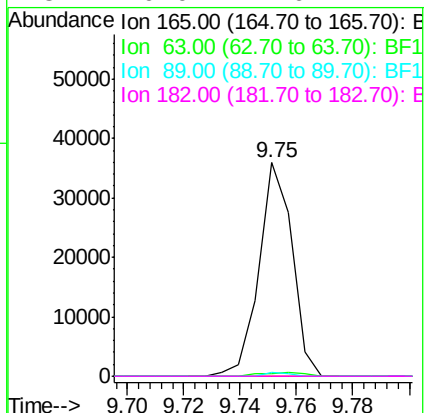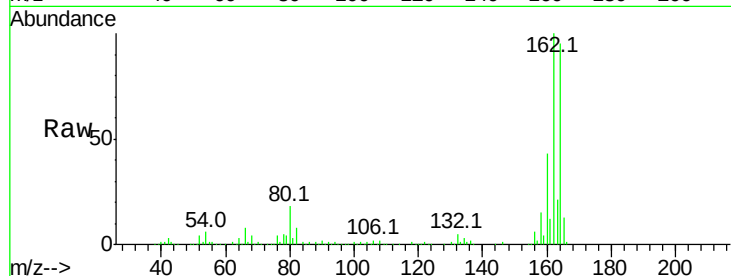

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.23 min Scan# 1555
Delta R.T. -0.01 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Tgt Ion:	188	Resp:	337552
Ion	Ratio	Lower	Upper
188	100		
94	9.8	8.5	12.7
80	10.8	9.2	13.8

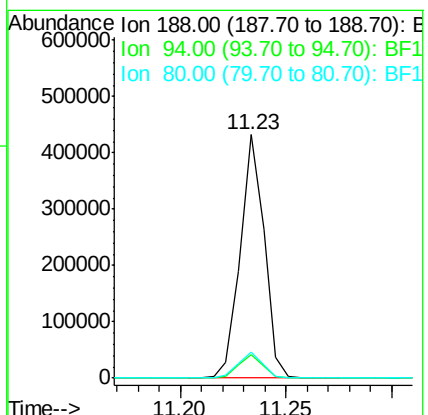



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.86 min Scan# 2002

Delta R.T. -0.02 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 231911

Ion Ratio Lower Upper

240 100

120 13.0 9.5 14.3




236 24.9 20.7 31.1

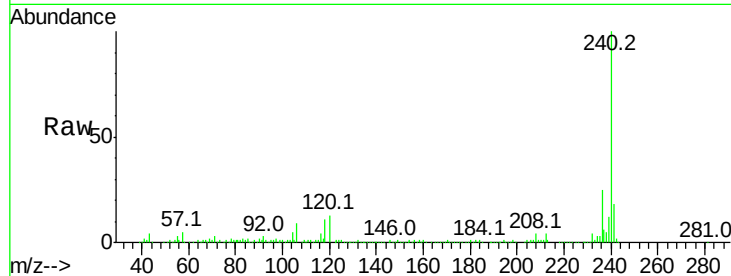

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

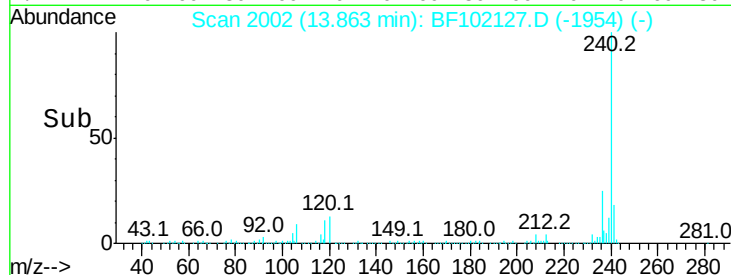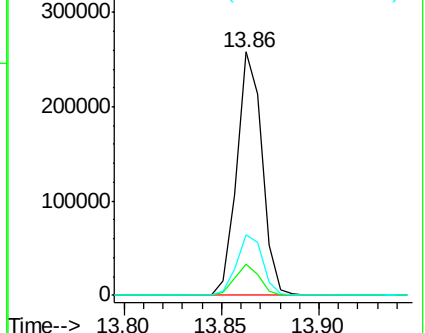

#78

Terphenyl-d14

Concen: 21.121 ng

RT: 12.82 min Scan# 1824

Delta R.T. -0.02 min

Lab File: BF102127.D

Acq: 16 Jan 2018 23:16


Tgt Ion:244 Resp: 235919

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 13.1 11.0 16.4

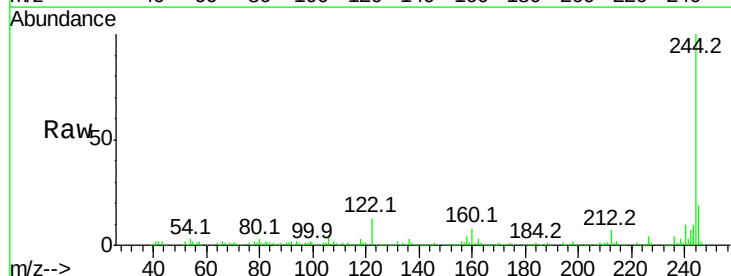


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

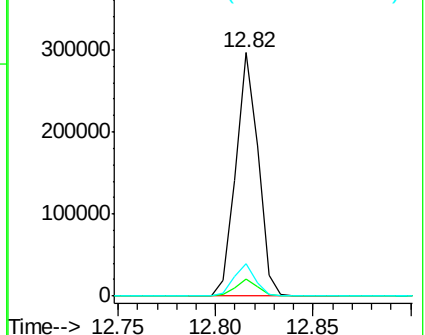


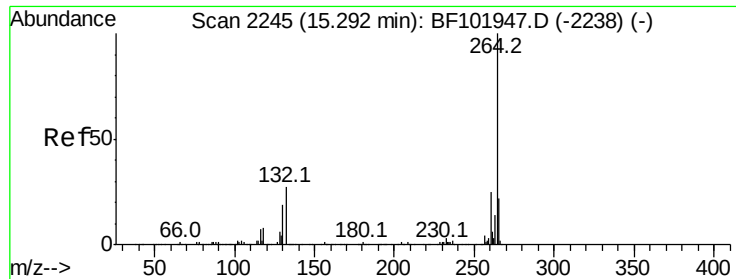

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.28 min Scan# 2243
Delta R.T. -0.01 min
Lab File: BF102127.D
Acq: 16 Jan 2018 23:16

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	20.6	17.5	26.3

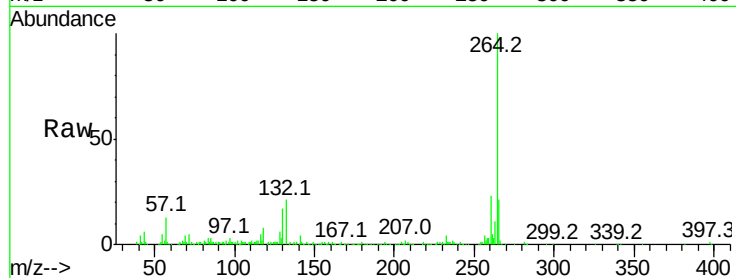

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

